

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042823\
 Data File : VY013523.D
 Acq On : 28 Apr 2023 14:07
 Operator : KP/MD
 Sample : 02503-10
 Misc : 5.23g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TR-305A-VOC-02

Quant Time: Apr 28 23:13:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	11335	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	18439	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	19051	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	7543	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	11659	93.830	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	187.660%#
35) Dibromofluoromethane	7.716	113	7997	68.956	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	137.920%
50) Toluene-d8	10.179	98	23657	57.342	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	114.680%
62) 4-Bromofluorobenzene	12.483	95	7486	53.823	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	107.640%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY042823\
Data File : VY013523.D
Acq On : 28 Apr 2023 14:07
Operator : KP/MD
Sample : 02503-10
Misc : 5.23g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TR-305A-VOC-02

Quant Time: Apr 28 23:13:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration




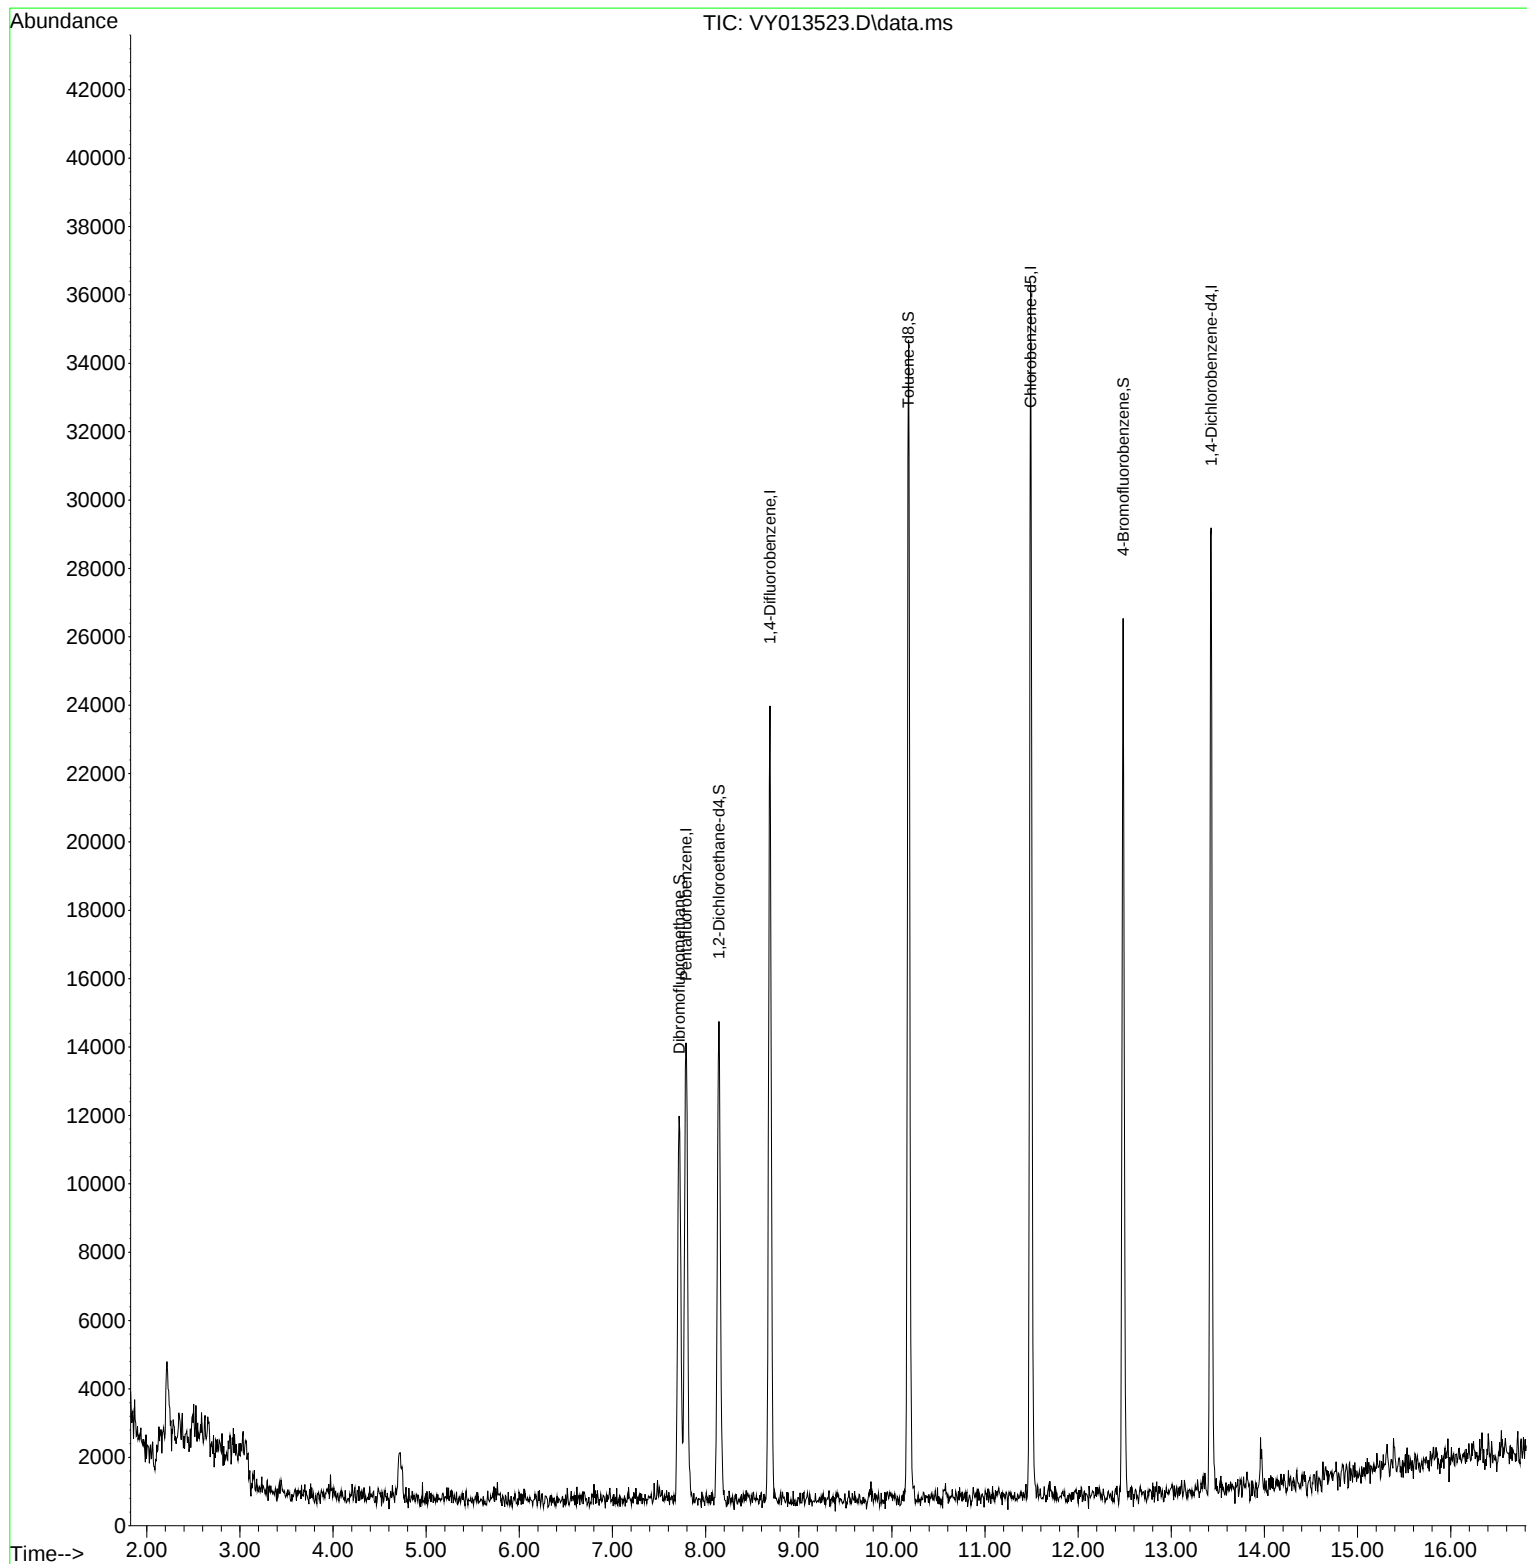


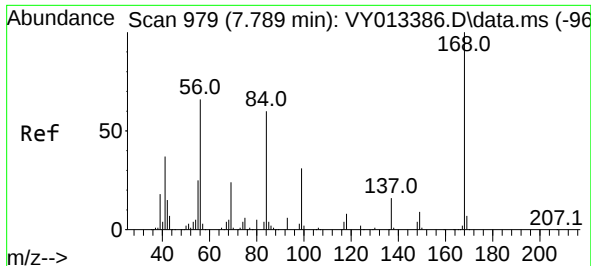

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY013523.D
Acq: 28 Apr 2023 14:07




Instrument :
MSVOA_Y
ClientSampleId :
TR-305A-VOC-02


Tgt Ion:168 Resp: 11335
Ion Ratio Lower Upper
168 100
99 46.6 41.8 62.6

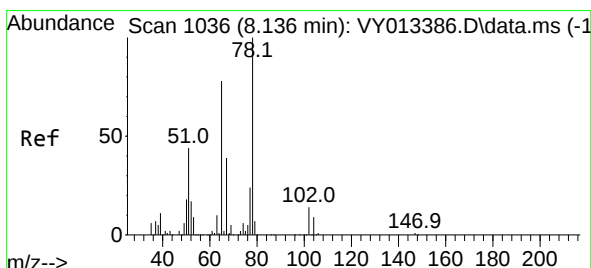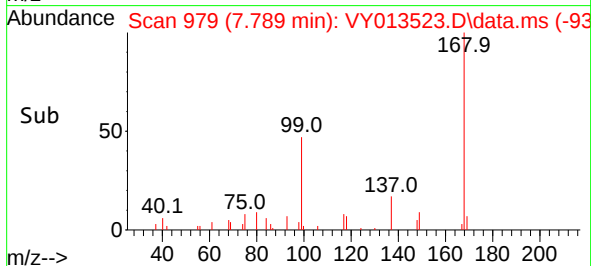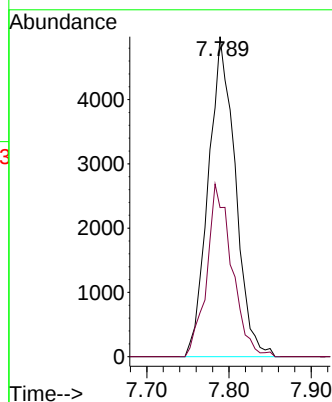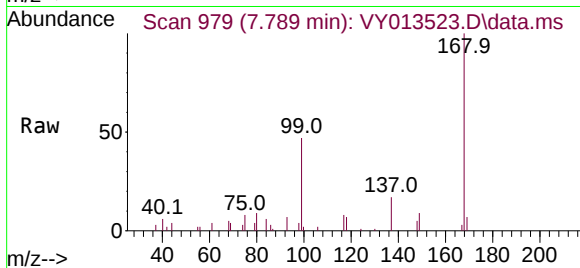

#33
1,2-Dichloroethane-d4
Concen: 93.830 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.007 min
Lab File: VY013523.D
Acq: 28 Apr 2023 14:07

Tgt Ion: 65 Resp: 11659
Ion Ratio Lower Upper
65 100
67 51.5 0.0 103.4


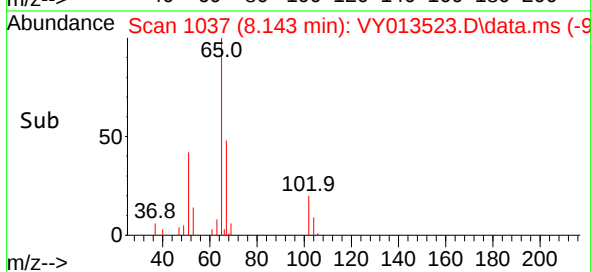
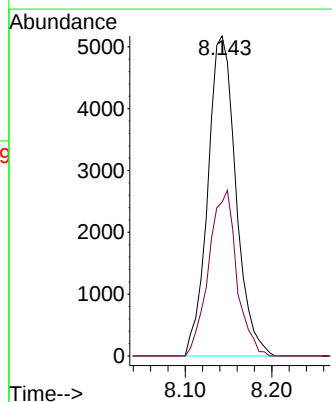
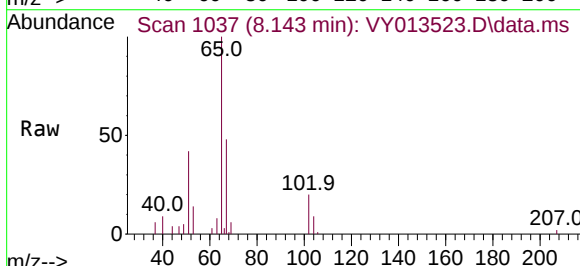


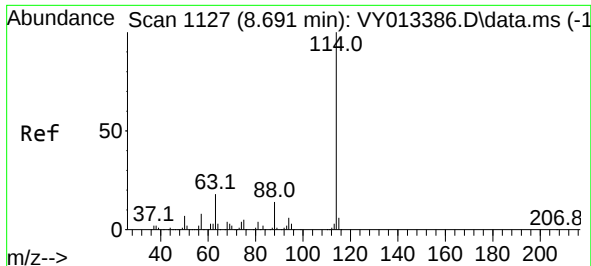

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VY013523.D
Acq: 28 Apr 2023 14:07




Instrument :
MSVOA_Y
ClientSampleId :
TR-305A-VOC-02


Tgt Ion:	114	Resp:	18439
Ion Ratio	Lower	Upper	
114	100		
63	21.8	0.0	36.6
88	15.6	0.0	28.8

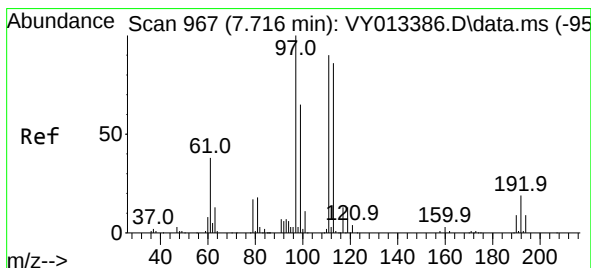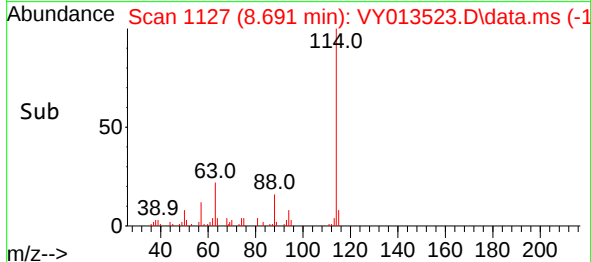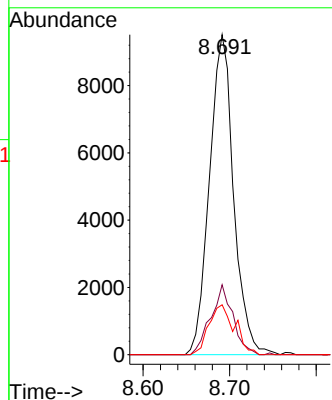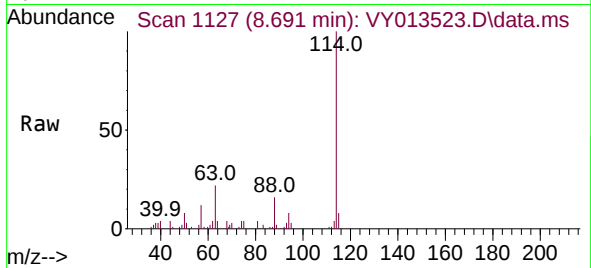

#35
Dibromofluoromethane
Concen: 68.956 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY013523.D
Acq: 28 Apr 2023 14:07

Tgt Ion:	113	Resp:	7997
Ion Ratio	Lower	Upper	
113	100		
111	100.3	82.2	123.2
192	24.2	16.7	25.1


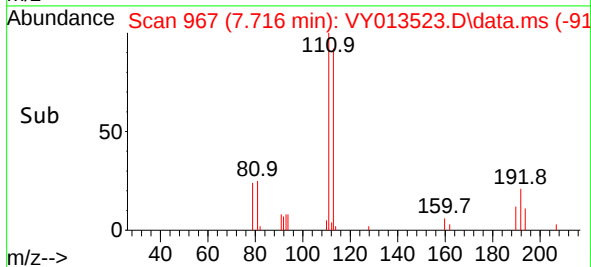
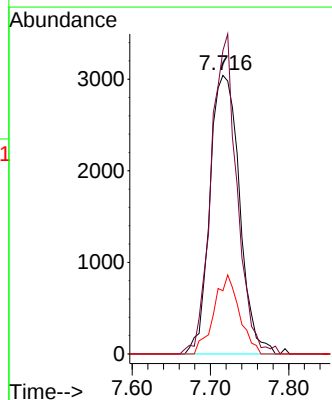
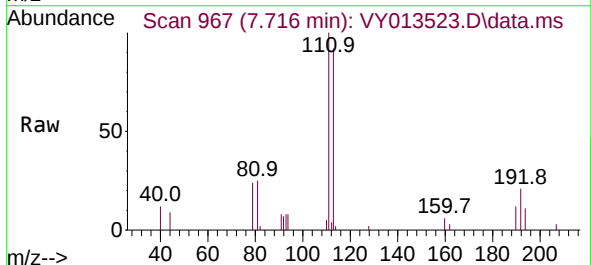


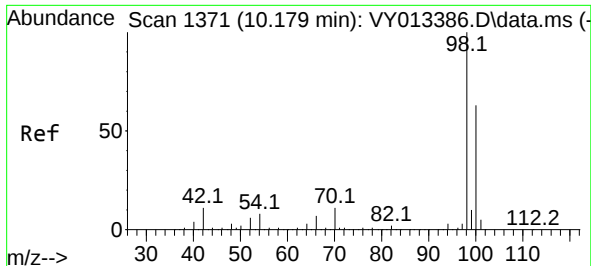

#50
Toluene-d8
Concen: 57.342 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013523.D
Acq: 28 Apr 2023 14:07




Instrument :
MSVOA_Y
ClientSampleId :
TR-305A-VOC-02


Tgt Ion: 98 Resp: 23657
Ion Ratio Lower Upper
98 100
100 58.4 50.5 75.7

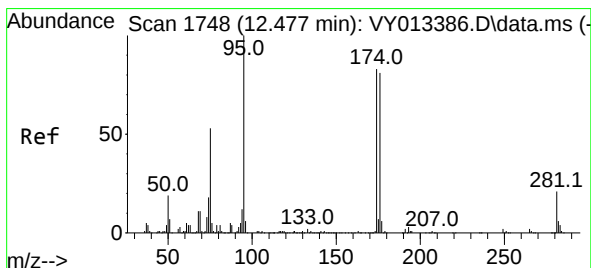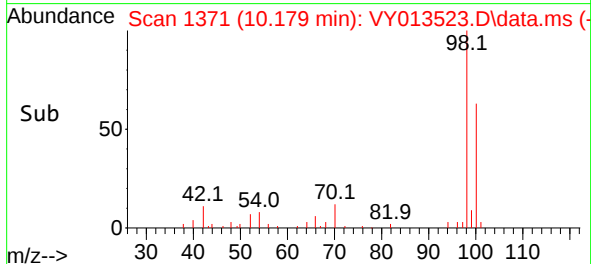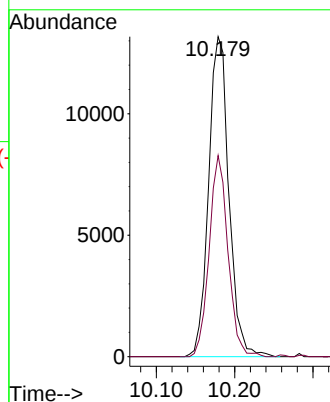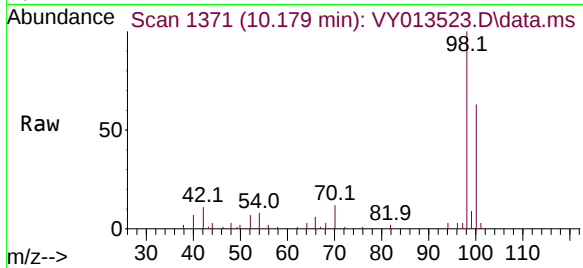

#62
4-Bromofluorobenzene
Concen: 53.823 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY013523.D
Acq: 28 Apr 2023 14:07

Tgt Ion: 95 Resp: 7486
Ion Ratio Lower Upper
95 100
174 94.9 0.0 182.0
176 88.2 0.0 175.4

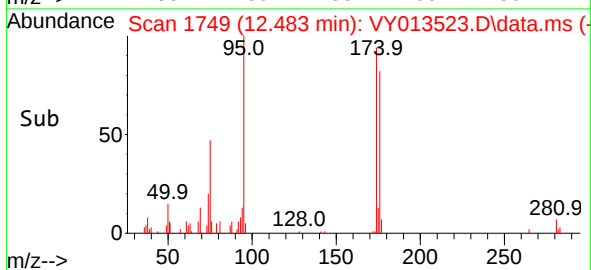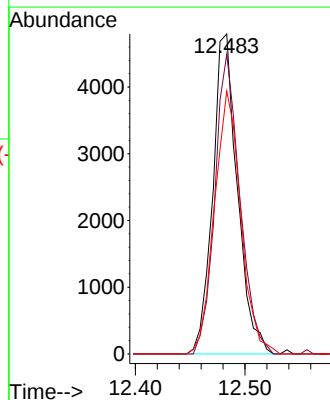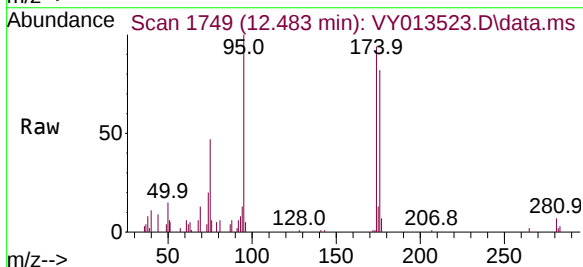

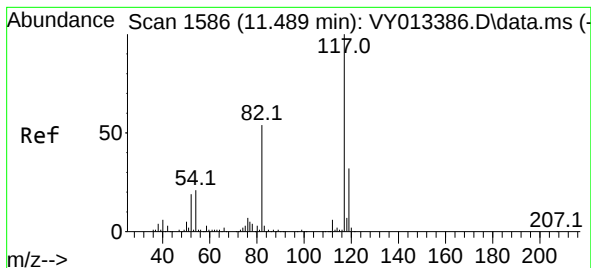

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.001 min

Lab File: VY013523.D

Acq: 28 Apr 2023 14:07

Instrument :

MSVOA_Y

ClientSampleId :

TR-305A-VOC-02





Tgt Ion:117 Resp: 19051

Ion Ratio Lower Upper

117 100

82 49.4 43.0 64.6

119 35.8 25.5 38.3

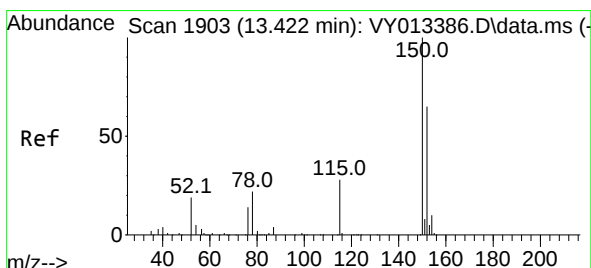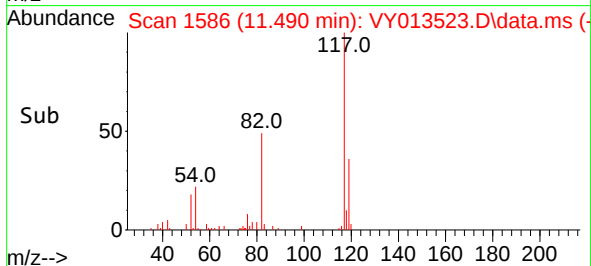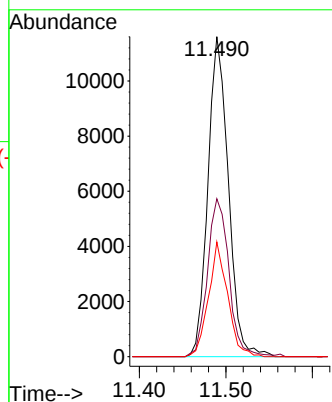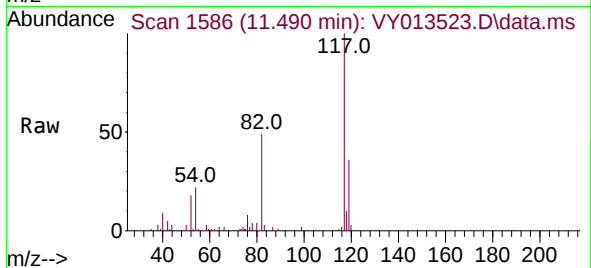

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY013523.D

Acq: 28 Apr 2023 14:07

Tgt Ion:152 Resp: 7543

Ion Ratio Lower Upper

152 100

115 57.4 28.1 84.2

150 159.8 0.0 352.0

