
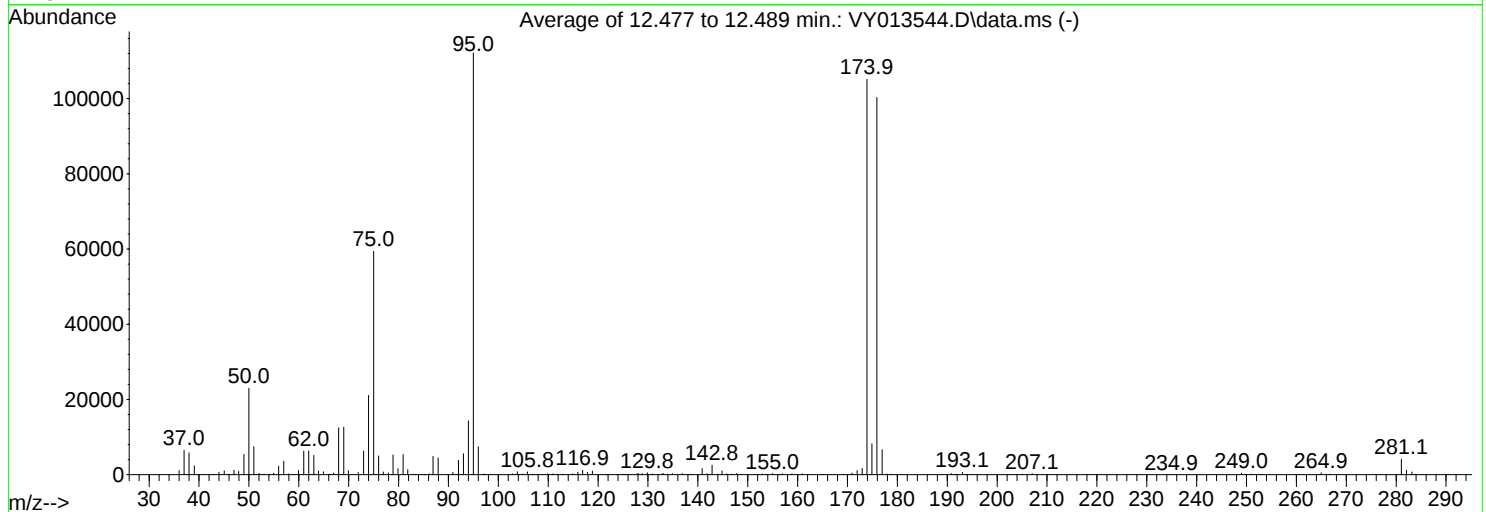


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050223\
Data File : VY013544.D
Acq On : 02 May 2023 09:21
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Title : SW846 8260
Last Update : Tue Apr 25 02:39:58 2023

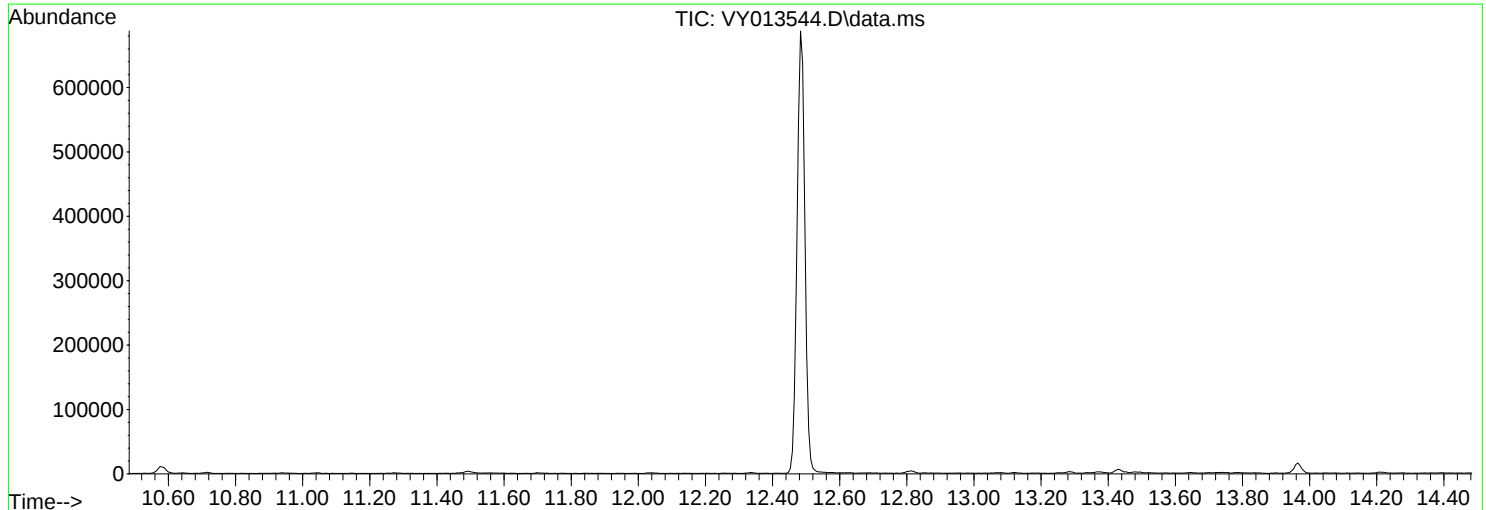

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	22965	PASS
75	95	30	60	53.0	59416	PASS
95	95	100	100	100.0	112195	PASS
96	95	5	9	6.6	7425	PASS
173	174	0.00	2	1.6	1648	PASS
174	95	50	100	93.7	105160	PASS
175	174	5	9	7.8	8201	PASS
176	174	95	101	95.4	100325	PASS
177	176	5	9	6.6	6649	PASS