
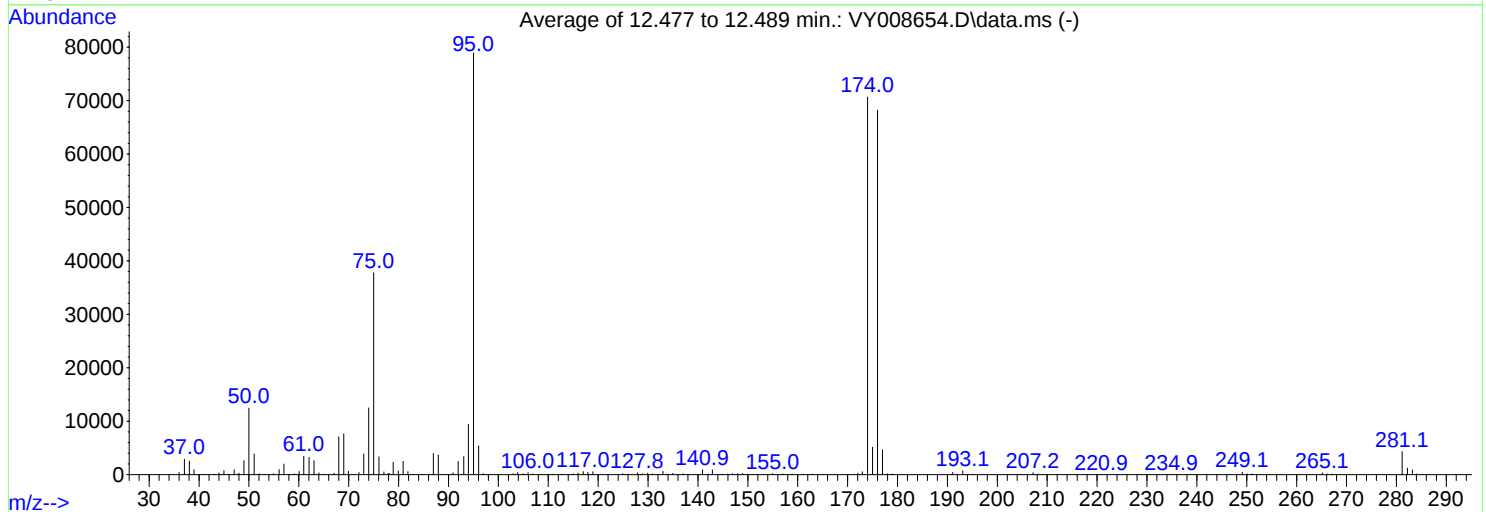


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY050922\
 Data File : VY008654.D
 Acq On : 09 May 2022 08:54
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y050922S.M
 Title : SW846 8260
 Last Update : Mon May 09 19:21:20 2022

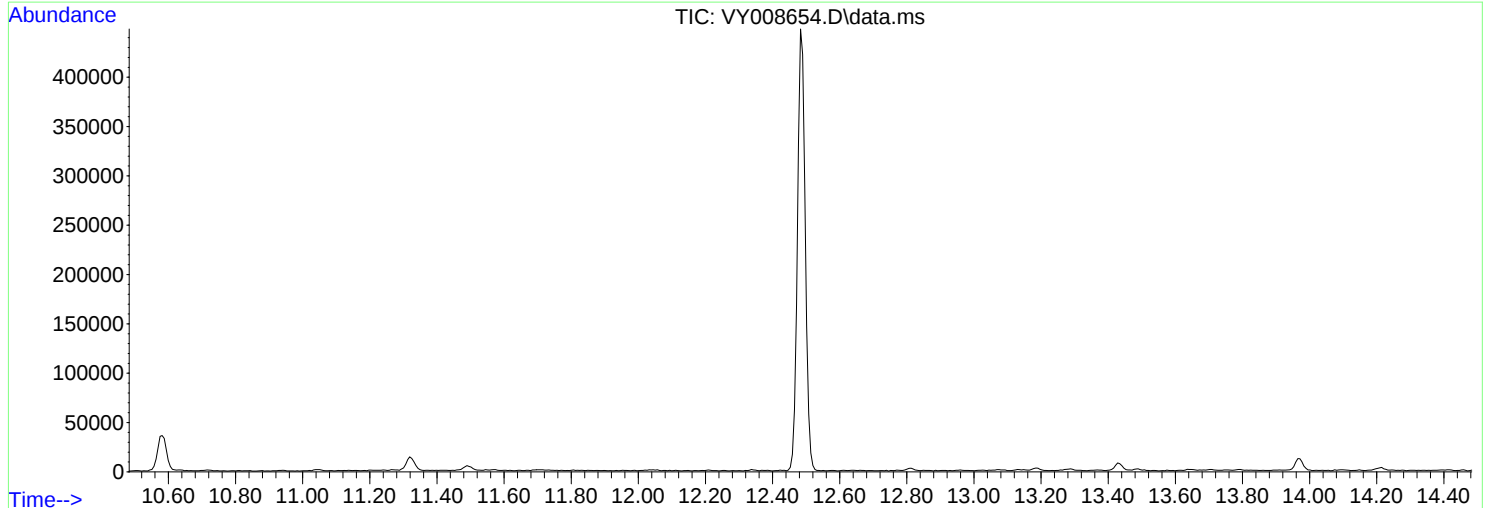

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	12444	PASS
75	95	30	60	47.9	37800	PASS
95	95	100	100	100.0	78944	PASS
96	95	5	9	6.8	5376	PASS
173	174	0.00	2	0.8	543	PASS
174	95	50	100	89.5	70683	PASS
175	174	5	9	7.3	5127	PASS
176	174	95	101	96.5	68197	PASS
177	176	5	9	6.8	4644	PASS