


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY050923\  
Data File : VY013655.D  
Acq On : 09 May 2023 09:11  
Operator : KP/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y042423S.M  
Title : SW846 8260  
Last Update : Tue Apr 25 02:39:58 2023

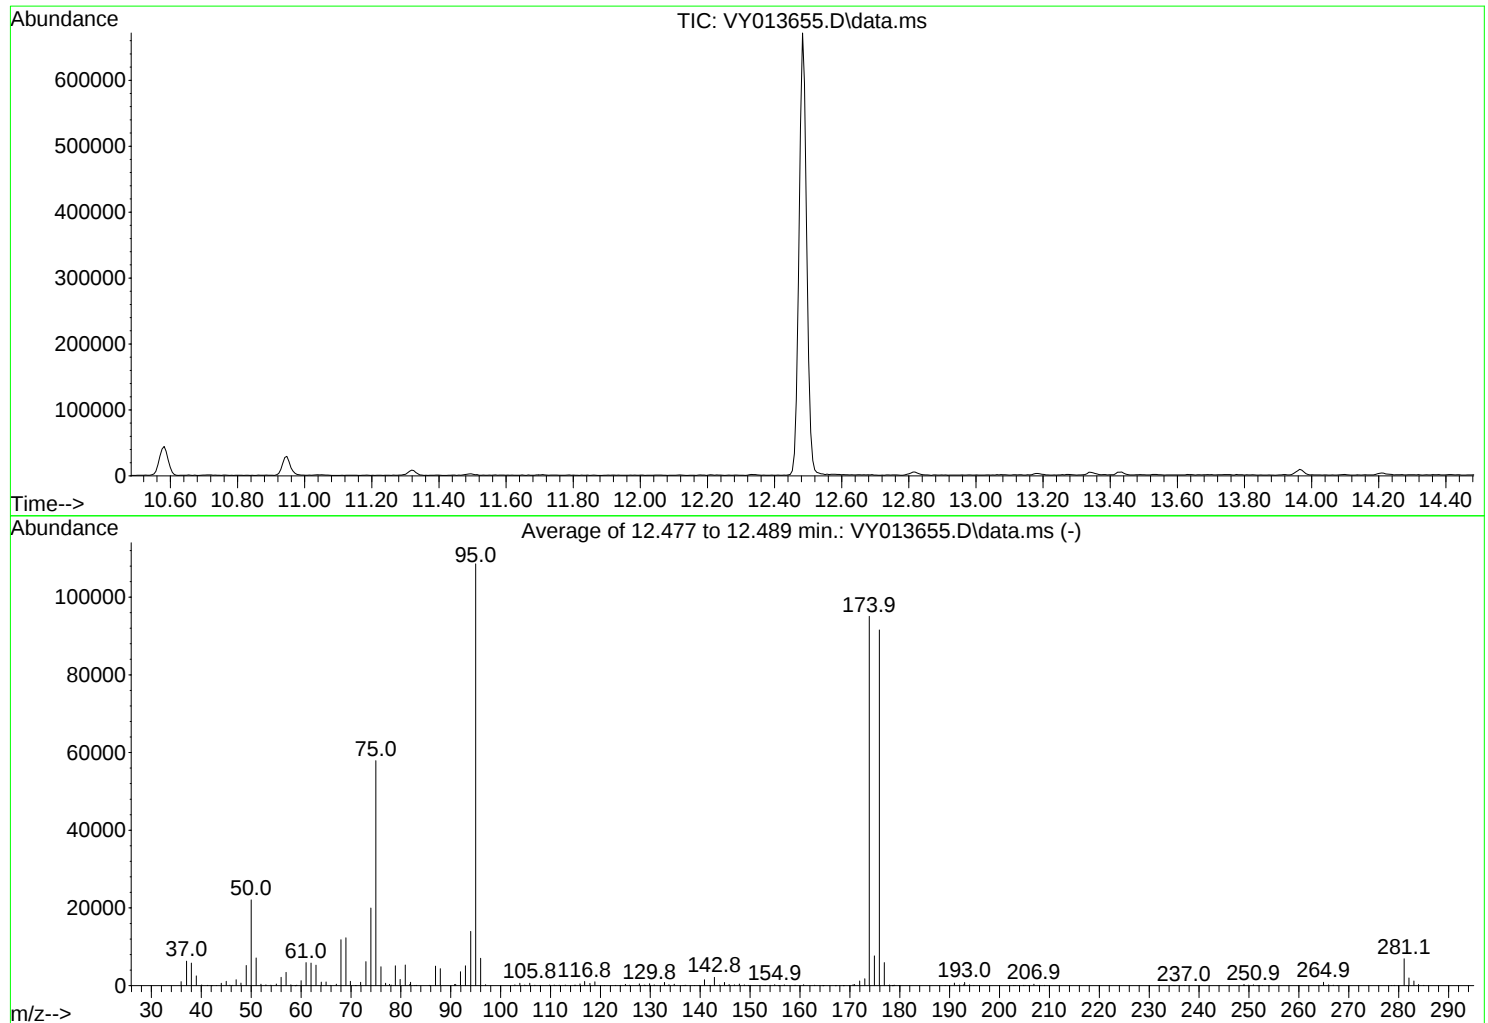

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 50     | 95      | 15     | 40     | 20.3  | 22061  | PASS      |
| 75     | 95      | 30     | 60     | 53.3  | 57912  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 108573 | PASS      |
| 96     | 95      | 5      | 9      | 6.5   | 7058   | PASS      |
| 173    | 174     | 0.00   | 2      | 1.9   | 1772   | PASS      |
| 174    | 95      | 50     | 100    | 87.5  | 95037  | PASS      |
| 175    | 174     | 5      | 9      | 8.0   | 7647   | PASS      |
| 176    | 174     | 95     | 101    | 96.3  | 91563  | PASS      |
| 177    | 176     | 5      | 9      | 6.5   | 5952   | PASS      |