

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051023\
 Data File : VY013691.D
 Acq On : 10 May 2023 16:30
 Operator : KP/MD
 Sample : VIBLK
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VIBLK

Quant Time: May 11 03:29:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	193562	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	328765	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	322237	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	148133	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	137772	64.930	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	129.860%
35) Dibromofluoromethane	7.716	113	112475	54.394	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.780%
50) Toluene-d8	10.179	98	403206	54.814	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	109.620%
62) 4-Bromofluorobenzene	12.483	95	130382	52.576	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	105.160%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051023\
Data File : VY013691.D
Acq On : 10 May 2023 16:30
Operator : KP/MD
Sample : VIBLK
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VIBLK

Quant Time: May 11 03:29:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration




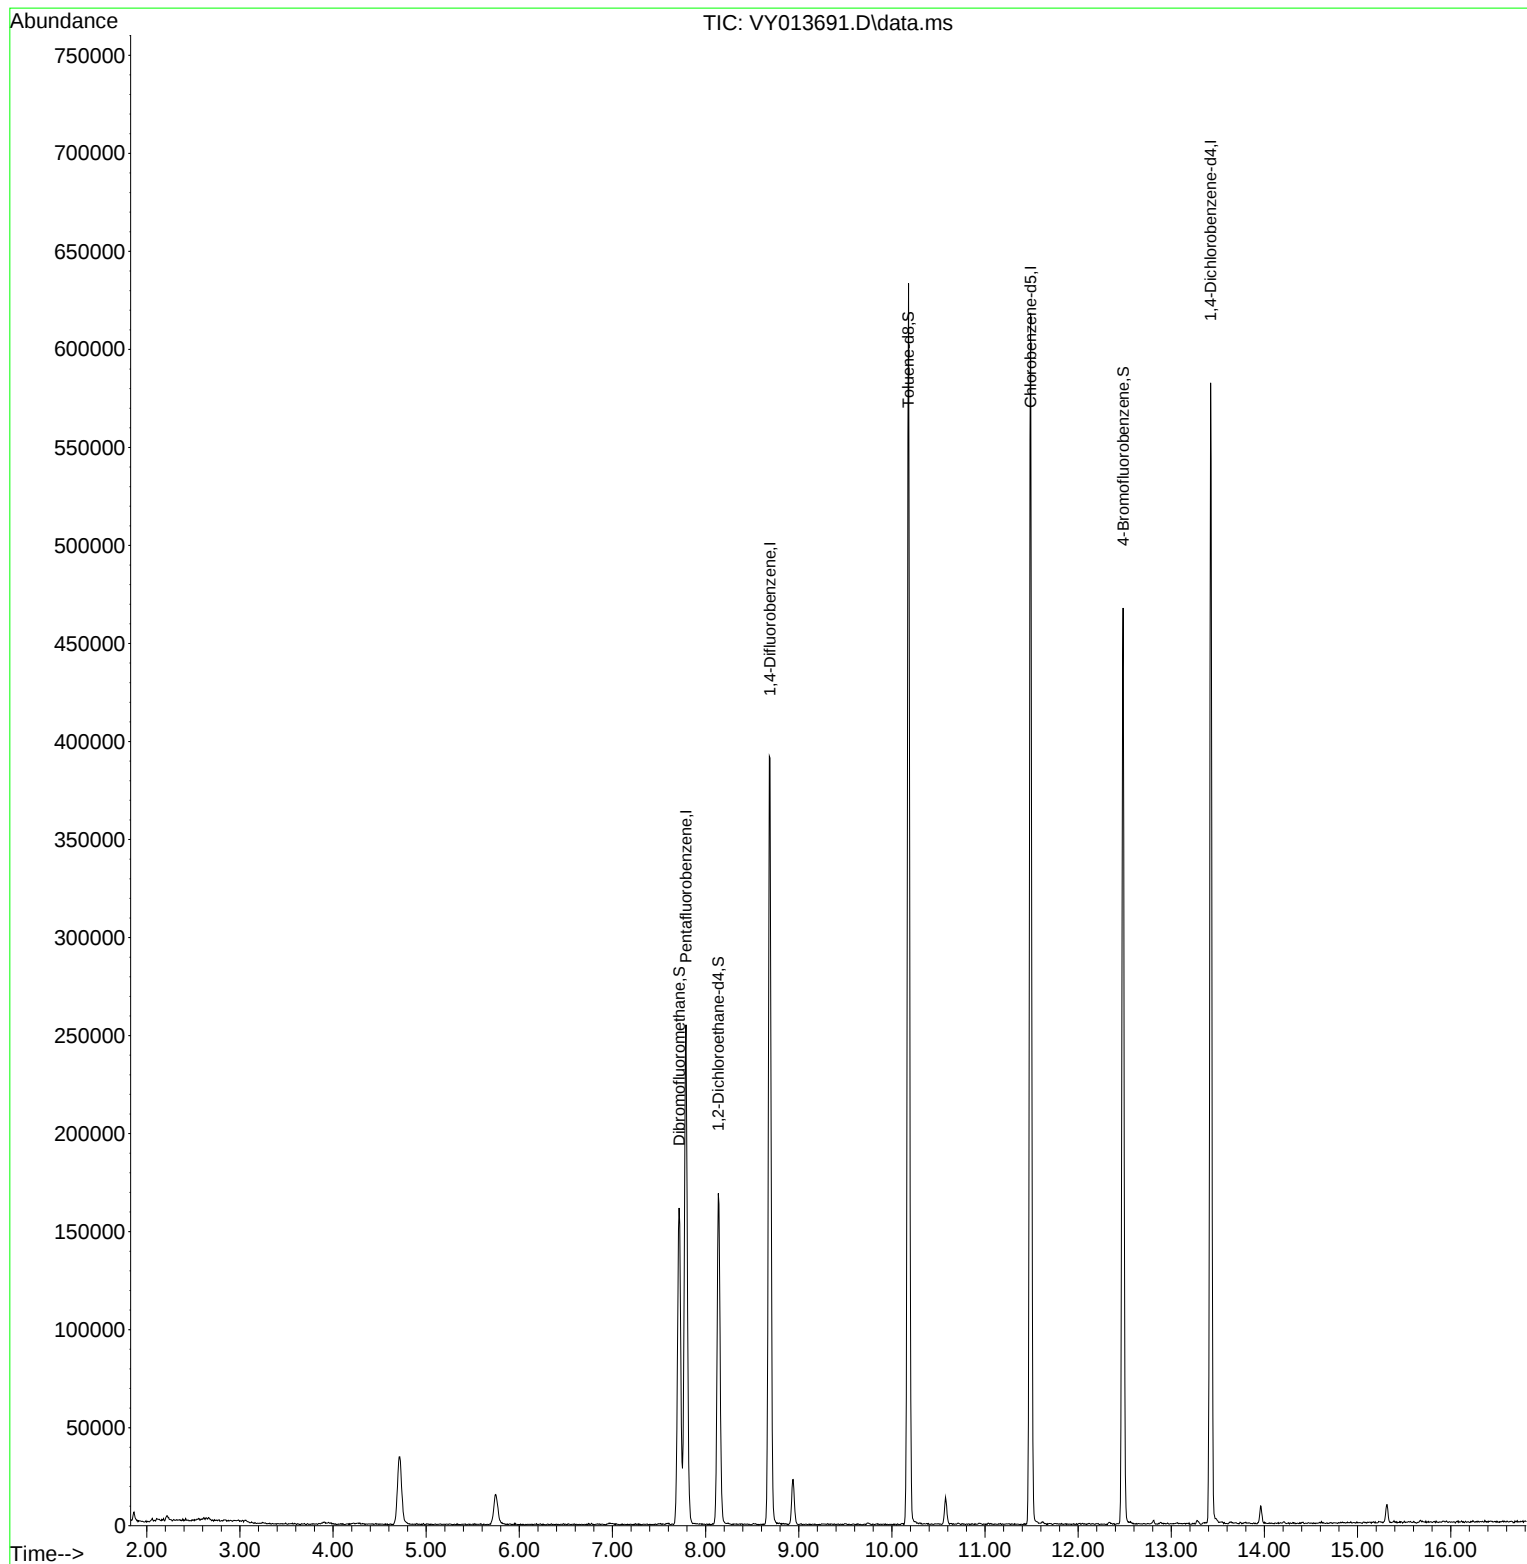




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY013691.D
Acq: 10 May 2023 16:30




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK

Tgt Ion:168 Resp: 193562
Ion Ratio Lower Upper
168 100
99 52.1 41.8 62.6

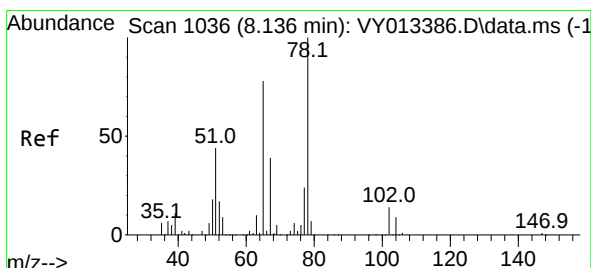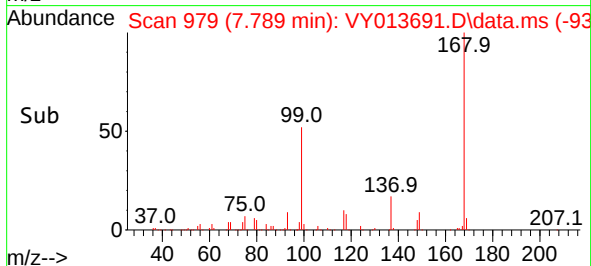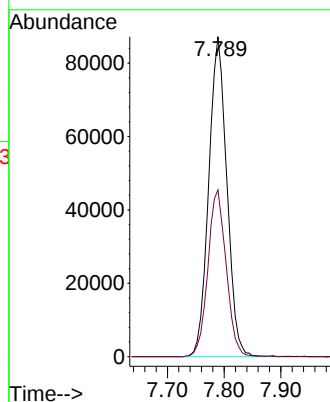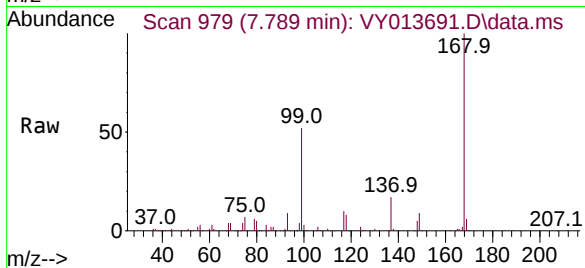

#33
1,2-Dichloroethane-d4
Concen: 64.930 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. 0.001 min
Lab File: VY013691.D
Acq: 10 May 2023 16:30

Tgt Ion: 65 Resp: 137772
Ion Ratio Lower Upper
65 100
67 51.3 0.0 103.4

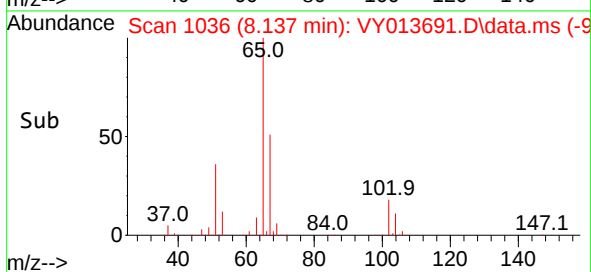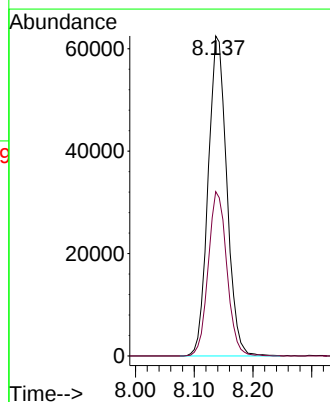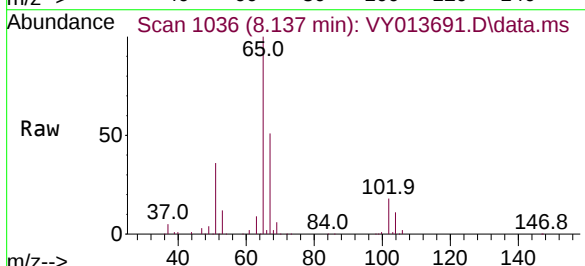



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY013691.D

Acq: 10 May 2023 16:30

Instrument :

MSVOA_Y

ClientSampleId :

VIBLK




Tgt Ion:114 Resp: 328765

Ion Ratio Lower Upper

114 100

63 20.9 0.0 36.6

88 14.7 0.0 28.8

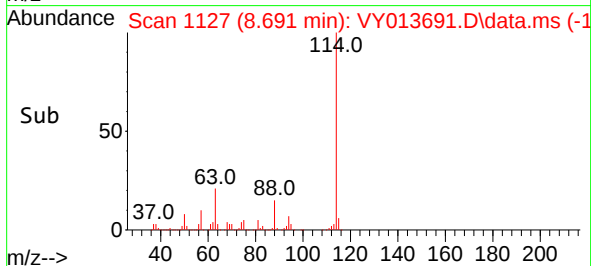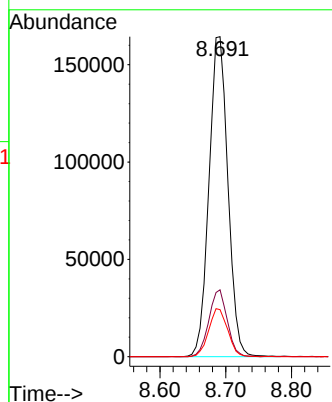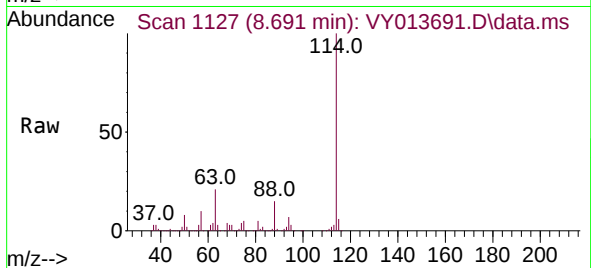

#35

Dibromofluoromethane

Concen: 54.394 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY013691.D

Acq: 10 May 2023 16:30




Tgt Ion:113 Resp: 112475


Ion Ratio Lower Upper

113 100

111 101.8 82.2 123.2

192 21.1 16.7 25.1


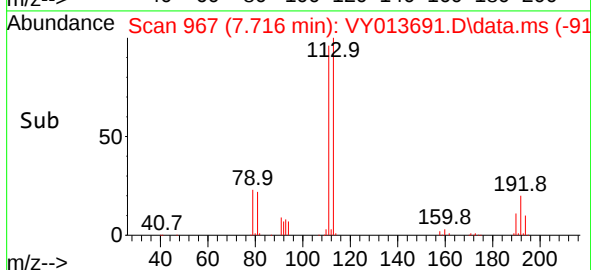
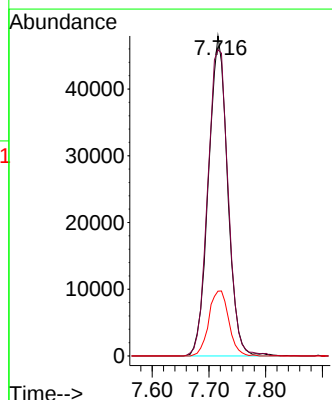
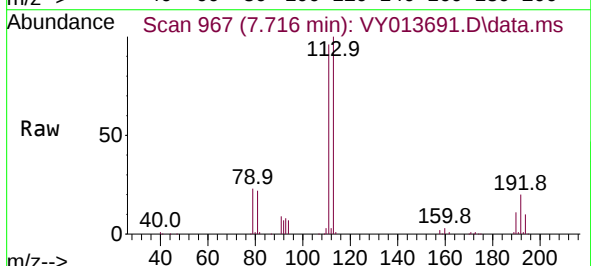


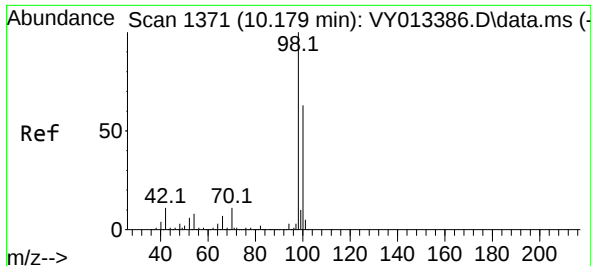

#50
Toluene-d8
Concen: 54.814 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY013691.D
Acq: 10 May 2023 16:30




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 403206
Ion Ratio Lower Upper
98 100
100 63.0 50.5 75.7

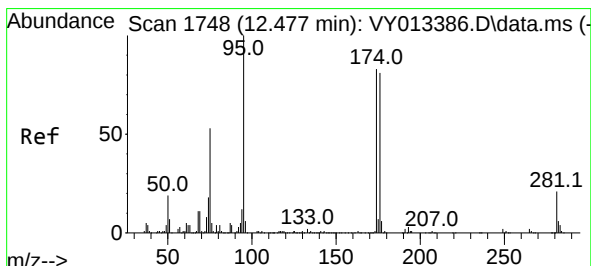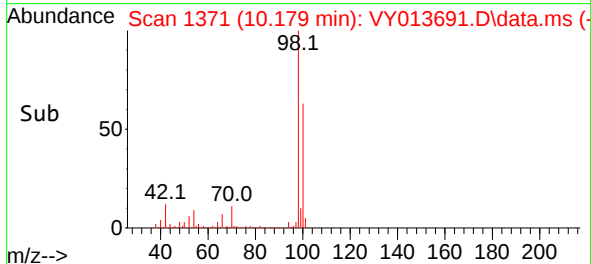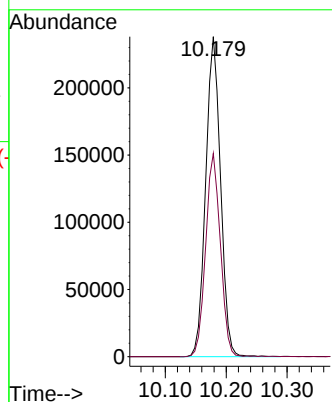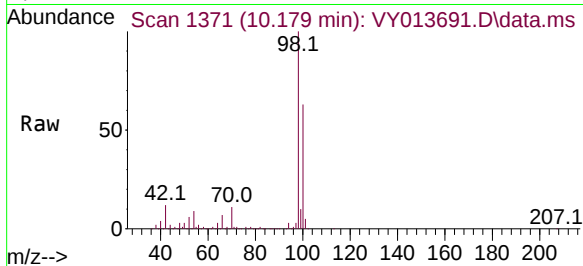

#62
4-Bromofluorobenzene
Concen: 52.576 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY013691.D
Acq: 10 May 2023 16:30

Tgt Ion: 95 Resp: 130382
Ion Ratio Lower Upper
95 100
174 92.3 0.0 182.0
176 89.7 0.0 175.4

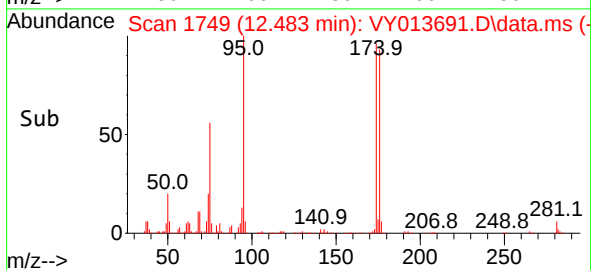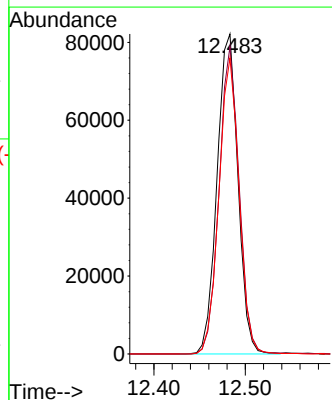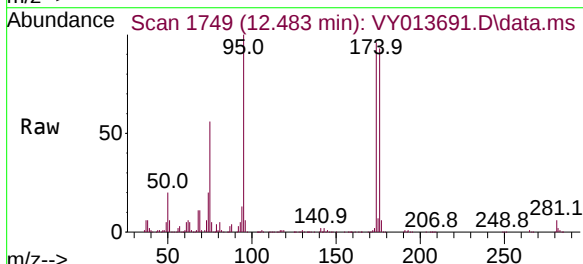

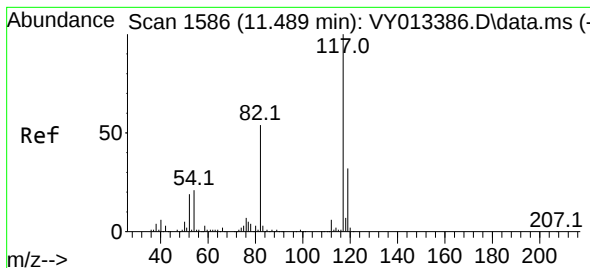

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.001 min

Lab File: VY013691.D

Acq: 10 May 2023 16:30

Instrument :

MSVOA_Y

ClientSampleId :

VIBLK





Tgt Ion:117 Resp: 322237

Ion Ratio Lower Upper

117 100

82 54.3 43.0 64.6

119 32.2 25.5 38.3

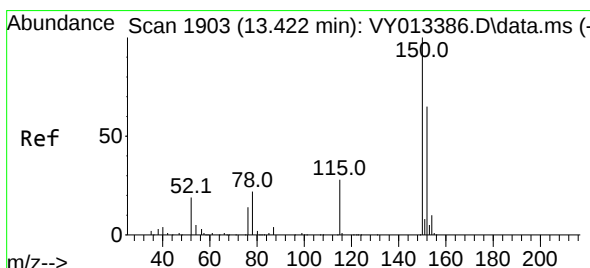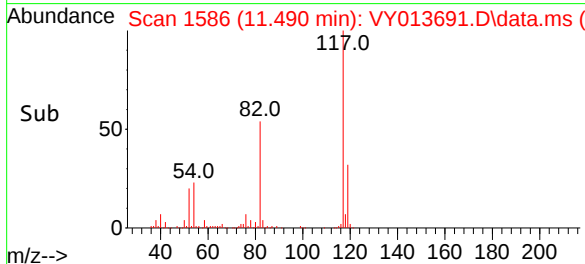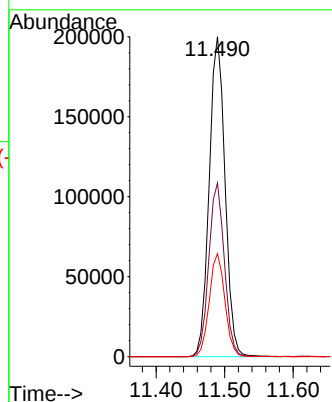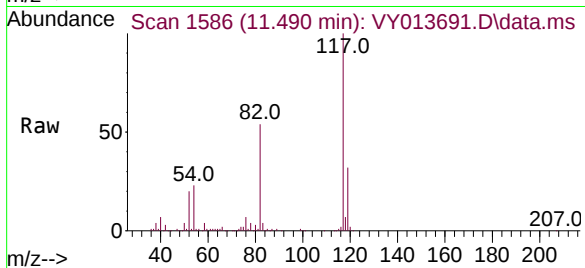

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY013691.D

Acq: 10 May 2023 16:30

Tgt Ion:152 Resp: 148133

Ion Ratio Lower Upper

152 100

115 56.8 28.1 84.2

150 156.7 0.0 352.0

