

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051322\
 Data File : VY008746.D
 Acq On : 13 May 2022 14:04
 Operator : KP/MD
 Sample : N2781-04
 Misc : 6.30g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 P003-SS003-1824-01

Quant Time: May 16 05:51:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051222S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 13 02:08:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	159557	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	273984	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	232499	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	93772	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	88618	55.769	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	111.540%
35) Dibromofluoromethane	7.716	113	84505	51.389	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.780%
50) Toluene-d8	10.179	98	324067	52.256	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.520%
62) 4-Bromofluorobenzene	12.483	95	87257	40.611	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	81.220%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051322\
Data File : VY008746.D
Acq On : 13 May 2022 14:04
Operator : KP/MD
Sample : N2781-04
Misc : 6.30g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
P003-SS003-1824-01

Quant Time: May 16 05:51:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051222S.M
Quant Title : SW846 8260
QLast Update : Fri May 13 02:08:33 2022
Response via : Initial Calibration




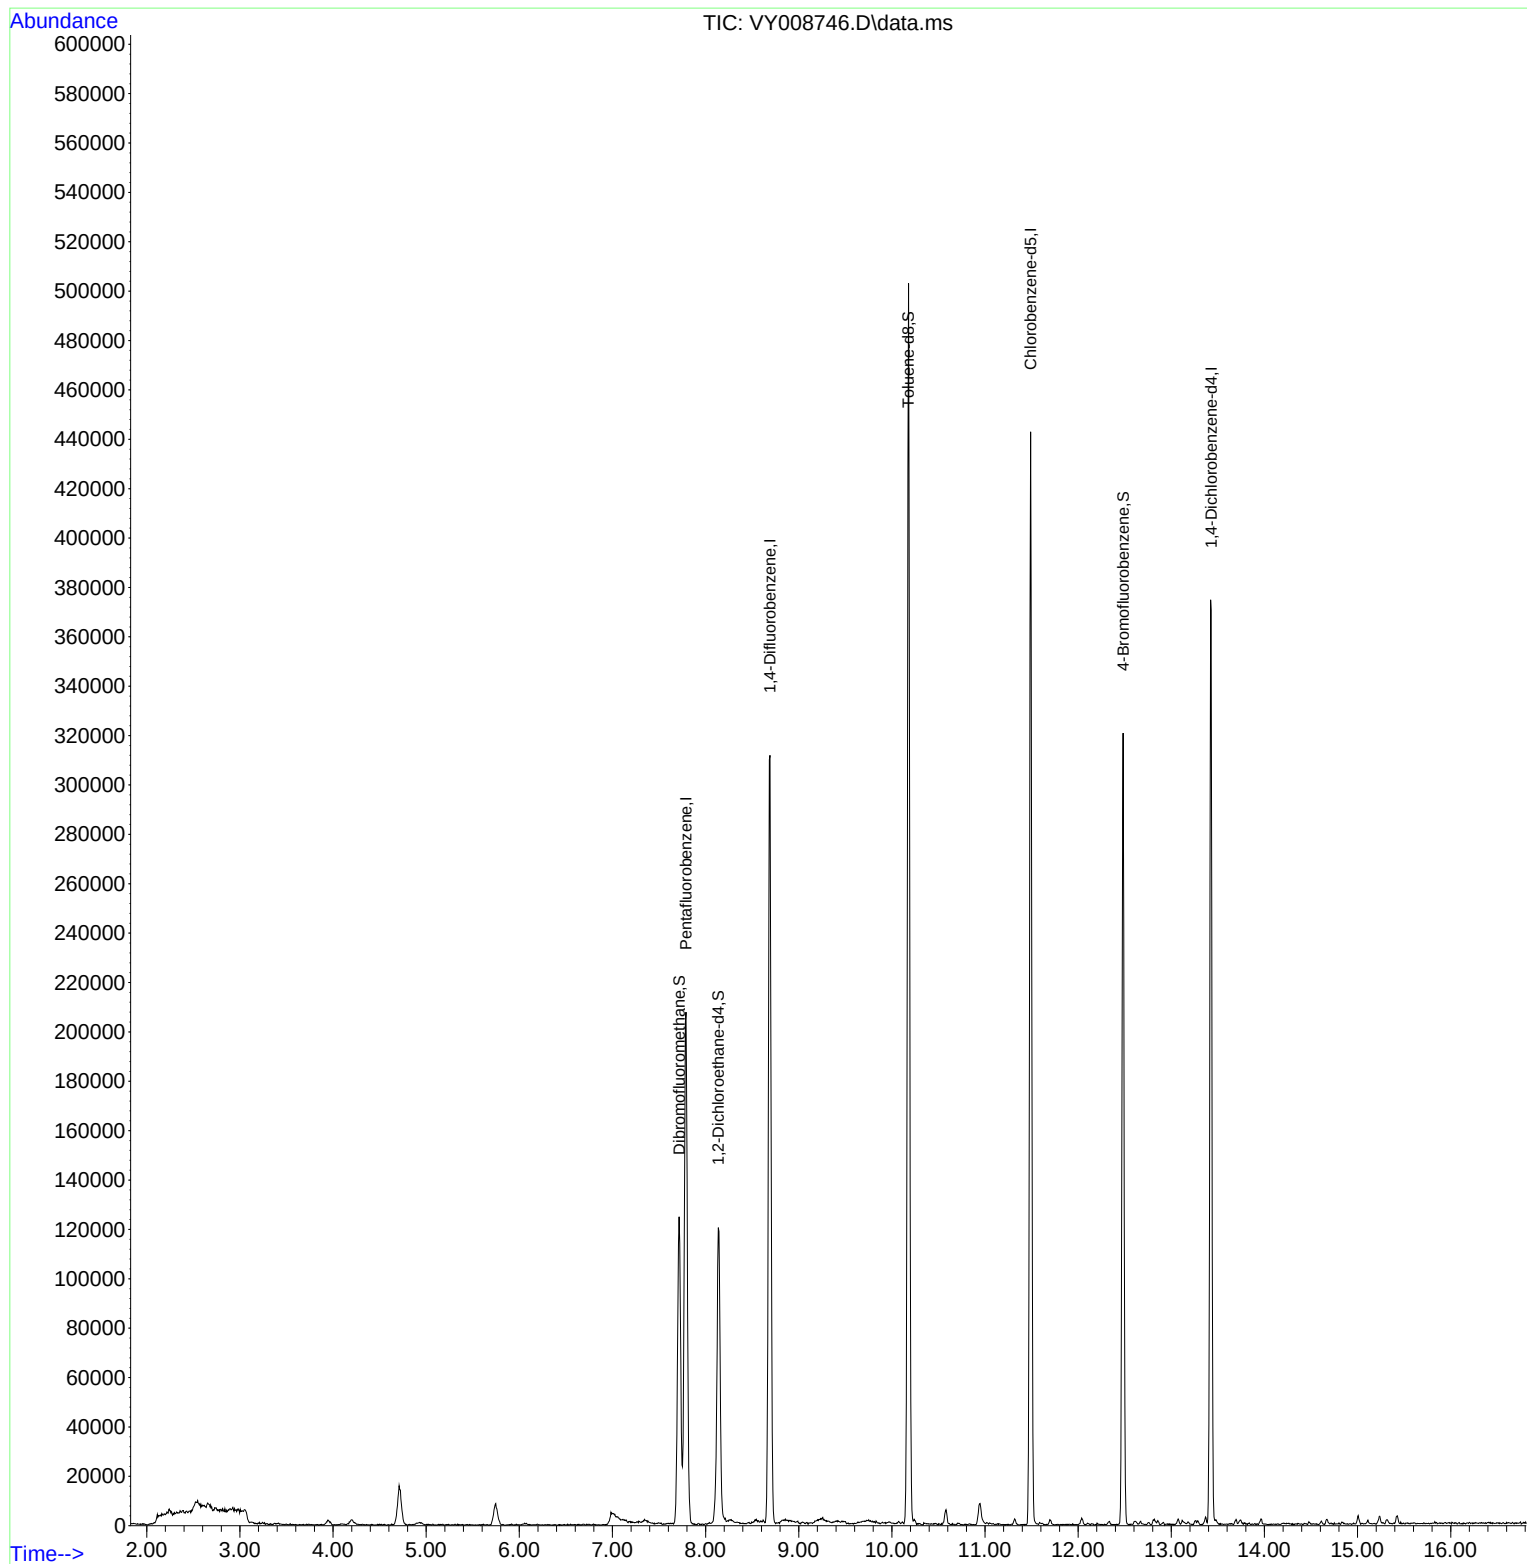


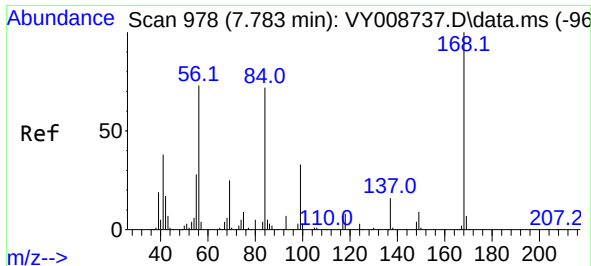

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY008746.D
Acq: 13 May 2022 14:04




Instrument :
MSVOA_Y
ClientSampleId :
P003-SS003-1824-01


Tgt Ion:168 Resp: 159557
Ion Ratio Lower Upper
168 100
99 54.3 42.3 63.5

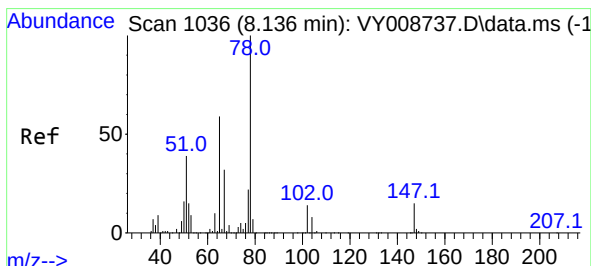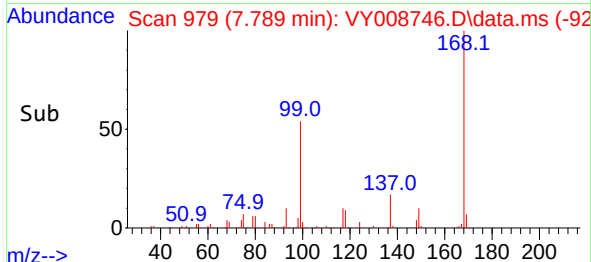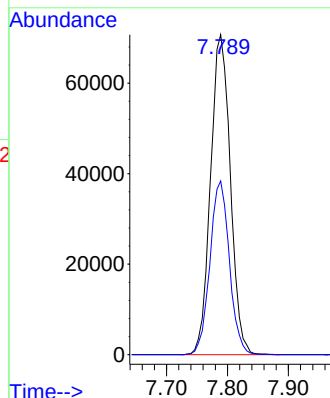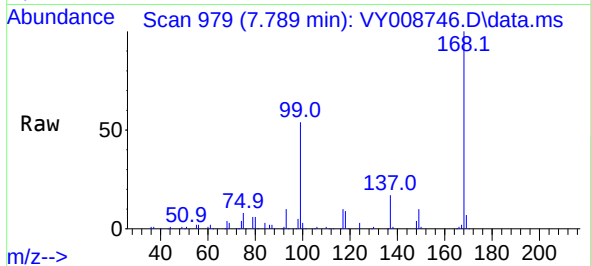

#33
1,2-Dichloroethane-d4
Concen: 55.769 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY008746.D
Acq: 13 May 2022 14:04

Tgt Ion: 65 Resp: 88618
Ion Ratio Lower Upper
65 100
67 53.0 0.0 110.0

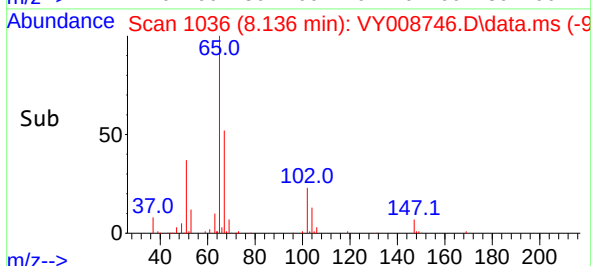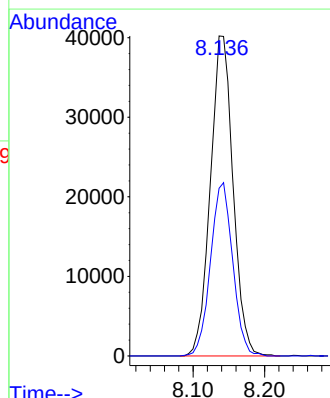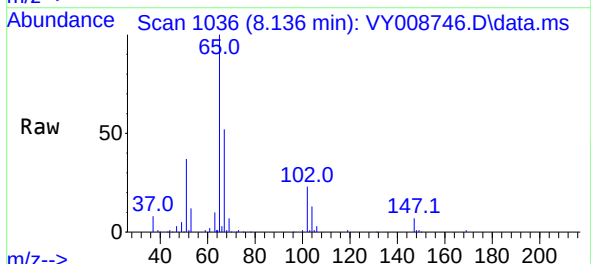

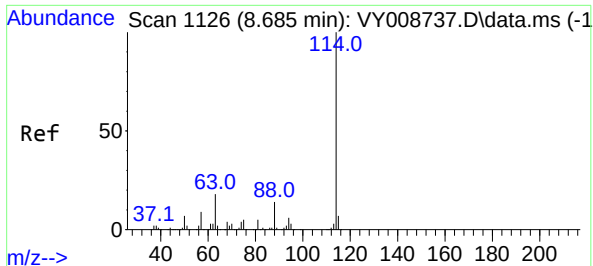

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY008746.D

Acq: 13 May 2022 14:04

Instrument :

MSVOA_Y

ClientSampleId :

P003-SS003-1824-01





Tgt Ion:114 Resp: 273984

Ion Ratio Lower Upper

114 100

63 17.9 0.0 36.4

88 13.1 0.0 27.4

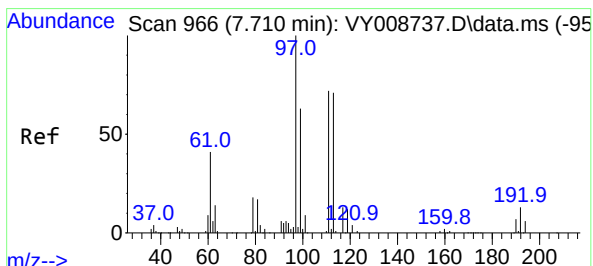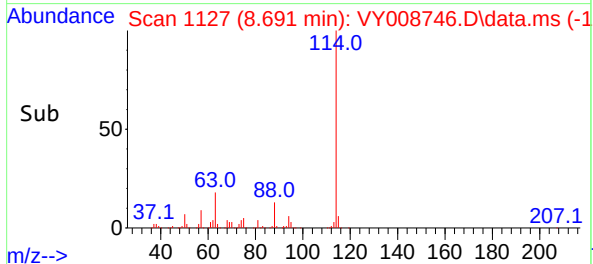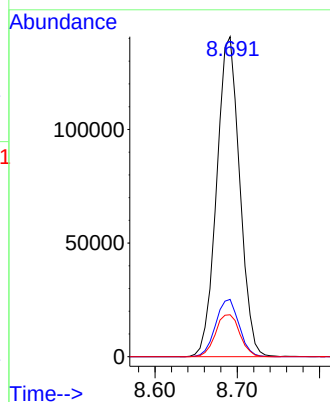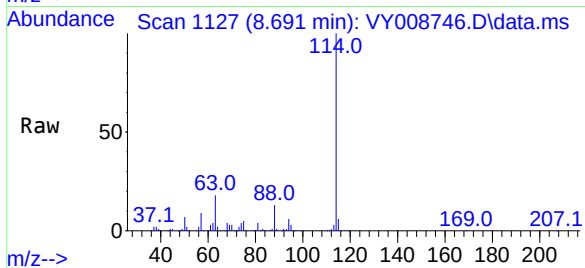

#35

Dibromofluoromethane

Concen: 51.389 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.006 min

Lab File: VY008746.D

Acq: 13 May 2022 14:04




Tgt Ion:113 Resp: 84505


Ion Ratio Lower Upper

113 100

111 103.9 81.8 122.6

192 18.6 14.5 21.7


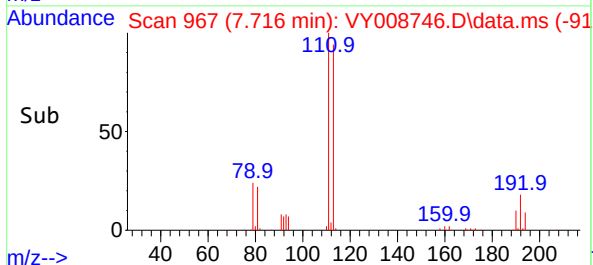
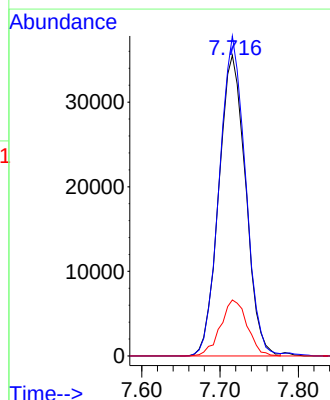
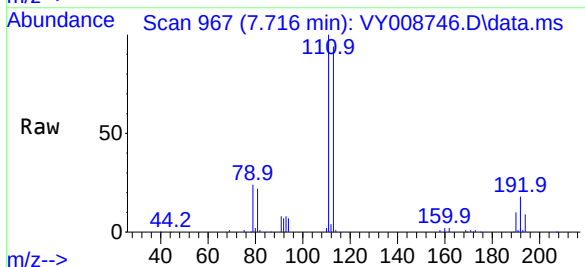


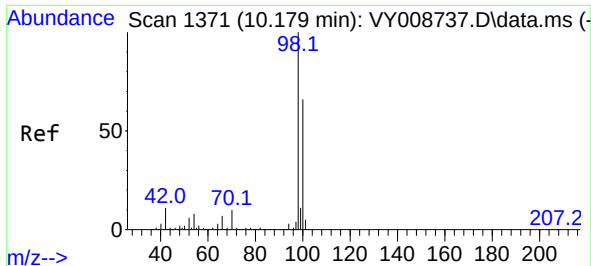

#50
Toluene-d8
Concen: 52.256 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.000 min
Lab File: VY008746.D
Acq: 13 May 2022 14:04




Instrument :
MSVOA_Y
ClientSampleId :
P003-SS003-1824-01


Tgt Ion: 98 Resp: 324067
Ion Ratio Lower Upper
98 100
100 64.2 52.8 79.2

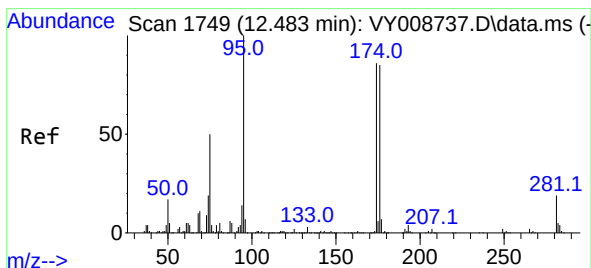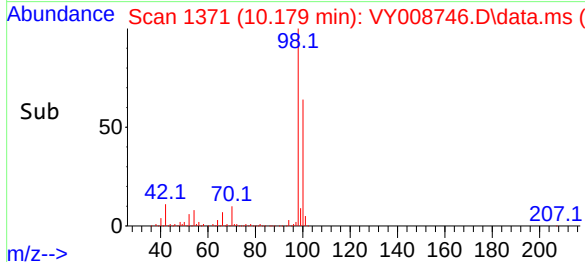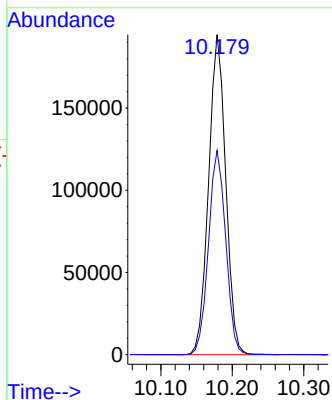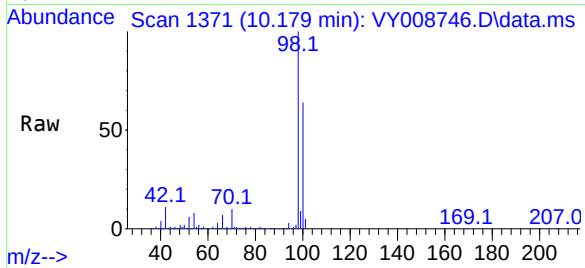

#62
4-Bromofluorobenzene
Concen: 40.611 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY008746.D
Acq: 13 May 2022 14:04

Tgt Ion: 95 Resp: 87257
Ion Ratio Lower Upper
95 100
174 87.1 0.0 171.2
176 85.4 0.0 168.8


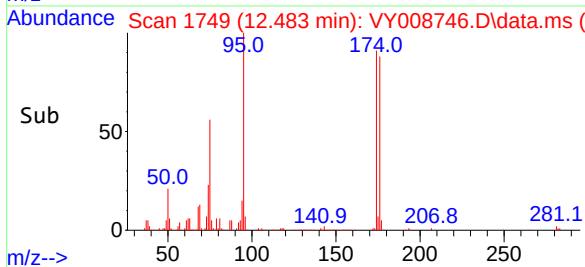
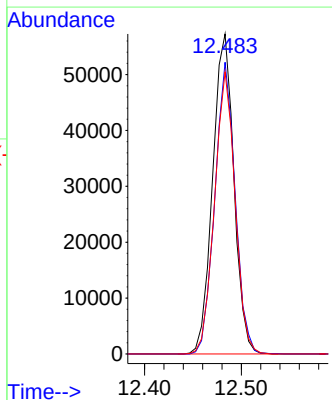
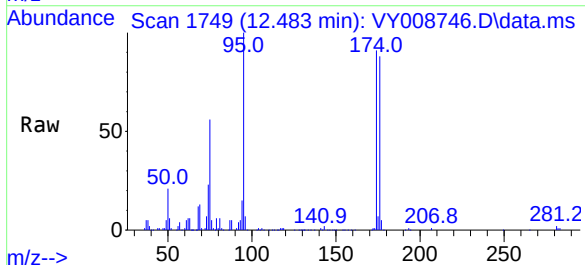


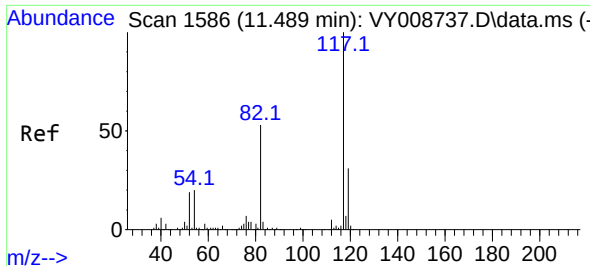

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY008746.D
Acq: 13 May 2022 14:04

Instrument :
MSVOA_Y
ClientSampleId :
P003-SS003-1824-01

Tgt Ion:117 Resp: 232499
Ion Ratio Lower Upper
117 100
82 53.8 42.3 63.5
119 31.6 24.6 37.0

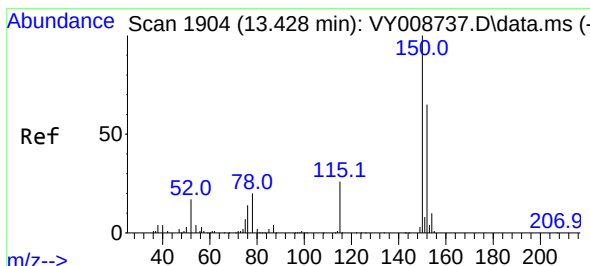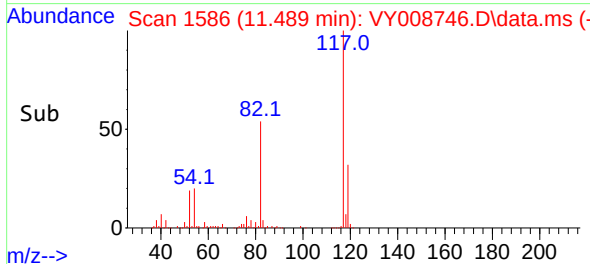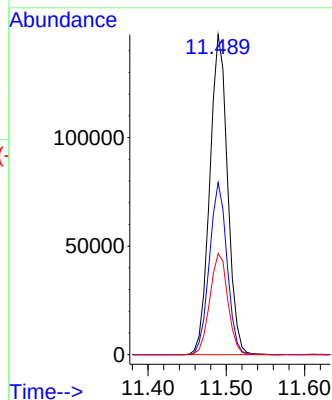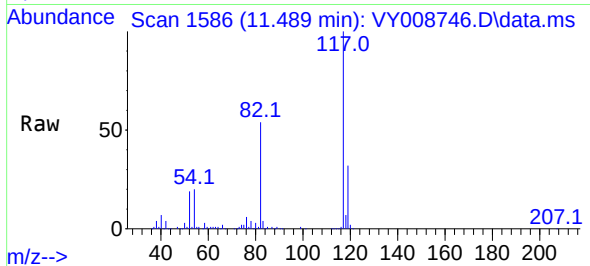

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY008746.D
Acq: 13 May 2022 14:04

Tgt Ion:152 Resp: 93772
Ion Ratio Lower Upper
152 100
115 57.7 28.2 84.7
150 157.9 0.0 348.2

