

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051523\
 Data File : VY013744.D
 Acq On : 15 May 2023 18:24
 Operator : KP/MD
 Sample : 02760-03
 Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 HR-4-051123

Quant Time: May 16 01:34:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 02:39:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	180979	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	317415	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	307591	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	145229	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	121226	61.104	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 122.200%	
35) Dibromofluoromethane	7.716	113	106977	53.585	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 107.180%	
50) Toluene-d8	10.179	98	388768	54.741	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 109.480%	
62) 4-Bromofluorobenzene	12.477	95	130902	54.673	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 109.340%	
Target Compounds						
					Qvalue	
13) Acrolein	3.497	56	19	Below Cal	#	16
16) Acetone	3.960	43	2137	2.735	ug/l	90
20) Methylene Chloride	4.710	84	24190	2.140	ug/l	93
31) Cyclohexane	7.789	56	4356	1.226	ug/l #	18
36) 1,1-Dichloropropene	7.789	75	14537	4.387	ug/l #	49
38) Carbon Tetrachloride	7.789	117	17700	5.097	ug/l #	15
76) 1,2,3-Trichloropropane	12.483	75	72350	36.940	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.483	75	72350	75.563	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051523\
Data File : VY013744.D
Acq On : 15 May 2023 18:24
Operator : KP/MD
Sample : 02760-03
Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
HR-4-051123

Quant Time: May 16 01:34:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 02:39:58 2023
Response via : Initial Calibration




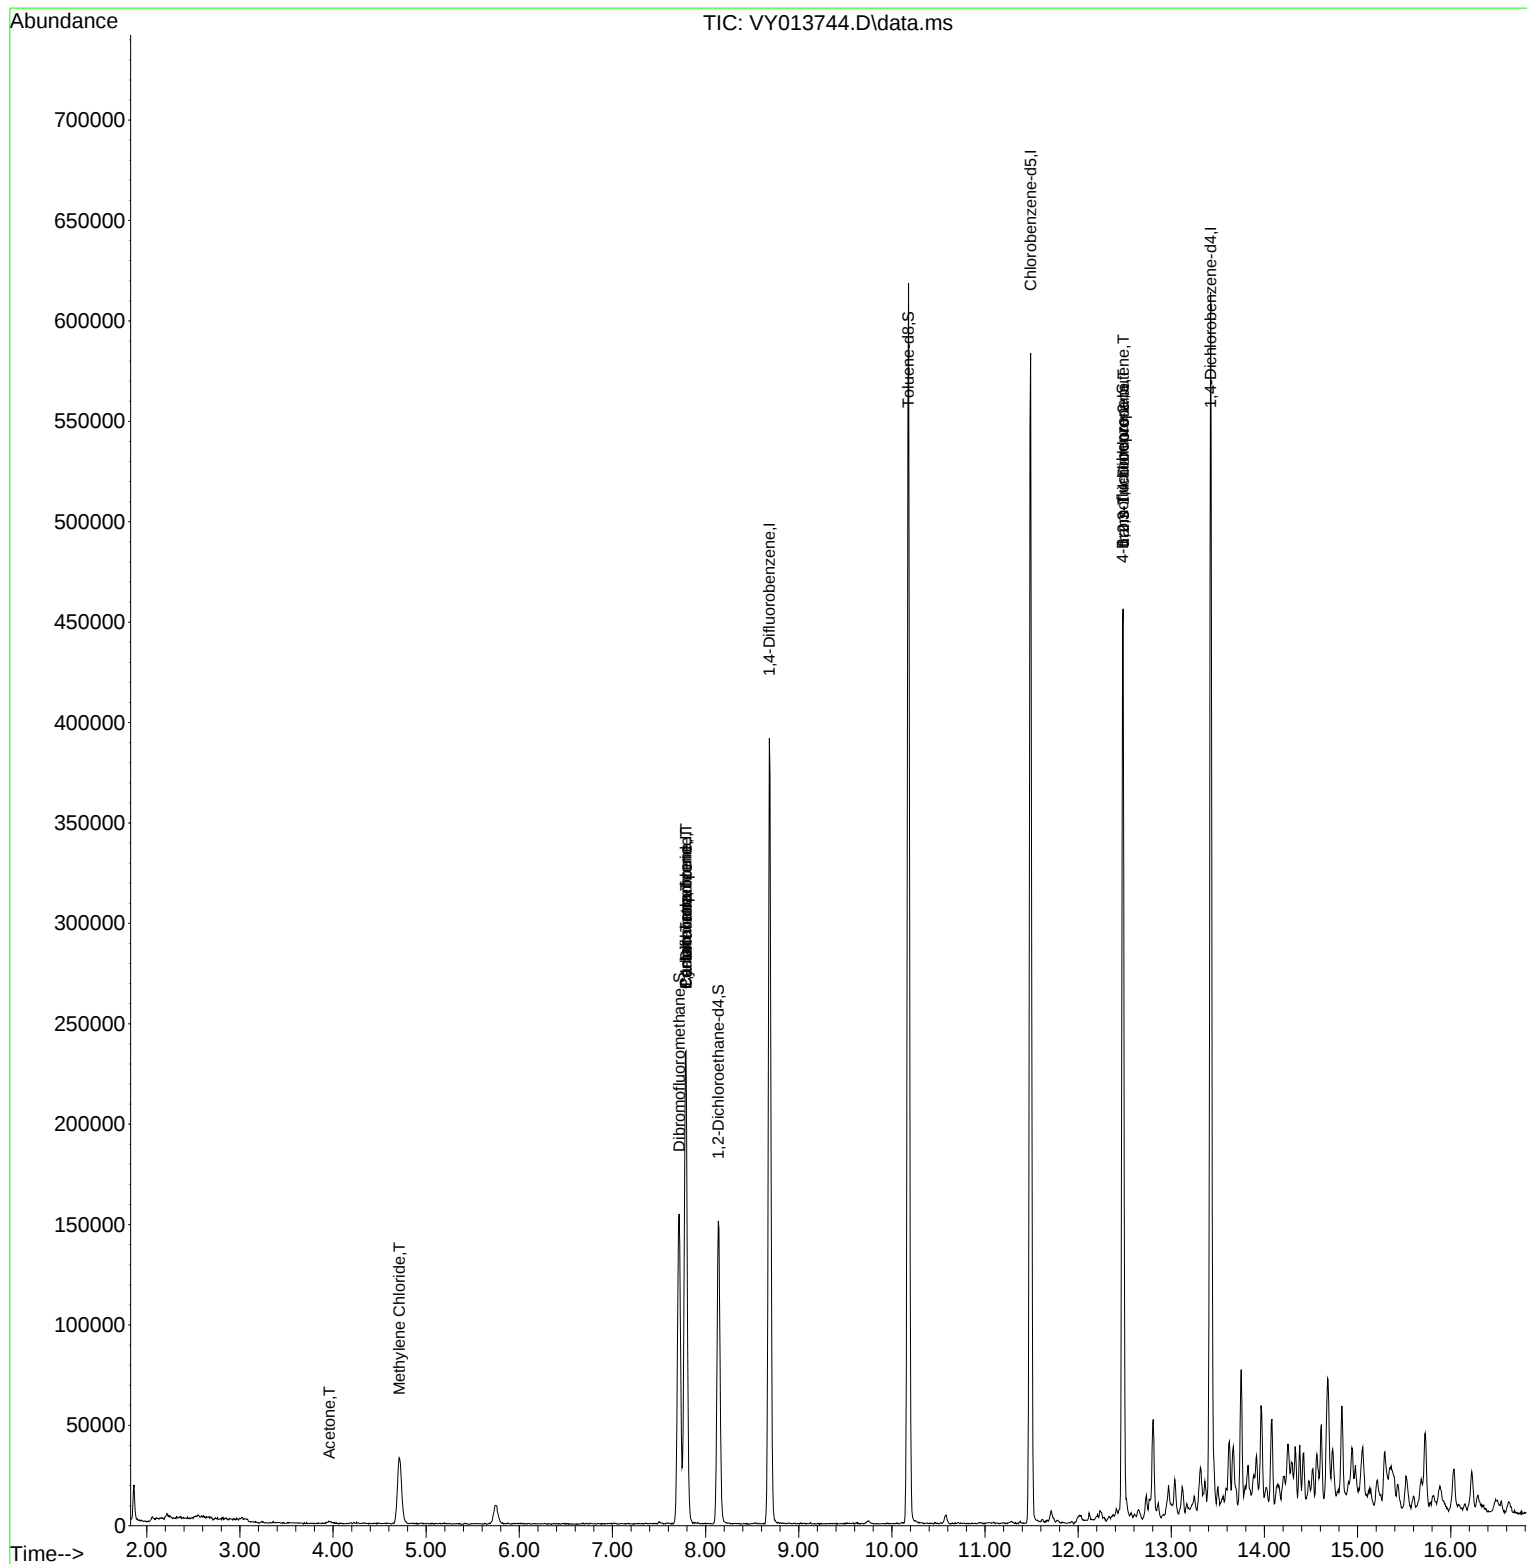


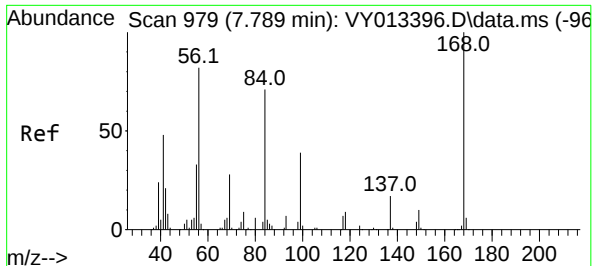

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24




Instrument :
MSVOA_Y
ClientSampleId :
HR-4-051123


Tgt Ion:168 Resp: 180979
Ion Ratio Lower Upper
168 100
99 51.4 41.8 62.6

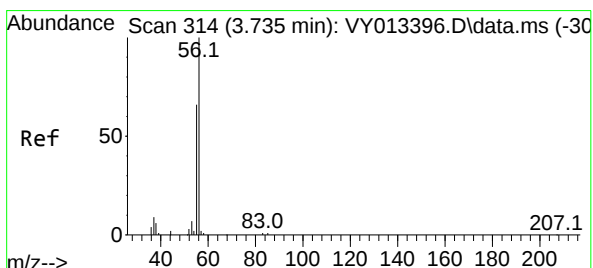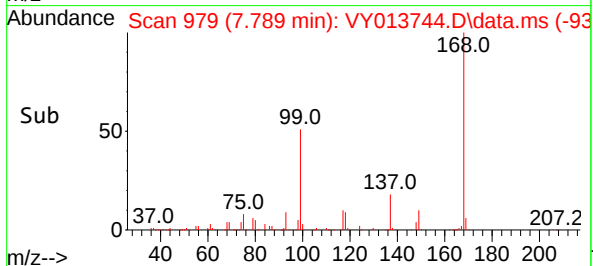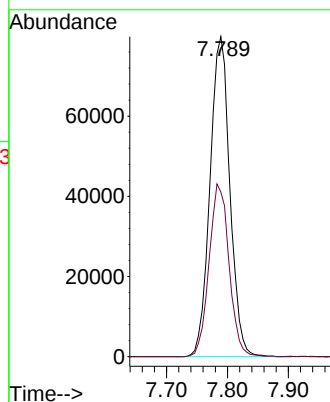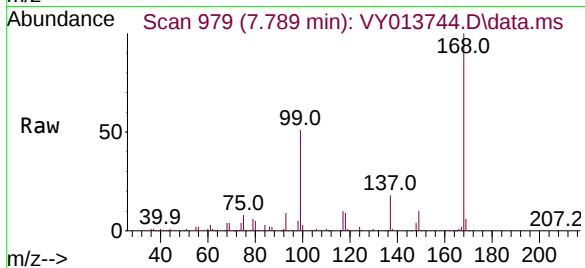

#13
Acrolein
Concen: Below Cal
RT: 3.497 min Scan# 275
Delta R.T. -0.232 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24

Tgt Ion: 56 Resp: 19
Ion Ratio Lower Upper
56 100
55 0.0 54.1 81.1#


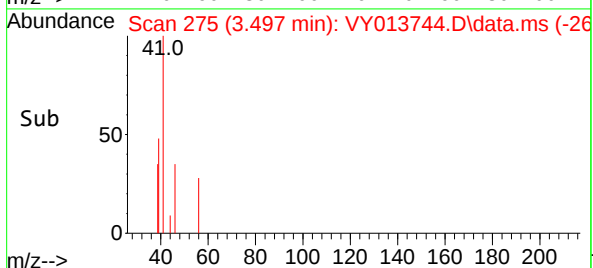
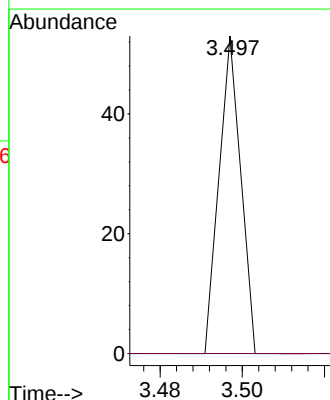
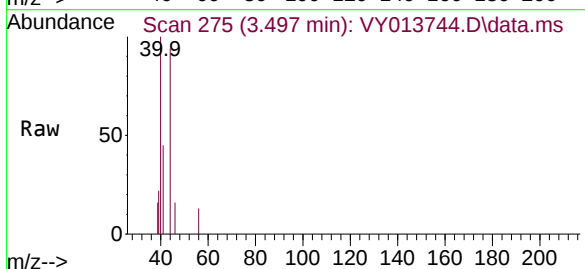


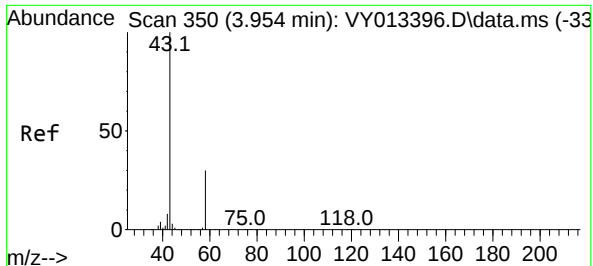

#16
Acetone
Concen: 2.735 ug/l
RT: 3.960 min Scan# 351
Delta R.T. 0.012 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24




Instrument :
MSVOA_Y
ClientSampleId :
HR-4-051123


Tgt Ion: 43 Resp: 2137
Ion Ratio Lower Upper
43 100
58 26.2 25.4 38.0

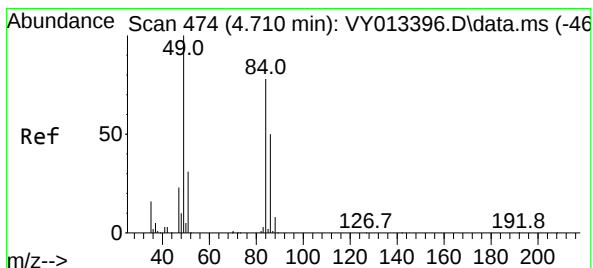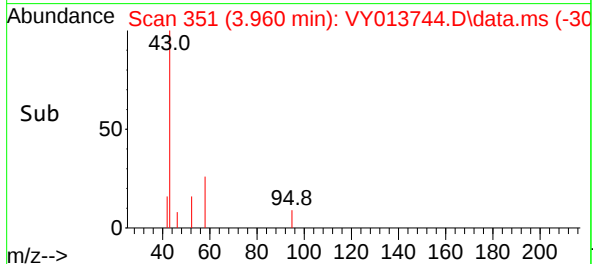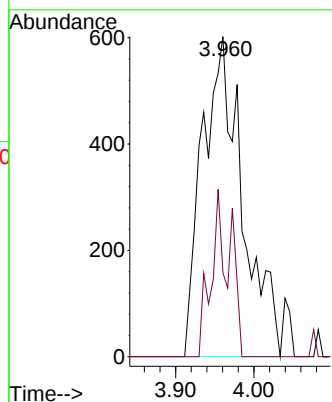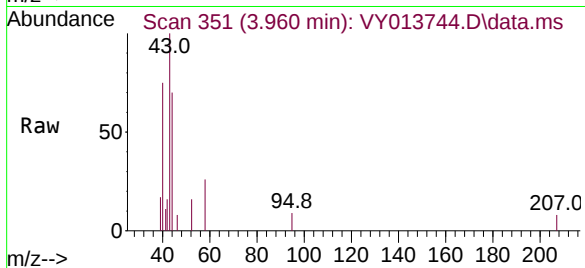

#20
Methylene Chloride
Concen: 2.140 ug/l
RT: 4.710 min Scan# 474
Delta R.T. -0.006 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24

Tgt Ion: 84 Resp: 24190
Ion Ratio Lower Upper
84 100
49 121.0 88.0 132.0
51 36.7 27.4 41.0
86 64.0 50.4 75.6


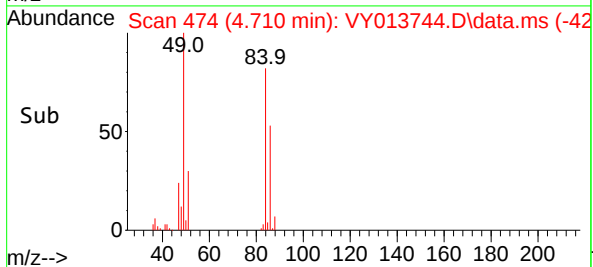
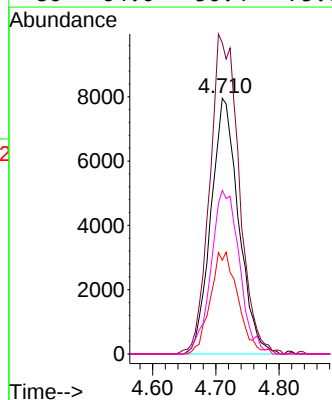
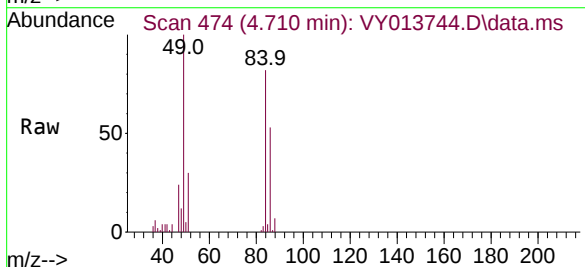


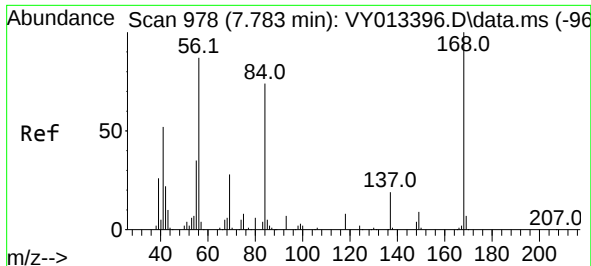

#31
Cyclohexane
Concen: 1.226 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24




Instrument :
MSVOA_Y
ClientSampleId :
HR-4-051123


Tgt Ion: 56 Resp: 4356
Ion Ratio Lower Upper
56 100
69 162.5 29.2 43.8#
84 119.5 73.0 109.6#

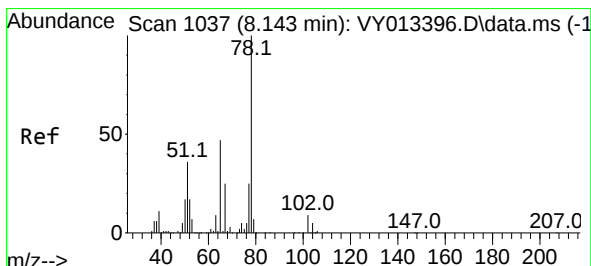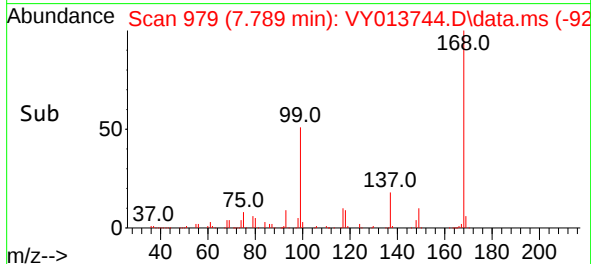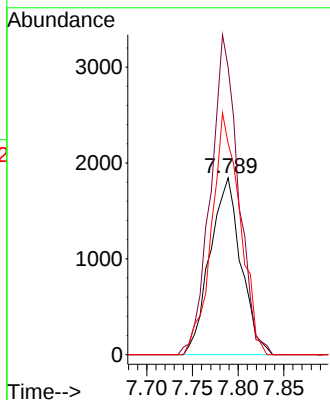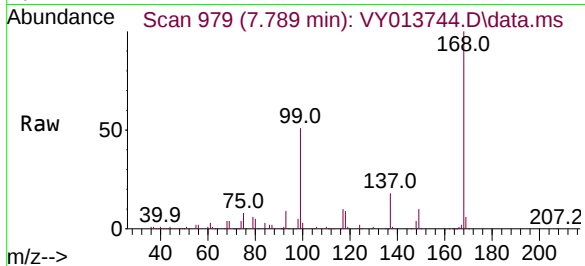

#33
1,2-Dichloroethane-d4
Concen: 61.104 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24

Tgt Ion: 65 Resp: 121226
Ion Ratio Lower Upper
65 100
67 52.1 0.0 103.4

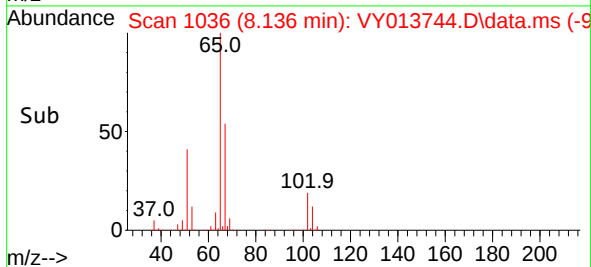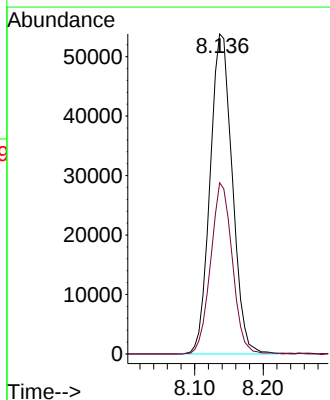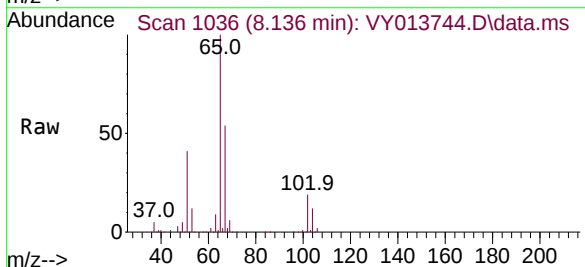

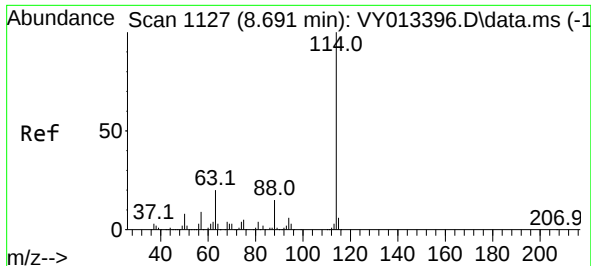

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.006 min

Lab File: VY013744.D

Acq: 15 May 2023 18:24

Instrument :

MSVOA_Y

ClientSampleId :

HR-4-051123





Tgt Ion:114 Resp: 317415

Ion Ratio Lower Upper

114 100

63 20.8 0.0 36.6

88 15.5 0.0 28.8

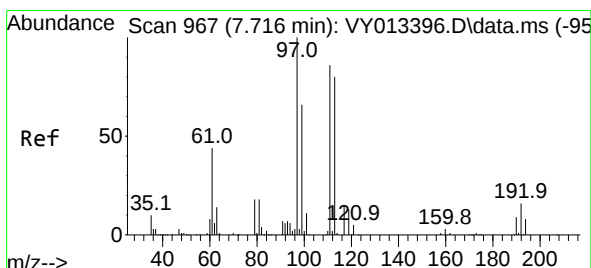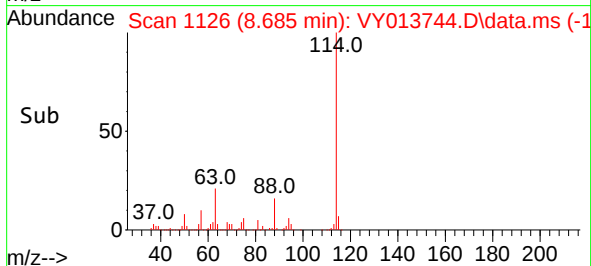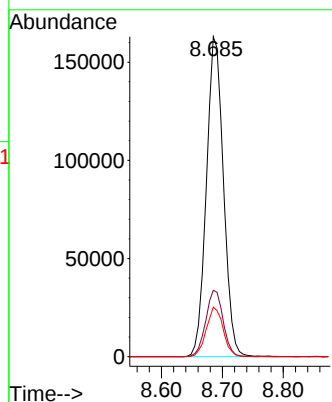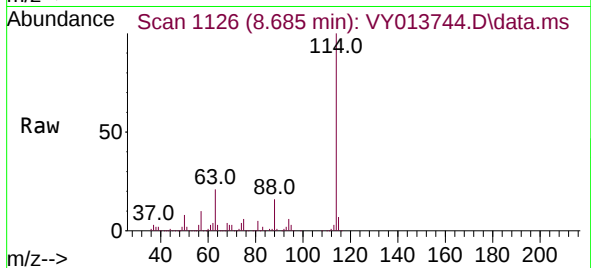

#35

Dibromofluoromethane

Concen: 53.585 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY013744.D

Acq: 15 May 2023 18:24




Tgt Ion:113 Resp: 106977


Ion Ratio Lower Upper

113 100

111 103.7 82.2 123.2

192 20.0 16.7 25.1

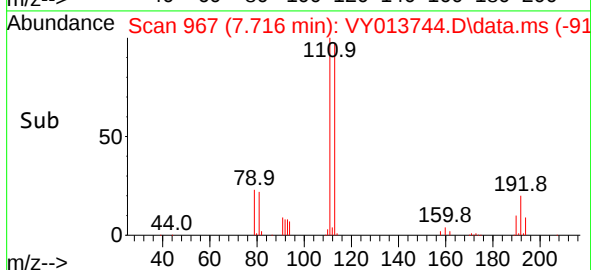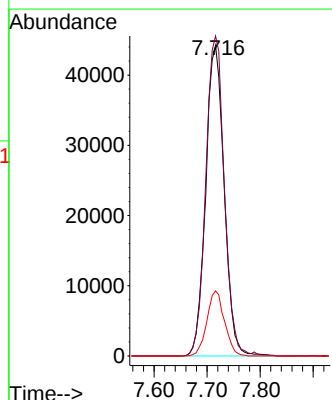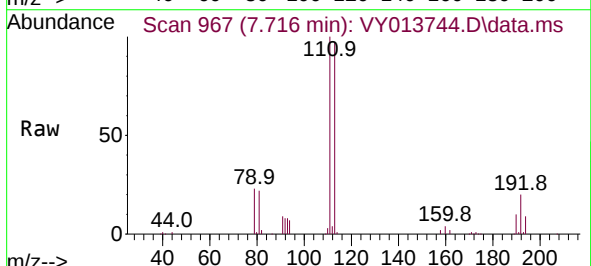

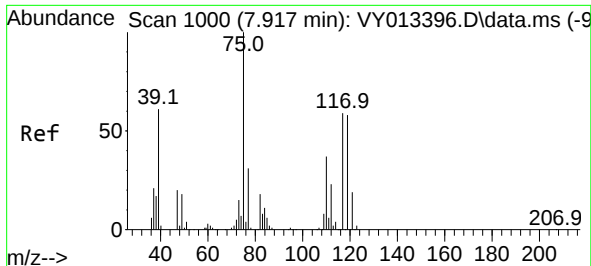

#36

1,1-Dichloropropene

Concen: 4.387 ug/l

RT: 7.789 min Scan# 91

Delta R.T. -0.128 min

Lab File: VY013744.D

Acq: 15 May 2023 18:24

Instrument :

MSVOA_Y

ClientSampleId :

HR-4-051123





Tgt Ion: 75 Resp: 14537

Ion Ratio Lower Upper

75 100

110 9.1 18.7 56.1#

77 0.0 24.6 37.0#

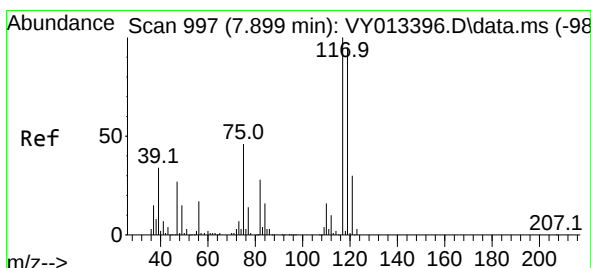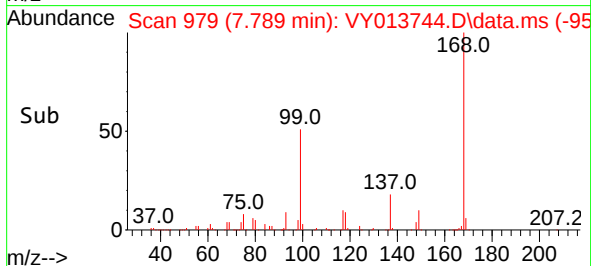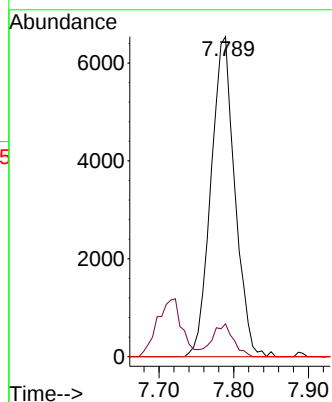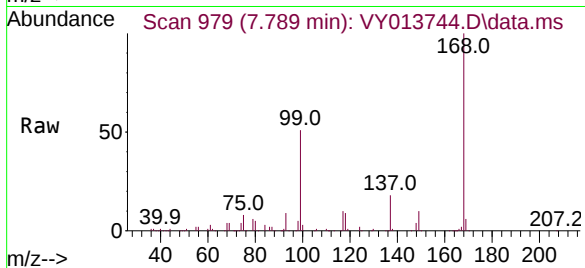

#38

Carbon Tetrachloride

Concen: 5.097 ug/l

RT: 7.789 min Scan# 979

Delta R.T. -0.110 min

Lab File: VY013744.D

Acq: 15 May 2023 18:24




Tgt Ion: 117 Resp: 17700


Ion Ratio Lower Upper

117 100

119 6.2 79.0 118.6#

121 0.0 26.6 40.0#


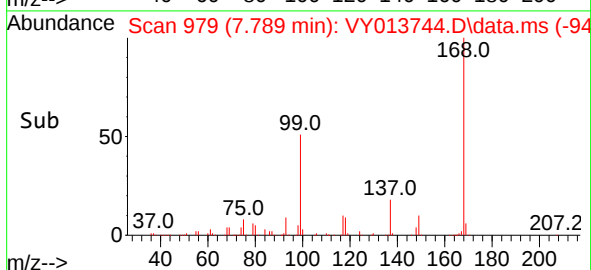
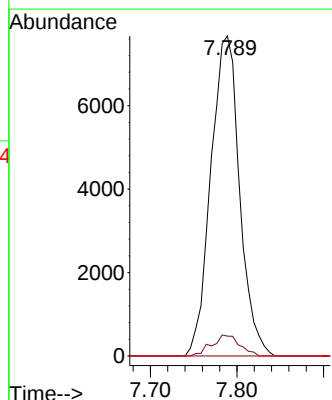
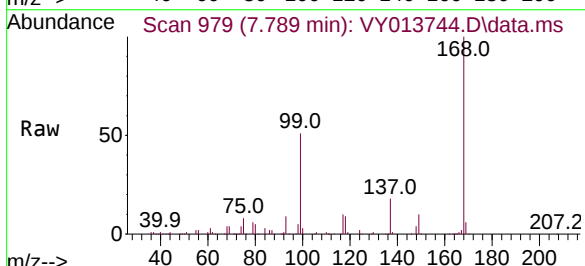


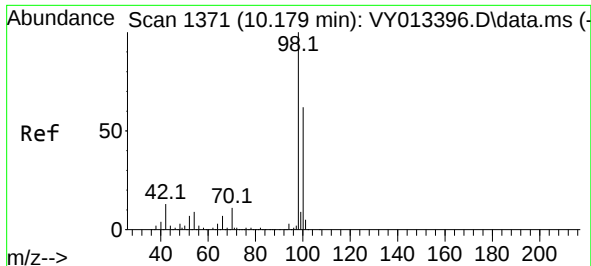

#50
Toluene-d8
Concen: 54.741 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24




Instrument :
MSVOA_Y
ClientSampleId :
HR-4-051123


Tgt Ion: 98 Resp: 388768
Ion Ratio Lower Upper
98 100
100 63.1 50.5 75.7

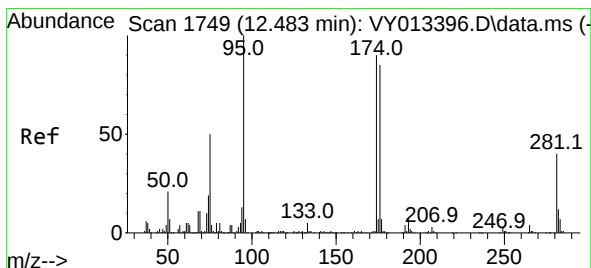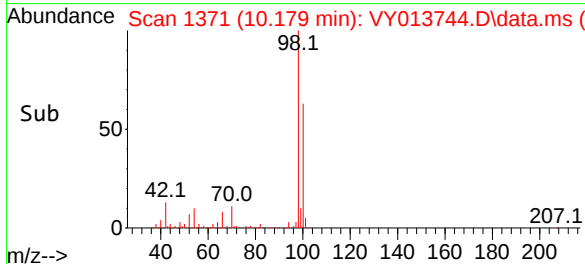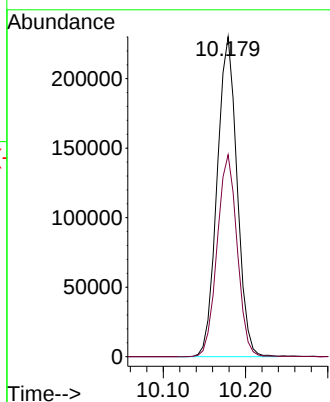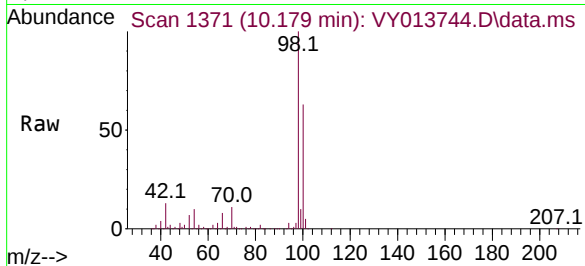

#62
4-Bromofluorobenzene
Concen: 54.673 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24

Tgt Ion: 95 Resp: 130902
Ion Ratio Lower Upper
95 100
174 88.4 0.0 182.0
176 85.0 0.0 175.4


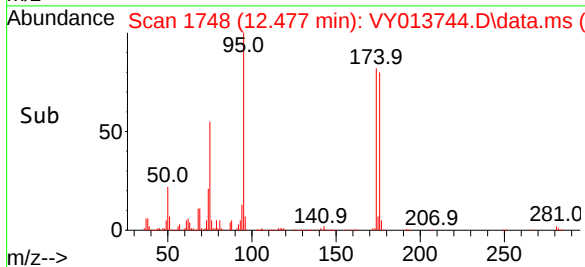
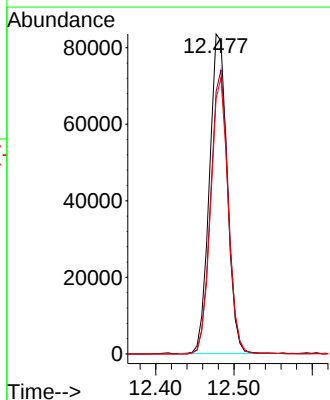
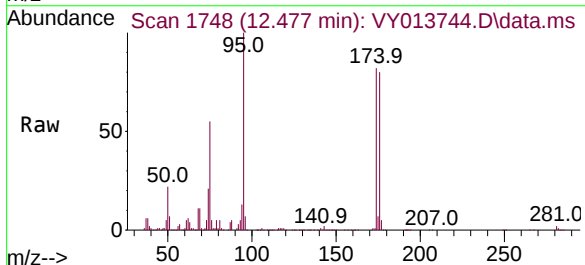


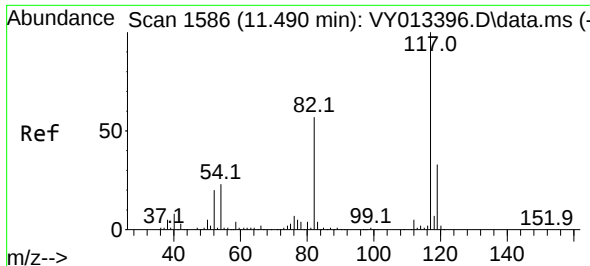

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24




Instrument :
MSVOA_Y
ClientSampleId :
HR-4-051123


Tgt Ion:117 Resp: 307591
Ion Ratio Lower Upper
117 100
82 54.6 43.0 64.6
119 31.2 25.5 38.3

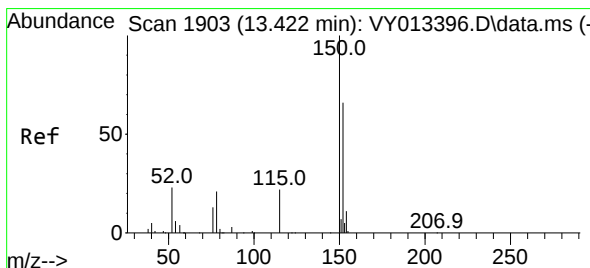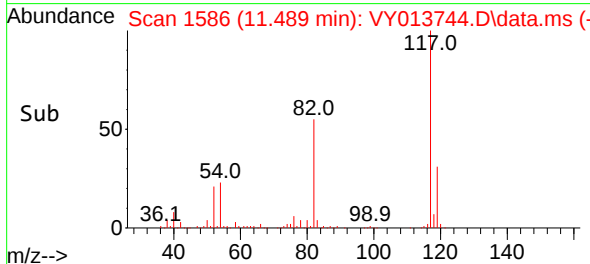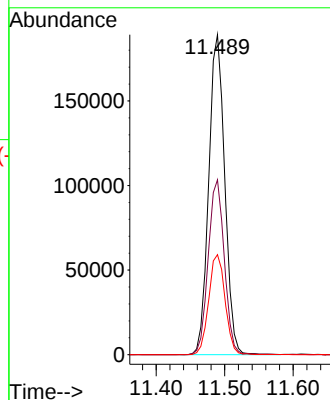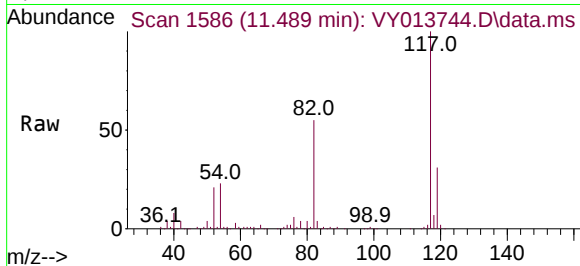

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24

Tgt Ion:152 Resp: 145229
Ion Ratio Lower Upper
152 100
115 57.7 28.1 84.2
150 155.5 0.0 352.0


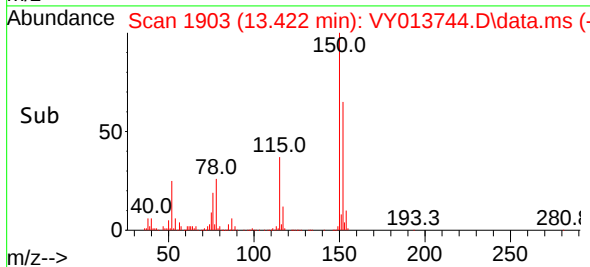
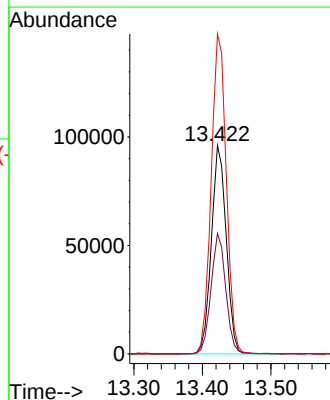
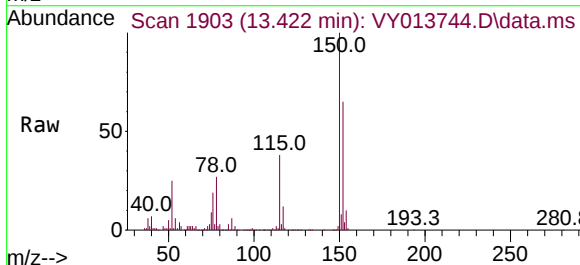


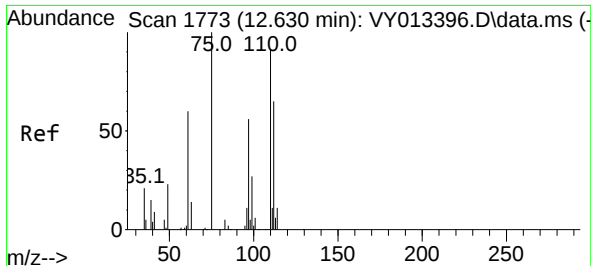

#76
1,2,3-Trichloropropane
Concen: 36.940 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.146 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24

Instrument :
MSVOA_Y
ClientSampleId :
HR-4-051123

Tgt Ion: 75 Resp: 72350
Ion Ratio Lower Upper
75 100
77 1.4 0.0 0.0#

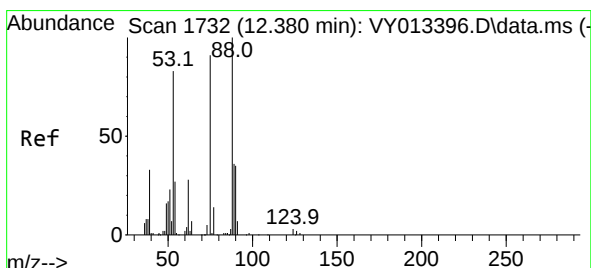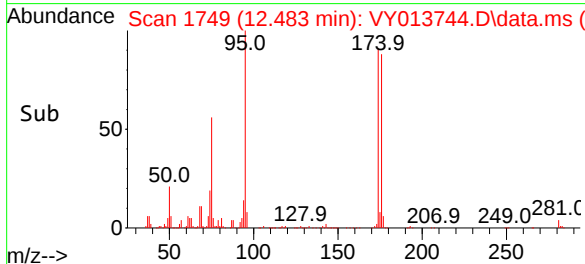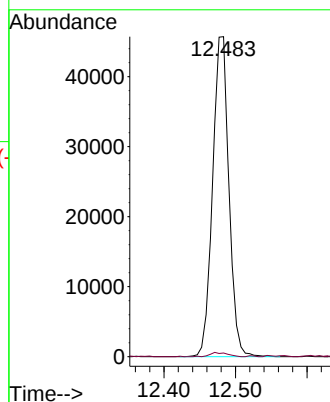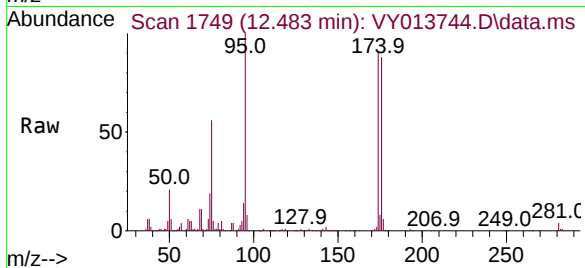

#81
trans-1,4-Dichloro-2-butene
Concen: 75.563 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.104 min
Lab File: VY013744.D
Acq: 15 May 2023 18:24

Tgt Ion: 75 Resp: 72350
Ion Ratio Lower Upper
75 100
53 0.3 73.2 109.8#
89 0.1 38.0 57.0#

