
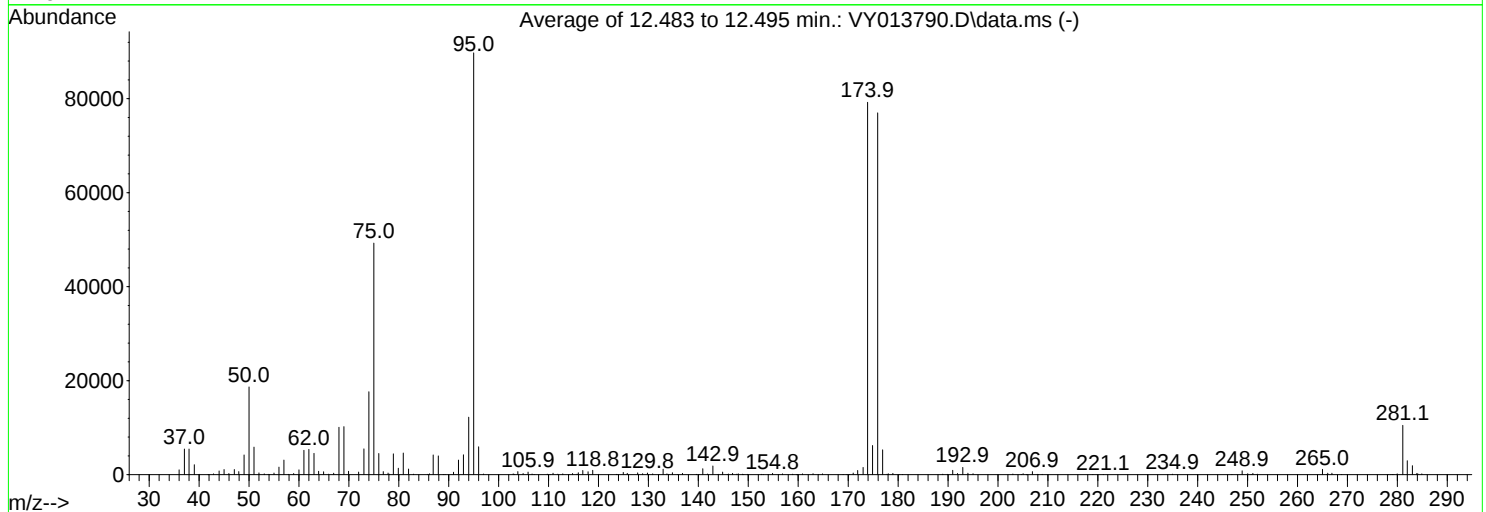


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY051823\
Data File : VY013790.D
Acq On : 18 May 2023 09:18
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y051723S.M
Title : SW846 8260
Last Update : Thu May 18 06:54:18 2023

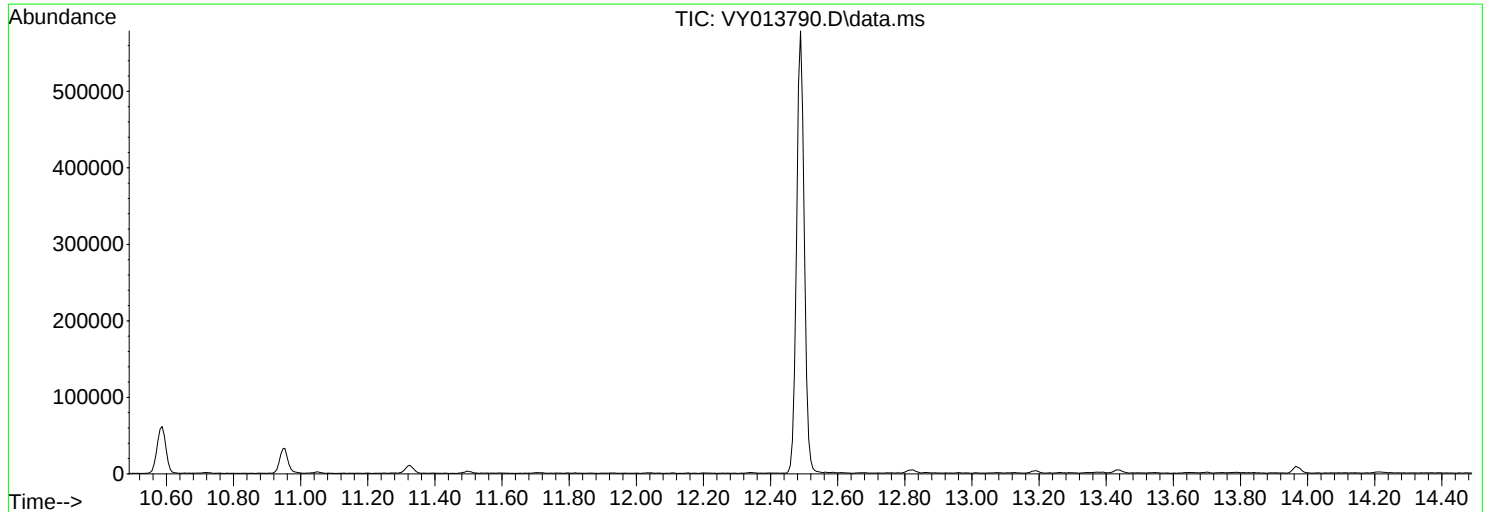

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	18668	PASS
75	95	30	60	54.9	49272	PASS
95	95	100	100	100.0	89752	PASS
96	95	5	9	6.6	5935	PASS
173	174	0.00	2	1.9	1536	PASS
174	95	50	100	88.3	79229	PASS
175	174	5	9	7.8	6214	PASS
176	174	95	101	97.2	76981	PASS
177	176	5	9	6.9	5285	PASS