

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052423\
 Data File : VY013842.D
 Acq On : 24 May 2023 13:38
 Operator : KP/MD
 Sample : 02899-01
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB06A

Quant Time: May 25 07:08:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052323S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 24 05:25:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	6583	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	11233	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	10957	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	3672	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	6313	82.893	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 165.780%#			
35) Dibromofluoromethane	7.716	113	4895	67.477	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 134.960%			
50) Toluene-d8	10.179	98	13700	49.689	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery = 99.380%			
62) 4-Bromofluorobenzene	12.483	95	3518	38.386	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery = 76.780%			
Target Compounds						Qvalue
3) Chloromethane	2.119	50	564	7.678	ug/l #	24
5) Bromomethane	2.668	94	528	8.844	ug/l	82
10) Methyl Iodide	4.100	142	572	7.030	ug/l #	68
13) Acrolein	3.747	56	174	19.827	ug/l #	62
15) Acrylonitrile	5.173	53	42	2.112	ug/l #	17
16) Acetone	3.948	43	707	31.278	ug/l #	81
20) Methylene Chloride	4.704	84	1255	13.821	ug/l #	83
38) Carbon Tetrachloride	7.795	117	662	5.268	ug/l #	13
48) Methyl methacrylate	9.404	41	101	1.751	ug/l #	16
51) 4-Methyl-2-Pentanone	10.069	43	78	1.192	ug/l #	38
60) Dibromochloromethane	10.727	129	81	1.022	ug/l #	11
68) m/p-Xylenes	11.703	106	173	1.106	ug/l	99
76) 1,2,3-Trichloropropane	12.477	75	2141	49.448	ug/l #	100
77) Bromobenzene	12.611	156	70	1.044	ug/l #	24
78) n-propylbenzene	12.672	91	377	1.117	ug/l #	53
79) 2-Chlorotoluene	12.757	91	225	1.193	ug/l #	39
81) trans-1,4-Dichloro-2-b...	12.477	75	2141	107.337	ug/l #	10
82) 4-Chlorotoluene	12.867	91	385	1.975	ug/l #	39
83) tert-Butylbenzene	13.081	119	216	1.099	ug/l #	86
85) sec-Butylbenzene	13.257	105	354	1.213	ug/l #	56
86) p-Isopropyltoluene	13.367	119	321	1.331	ug/l #	74
87) 1,3-Dichlorobenzene	13.373	146	349	2.695	ug/l	77
88) 1,4-Dichlorobenzene	13.446	146	295	2.288	ug/l	92
89) n-Butylbenzene	13.702	91	350	1.513	ug/l #	82
90) Hexachloroethane	13.965	117	67	1.353	ug/l #	7
91) 1,2-Dichlorobenzene	13.733	146	352	3.058	ug/l #	68
92) 1,2-Dibromo-3-Chloropr...	14.355	75	64	6.457	ug/l #	2
93) 1,2,4-Trichlorobenzene	15.007	180	365	5.115	ug/l #	61
94) Hexachlorobutadiene	15.105	225	160	3.556	ug/l	73
95) Naphthalene	15.233	128	632	8.215	ug/l #	80
96) 1,2,3-Trichlorobenzene	15.422	180	292	4.601	ug/l #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY052423\
Data File : VY013842.D
Acq On : 24 May 2023 13:38
Operator : KP/MD
Sample : 02899-01
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB06A

Quant Time: May 25 07:08:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052323S.M
Quant Title : SW846 8260
QLast Update : Wed May 24 05:25:47 2023
Response via : Initial Calibration




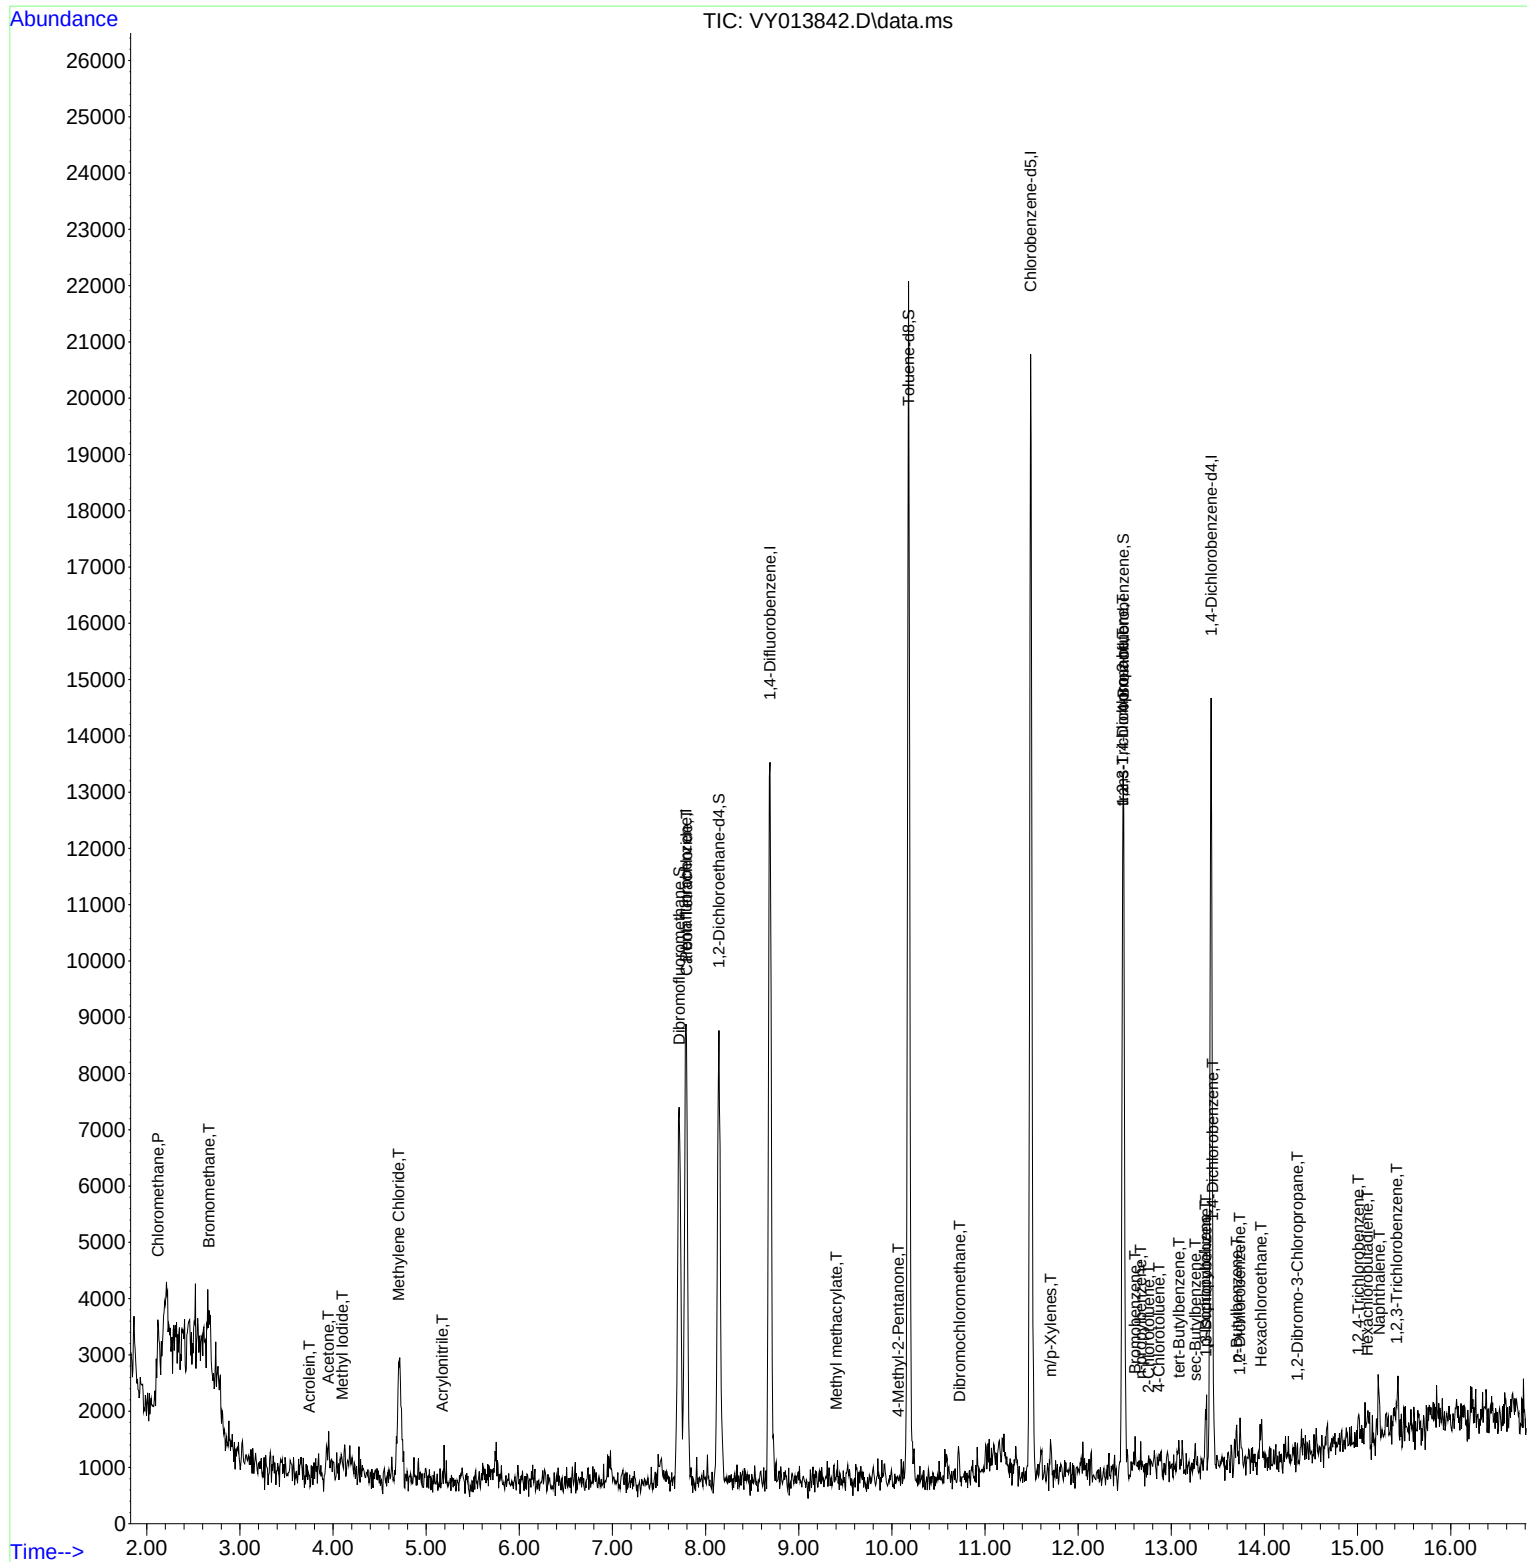




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion:168 Resp: 6583
Ion Ratio Lower Upper
168 100
99 61.1 43.4 65.2



#3
Chloromethane
Concen: 7.678 ug/l
RT: 2.119 min Scan# 49
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion: 50 Resp: 564
Ion Ratio Lower Upper
50 100
52 74.7 25.7 38.5#







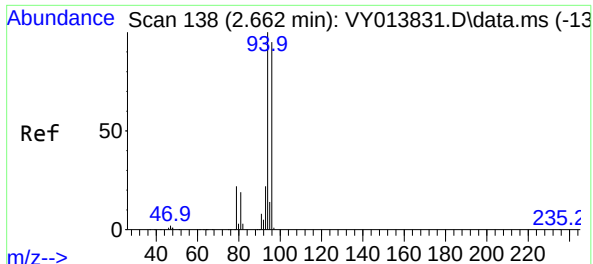

#5
Bromomethane
Concen: 8.844 ug/l
RT: 2.668 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion: 94 Resp: 528
Ion Ratio Lower Upper
94 100
96 78.1 76.2 114.2

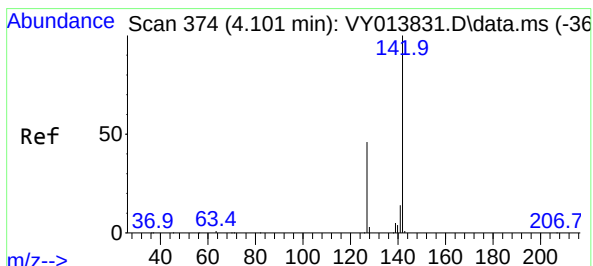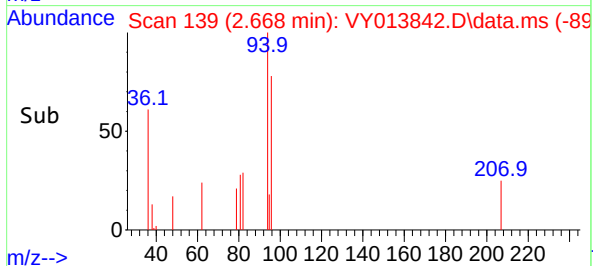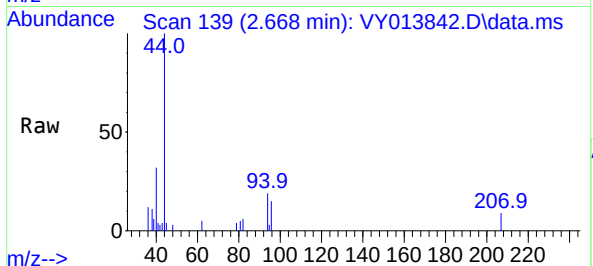

#10
Methyl Iodide
Concen: 7.030 ug/l
RT: 4.100 min Scan# 374
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion:142 Resp: 572
Ion Ratio Lower Upper
142 100
127 67.0 37.0 55.4#
141 0.0 11.8 17.6#


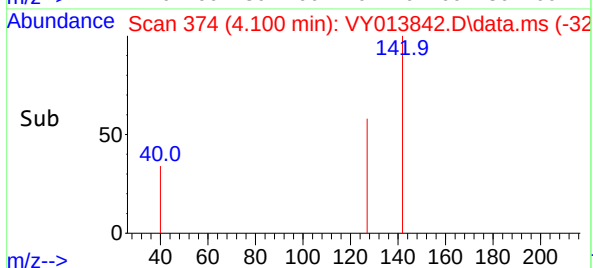
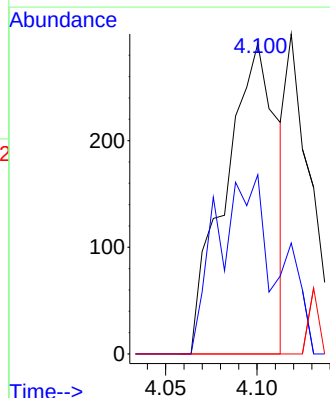
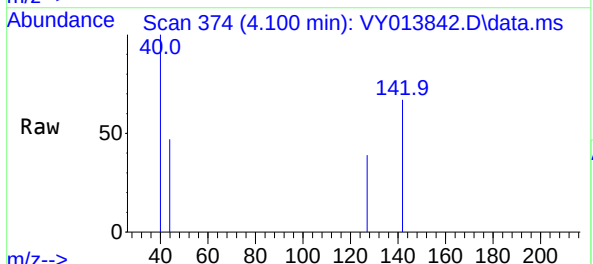




#13
Acrolein
Concen: 19.827 ug/l
RT: 3.747 min Scan# 314
Delta R.T. 0.012 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion: 56 Resp: 174
Ion Ratio Lower Upper
56 100
55 39.1 56.2 84.2#



#15
Acrylonitrile
Concen: 2.112 ug/l
RT: 5.173 min Scan# 550
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion: 53 Resp: 42
Ion Ratio Lower Upper
53 100
52 0.0 67.2 100.8#
51 0.0 30.2 45.2#


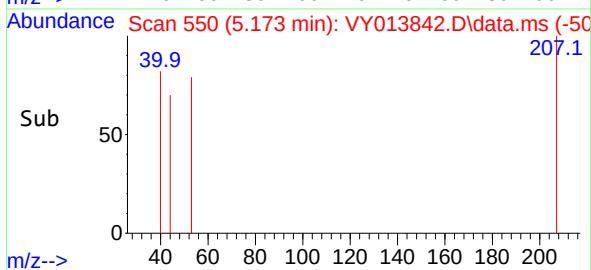

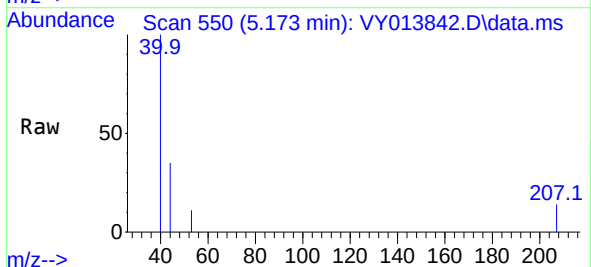




#16
Acetone
Concen: 31.278 ug/l
RT: 3.948 min Scan# 34
Delta R.T. -0.012 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion: 43 Resp: 707
Ion Ratio Lower Upper
43 100
58 18.9 23.3 34.9#



#20
Methylene Chloride
Concen: 13.821 ug/l
RT: 4.704 min Scan# 473
Delta R.T. -0.024 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion: 84 Resp: 1255
Ion Ratio Lower Upper
84 100
49 113.9 106.2 159.2
51 56.1 31.4 47.0#
86 54.4 50.6 75.8

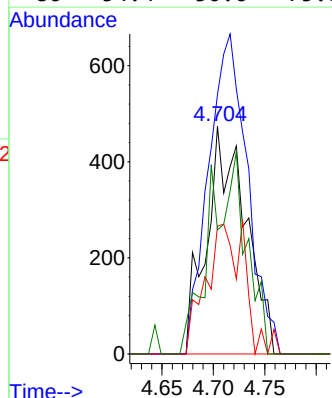

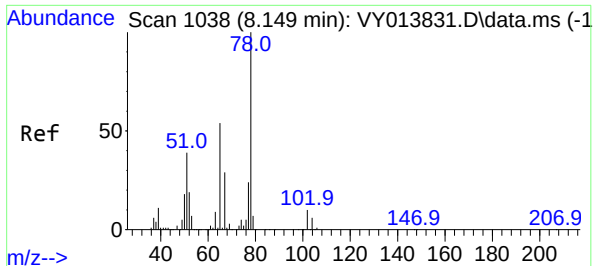

#33

1,2-Dichloroethane-d4

Concen: 82.893 ug/l

RT: 8.142 min Scan# 1037

Delta R.T. -0.006 min

Lab File: VY013842.D

Acq: 24 May 2023 13:38

Instrument :

MSVOA_Y

ClientSampleId :





SB06A

Tgt Ion: 65 Resp: 6313

Ion Ratio Lower Upper

65 100

67 51.3 0.0 104.4

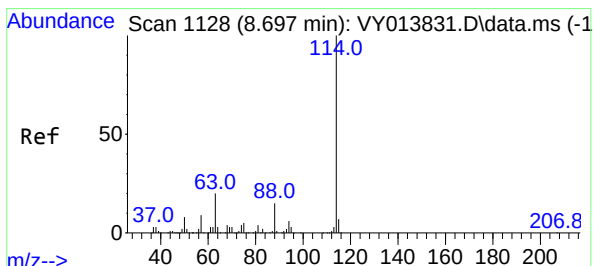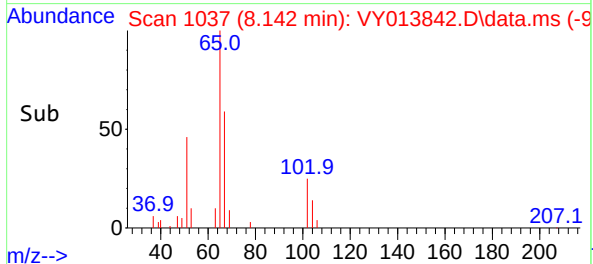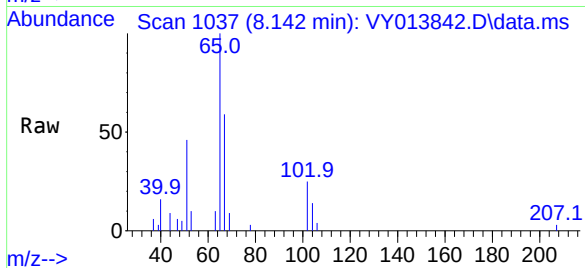

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. -0.006 min

Lab File: VY013842.D

Acq: 24 May 2023 13:38




Tgt Ion: 114 Resp: 11233


Ion Ratio Lower Upper

114 100

63 18.3 0.0 40.2


88 15.0 0.0 30.0

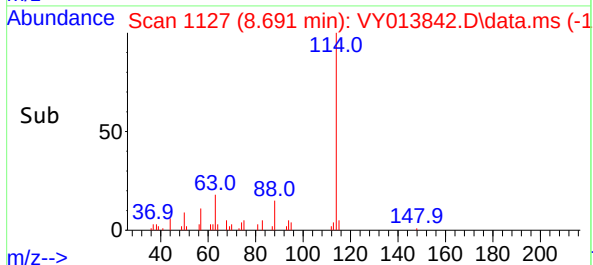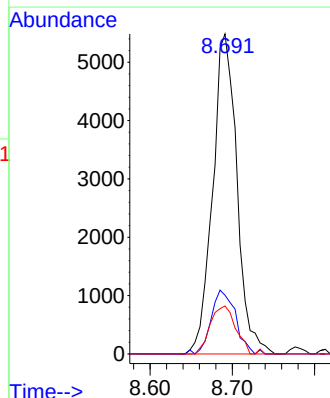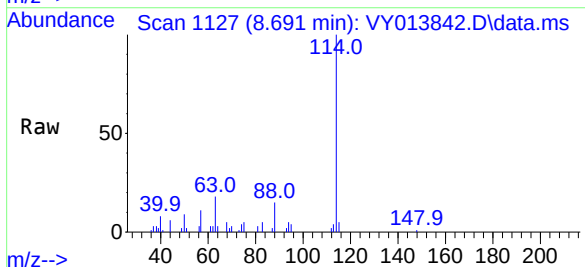



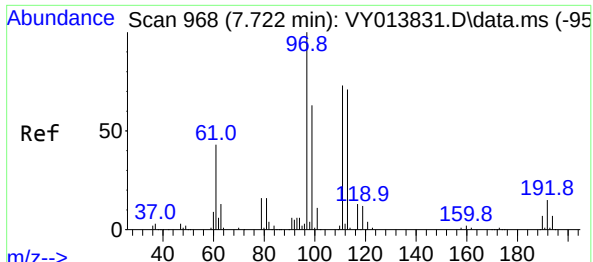


#35
Dibromofluoromethane
Concen: 67.477 ug/l
RT: 7.716 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38


Instrument :
MSVOA_Y
ClientSampleId :
SB06A

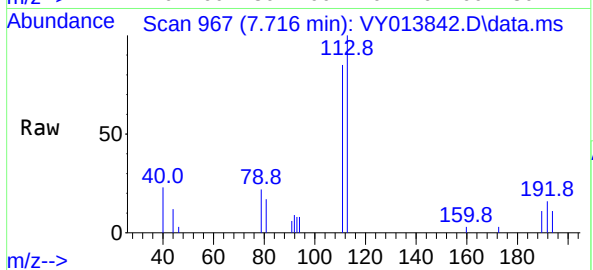



Tgt Ion:113 Resp: 4895
Ion Ratio Lower Upper
113 100
111 96.4 80.4 120.6
192 20.3 16.6 25.0

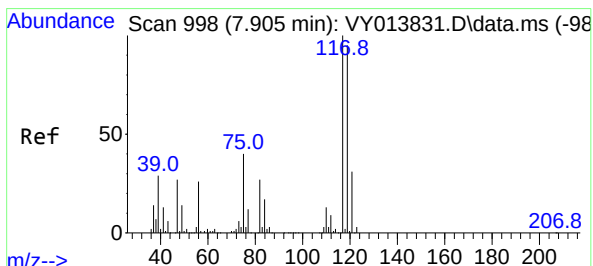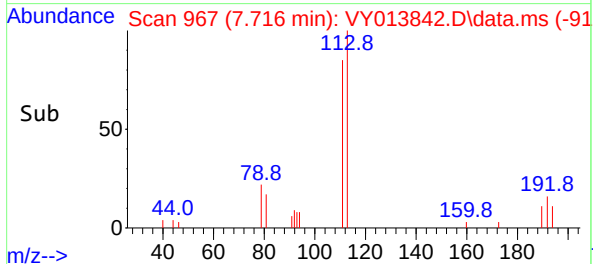


#38
Carbon Tetrachloride
Concen: 5.268 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.110 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

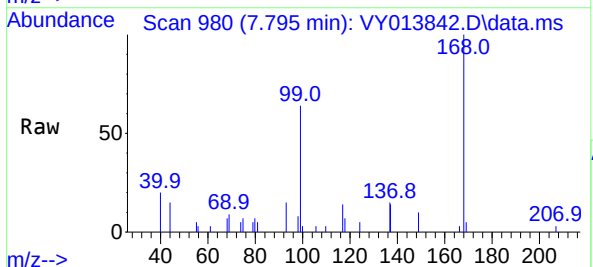

Tgt Ion:117 Resp: 662
Ion Ratio Lower Upper
117 100
119 0.0 75.6 113.4#
121 0.0 24.8 37.2#

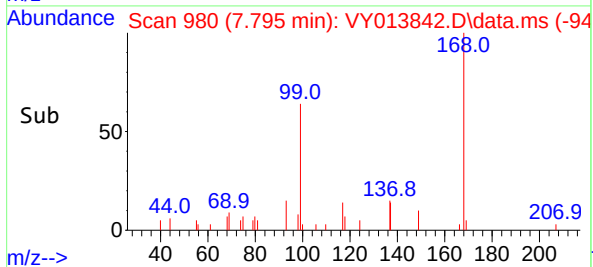

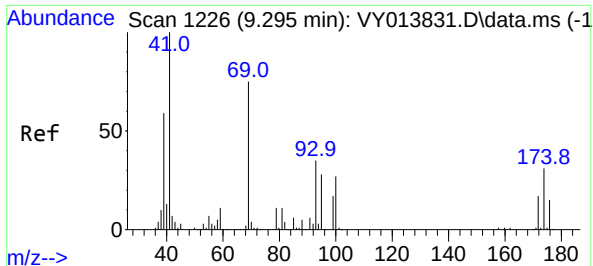

#48

Methyl methacrylate

Concen: 1.751 ug/l

RT: 9.404 min Scan# 1

Delta R.T. 0.110 min

Lab File: VY013842.D

Acq: 24 May 2023 13:38

Instrument :

MSVOA_Y

ClientSampleId :

SB06A





Tgt Ion: 41 Resp: 101

Ion Ratio Lower Upper

41 100

69 0.0 62.0 93.0#

39 0.0 45.7 68.5#

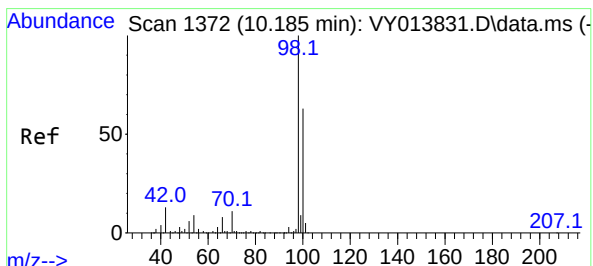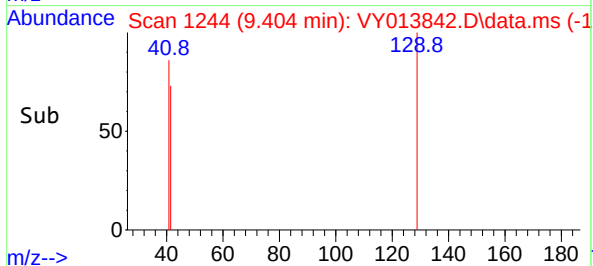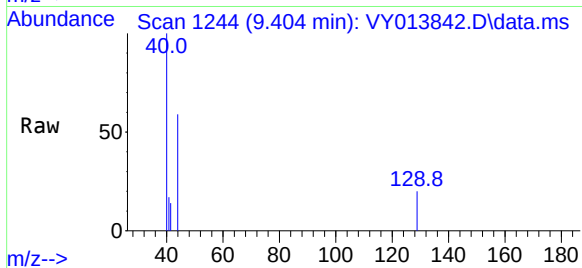

#50

Toluene-d8

Concen: 49.689 ug/l

RT: 10.179 min Scan# 1371

Delta R.T. -0.006 min

Lab File: VY013842.D




Acq: 24 May 2023 13:38


Tgt Ion: 98 Resp: 13700

Ion Ratio Lower Upper

98 100

100 59.9 50.8 76.2


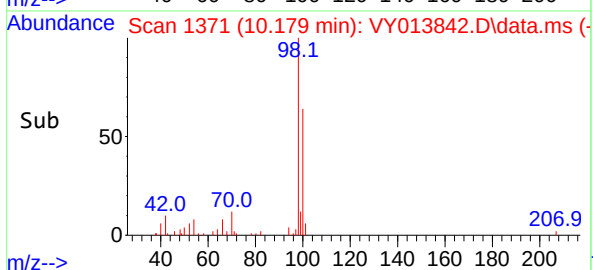

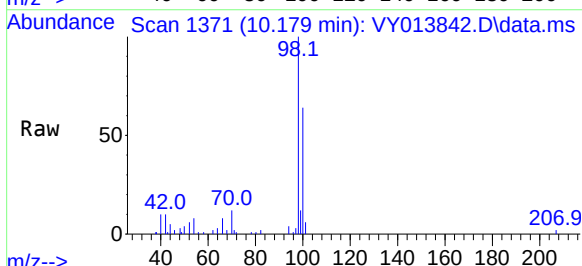




#51
4-Methyl-2-Pentanone
Concen: 1.192 ug/l
RT: 10.069 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion: 43 Resp: 78
Ion Ratio Lower Upper
43 100
58 0.0 29.1 43.7#

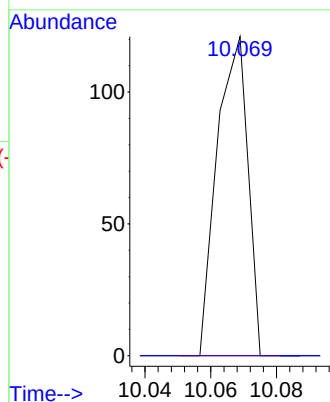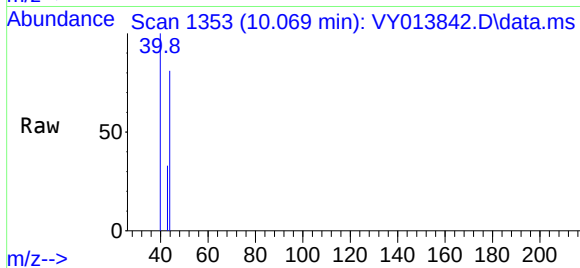

#60
Dibromochloromethane
Concen: 1.022 ug/l
RT: 10.727 min Scan# 1461
Delta R.T. -0.256 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion: 129 Resp: 81
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#


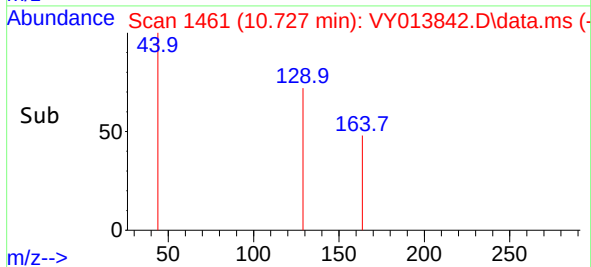
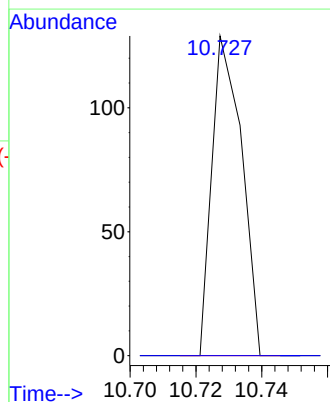
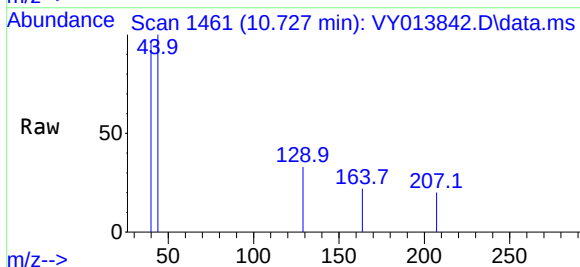




#62
4-Bromofluorobenzene
Concen: 38.386 ug/l
RT: 12.483 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion:	95	Resp:	3518
Ion	Ratio	Lower	Upper
95	100		
174	106.0	0.0	176.0
176	104.7	0.0	170.2

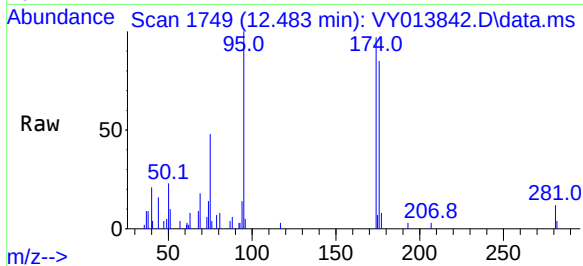

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion:	117	Resp:	10957
Ion	Ratio	Lower	Upper
117	100		
82	54.2	44.2	66.4
119	26.4	25.7	38.5


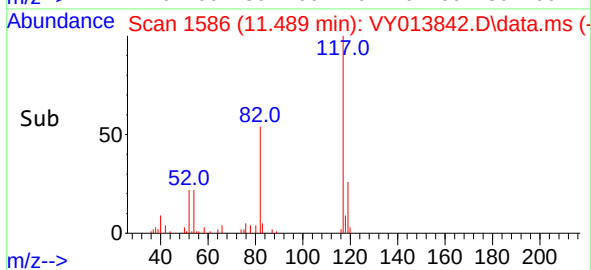

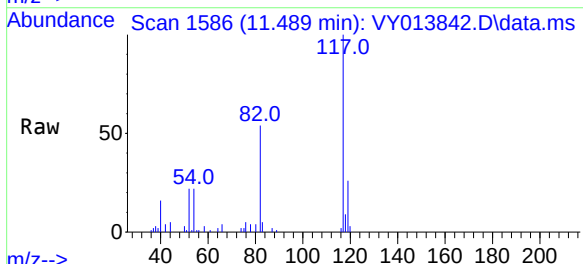




#68
m/p-Xylenes
Concen: 1.106 ug/l
RT: 11.703 min Scan# 1621
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion:106 Resp: 173
Ion Ratio Lower Upper
106 100
91 204.6 164.9 247.3

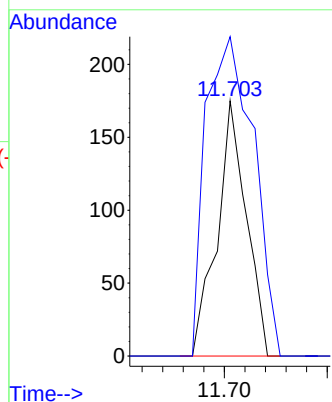

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion:152 Resp: 3672
Ion Ratio Lower Upper
152 100
115 53.8 28.8 86.5
150 152.6 0.0 353.4


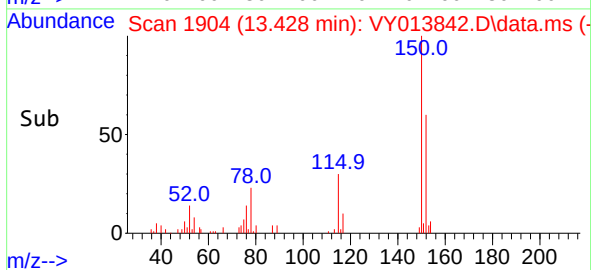






#76
1,2,3-Trichloropropane
Concen: 49.448 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.159 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion: 75 Resp: 2141
Ion Ratio Lower Upper
75 100
77 0.0 0.0 0.0

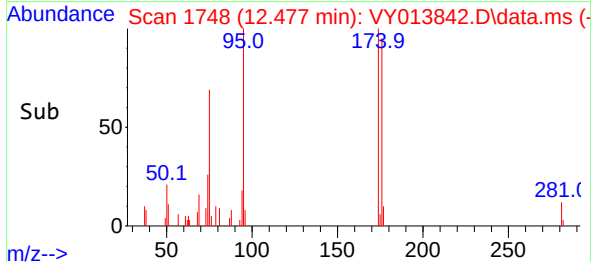

#77
Bromobenzene
Concen: 1.044 ug/l
RT: 12.611 min Scan# 1770
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion: 156 Resp: 70
Ion Ratio Lower Upper
156 100
77 301.4 91.6 274.8#
158 34.3 48.9 146.6#


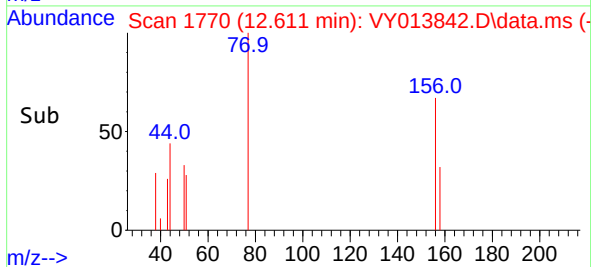

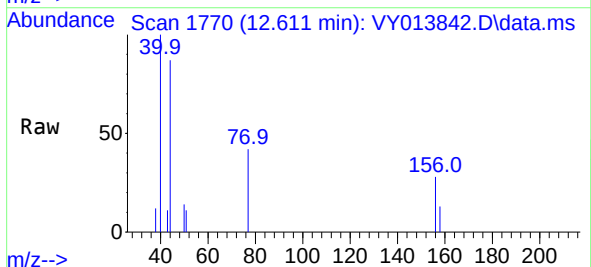




#78
n-propylbenzene
Concen: 1.117 ug/l
RT: 12.672 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion: 91 Resp: 377
Ion Ratio Lower Upper
91 100
120 0.0 11.3 33.9#



#79
2-Chlorotoluene
Concen: 1.193 ug/l
RT: 12.757 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion: 91 Resp: 225
Ion Ratio Lower Upper
91 100
126 0.0 17.8 53.4#


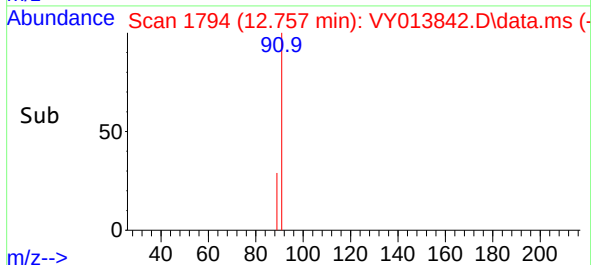
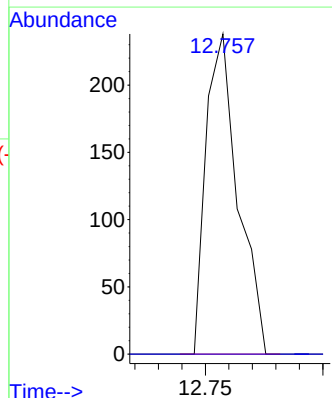
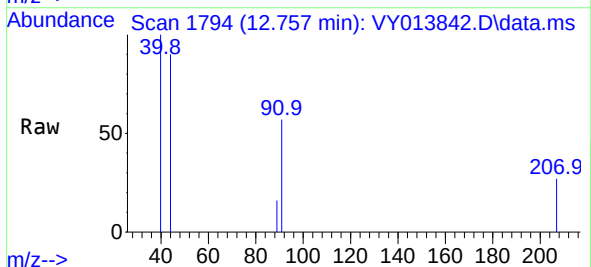




#81
trans-1,4-Dichloro-2-butene
Concen: 107.337 ug/l
RT: 12.477 min Scan# 11
Delta R.T. 0.097 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion: 75 Resp: 2141
Ion Ratio Lower Upper
75 100
53 0.0 79.7 119.5#
89 0.0 36.4 54.6#

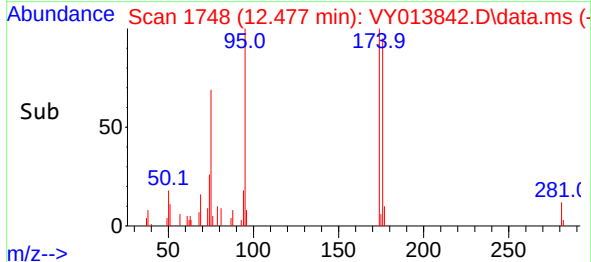

#82
4-Chlorotoluene
Concen: 1.975 ug/l
RT: 12.867 min Scan# 1812
Delta R.T. 0.012 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion: 91 Resp: 385
Ion Ratio Lower Upper
91 100
126 0.0 17.9 53.7#


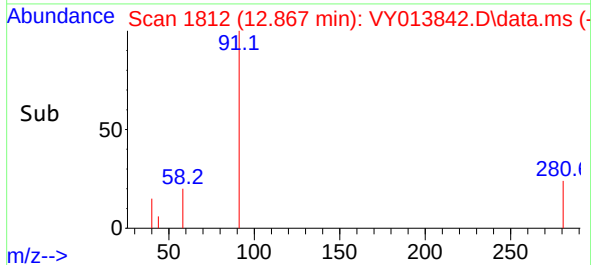

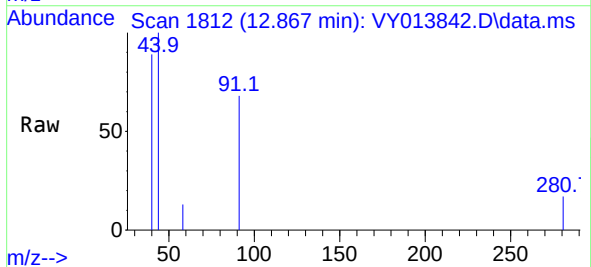




#83
tert-Butylbenzene
Concen: 1.099 ug/l
RT: 13.081 min Scan# 1846
Delta R.T. 0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion:119 Resp: 216
Ion Ratio Lower Upper
119 100
91 72.7 33.7 101.0
134 9.3 13.1 39.1#



#85
sec-Butylbenzene
Concen: 1.213 ug/l
RT: 13.257 min Scan# 1876
Delta R.T. 0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion:105 Resp: 354
Ion Ratio Lower Upper
105 100
134 0.0 10.3 30.8#


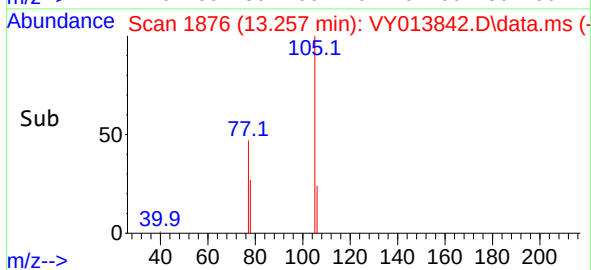






#86
p-Isopropyltoluene
Concen: 1.331 ug/l
RT: 13.367 min Scan# 1894
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion:	119	Resp:	321
Ion	Ratio	Lower	Upper
119	100		
134	24.9	13.3	39.9
91	0.0	12.4	37.4#

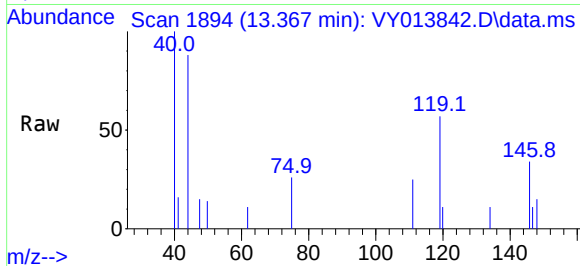

#87
1,3-Dichlorobenzene
Concen: 2.695 ug/l
RT: 13.373 min Scan# 1895
Delta R.T. 0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion:	146	Resp:	349
Ion	Ratio	Lower	Upper
146	100		
111	35.5	19.1	57.5
148	37.0	31.8	95.3


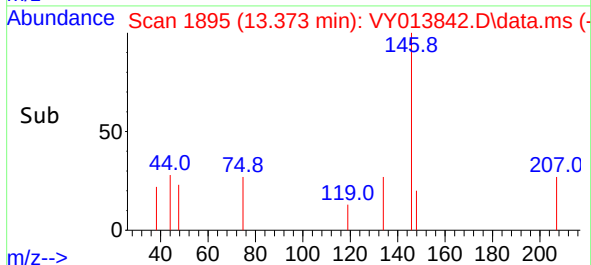
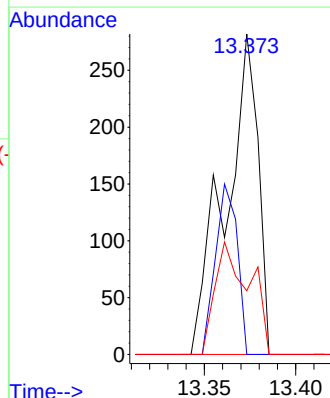
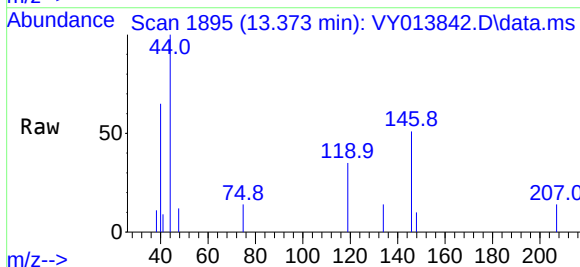




#88
1,4-Dichlorobenzene
Concen: 2.288 ug/l
RT: 13.446 min Scan# 1907
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion:	146	Resp:	295
Ion	Ratio	Lower	Upper
146	100		
111	44.4	18.6	55.8
148	69.2	32.4	97.2

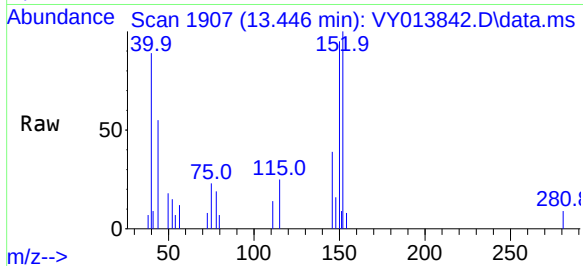

#89
n-Butylbenzene
Concen: 1.513 ug/l
RT: 13.702 min Scan# 1949
Delta R.T. 0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion:	91	Resp:	350
Ion	Ratio	Lower	Upper
91	100		
92	42.3	25.6	76.6
134	11.4	13.0	38.9


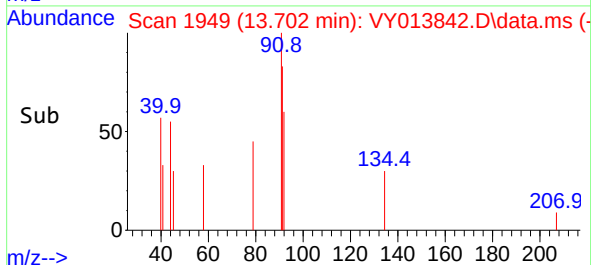
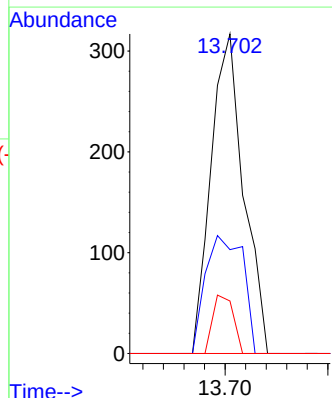
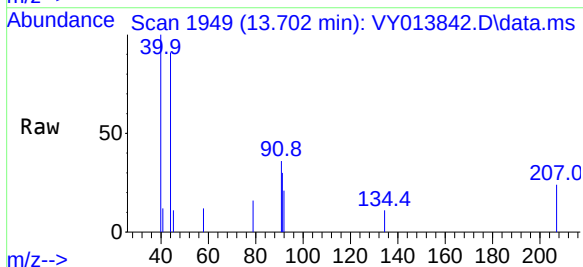




#90
Hexachloroethane
Concen: 1.353 ug/l
RT: 13.965 min Scan# 1992
Delta R.T. 0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion:117 Resp: 67
Ion Ratio Lower Upper
117 100
201 0.0 42.3 126.8#

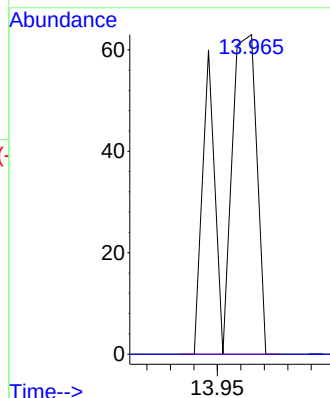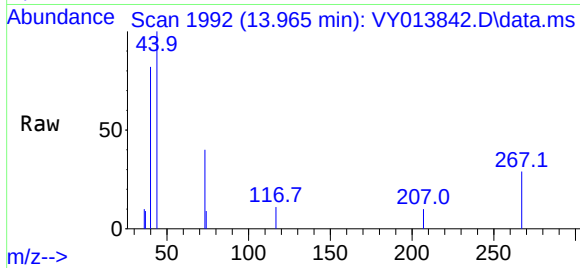

#91
1,2-Dichlorobenzene
Concen: 3.058 ug/l
RT: 13.733 min Scan# 1954
Delta R.T. -0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion:146 Resp: 352
Ion Ratio Lower Upper
146 100
111 46.0 19.6 58.8
148 28.7 32.1 96.5#


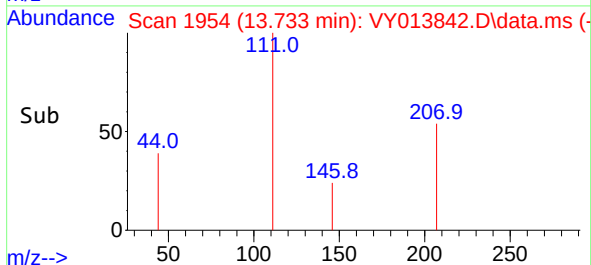
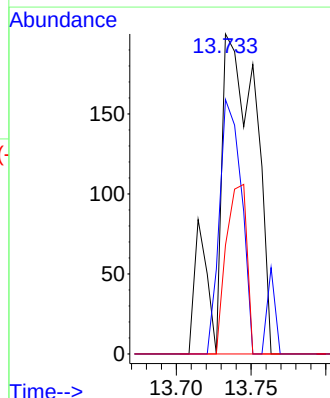
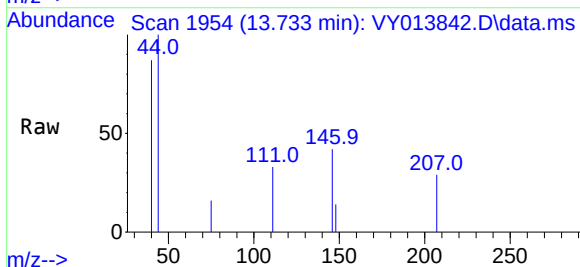




#92
1,2-Dibromo-3-Chloropropane
Concen: 6.457 ug/l
RT: 14.355 min Scan# 2056
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion: 75 Resp: 64
Ion Ratio Lower Upper
75 100
155 0.0 39.9 119.6#
157 0.0 54.6 163.8#

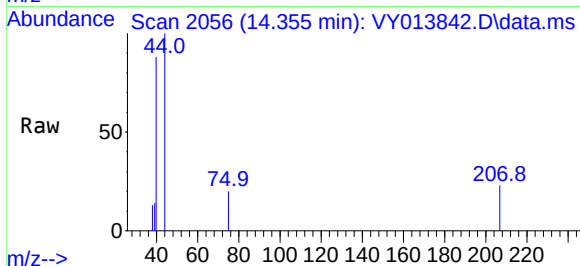

#93
1,2,4-Trichlorobenzene
Concen: 5.115 ug/l
RT: 15.007 min Scan# 2163
Delta R.T. -0.000 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38

Tgt Ion: 180 Resp: 365
Ion Ratio Lower Upper
180 100
182 59.5 48.1 144.3
145 6.3 14.8 44.4#


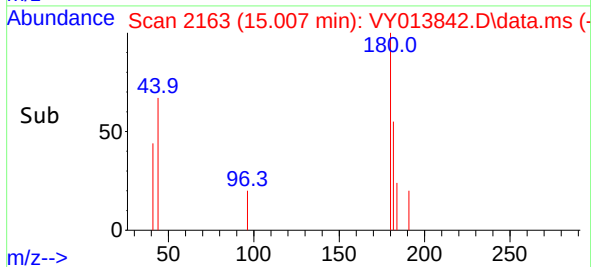

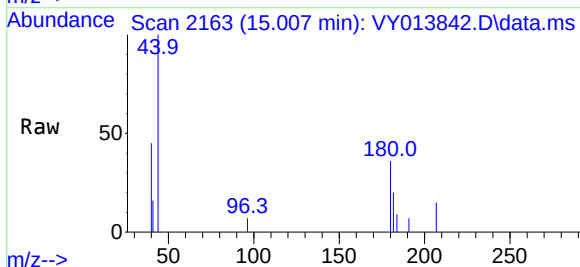




#94
Hexachlorobutadiene
Concen: 3.556 ug/l
RT: 15.105 min Scan# 21
Delta R.T. -0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38




Instrument :
MSVOA_Y
ClientSampleId :
SB06A


Tgt Ion:	225	Resp:	160
Ion	Ratio	Lower	Upper
225	100		
223	85.0	31.3	93.9
227	45.0	32.9	98.6



#95
Naphthalene
Concen: 8.215 ug/l
RT: 15.233 min Scan# 2200
Delta R.T. -0.006 min
Lab File: VY013842.D
Acq: 24 May 2023 13:38


Tgt Ion:	128	Resp:	632
Ion	Ratio	Lower	Upper
128	100		
127	8.2	10.7	16.1#
129	0.0	9.0	13.4#

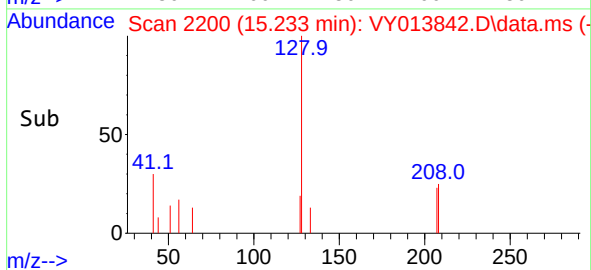



#96
 1,2,3-Trichlorobenzene
 Concen: 4.601 ug/l
 RT: 15.422 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VY013842.D
 Acq: 24 May 2023 13:38

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB06A



Tgt Ion:180 Resp: 292
 Ion Ratio Lower Upper
 180 100
 182 69.5 47.4 142.2
 145 0.0 15.5 46.5#

