

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060622\
 Data File : VY009137.D
 Acq On : 06 Jun 2022 11:10
 Operator : KP/MD
 Sample : VY0606SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0606SBL01

Quant Time: Jun 07 02:29:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
 Quant Title : SW846 8260
 QLast Update : Fri May 20 23:50:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	116767	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	209195	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	197003	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	83350	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	73662	61.296	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	122.600%
35) Dibromofluoromethane	7.716	113	66471	51.098	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.200%
50) Toluene-d8	10.179	98	258685	53.903	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	107.800%
62) 4-Bromofluorobenzene	12.483	95	74458	38.462	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	76.920%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060622\
Data File : VY009137.D
Acq On : 06 Jun 2022 11:10
Operator : KP/MD
Sample : VY0606SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0606SBL01

Quant Time: Jun 07 02:29:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y052022S.M
Quant Title : SW846 8260
QLast Update : Fri May 20 23:50:52 2022
Response via : Initial Calibration




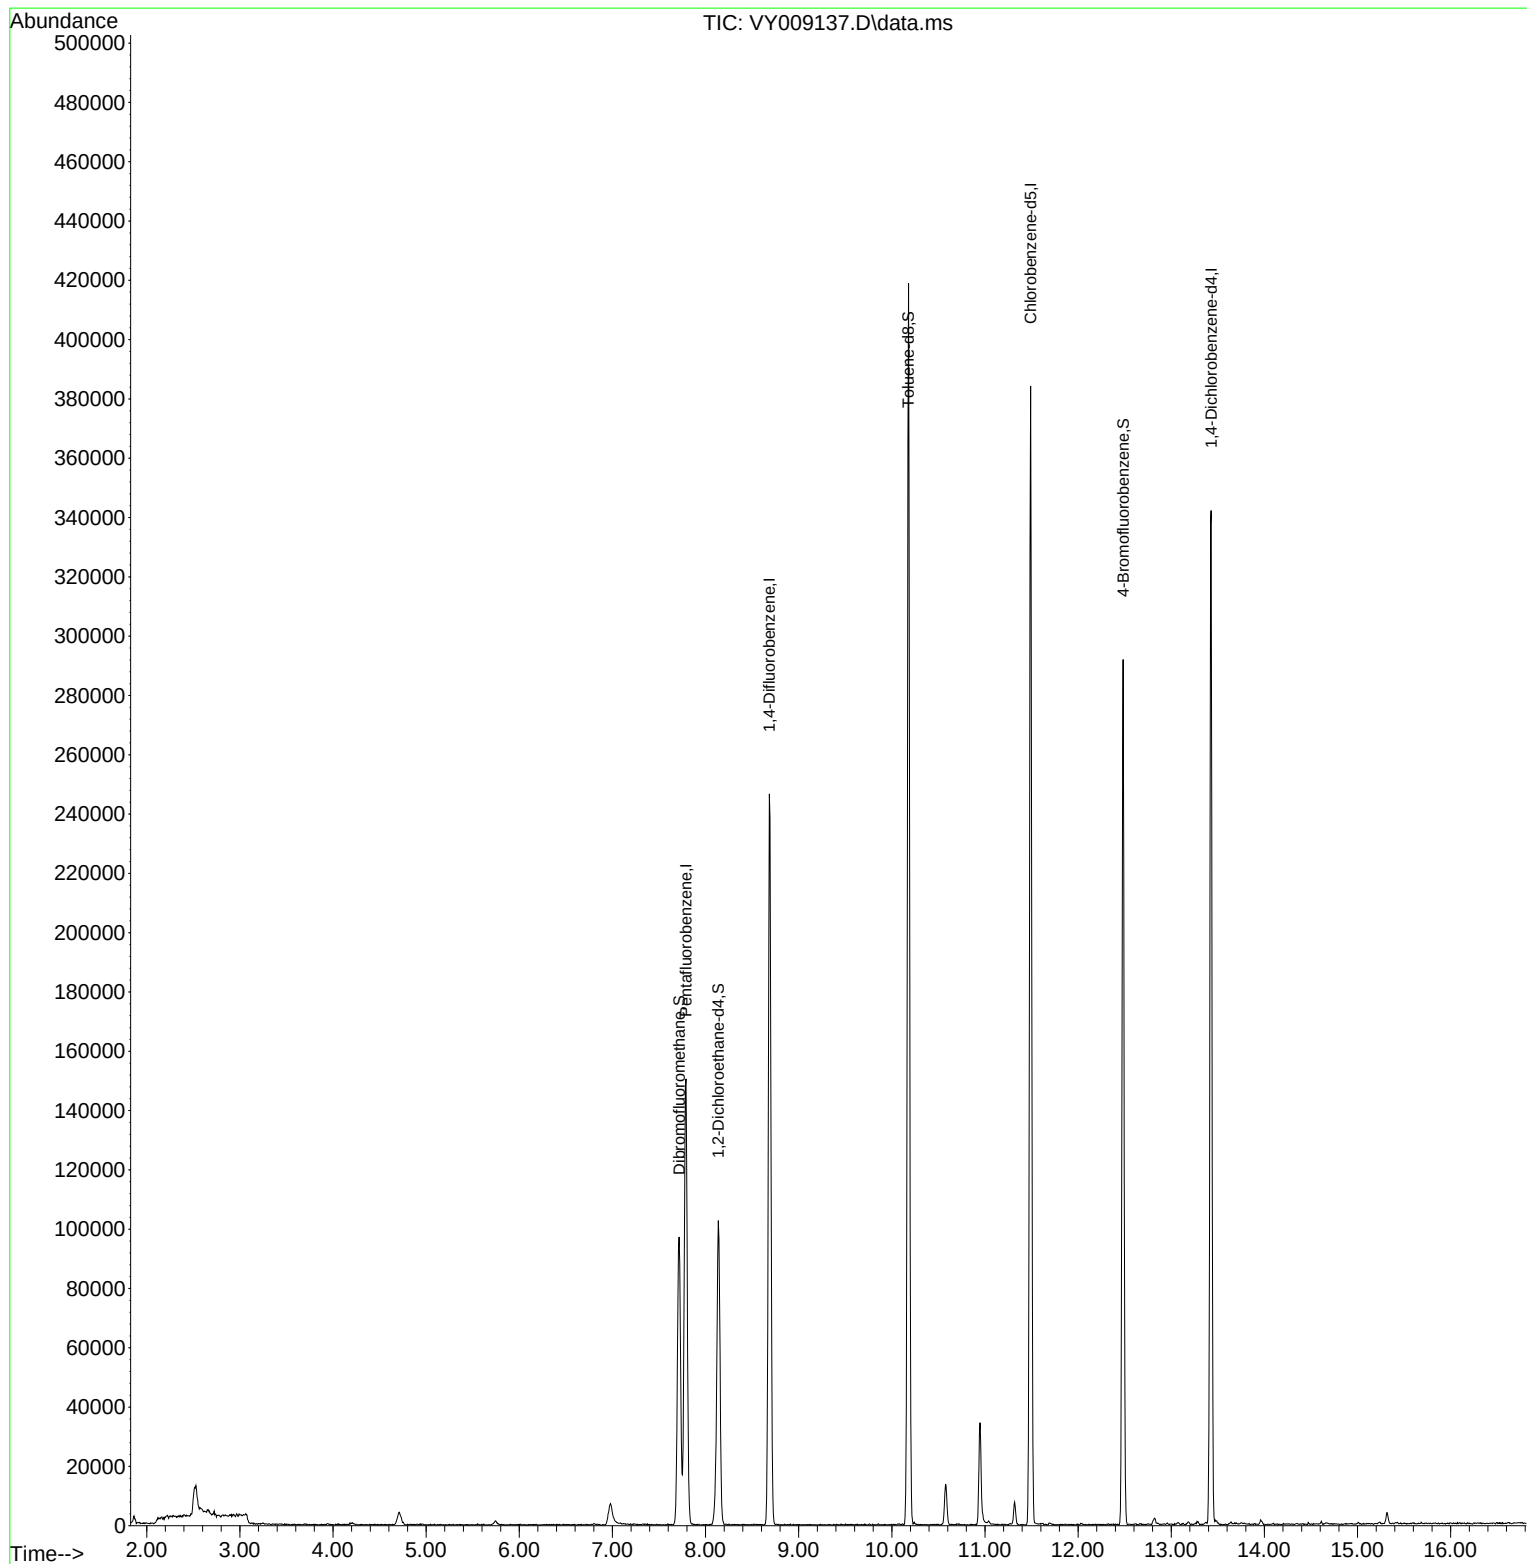


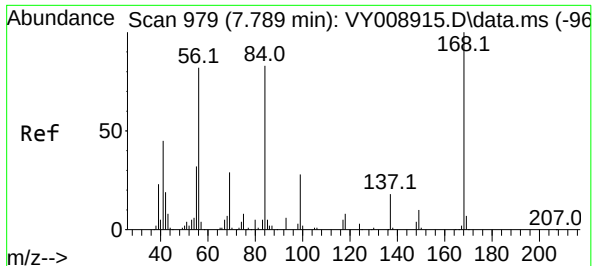

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY009137.D
Acq: 06 Jun 2022 11:10




Instrument :
MSVOA_Y
ClientSampleId :
VY0606SBL01


Tgt Ion:168 Resp: 116767
Ion Ratio Lower Upper
168 100
99 49.4 46.9 70.3

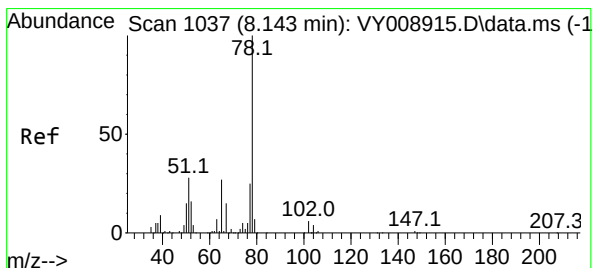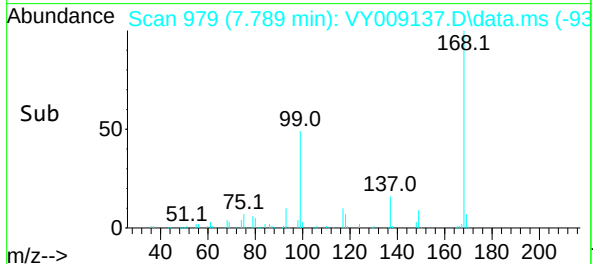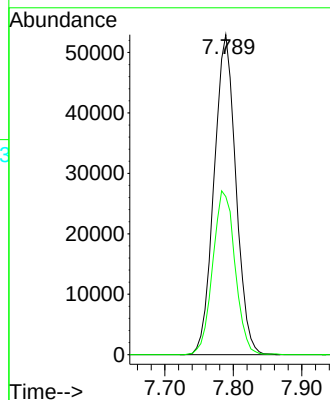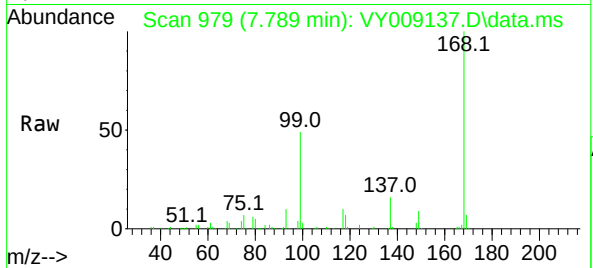

#33
1,2-Dichloroethane-d4
Concen: 61.296 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VY009137.D
Acq: 06 Jun 2022 11:10

Tgt Ion: 65 Resp: 73662
Ion Ratio Lower Upper
65 100
67 51.6 0.0 99.4


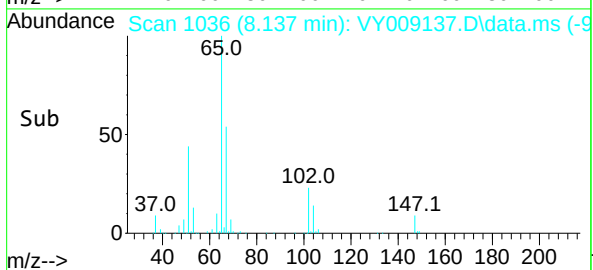
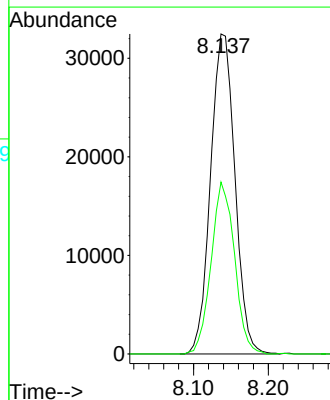
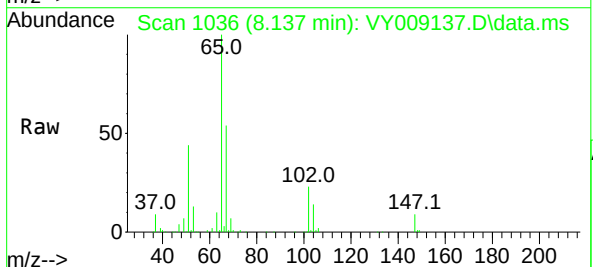


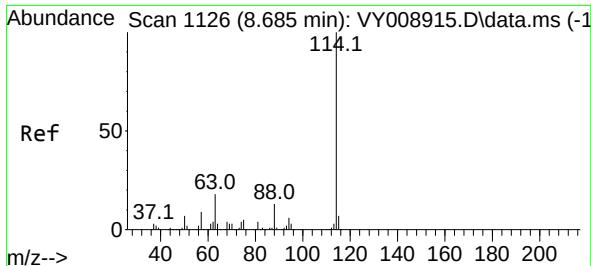

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VY009137.D
Acq: 06 Jun 2022 11:10




Instrument :
MSVOA_Y
ClientSampleId :
VY0606SBL01


Tgt Ion:114 Resp: 209195
Ion Ratio Lower Upper
114 100
63 19.0 0.0 43.2
88 12.9 0.0 31.8

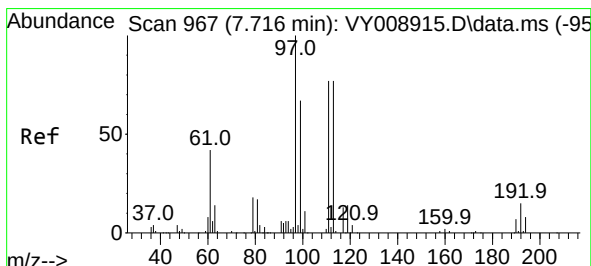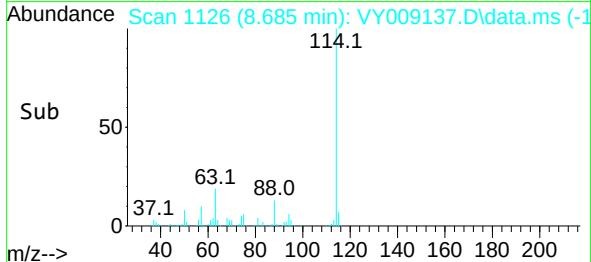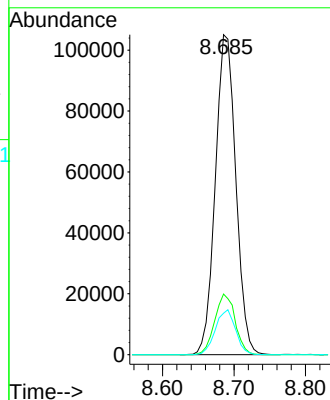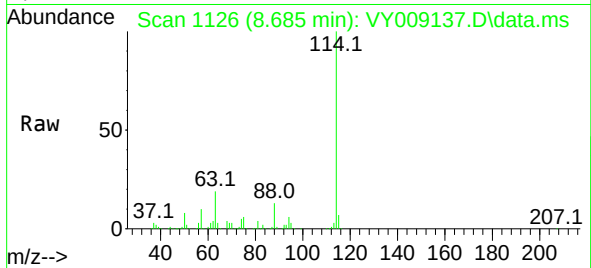

#35
Dibromofluoromethane
Concen: 51.098 ug/l
RT: 7.716 min Scan# 967
Delta R.T. -0.000 min
Lab File: VY009137.D
Acq: 06 Jun 2022 11:10

Tgt Ion:113 Resp: 66471
Ion Ratio Lower Upper
113 100
111 103.7 82.6 124.0
192 19.2 17.6 26.4


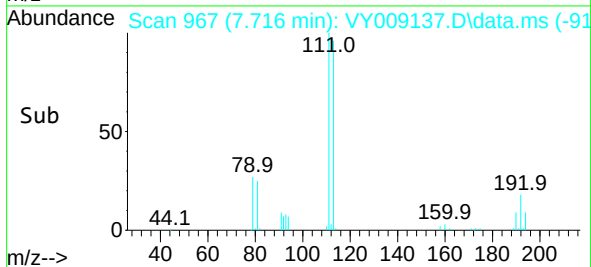
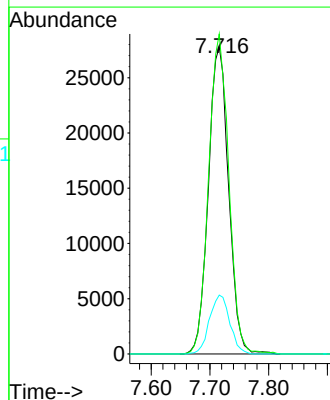
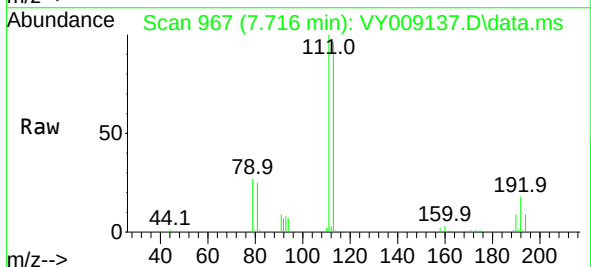


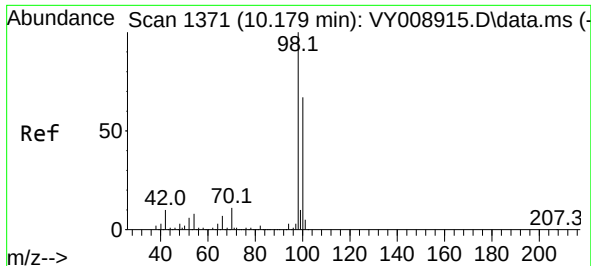

#50
Toluene-d8
Concen: 53.903 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY009137.D
Acq: 06 Jun 2022 11:10




Instrument :
MSVOA_Y
ClientSampleId :
VY0606SBL01


Tgt Ion: 98 Resp: 258685
Ion Ratio Lower Upper
98 100
100 64.6 50.2 75.2

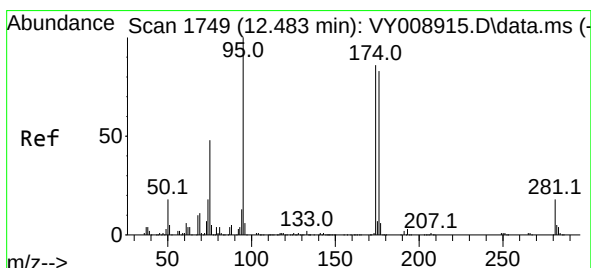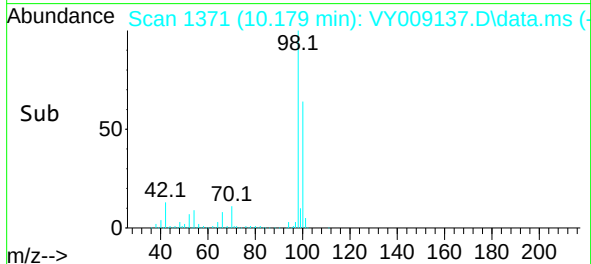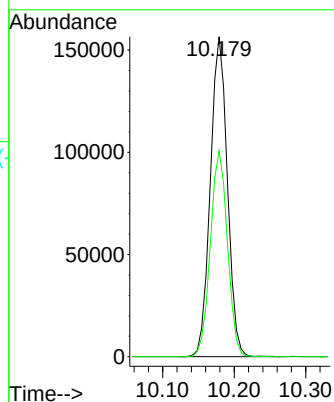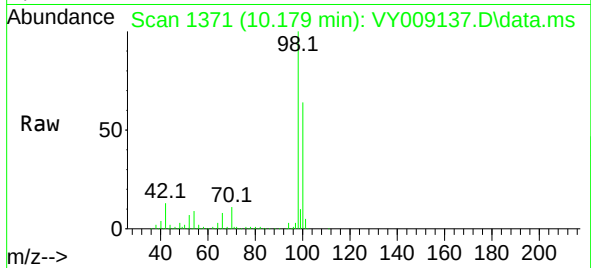

#62
4-Bromofluorobenzene
Concen: 38.462 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY009137.D
Acq: 06 Jun 2022 11:10

Tgt Ion: 95 Resp: 74458
Ion Ratio Lower Upper
95 100
174 91.1 0.0 177.0
176 86.6 0.0 175.8


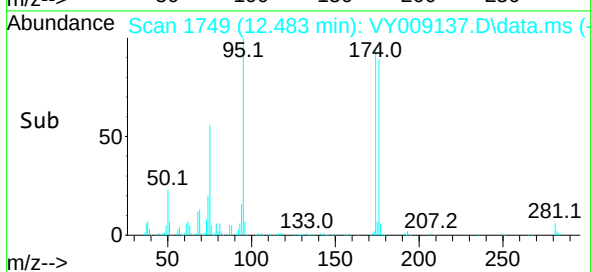
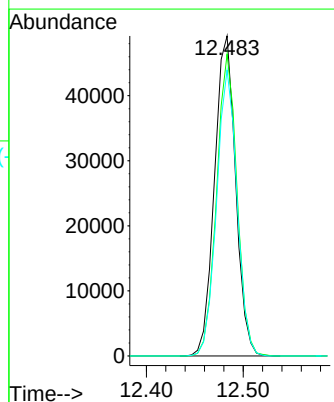
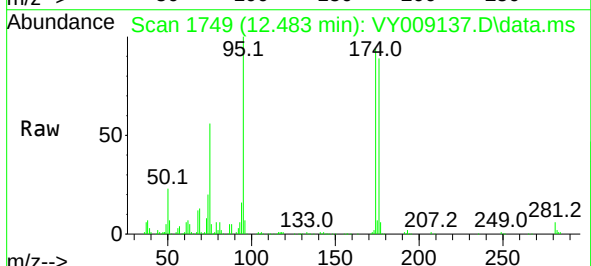


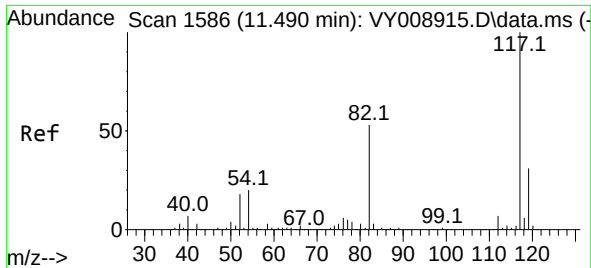

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY009137.D
Acq: 06 Jun 2022 11:10

Instrument :
MSVOA_Y
ClientSampleId :
VY0606SBL01

Tgt Ion:117 Resp: 197003
Ion Ratio Lower Upper
117 100
82 52.0 43.0 64.4
119 31.2 25.4 38.0

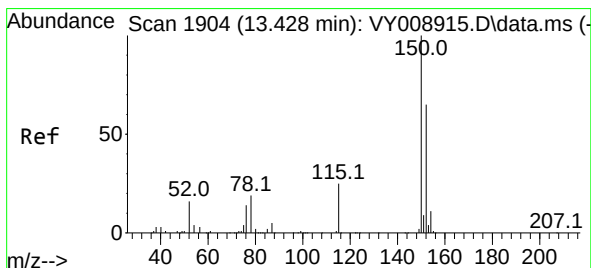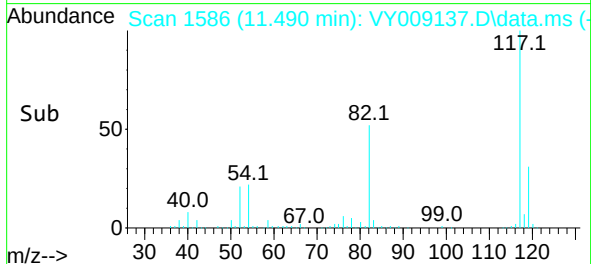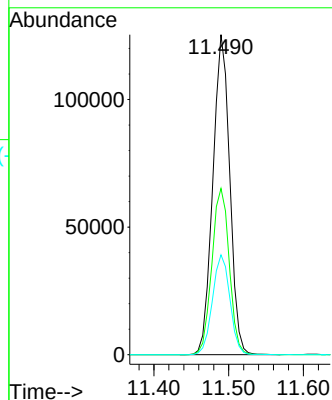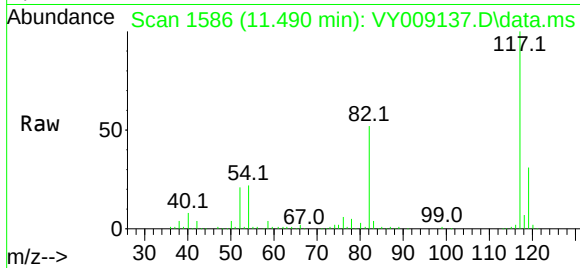

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY009137.D
Acq: 06 Jun 2022 11:10

Tgt Ion:152 Resp: 83350
Ion Ratio Lower Upper
152 100
115 55.7 28.2 84.7
150 155.6 0.0 347.6

