
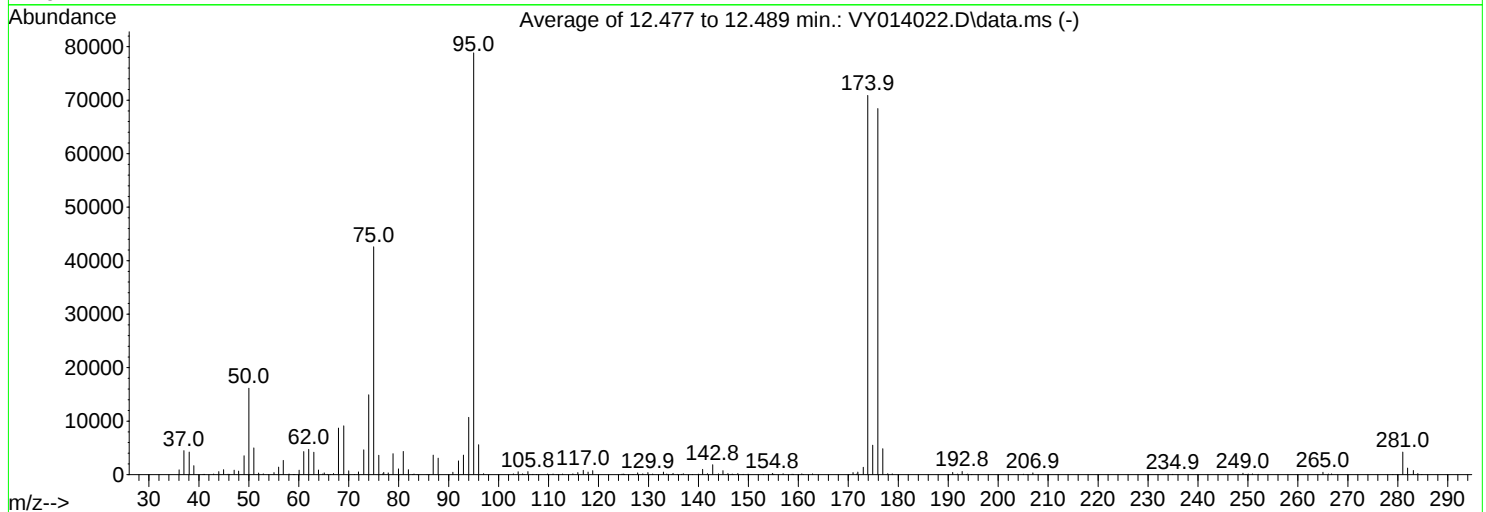


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060623\
Data File : VY014022.D
Acq On : 06 Jun 2023 09:53
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060123S.M
Title : SW846 8260
Last Update : Fri Jun 02 07:00:14 2023

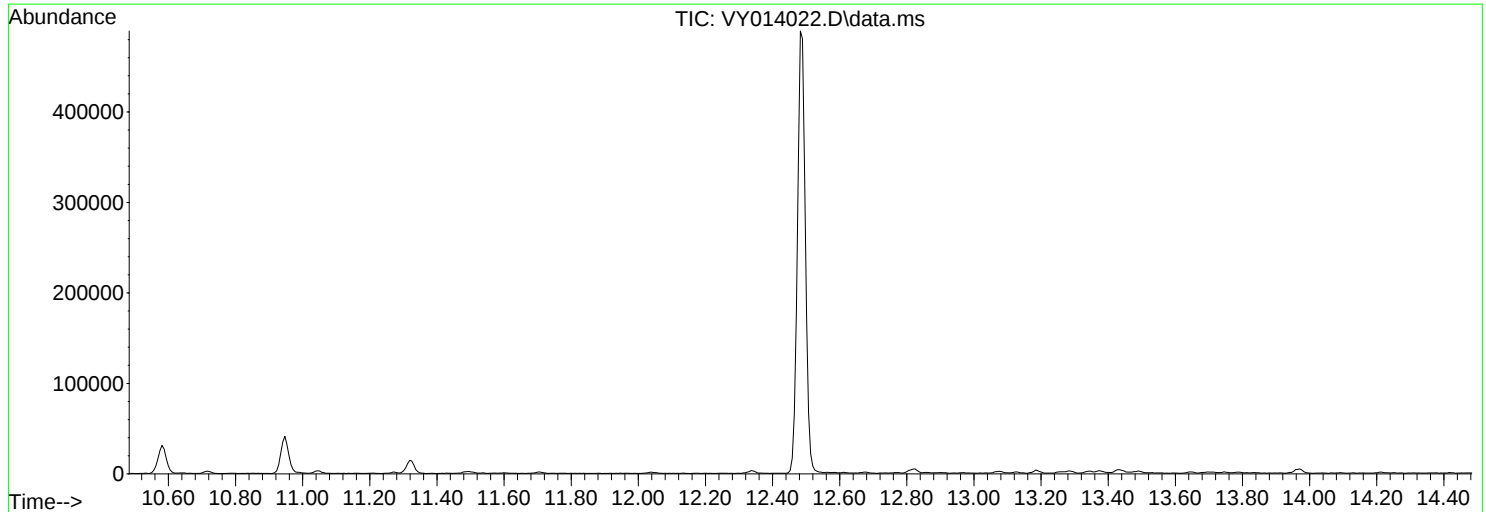

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	16154	PASS
75	95	30	60	54.0	42605	PASS
95	95	100	100	100.0	78851	PASS
96	95	5	9	7.1	5592	PASS
173	174	0.00	2	2.0	1387	PASS
174	95	50	100	89.9	70891	PASS
175	174	5	9	7.8	5515	PASS
176	174	95	101	96.5	68443	PASS
177	176	5	9	7.1	4846	PASS