
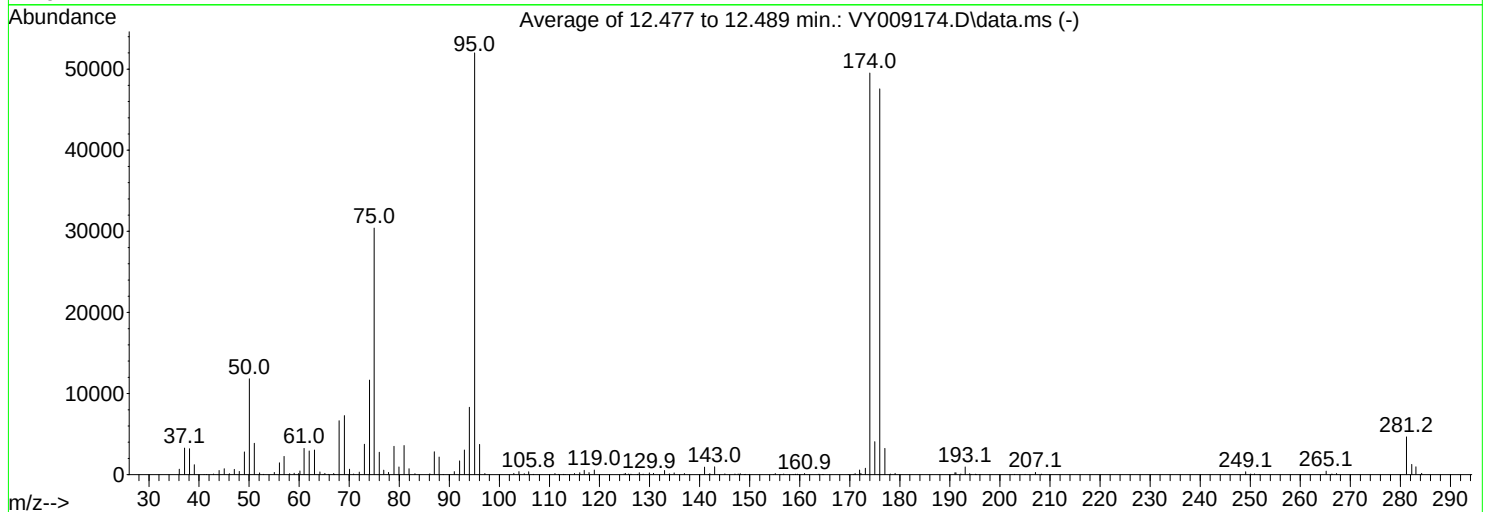


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060822\
Data File : VY009174.D
Acq On : 08 Jun 2022 16:47
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060822S.M
Title : SW846 8260
Last Update : Thu Jun 09 10:00:49 2022

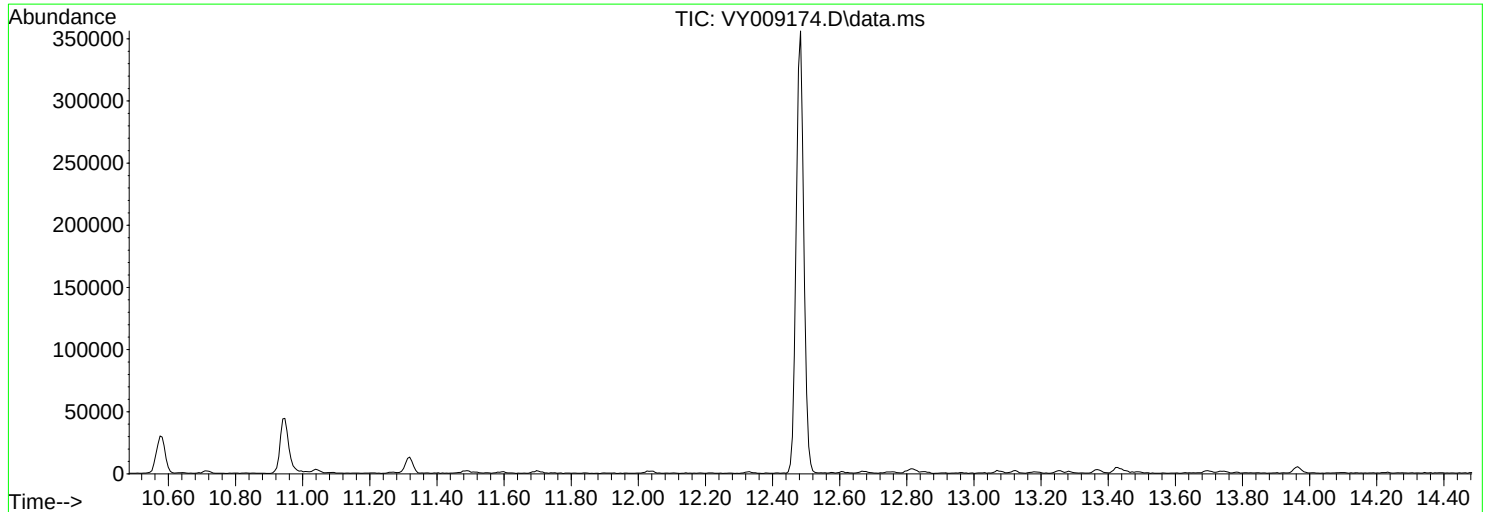

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	11820	PASS
75	95	30	60	58.4	30397	PASS
95	95	100	100	100.0	52008	PASS
96	95	5	9	7.2	3739	PASS
173	174	0.00	2	1.6	794	PASS
174	95	50	100	95.2	49528	PASS
175	174	5	9	8.2	4062	PASS
176	174	95	101	96.1	47573	PASS
177	176	5	9	6.8	3228	PASS