

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060823\
 Data File : VY014082.D
 Acq On : 08 Jun 2023 18:49
 Operator : KP/MD
 Sample : 03072-01
 Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 30999

Quant Time: Jun 09 04:23:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060123S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 02 07:00:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	153315	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	263842	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	276421	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	137963	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	108819	53.618	ug/l	0.00
Spiked Amount	50.000	Range 50 - 163	Recovery	= 107.240%		
35) Dibromofluoromethane	7.722	113	90534	53.994	ug/l	0.01
Spiked Amount	50.000	Range 54 - 147	Recovery	= 107.980%		
50) Toluene-d8	10.178	98	347067	54.265	ug/l	0.00
Spiked Amount	50.000	Range 58 - 134	Recovery	= 108.520%		
62) 4-Bromofluorobenzene	12.483	95	119073	54.609	ug/l	0.00
Spiked Amount	50.000	Range 30 - 143	Recovery	= 109.220%		
Target Compounds						
					Qvalue	
16) Acetone	3.960	43	75834	109.213	ug/l	97
17) Carbon Disulfide	4.204	76	14562	2.922	ug/l #	95
25) 2-Butanone	6.996	43	17966	20.769	ug/l	94
51) 4-Methyl-2-Pentanone	10.069	43	17866	9.020	ug/l	96
59) 2-Hexanone	10.831	43	9109	6.351	ug/l	79
95) Naphthalene	15.239	128	1494	4.095	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060823\
Data File : VY014082.D
Acq On : 08 Jun 2023 18:49
Operator : KP/MD
Sample : 03072-01
Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
30999

Quant Time: Jun 09 04:23:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060123S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 02 07:00:14 2023
Response via : Initial Calibration




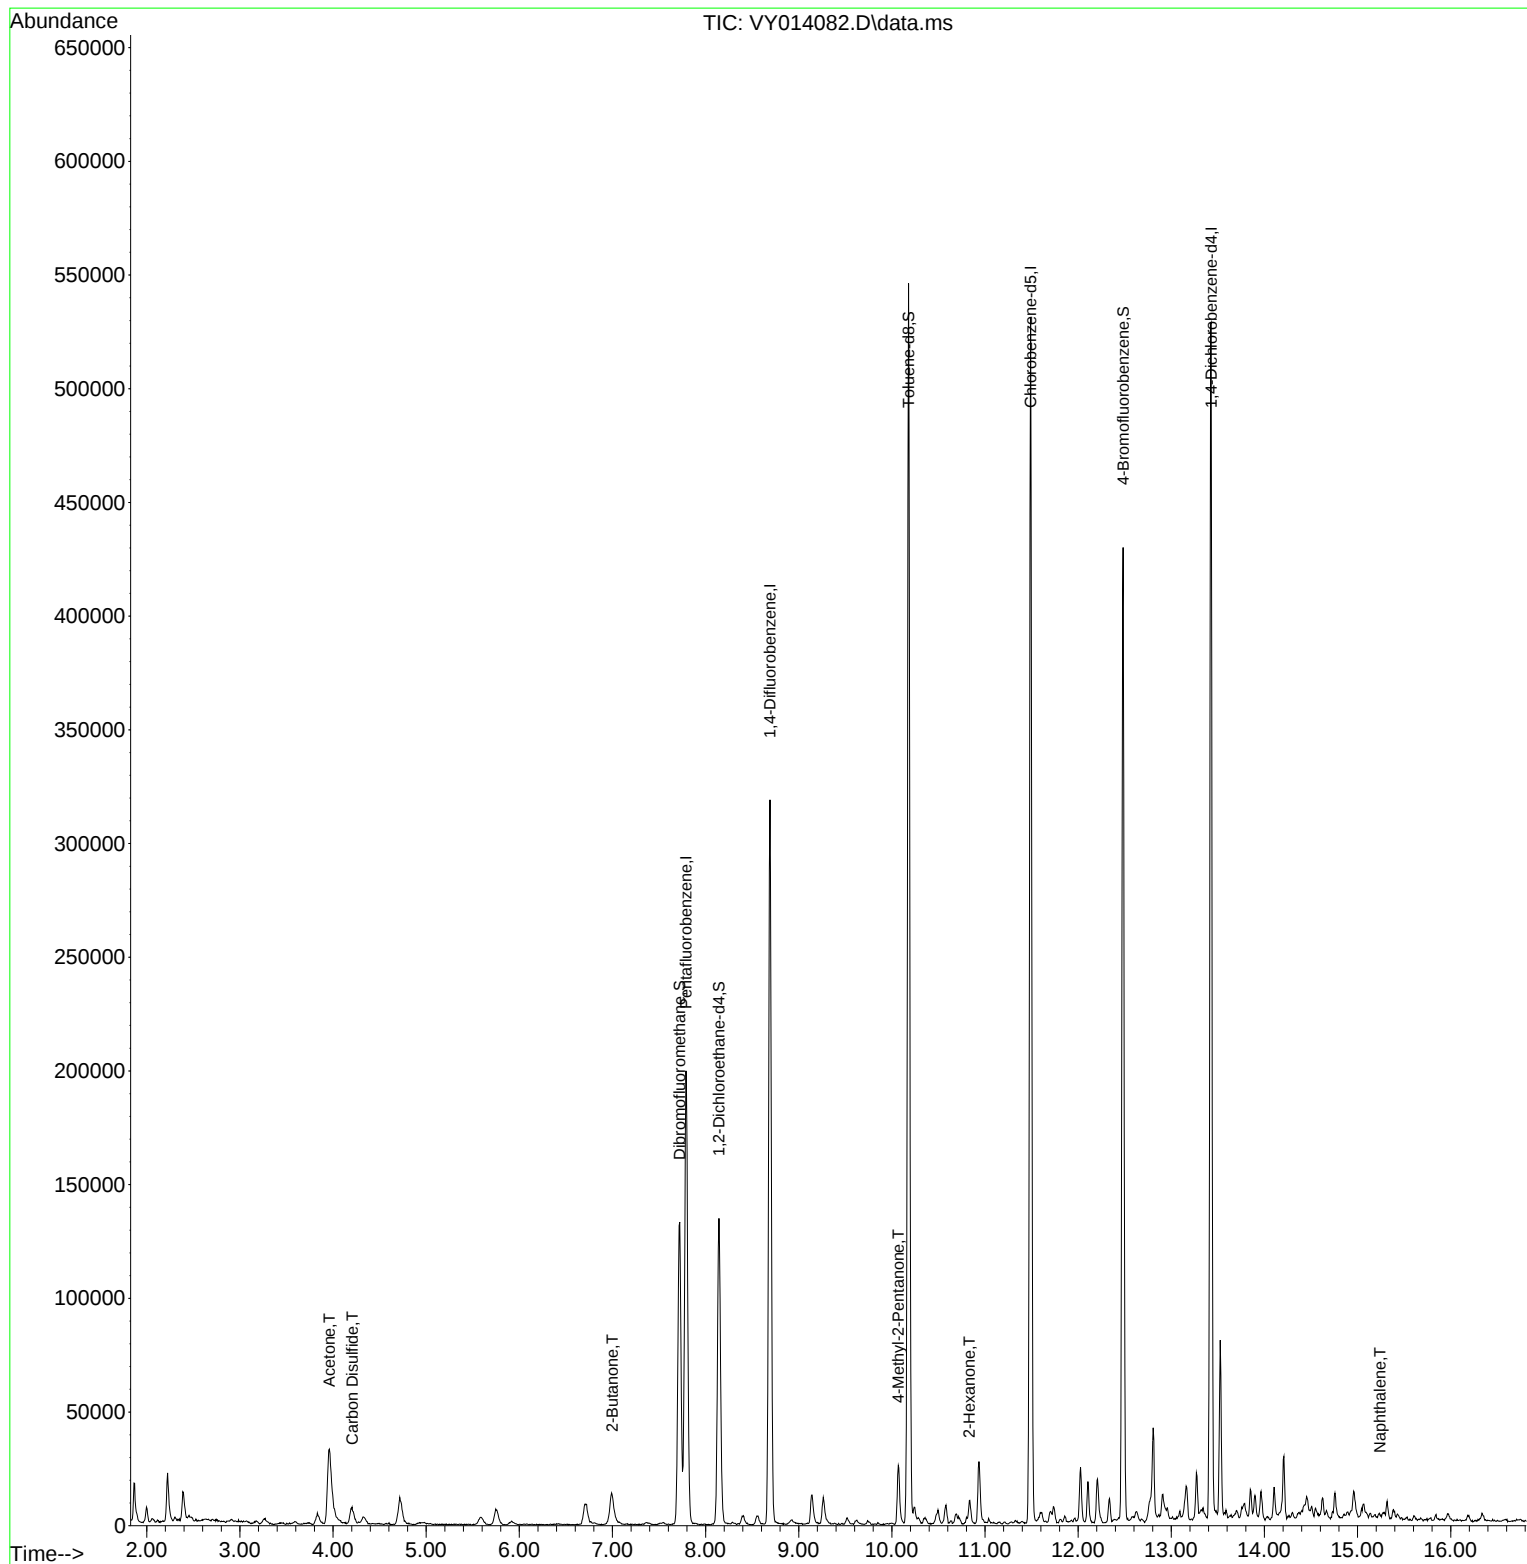


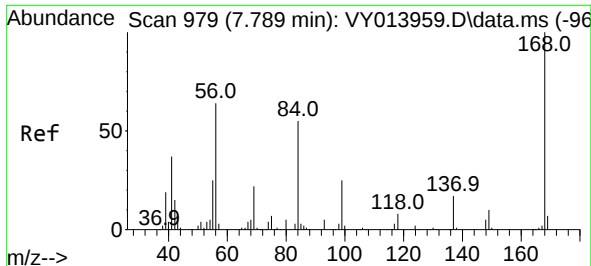

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49




Instrument :
MSVOA_Y
ClientSampleId :
30999


Tgt Ion:168 Resp: 153315
Ion Ratio Lower Upper
168 100
99 53.6 43.4 65.0

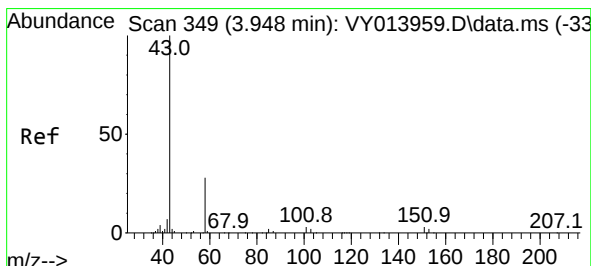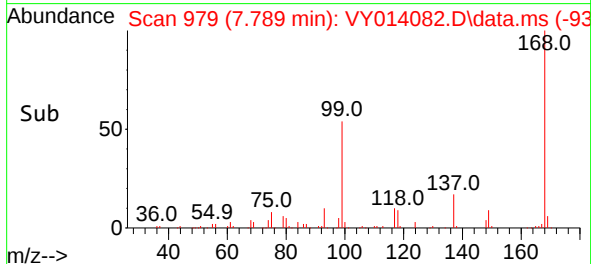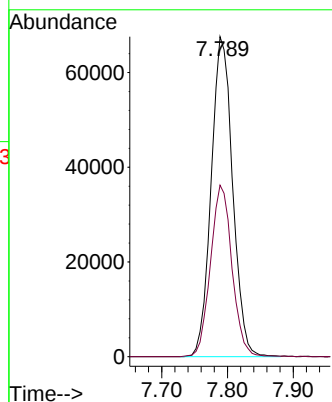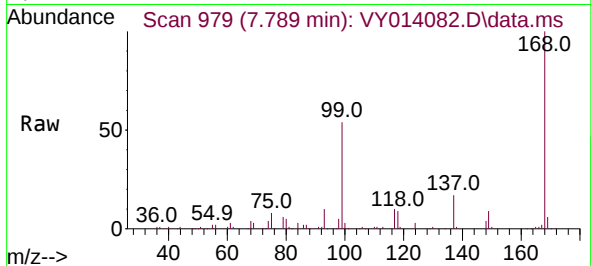

#16
Acetone
Concen: 109.213 ug/l
RT: 3.960 min Scan# 351
Delta R.T. 0.012 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49

Tgt Ion: 43 Resp: 75834
Ion Ratio Lower Upper
43 100
58 29.8 22.7 34.1


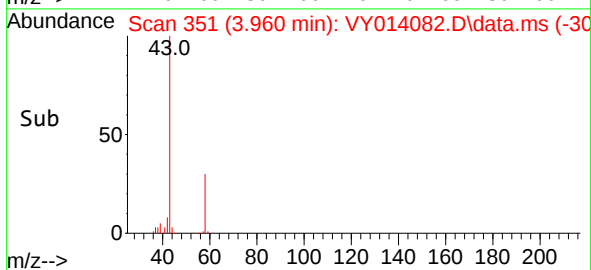
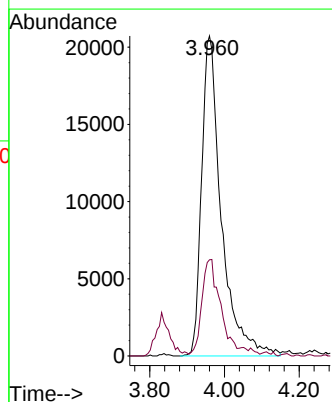
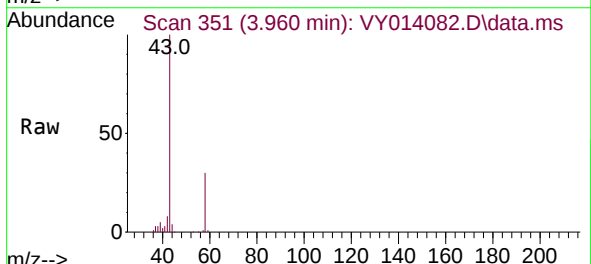


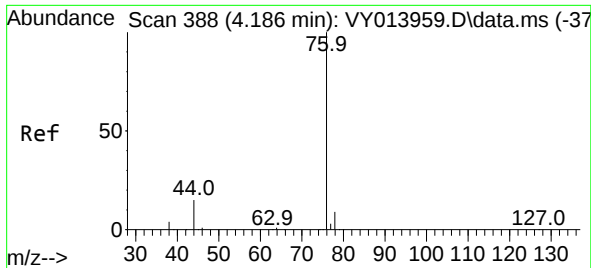

#17
Carbon Disulfide
Concen: 2.922 ug/l
RT: 4.204 min Scan# 391
Delta R.T. 0.018 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49




Instrument :
MSVOA_Y
ClientSampleId :
30999


Tgt Ion: 76 Resp: 14562
Ion Ratio Lower Upper
76 100
78 10.6 7.0 10.4#

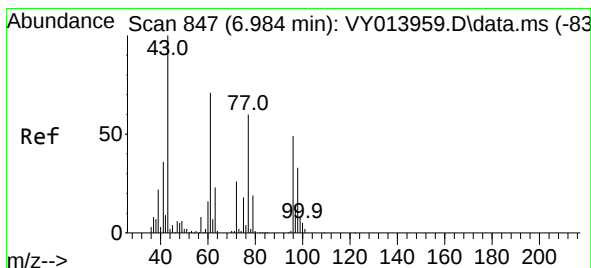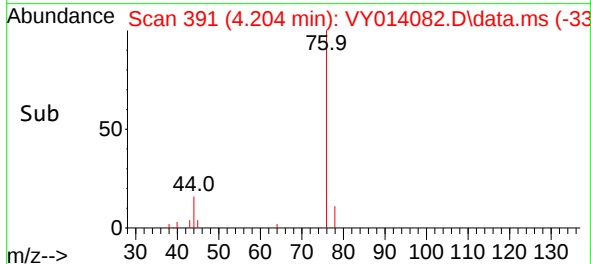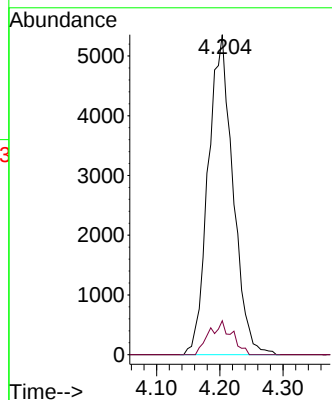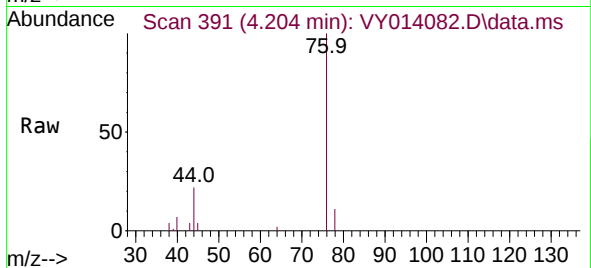

#25
2-Butanone
Concen: 20.769 ug/l
RT: 6.996 min Scan# 849
Delta R.T. 0.012 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49

Tgt Ion: 43 Resp: 17966
Ion Ratio Lower Upper
43 100
72 28.5 20.5 30.7

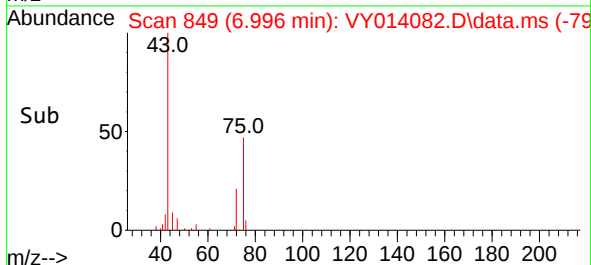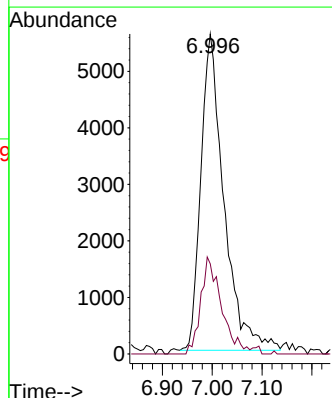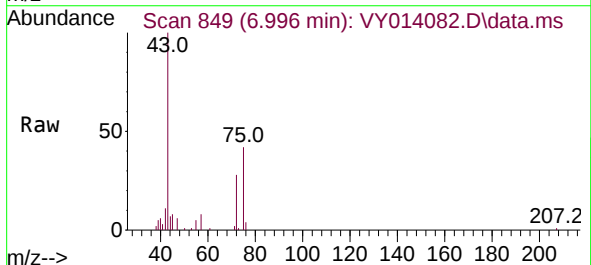

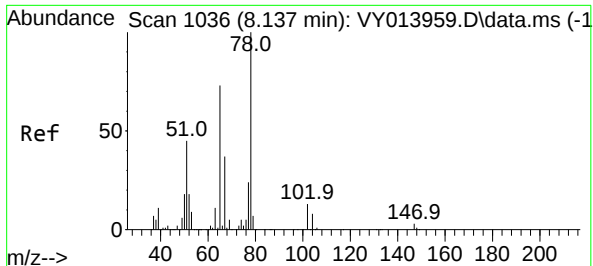

#33

1,2-Dichloroethane-d4

Concen: 53.618 ug/l

RT: 8.142 min Scan# 110

Delta R.T. 0.006 min

Lab File: VY014082.D

Acq: 08 Jun 2023 18:49

Instrument :

MSVOA_Y

ClientSampleId :





30999

Tgt Ion: 65 Resp: 108819

Ion Ratio Lower Upper

65 100

67 49.5 0.0 101.8

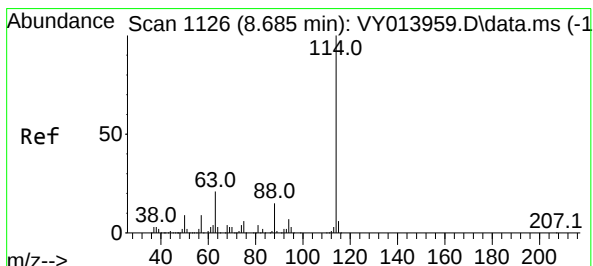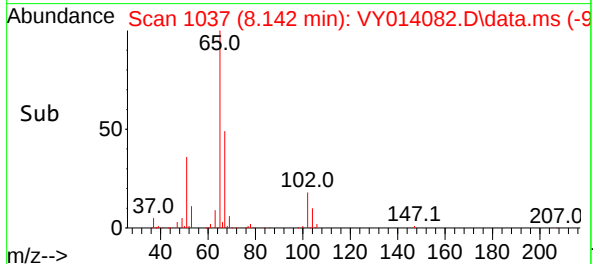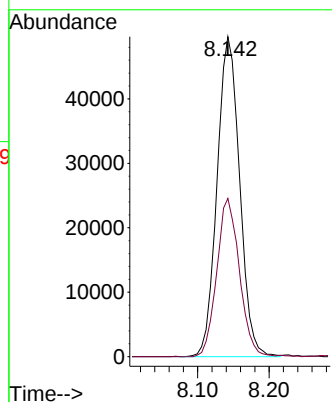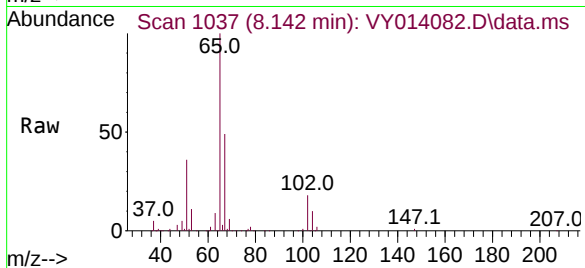

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY014082.D

Acq: 08 Jun 2023 18:49




Tgt Ion:114 Resp: 263842


Ion Ratio Lower Upper

114 100

63 19.5 0.0 42.4

88 14.4 0.0 30.6


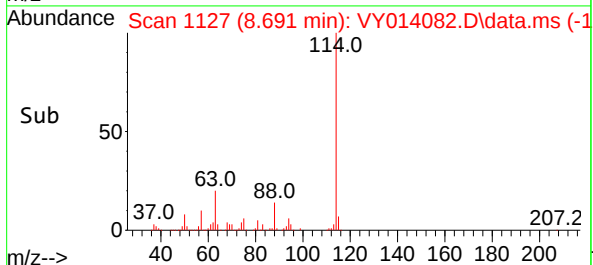
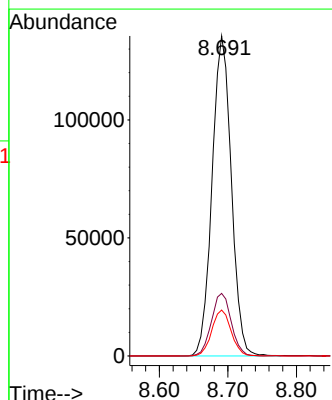
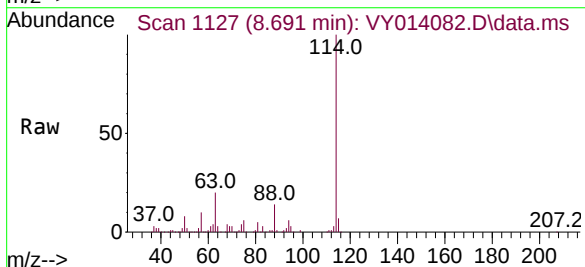


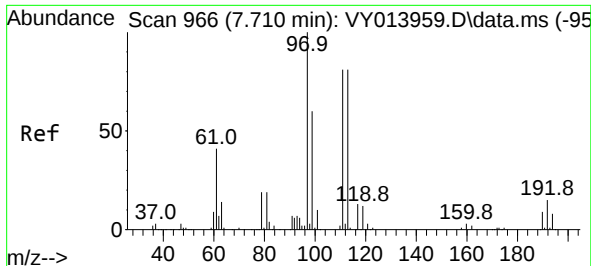

#35
Dibromofluoromethane
Concen: 53.994 ug/l
RT: 7.722 min Scan# 90
Delta R.T. 0.012 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49




Instrument :
MSVOA_Y
ClientSampleId :
30999


Tgt Ion:113 Resp: 90534
Ion Ratio Lower Upper
113 100
111 103.0 81.3 121.9
192 20.8 16.9 25.3

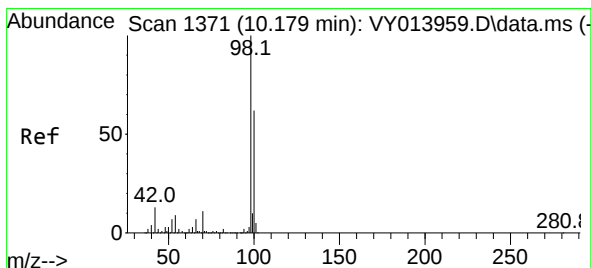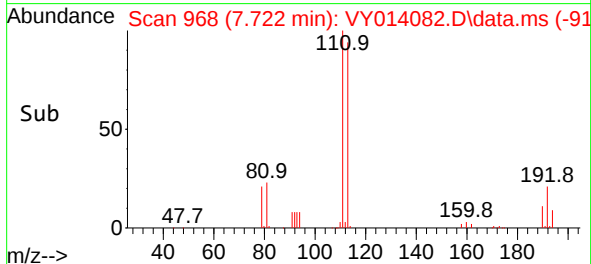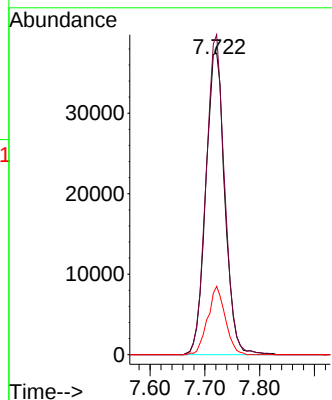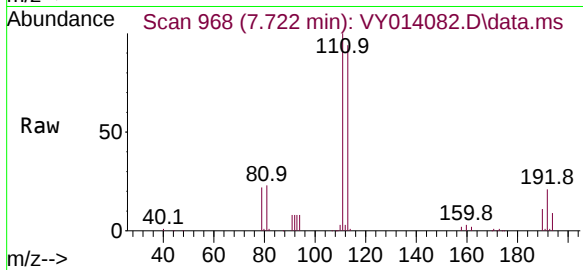

#50
Toluene-d8
Concen: 54.265 ug/l
RT: 10.178 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49

Tgt Ion: 98 Resp: 347067
Ion Ratio Lower Upper
98 100
100 62.1 50.1 75.1


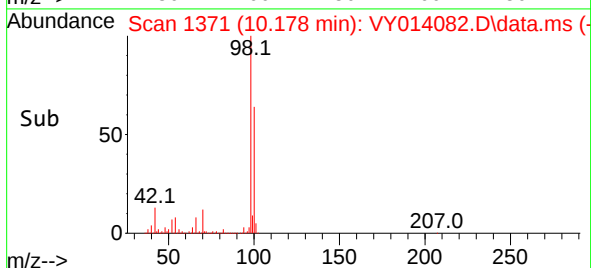
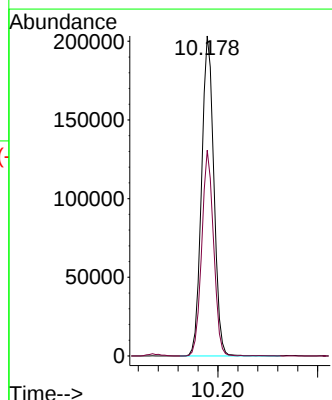
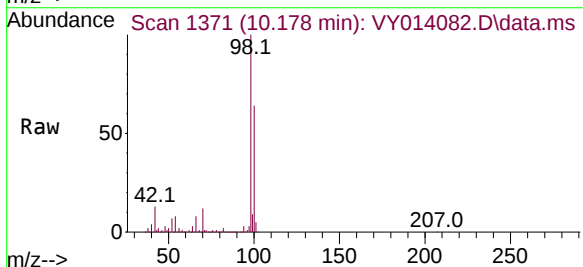


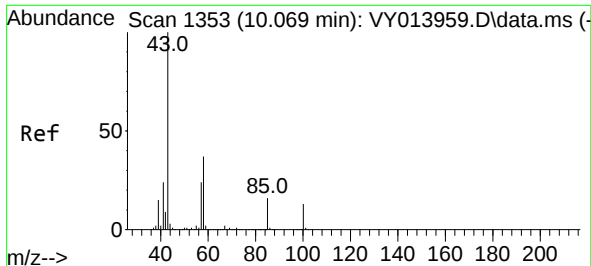

#51
4-Methyl-2-Pentanone
Concen: 9.020 ug/l
RT: 10.069 min Scan# 1353
Delta R.T. -0.000 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49




Instrument :
MSVOA_Y
ClientSampleId :
30999


Tgt Ion: 43 Resp: 17866
Ion Ratio Lower Upper
43 100
58 33.8 29.0 43.6

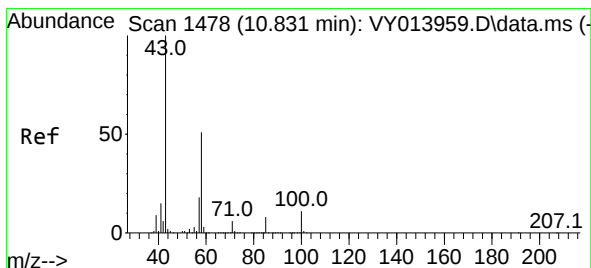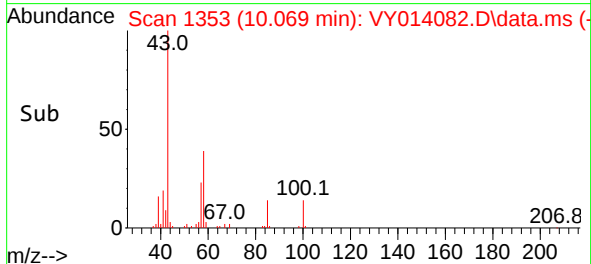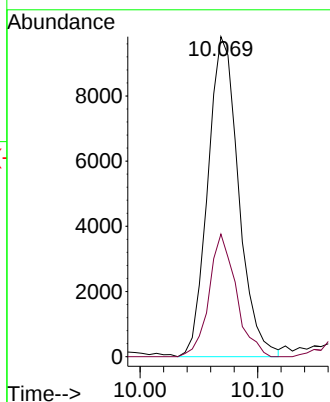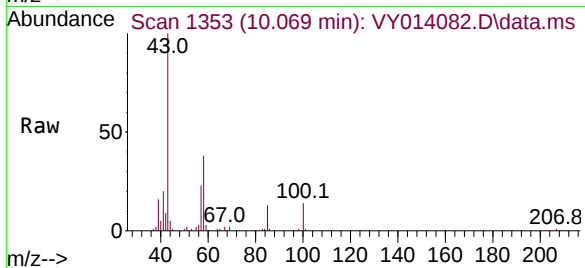

#59
2-Hexanone
Concen: 6.351 ug/l
RT: 10.831 min Scan# 1478
Delta R.T. -0.000 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49

Tgt Ion: 43 Resp: 9109
Ion Ratio Lower Upper
43 100
58 35.8 25.1 75.3


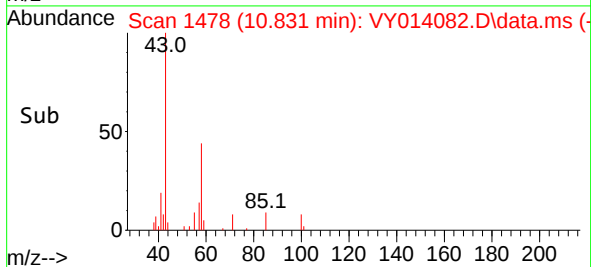
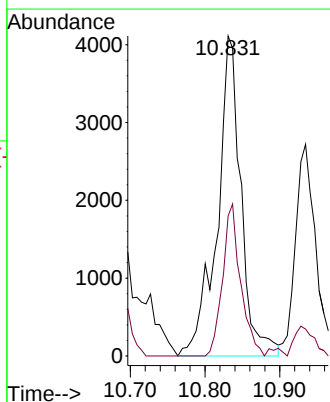
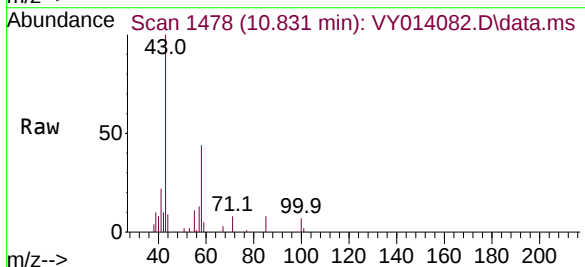


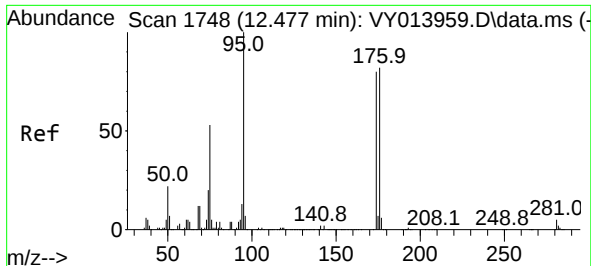

#62
4-Bromofluorobenzene
Concen: 54.609 ug/l
RT: 12.483 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49




Instrument :
MSVOA_Y
ClientSampleId :
30999


Tgt Ion: 95 Resp: 119073
Ion Ratio Lower Upper
95 100
174 93.7 0.0 178.2
176 90.5 0.0 173.8

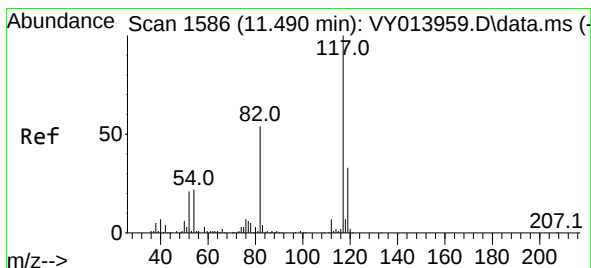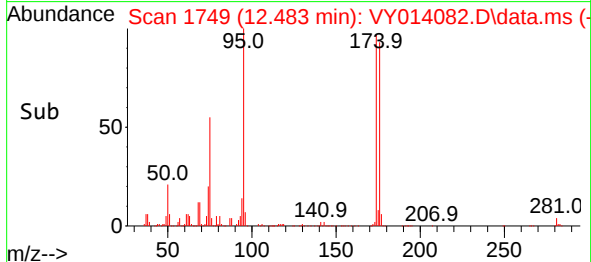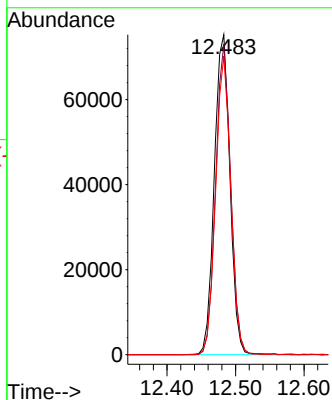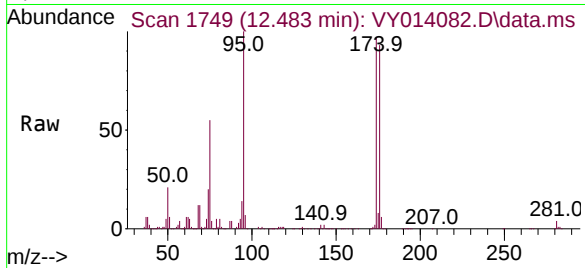

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49

Tgt Ion: 117 Resp: 276421
Ion Ratio Lower Upper
117 100
82 53.9 43.4 65.0
119 32.2 26.3 39.5


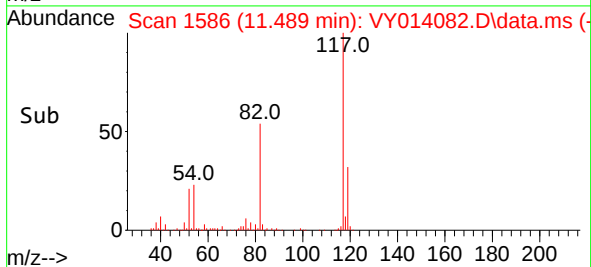
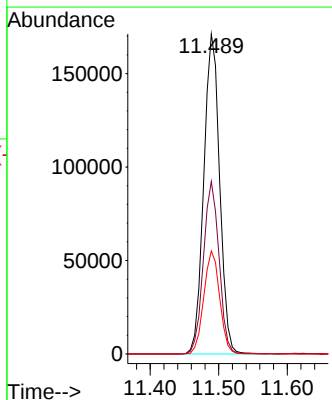
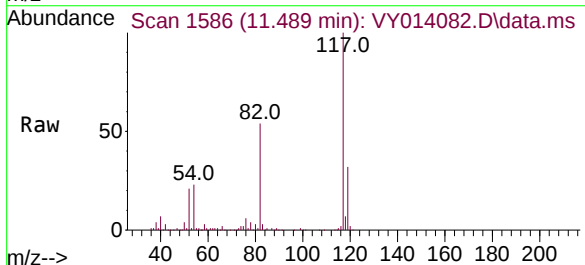


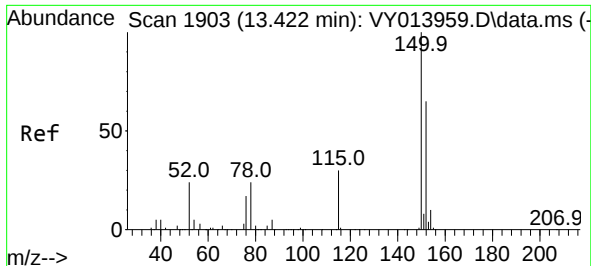

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1903
Delta R.T. 0.006 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49

Instrument :
MSVOA_Y
ClientSampleId :
30999

Tgt Ion:152 Resp: 137963
Ion Ratio Lower Upper
152 100
115 56.7 28.8 86.5
150 155.5 0.0 348.8

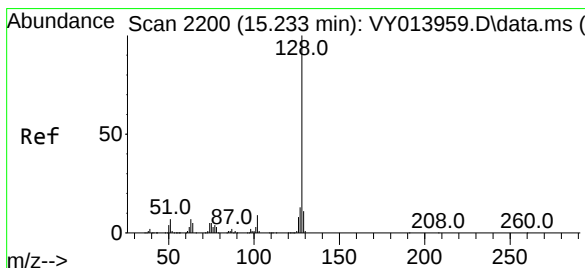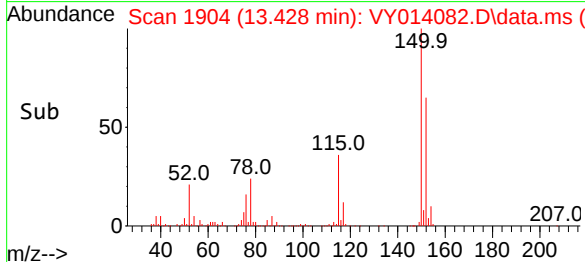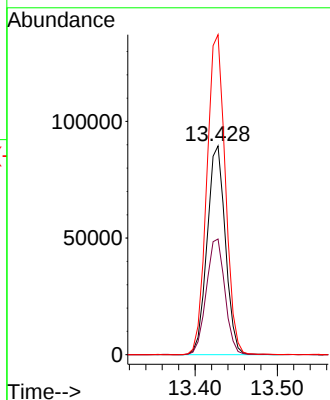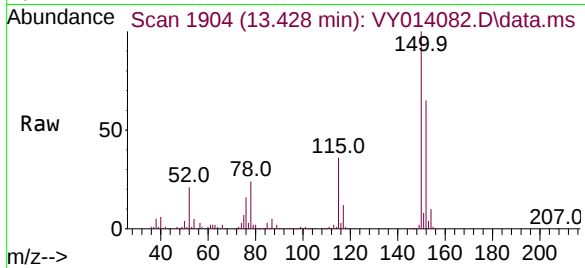

#95
Naphthalene
Concen: 4.095 ug/l
RT: 15.239 min Scan# 2201
Delta R.T. 0.005 min
Lab File: VY014082.D
Acq: 08 Jun 2023 18:49

Tgt Ion:128 Resp: 1494
Ion Ratio Lower Upper
128 100
127 13.8 10.8 16.2
129 12.7 8.6 13.0

