
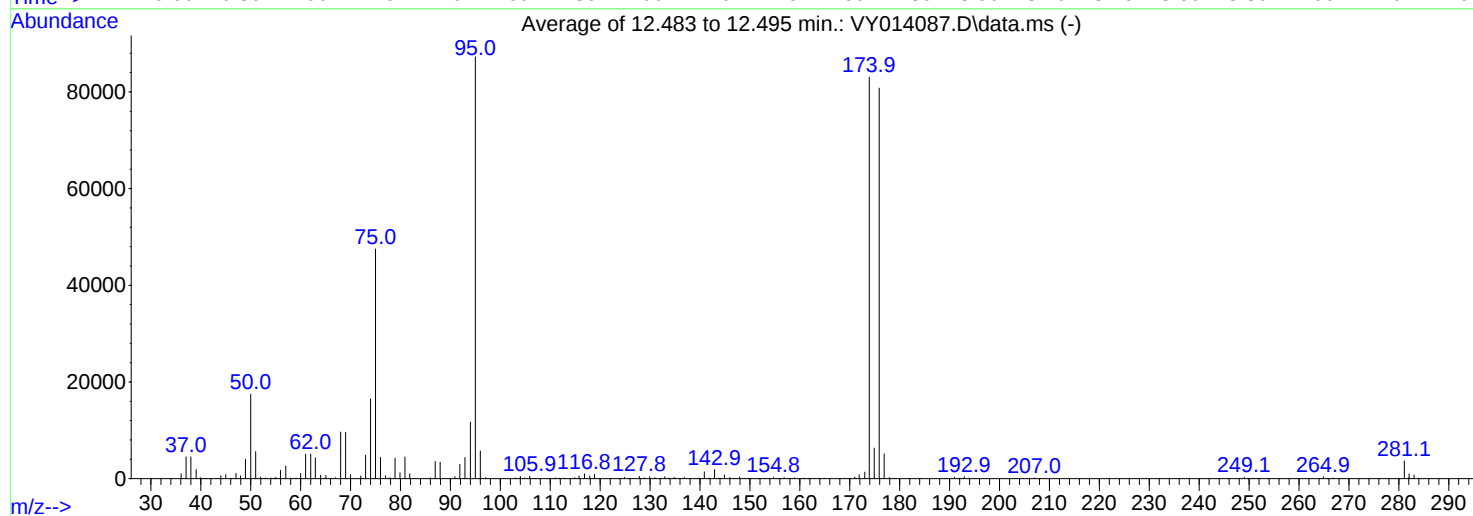


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY060923\
Data File : VY014087.D
Acq On : 09 Jun 2023 09:02
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y060923S.M
Title : SW846 8260
Last Update : Fri Jun 09 18:07:13 2023

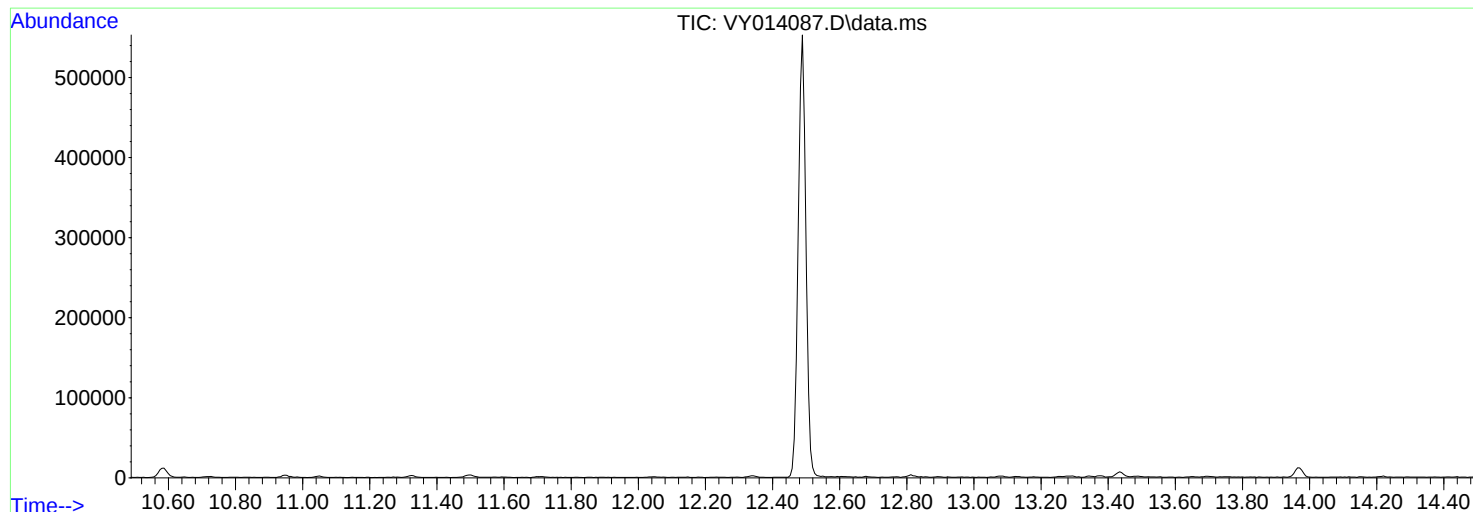

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	17451	PASS
75	95	30	60	54.4	47496	PASS
95	95	100	100	100.0	87253	PASS
96	95	5	9	6.6	5736	PASS
173	174	0.00	2	1.6	1367	PASS
174	95	50	100	95.2	83048	PASS
175	174	5	9	7.6	6322	PASS
176	174	95	101	97.3	80789	PASS
177	176	5	9	6.3	5128	PASS