
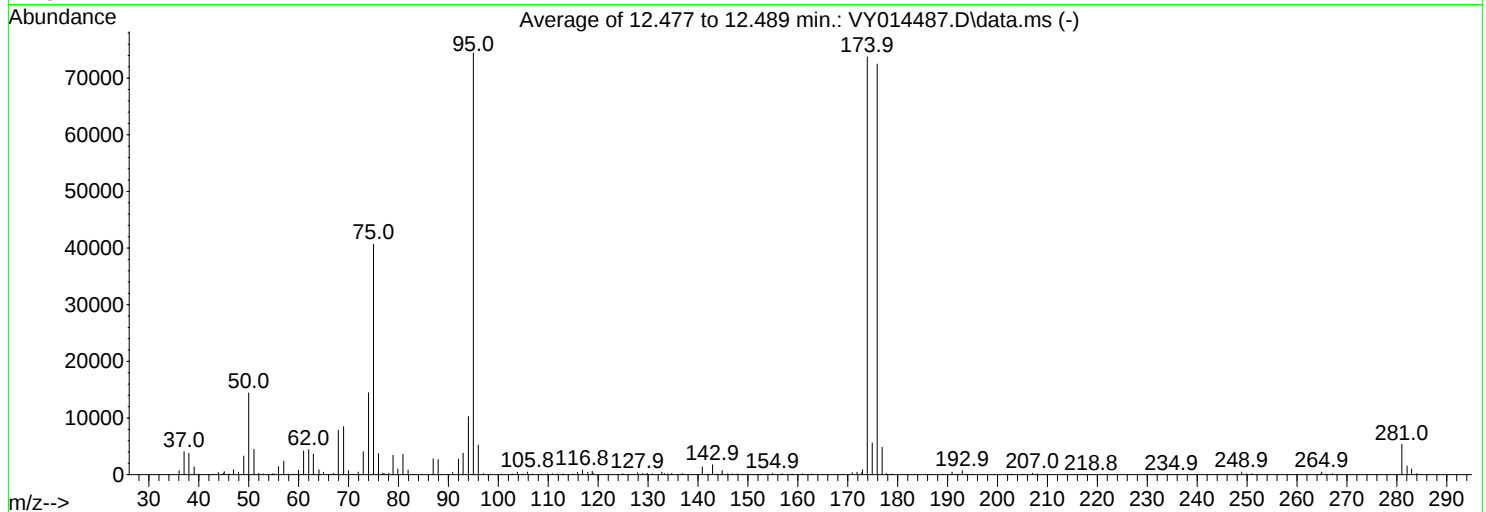


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY062923\  
Data File : VY014487.D  
Acq On : 29 Jun 2023 08:57  
Operator : KP/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y062323S.M  
Title : SW846 8260  
Last Update : Fri Jun 23 17:18:46 2023

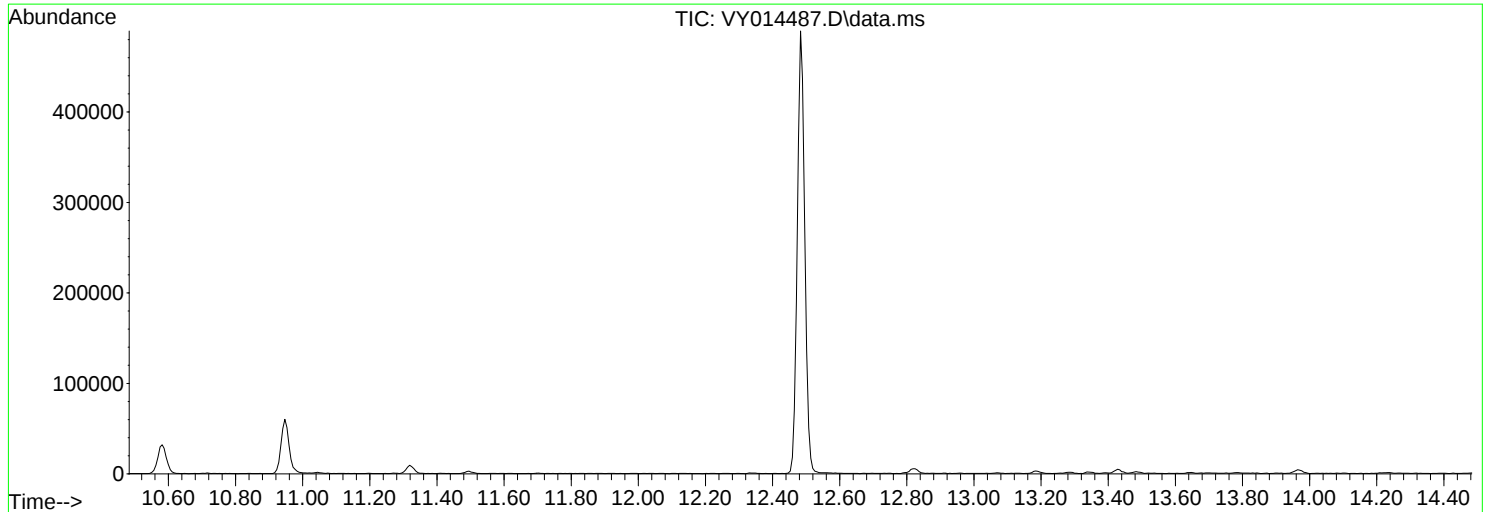

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.4  | 14449 | PASS      |
| 75     | 95      | 30     | 60     | 54.6  | 40688 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 74469 | PASS      |
| 96     | 95      | 5      | 9      | 7.0   | 5205  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.1   | 840   | PASS      |
| 174    | 95      | 50     | 100    | 99.0  | 73747 | PASS      |
| 175    | 174     | 5      | 9      | 7.6   | 5608  | PASS      |
| 176    | 174     | 95     | 101    | 98.3  | 72480 | PASS      |
| 177    | 176     | 5      | 9      | 6.7   | 4831  | PASS      |