
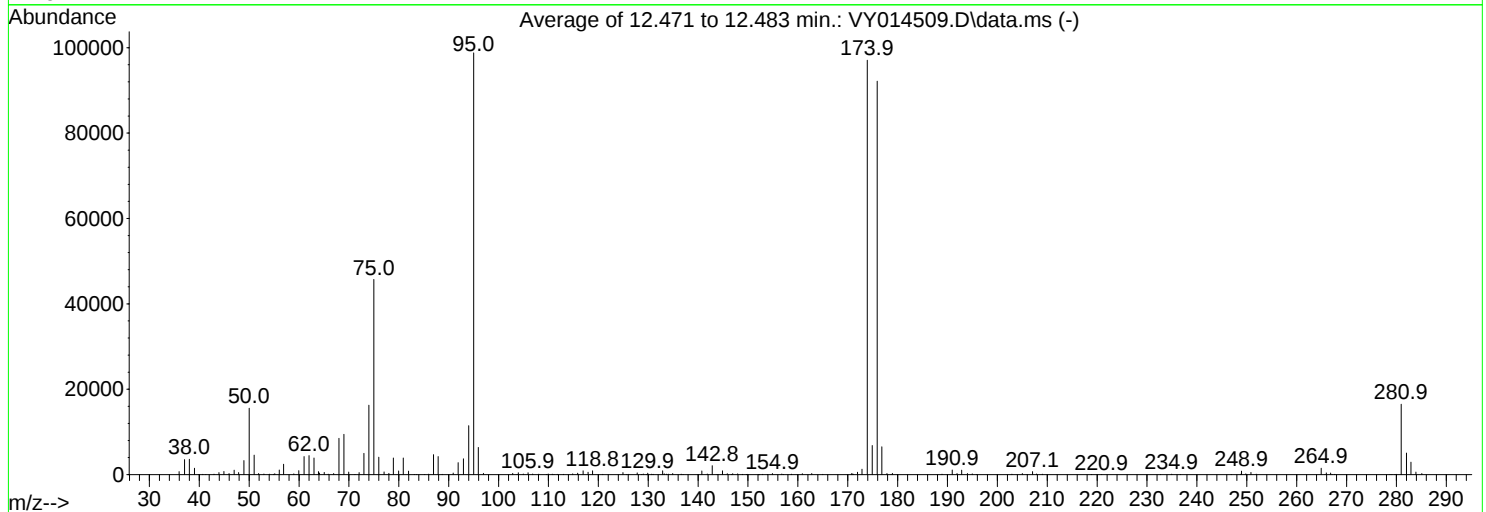


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY063023\  
Data File : VY014509.D  
Acq On : 30 Jun 2023 10:57  
Operator : KP/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y063023S.M  
Title : SW846 8260  
Last Update : Fri Jun 30 19:02:11 2023

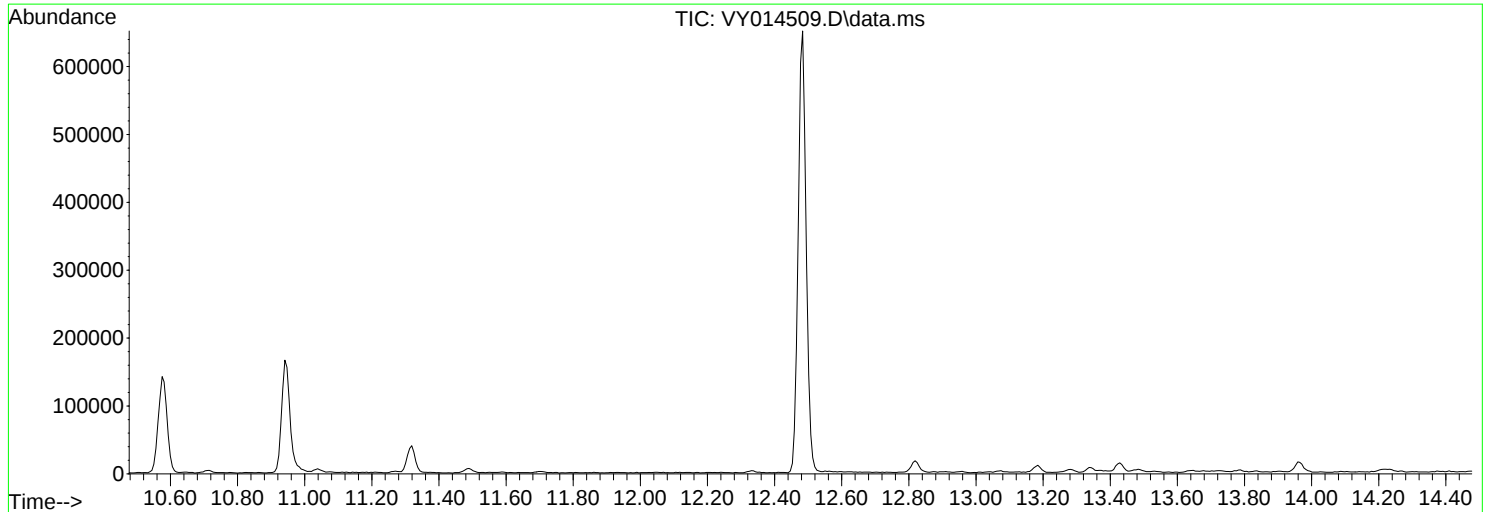

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 15.7         | 15545      | PASS                |
| 75             | 95              | 30              | 60              | 46.3         | 45720      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 98795      | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 6382       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.3          | 1275       | PASS                |
| 174            | 95              | 50              | 100             | 98.2         | 97059      | PASS                |
| 175            | 174             | 5               | 9               | 7.0          | 6805       | PASS                |
| 176            | 174             | 95              | 101             | 95.0         | 92171      | PASS                |
| 177            | 176             | 5               | 9               | 7.1          | 6521       | PASS                |