
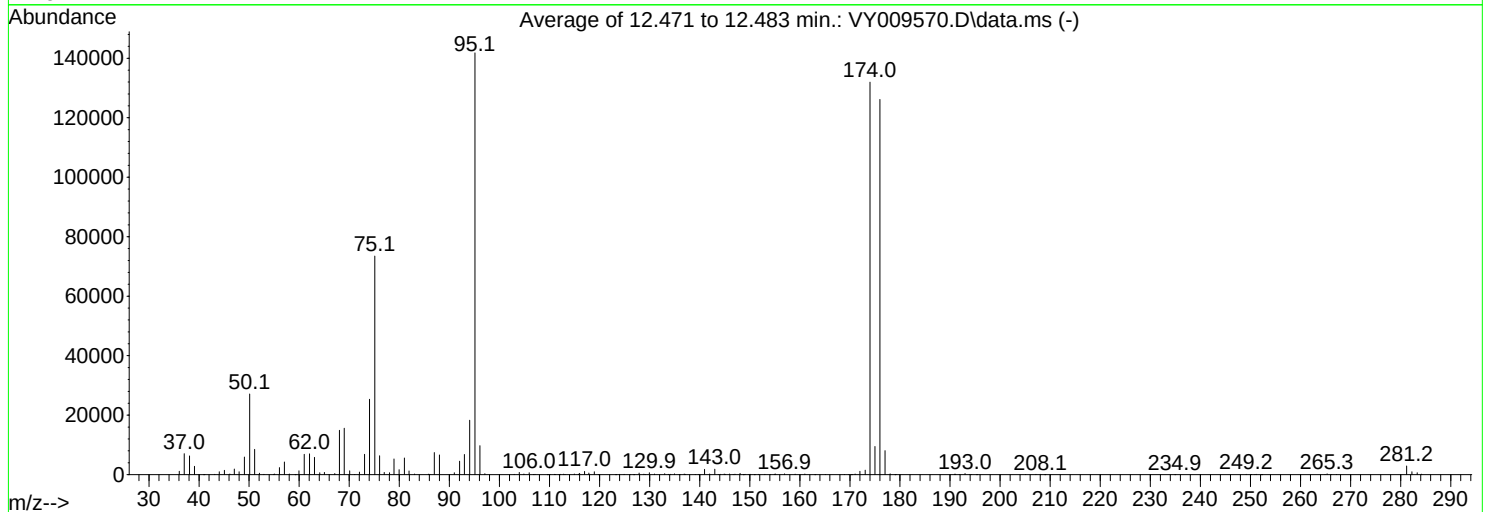


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071822\
 Data File : VY009570.D
 Acq On : 18 Jul 2022 09:38
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071822S.M
 Title : SW846 8260
 Last Update : Tue Jul 19 04:22:09 2022

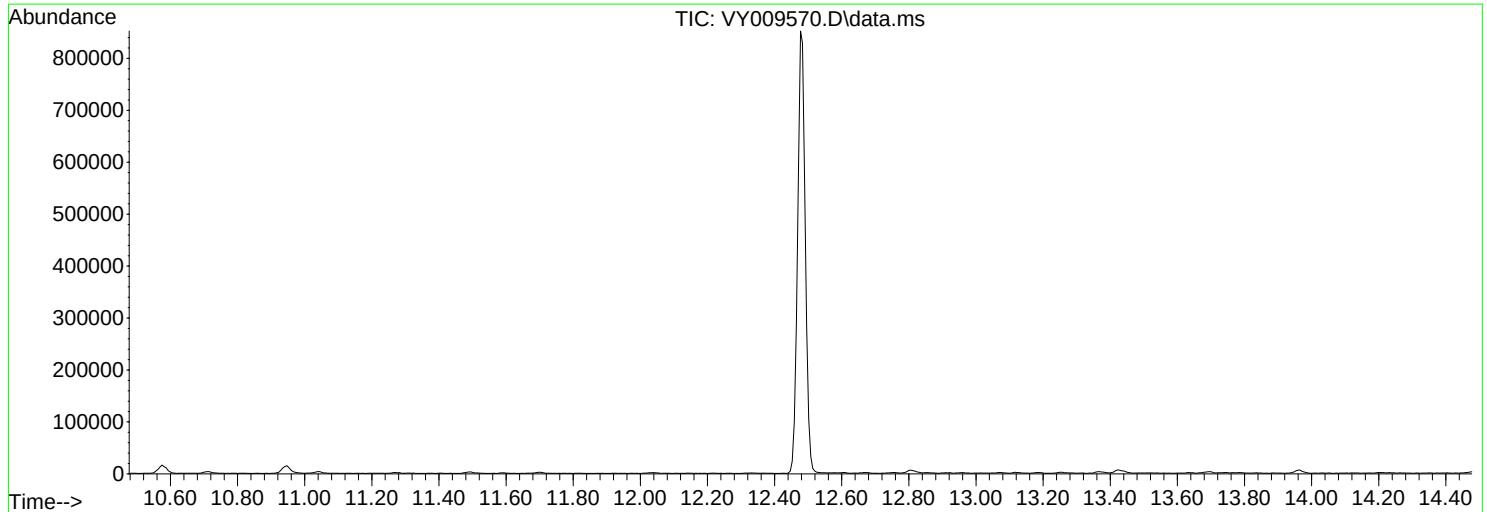

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	27141	PASS
75	95	30	60	51.8	73515	PASS
95	95	100	100	100.0	141813	PASS
96	95	5	9	6.9	9720	PASS
173	174	0.00	2	1.1	1488	PASS
174	95	50	100	93.0	131944	PASS
175	174	5	9	7.2	9481	PASS
176	174	95	101	95.6	126173	PASS
177	176	5	9	6.4	8094	PASS