


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071922\
Data File : VY009579.D
Acq On : 19 Jul 2022 09:10
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071822S.M
Title : SW846 8260
Last Update : Tue Jul 19 04:22:09 2022

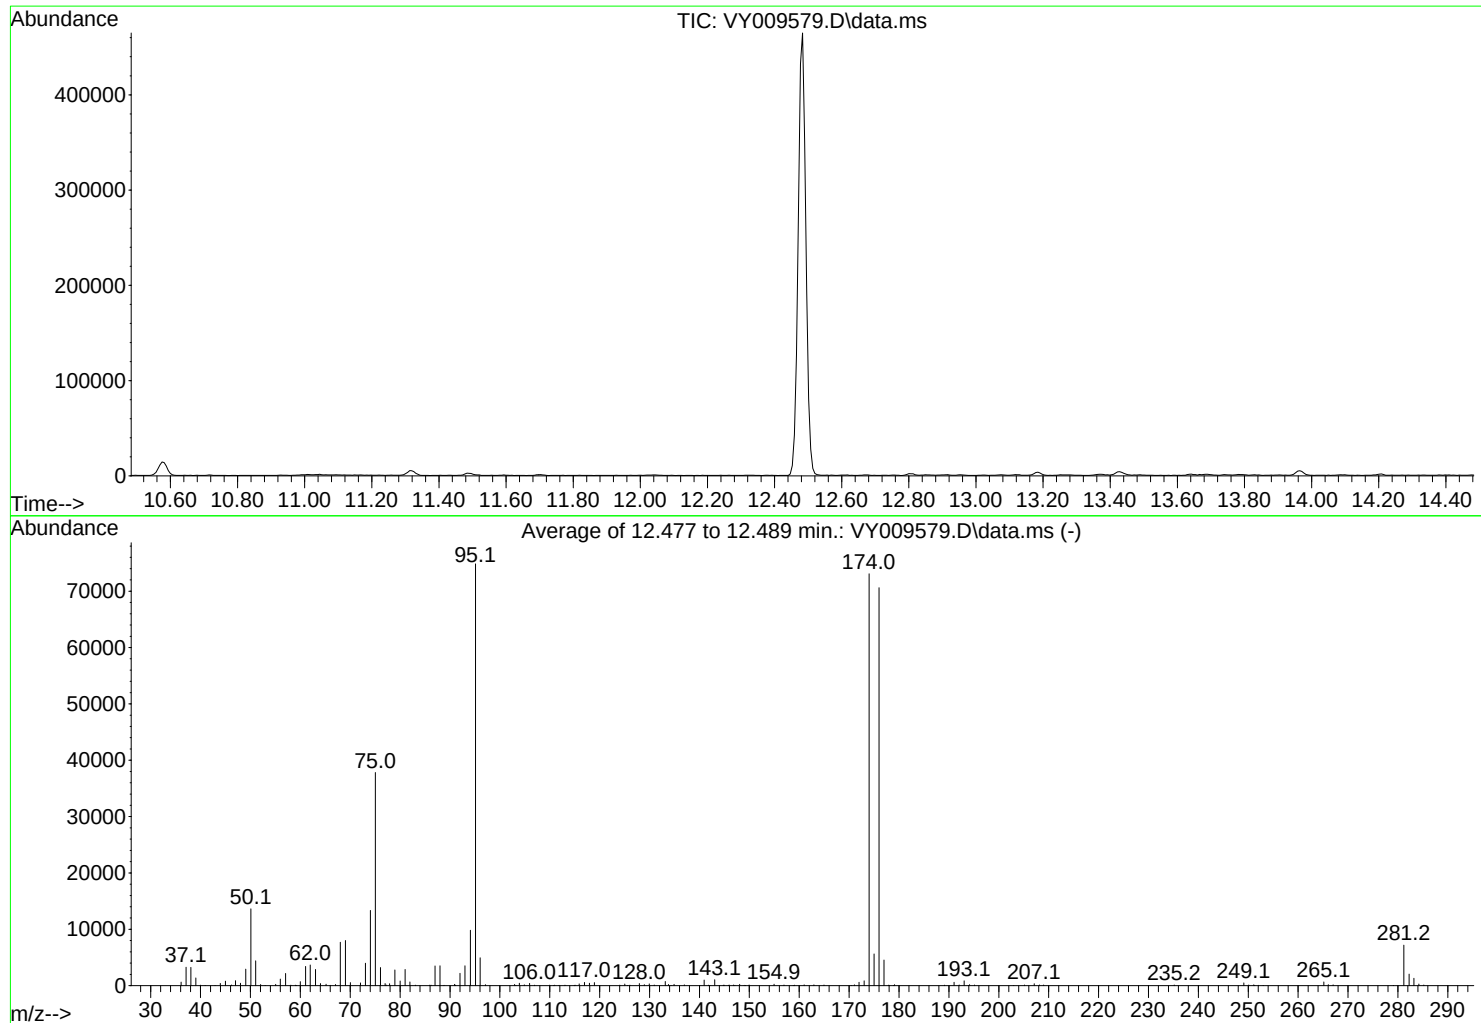

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	13638	PASS
75	95	30	60	50.5	37813	PASS
95	95	100	100	100.0	74856	PASS
96	95	5	9	6.6	4944	PASS
173	174	0.00	2	1.2	846	PASS
174	95	50	100	97.6	73085	PASS
175	174	5	9	7.7	5632	PASS
176	174	95	101	96.6	70608	PASS
177	176	5	9	6.5	4556	PASS