

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY072120\
 Data File : VY003264.D
 Acq On : 21 Jul 2020 21:15
 Operator : SY/MD
 Sample : L3344-10
 Misc : 7.74G/5ML/MSVOA Y/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-14-D2

Quant Time: Jul 22 04:05:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 10 13:18:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	397010	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	621334	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	578495	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	285313	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	202033	60.29	ug/l	0.00
Spiked Amount	50.000		Recovery	=	120.58%	
35) Dibromofluoromethane	7.72	113	193710	54.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.36%	
50) Toluene-d8	10.18	98	754547	56.76	ug/l	0.00
Spiked Amount	50.000		Recovery	=	113.52%	
62) 4-Bromofluorobenzene	12.48	95	242291	50.45	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.90%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY072120\
Data File : VY003264.D
Acq On : 21 Jul 2020 21:15
Operator : SY/MD
Sample : L3344-10
Misc : 7.74G/5ML/MSVOA Y/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-14-D2

Quant Time: Jul 22 04:05:15 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 10 13:18:03 2020
Response via : Initial Calibration

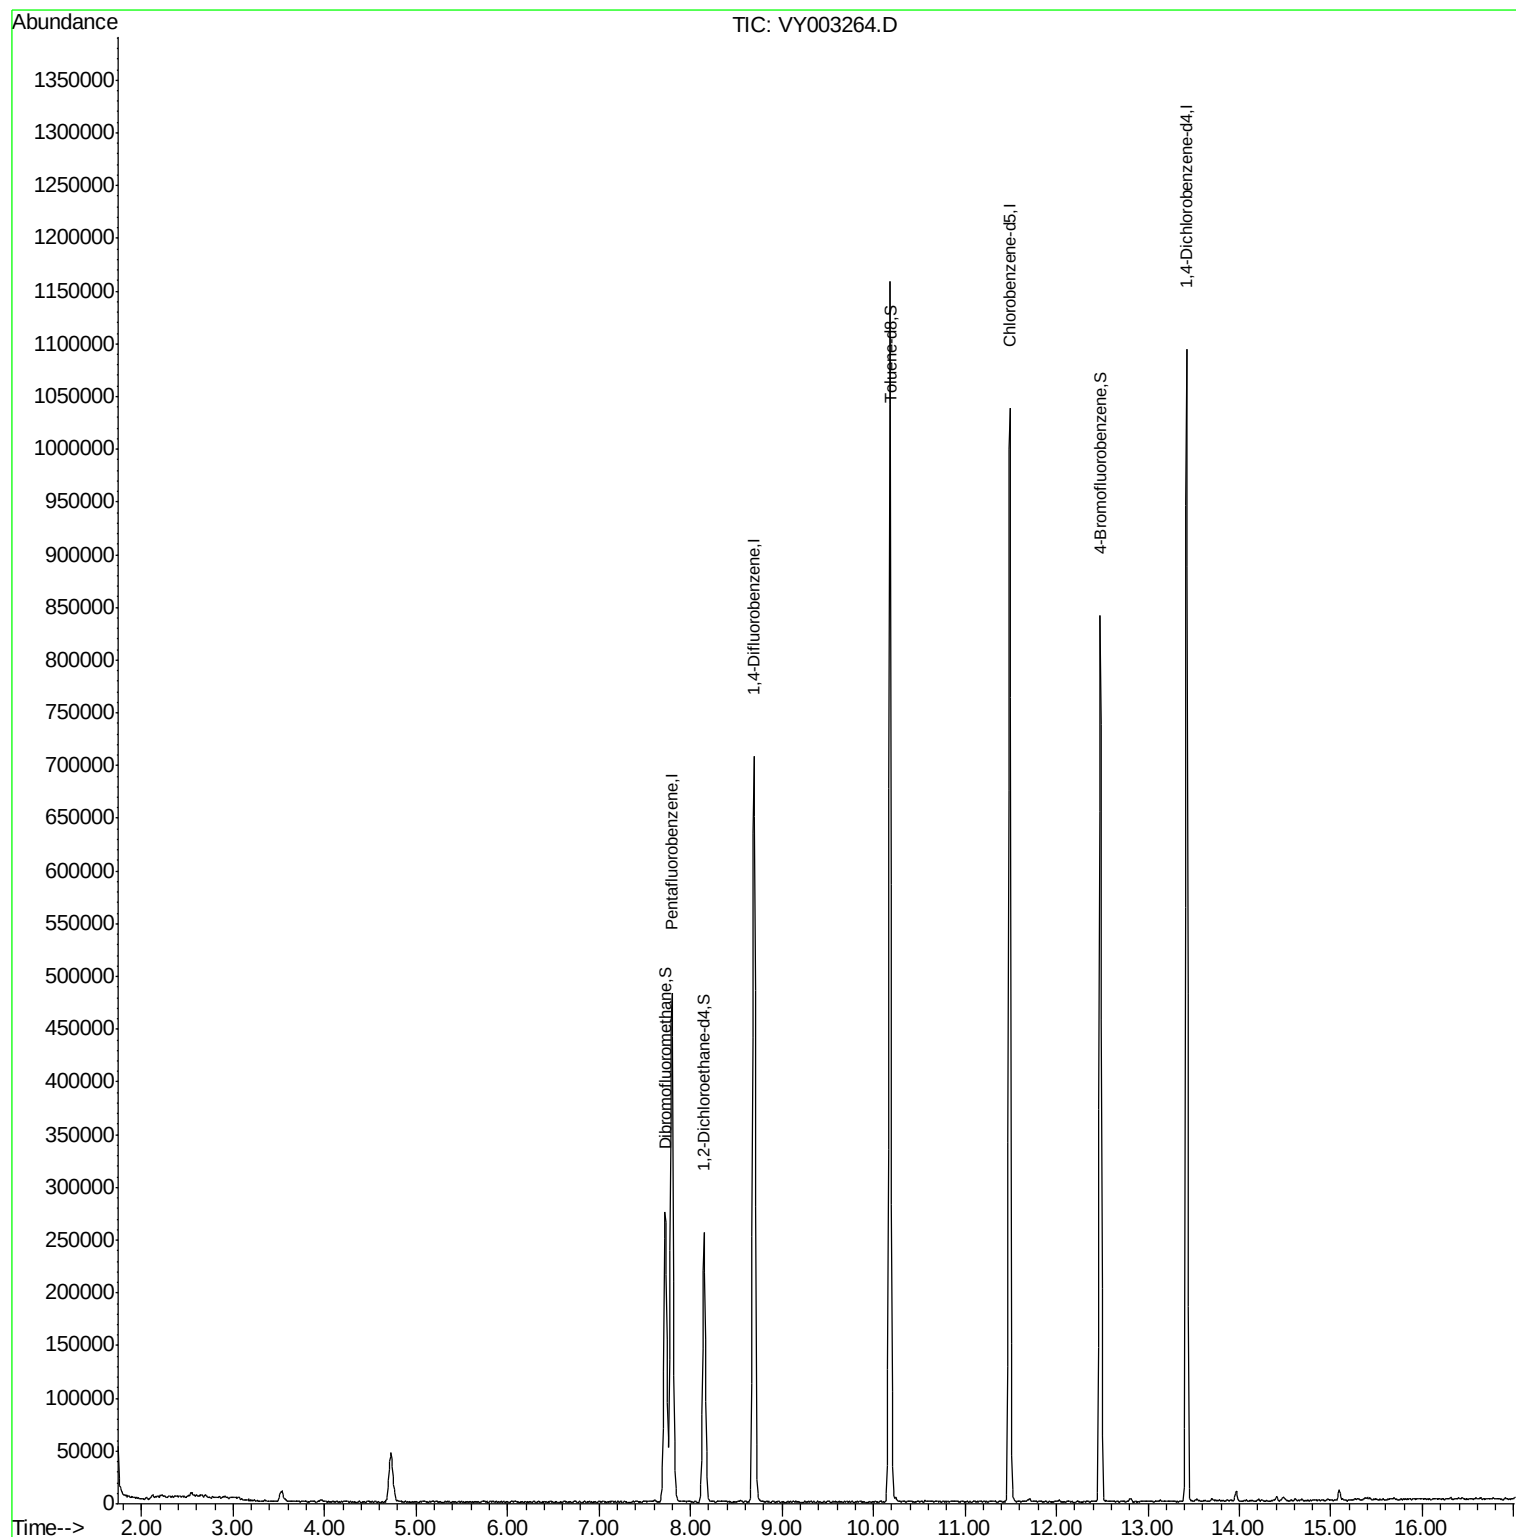

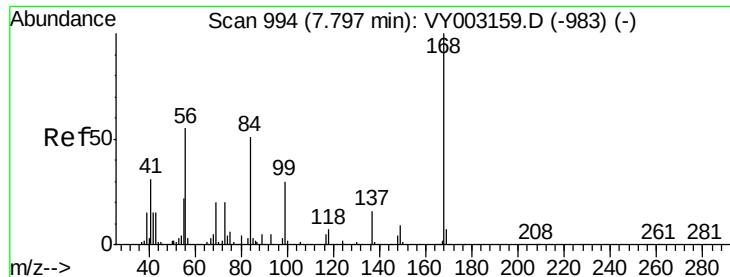

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. -0.00 min

Lab File: VY003264.D

Acq: 21 Jul 2020 21:15

Instrument :

MSVOA_Y

ClientSampleId :


TP-14-D2

Tot Ion:168 Resp: 397010

Ion Ratio Lower Upper

168 100

99 49.0 37.3 55.9

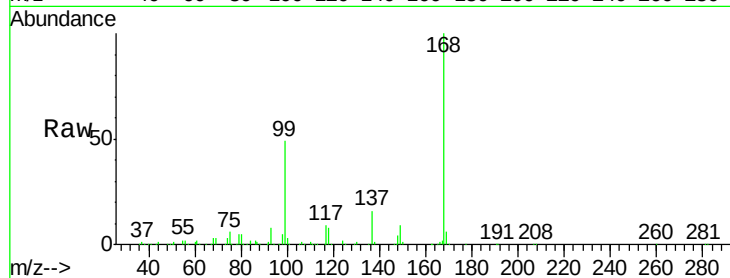

Abundance Ion 167.90 (167.60 to 168.60): VY003264.D (-945) (-)

Ion 98.90 (98.60 to 99.60): VY003264.D (-945) (-)

7.80



150000

100000

50000

0

Time-->

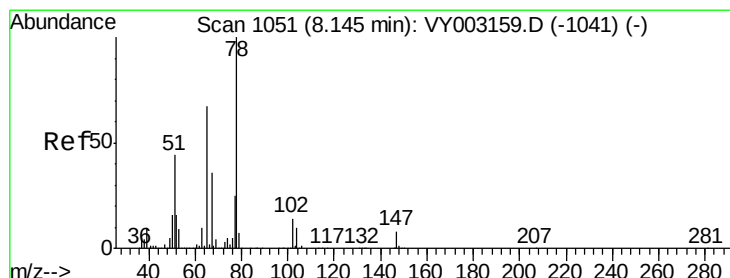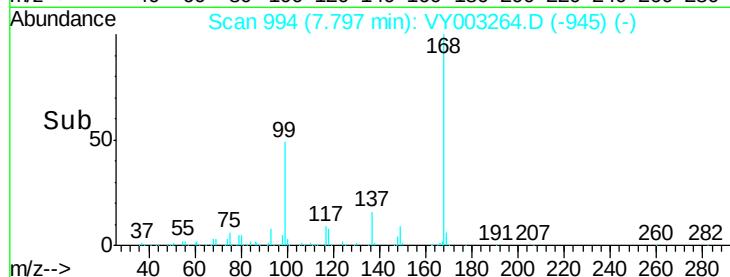

#33

1,2-Dichloroethane-d4

Concen: 60.292 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. 0.01 min

Lab File: VY003264.D


Acq: 21 Jul 2020 21:15

Tgt Ion: 65 Resp: 202033

Ion Ratio Lower Upper

65 100

67 53.3 0.0 105.2

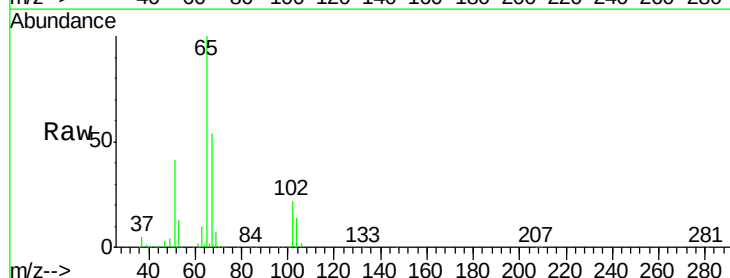

Abundance Ion 64.90 (64.60 to 65.60): VY003264.D (-1002) (-)

Ion 66.90 (66.60 to 67.60): VY003264.D (-1002) (-)

8.15

100000

80000


60000


40000

20000

0

Time-->




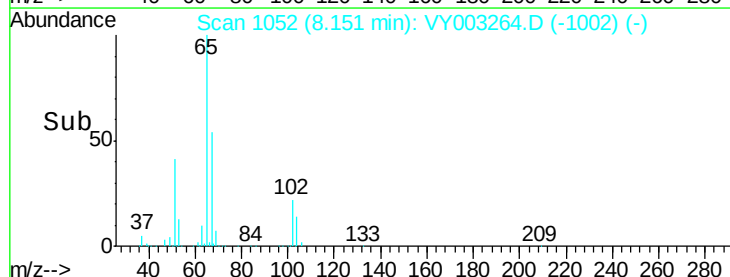


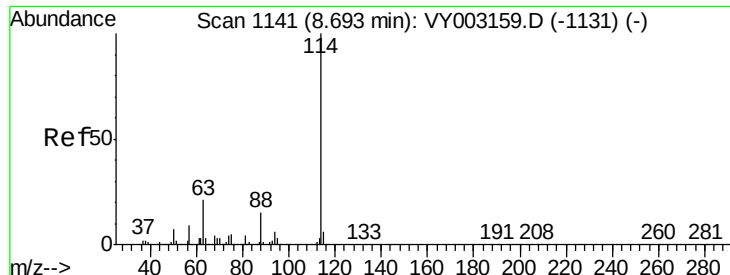

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.69 min Scan# 1141
 Delta R.T. -0.00 min
 Lab File: VY003264.D
 Acq: 21 Jul 2020 21:15




Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-14-D2


Tot Ion:114 Resp: 621334
 Ion Ratio Lower Upper
 114 100
 63 19.9 0.0 41.2
 88 15.0 0.0 30.2

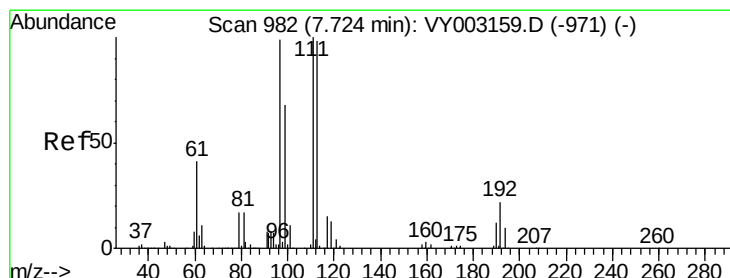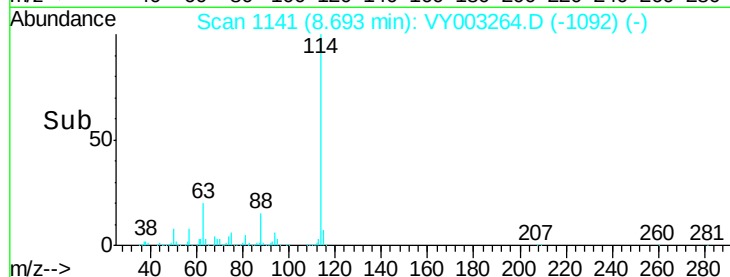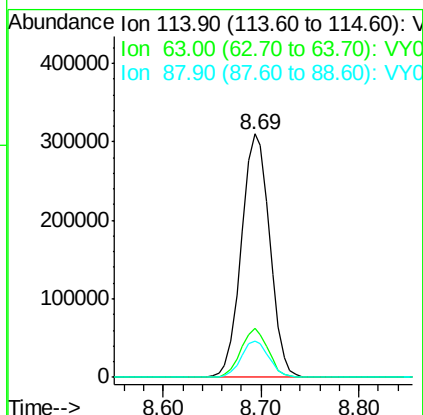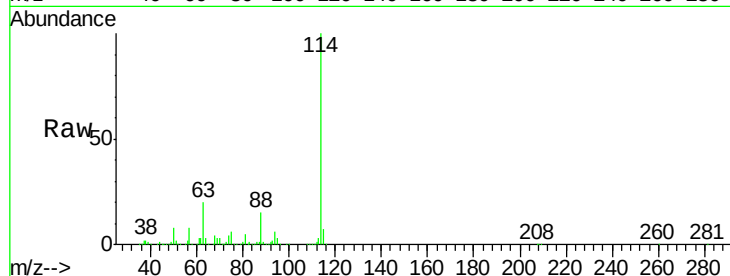

#35
 Dibromofluoromethane
 Concen: 54.175 ug/l
 RT: 7.72 min Scan# 982
 Delta R.T. -0.00 min
 Lab File: VY003264.D
 Acq: 21 Jul 2020 21:15

Tgt Ion:113 Resp: 193710
 Ion Ratio Lower Upper
 113 100
 111 103.3 82.1 123.1
 192 22.5 18.8 28.2


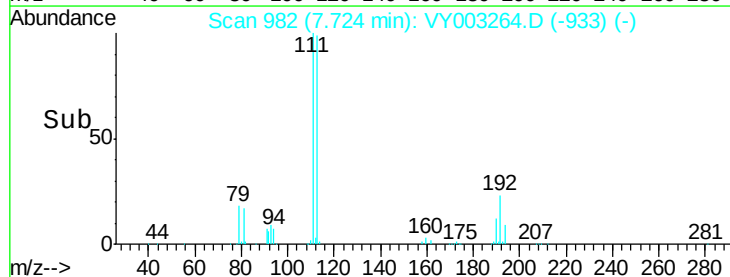
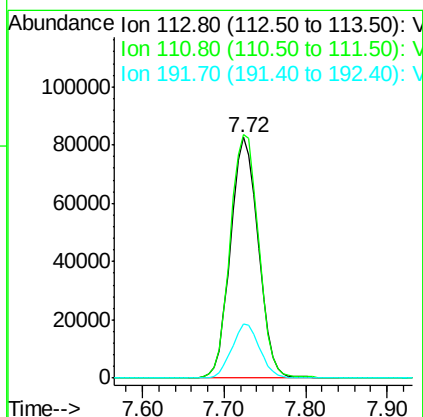
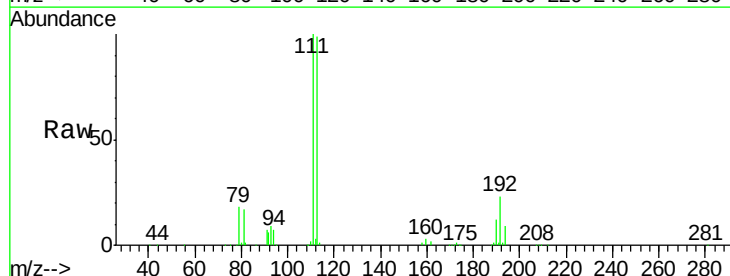


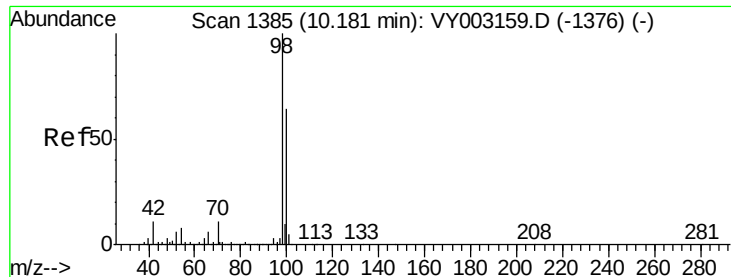

#50
Toluene-d8
Concen: 56.760 ug/l
RT: 10.18 min Scan# 1385
Delta R.T. -0.00 min
Lab File: VY003264.D
Acq: 21 Jul 2020 21:15




Instrument :
MSVOA_Y
ClientSampleId :
TP-14-D2


Tot Ion: 98 Resp: 754547
Ion Ratio Lower Upper
98 100
100 64.0 50.7 76.1

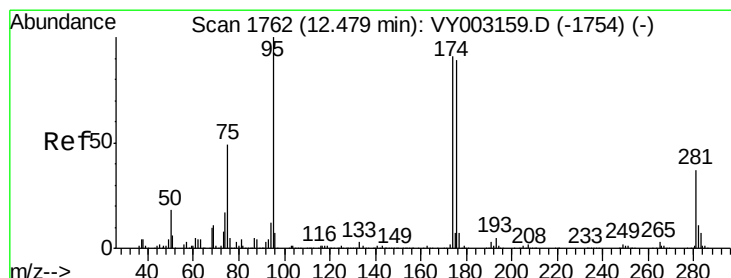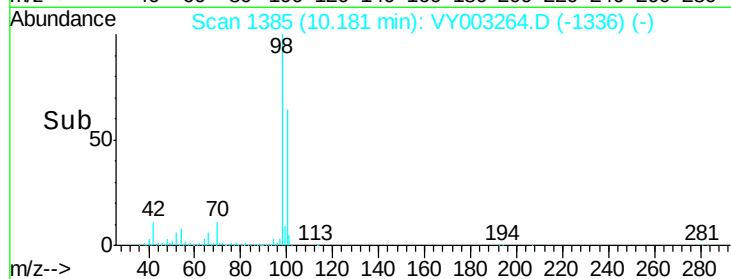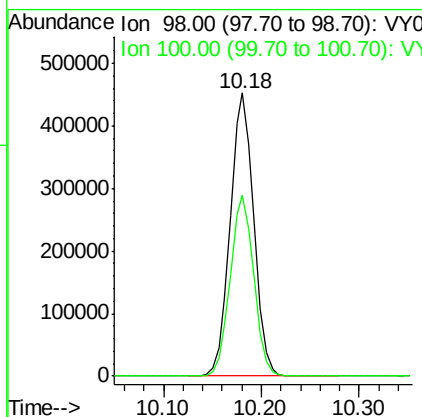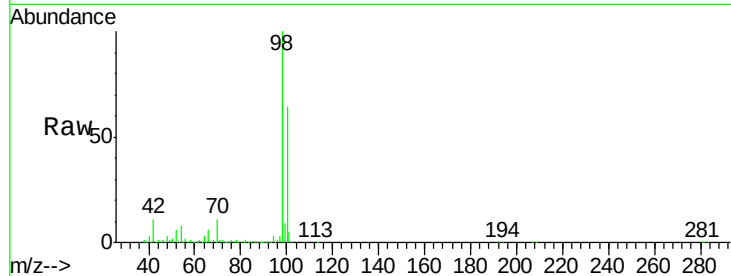

#62
4-Bromofluorobenzene
Concen: 50.452 ug/l
RT: 12.48 min Scan# 1762
Delta R.T. -0.00 min
Lab File: VY003264.D
Acq: 21 Jul 2020 21:15

Tgt Ion: 95 Resp: 242291
Ion Ratio Lower Upper
95 100
174 97.0 0.0 190.6
176 94.4 0.0 186.4

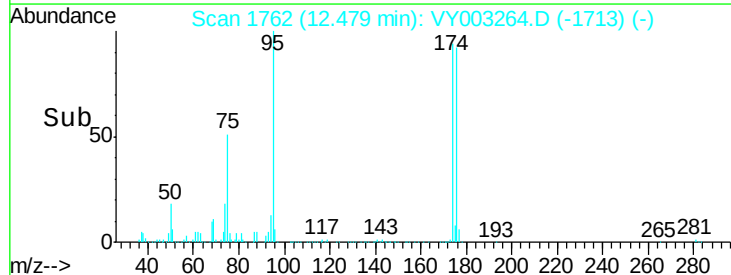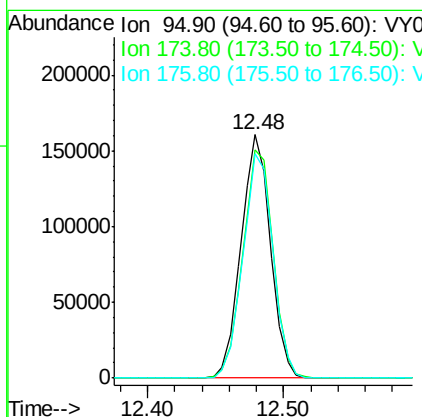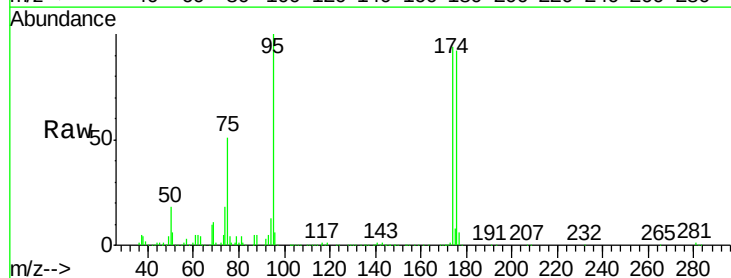


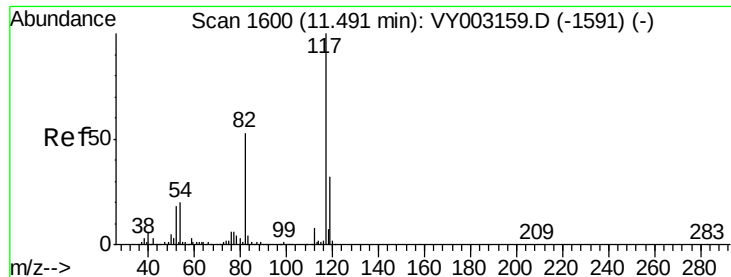




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. -0.00 min
Lab File: VY003264.D
Acq: 21 Jul 2020 21:15

Instrument :
MSVOA_Y
ClientSampleId :
TP-14-D2

Tot Ion:117 Resp: 578495
Ion Ratio Lower Upper
117 100
82 52.3 42.0 63.0
119 32.2 25.5 38.3

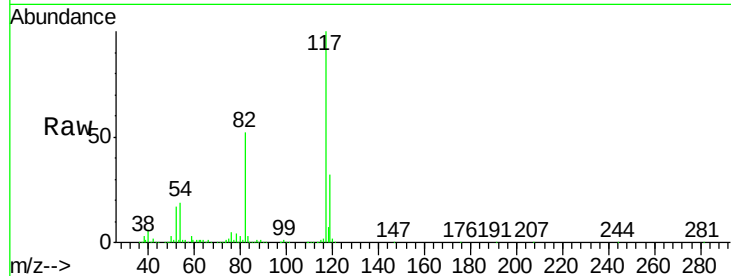


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

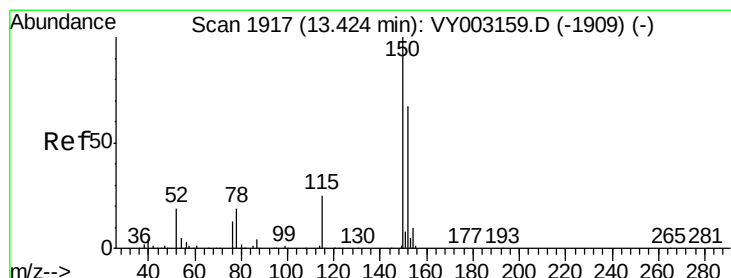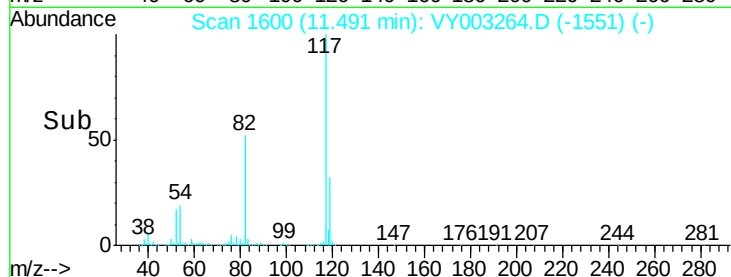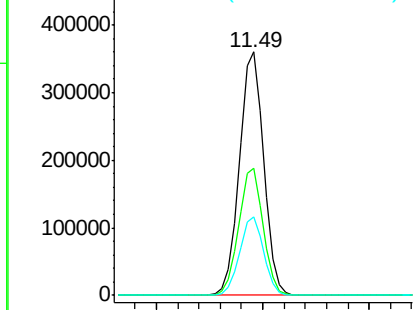

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. -0.00 min
Lab File: VY003264.D
Acq: 21 Jul 2020 21:15

Tgt Ion:152 Resp: 285313
Ion Ratio Lower Upper
152 100
115 54.0 26.9 80.7
150 156.0 0.0 338.0

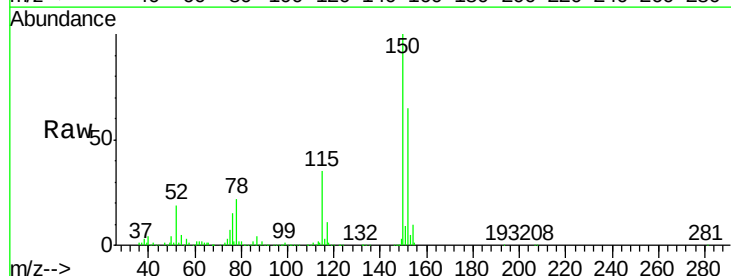

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

