


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv072120\
 Data File : VY003252.D
 Acq On : 21 Jul 2020 15:57
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
 Title : SW846 8260
 Last Update : Fri Jul 10 13:18:03 2020

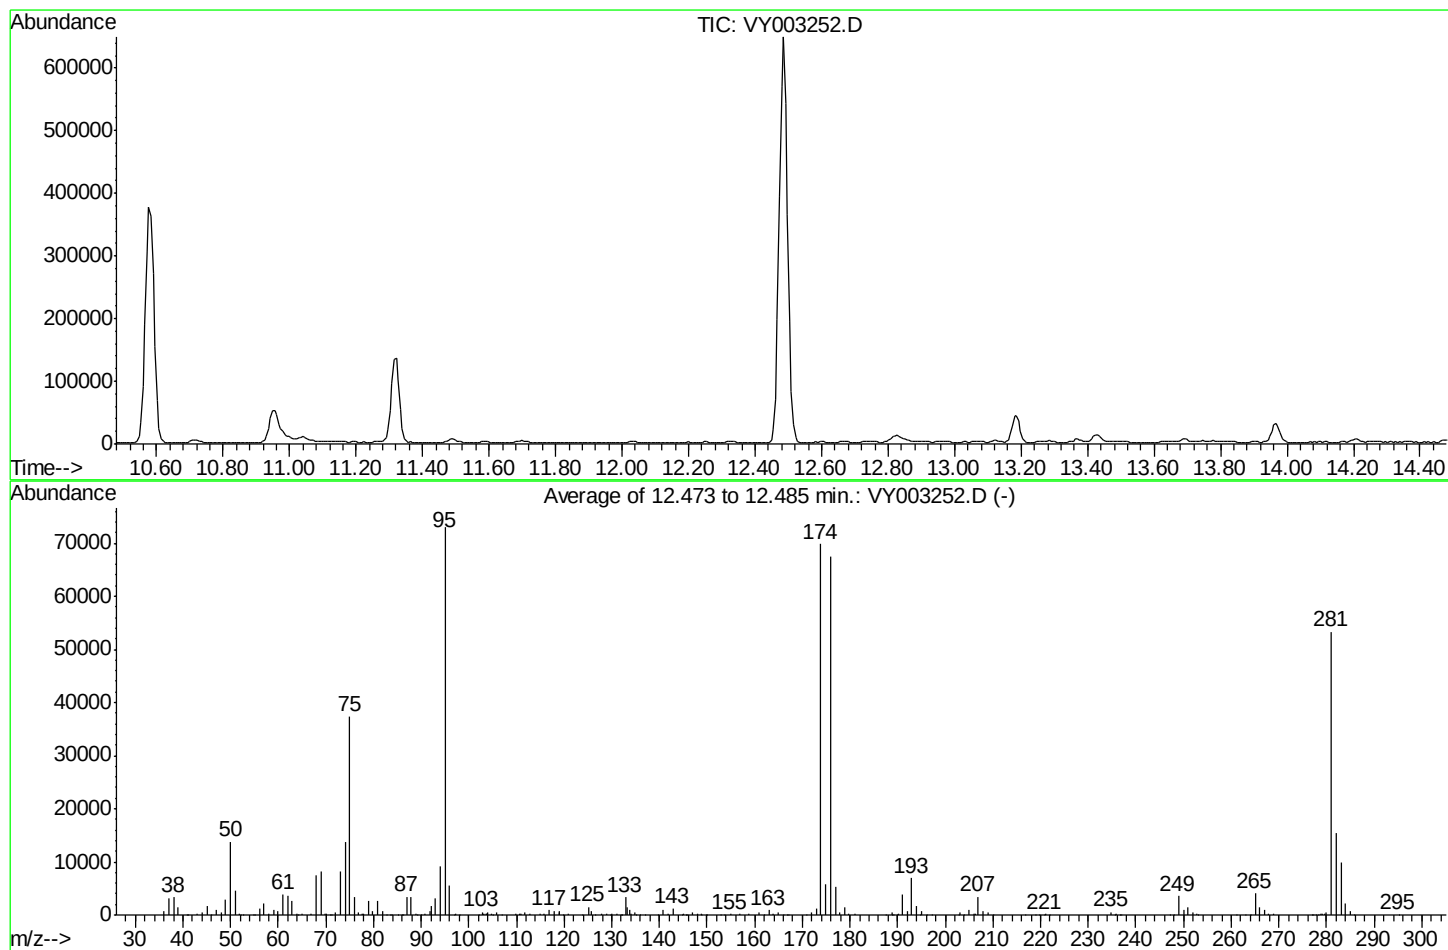

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	13795	PASS
75	95	30	60	51.0	37240	PASS
95	95	100	100	100.0	72973	PASS
96	95	5	9	7.5	5508	PASS
173	174	0.00	2	1.6	1103	PASS
174	95	50	100	95.6	69786	PASS
175	174	5	9	8.2	5697	PASS
176	174	95	101	96.5	67376	PASS
177	176	5	9	7.9	5304	PASS