

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY072220\
 Data File : VY003303.D
 Acq On : 22 Jul 2020 21:09
 Operator : SY/MD
 Sample : L3308-19RE
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 19

Quant Time: Jul 23 06:34:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 10 13:18:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	277677	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	424865	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	389548	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	186264	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	146370	62.45	ug/l	0.00
Spiked Amount	50.000		Recovery	=	124.90%	
35) Dibromofluoromethane	7.72	113	136008	55.63	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.26%	
50) Toluene-d8	10.18	98	511466	56.27	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.54%	
62) 4-Bromofluorobenzene	12.48	95	161453	49.17	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.34%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY072220\
Data File : VY003303.D
Acq On : 22 Jul 2020 21:09
Operator : SY/MD
Sample : L3308-19RE
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
19

Quant Time: Jul 23 06:34:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 10 13:18:03 2020
Response via : Initial Calibration

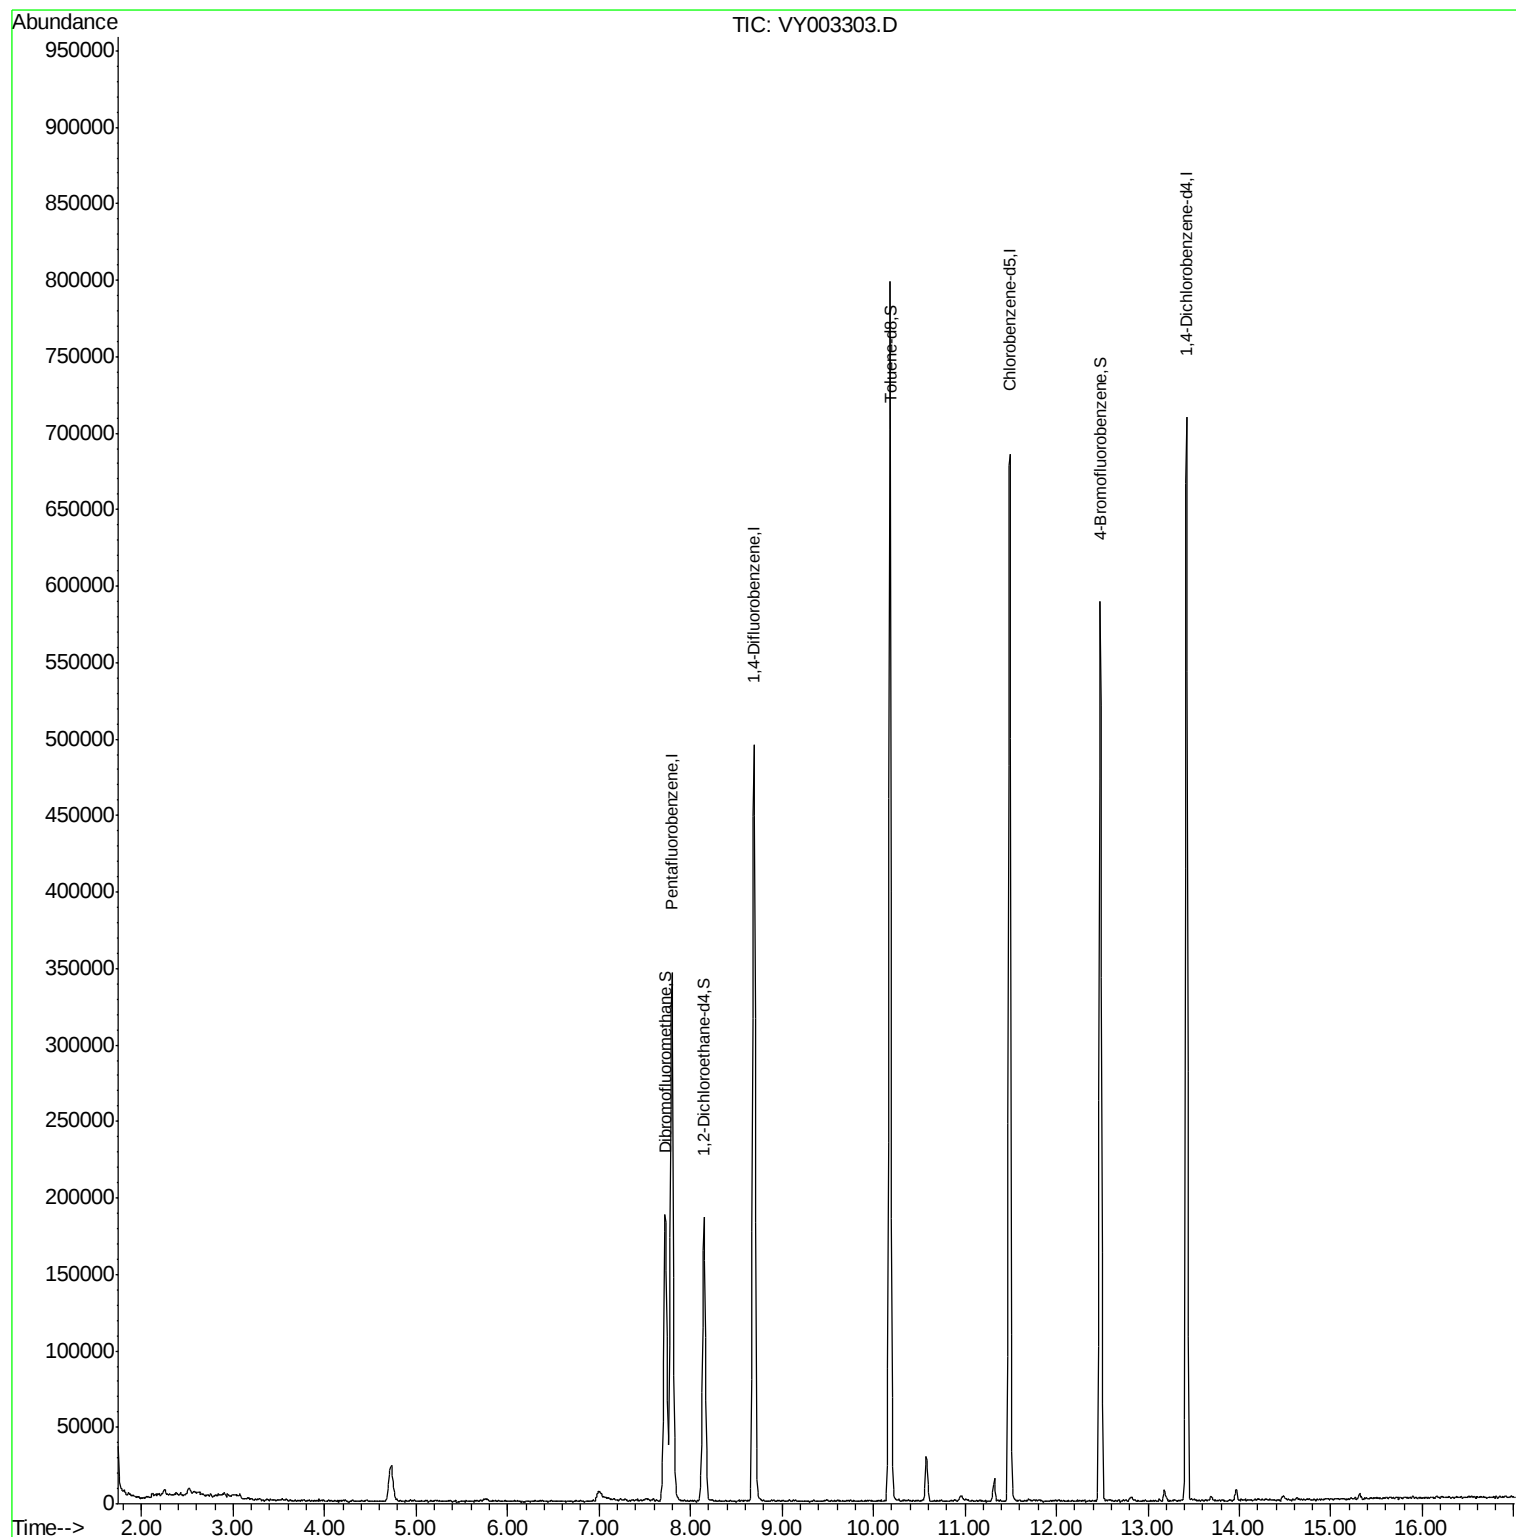

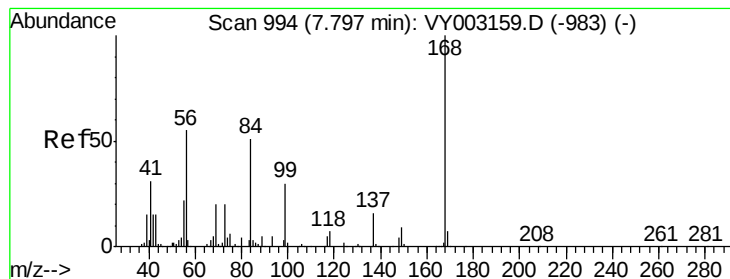

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. 0.00 min

Lab File: VY003303.D

Acq: 22 Jul 2020 21:09


Instrument :
MSVOA_Y
ClientSampled :
19

Tot Ion:168 Resp: 277677

Ion Ratio Lower Upper

168 100

99 53.3 37.3 55.9

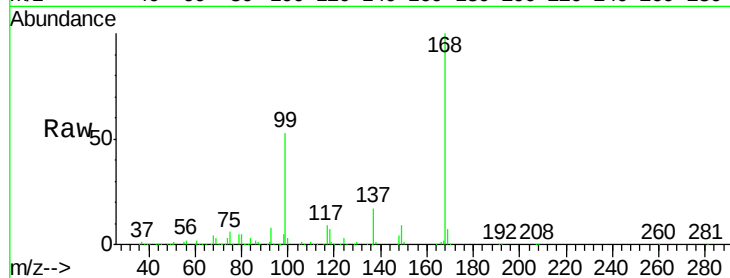

Abundance Ion 167.90 (167.60 to 168.60): VY003303.D (-945) (-)

Ion 98.90 (98.60 to 99.60): VY003303.D (-945) (-)

7.80



100000

50000

0

7.70 7.80 7.90 8.00

Time-->

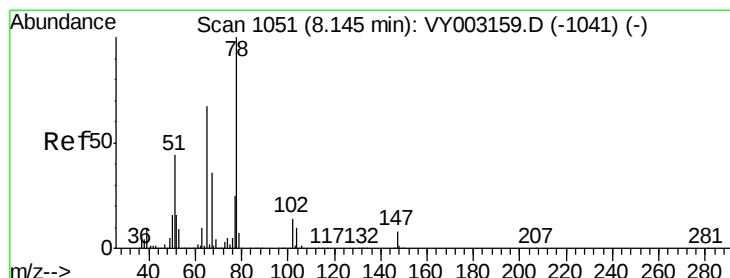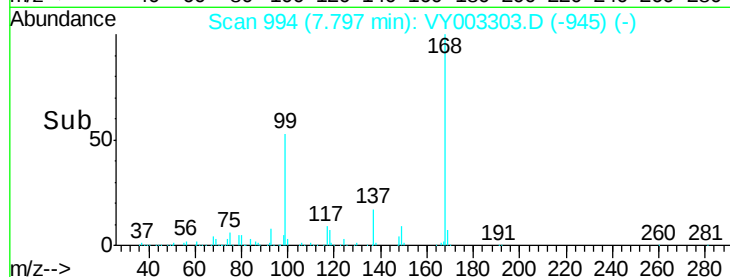

#33

1,2-Dichloroethane-d4

Concen: 62.453 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. 0.01 min

Lab File: VY003303.D


Acq: 22 Jul 2020 21:09

Tgt Ion: 65 Resp: 146370

Ion Ratio Lower Upper

65 100

67 53.7 0.0 105.2

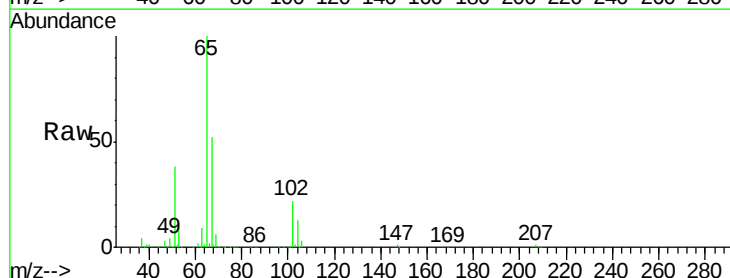

Abundance Ion 64.90 (64.60 to 65.60): VY003303.D (-1002) (-)

Ion 66.90 (66.60 to 67.60): VY003303.D (-1002) (-)

8.15

60000


40000


20000

0

8.00 8.10 8.20 8.30

Time-->




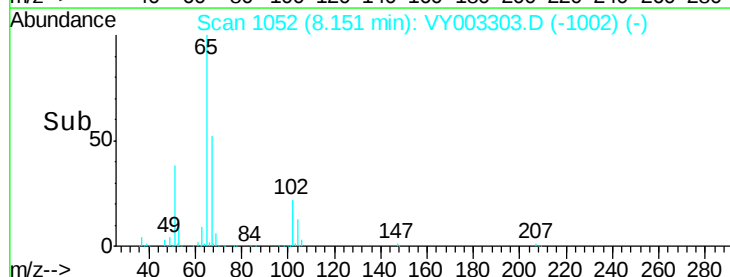


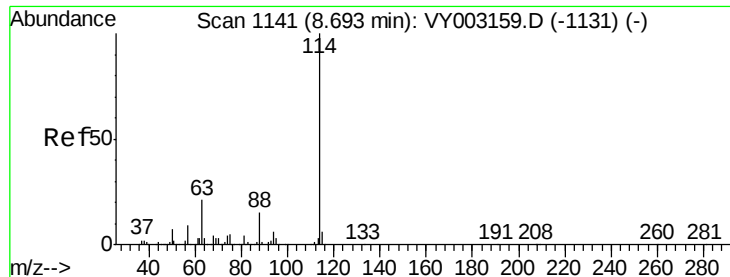

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.69 min Scan# 1141
 Delta R.T. 0.00 min
 Lab File: VY003303.D
 Acq: 22 Jul 2020 21:09




Instrument :
 MSVOA_Y
 ClientSampleId :
 19


Tot Ion	Ratio	Lower	Upper
114	100		
63	19.3	0.0	41.2
88	14.5	0.0	30.2

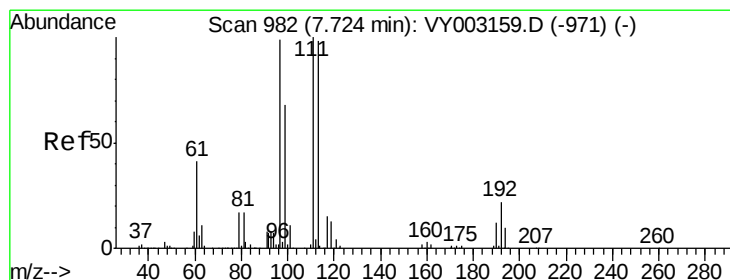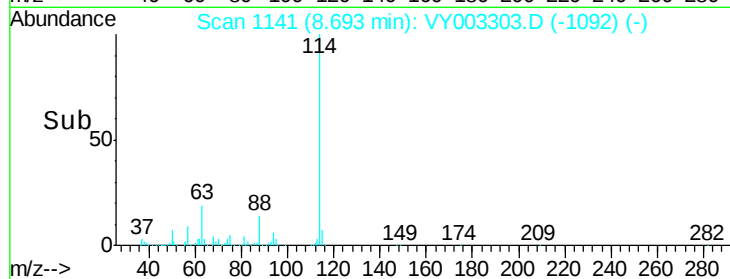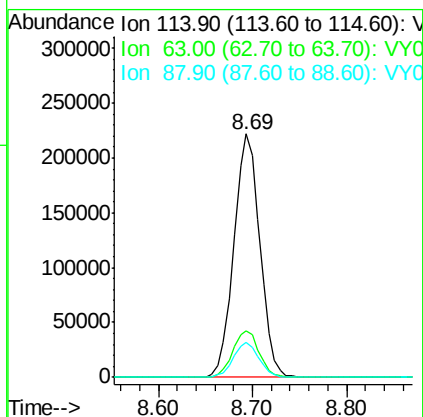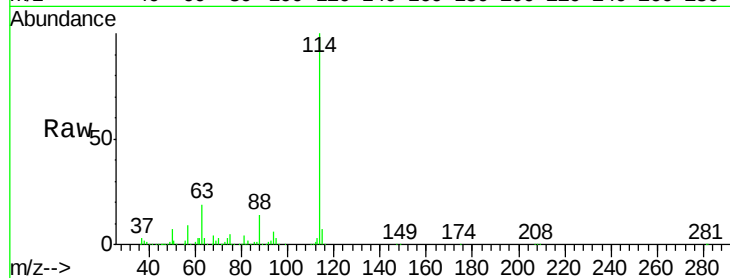

#35
 Dibromofluoromethane
 Concen: 55.627 ug/l
 RT: 7.72 min Scan# 982
 Delta R.T. 0.00 min
 Lab File: VY003303.D
 Acq: 22 Jul 2020 21:09

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.7	82.1	123.1
192	22.6	18.8	28.2

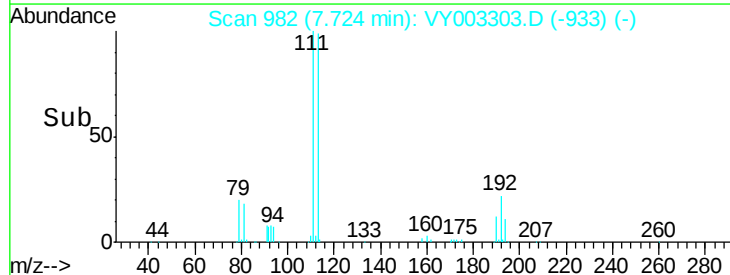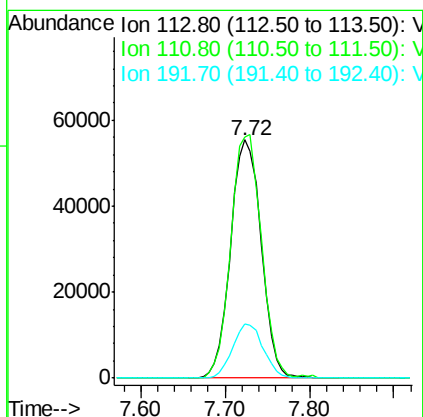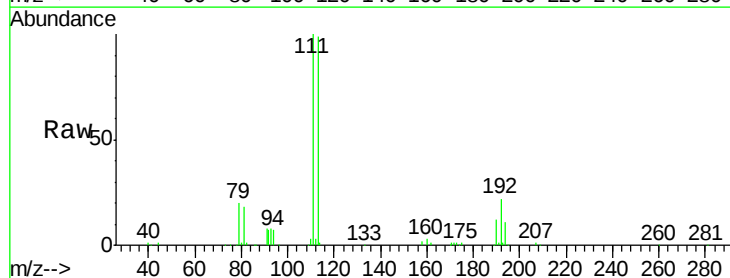

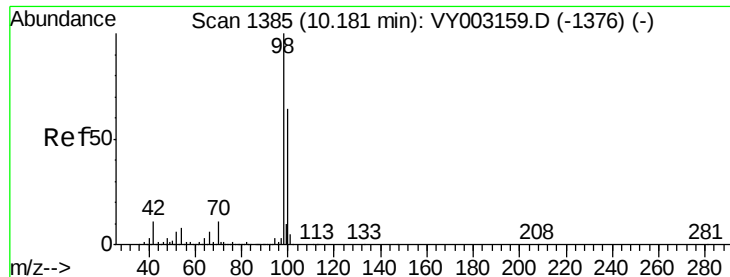

#50

Toluene-d8

Concen: 56.266 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. 0.00 min

Lab File: VY003303.D

Acq: 22 Jul 2020 21:09

Instrument :

MSVOA_Y

ClientSampleId :





19

Tot Ion: 98 Resp: 511466

Ion Ratio Lower Upper

98 100

100 64.2 50.7 76.1

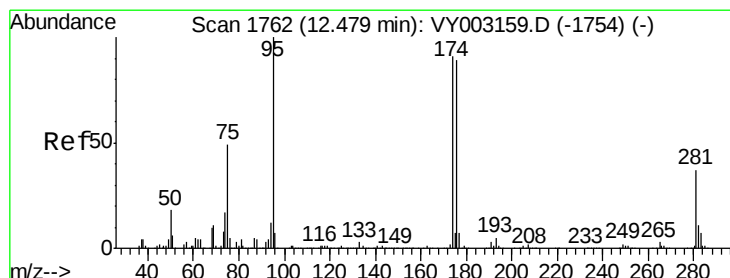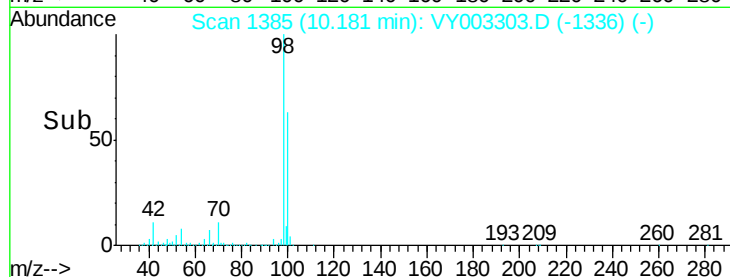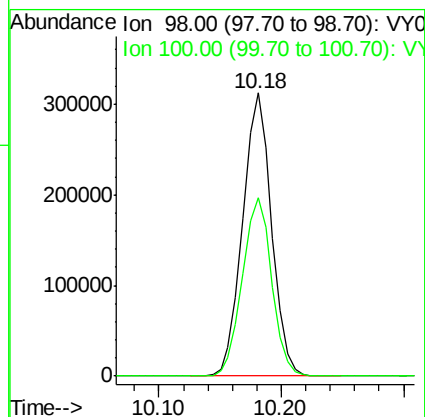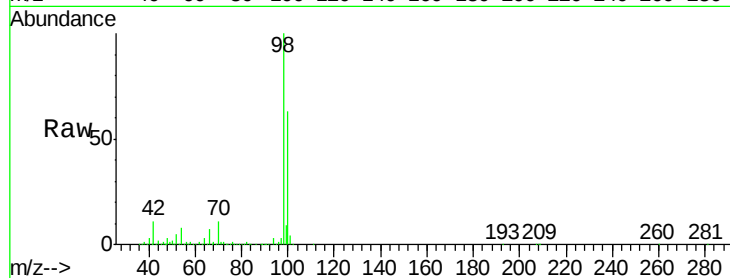

#62

4-Bromofluorobenzene

Concen: 49.165 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. 0.00 min

Lab File: VY003303.D

Acq: 22 Jul 2020 21:09




Tgt Ion: 95 Resp: 161453


Ion Ratio Lower Upper

95 100

174 97.7 0.0 190.6

176 93.7 0.0 186.4

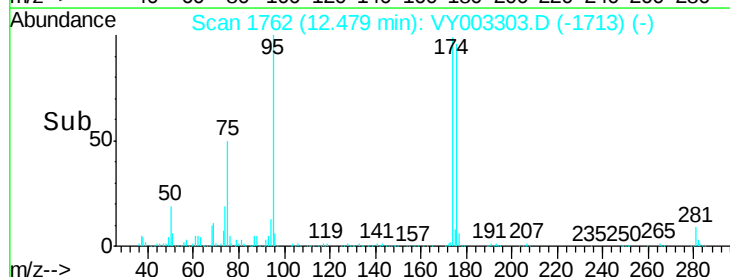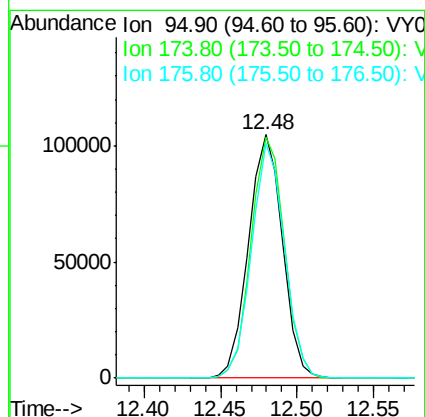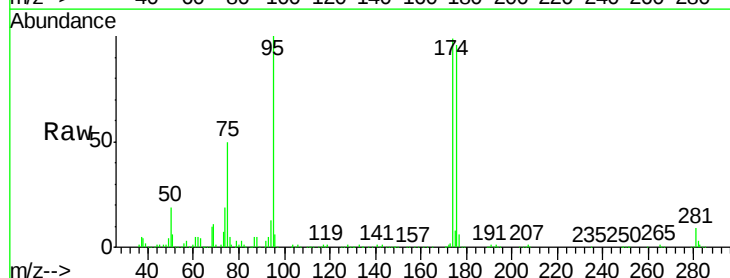


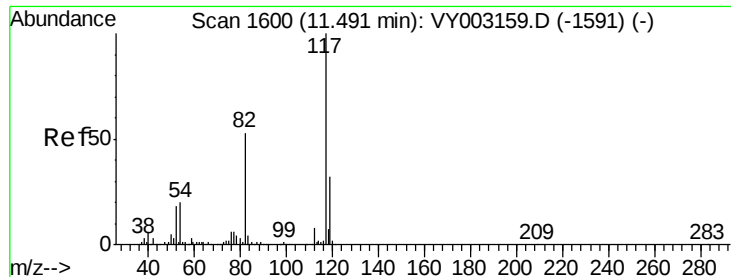




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. 0.00 min
Lab File: VY003303.D
Acq: 22 Jul 2020 21:09

Instrument :
MSVOA_Y
ClientSampleId :
19

Tot Ion:117 Resp: 389548
Ion Ratio Lower Upper
117 100
82 51.8 42.0 63.0
119 32.2 25.5 38.3

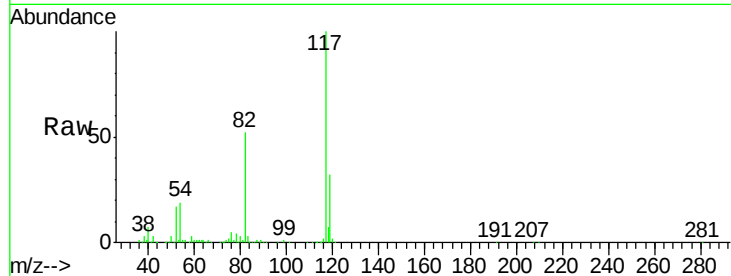


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

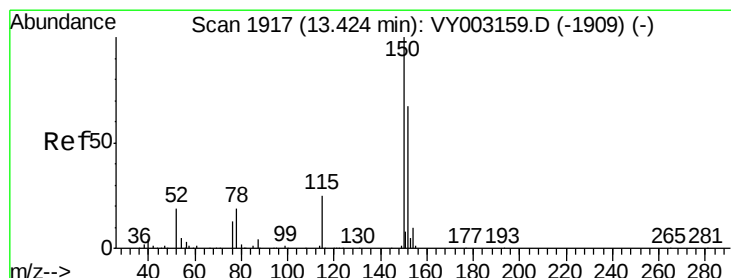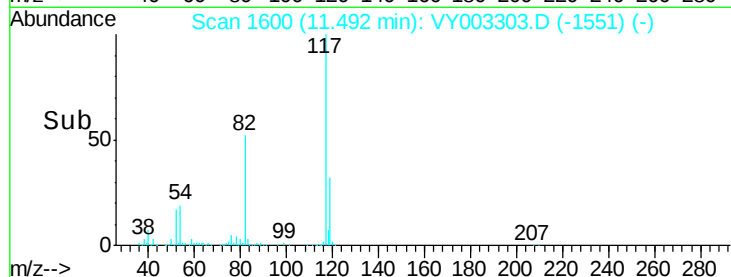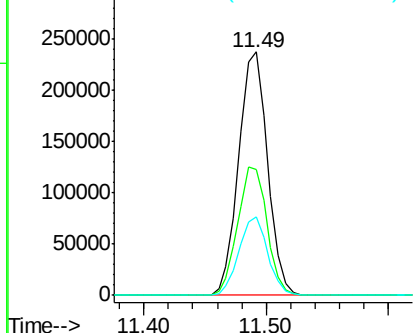

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. 0.00 min
Lab File: VY003303.D
Acq: 22 Jul 2020 21:09

Tgt Ion:152 Resp: 186264
Ion Ratio Lower Upper
152 100
115 54.9 26.9 80.7
150 158.5 0.0 338.0

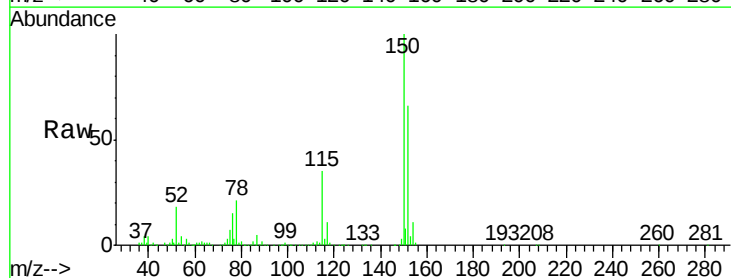

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

