


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv072220\
 Data File : VY003277.D
 Acq On : 22 Jul 2020 09:47
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
 Title : SW846 8260
 Last Update : Fri Jul 10 13:18:03 2020

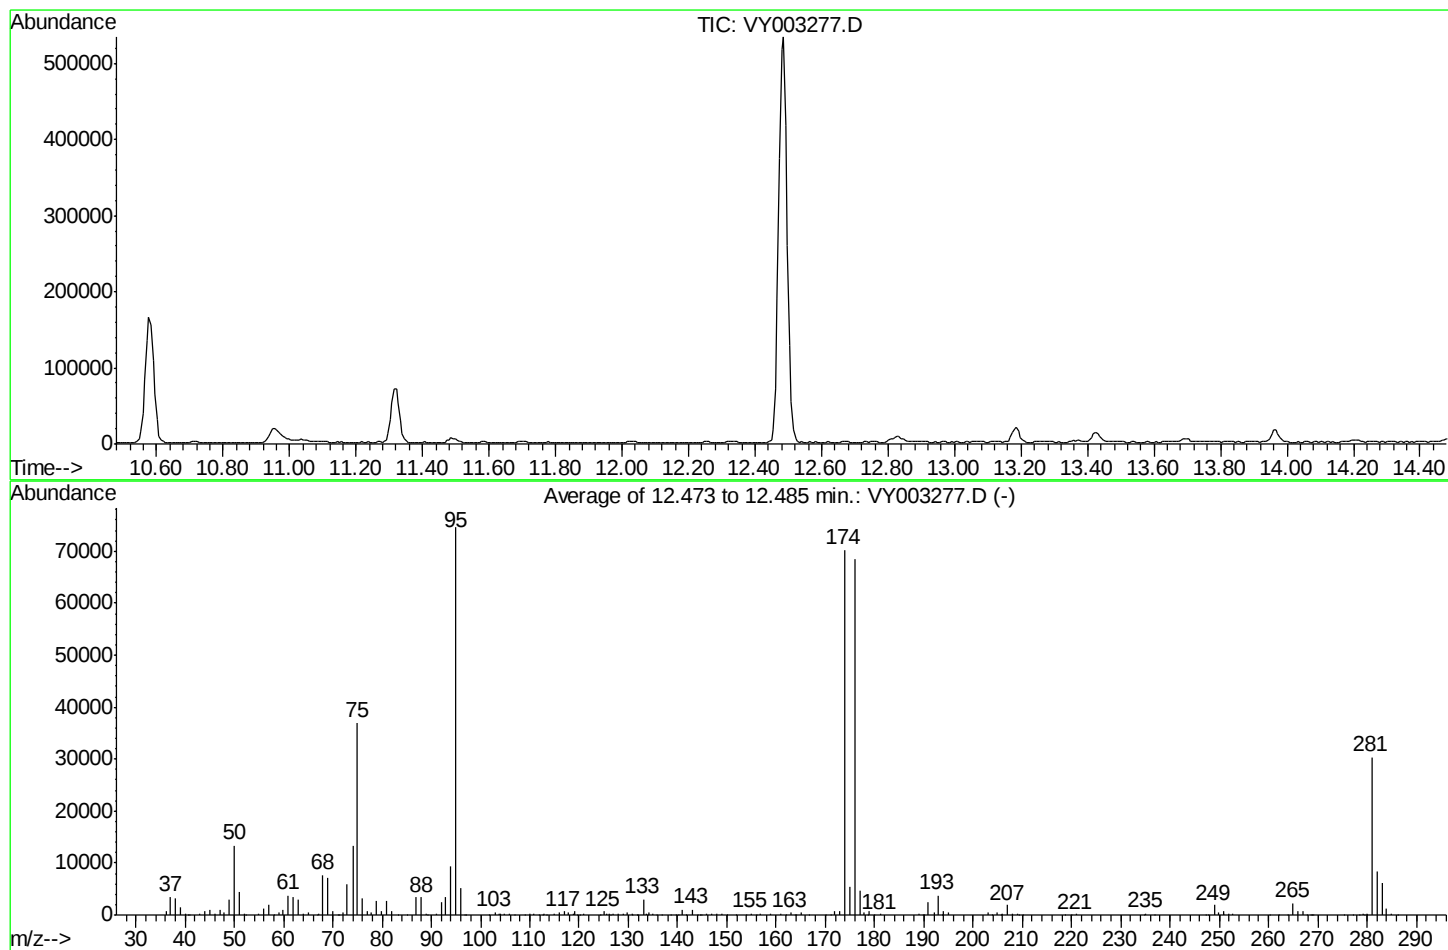

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	13387	PASS
75	95	30	60	49.6	37016	PASS
95	95	100	100	100.0	74605	PASS
96	95	5	9	6.9	5158	PASS
173	174	0.00	2	1.0	722	PASS
174	95	50	100	94.2	70245	PASS
175	174	5	9	7.8	5488	PASS
176	174	95	101	97.4	68410	PASS
177	176	5	9	6.9	4732	PASS