
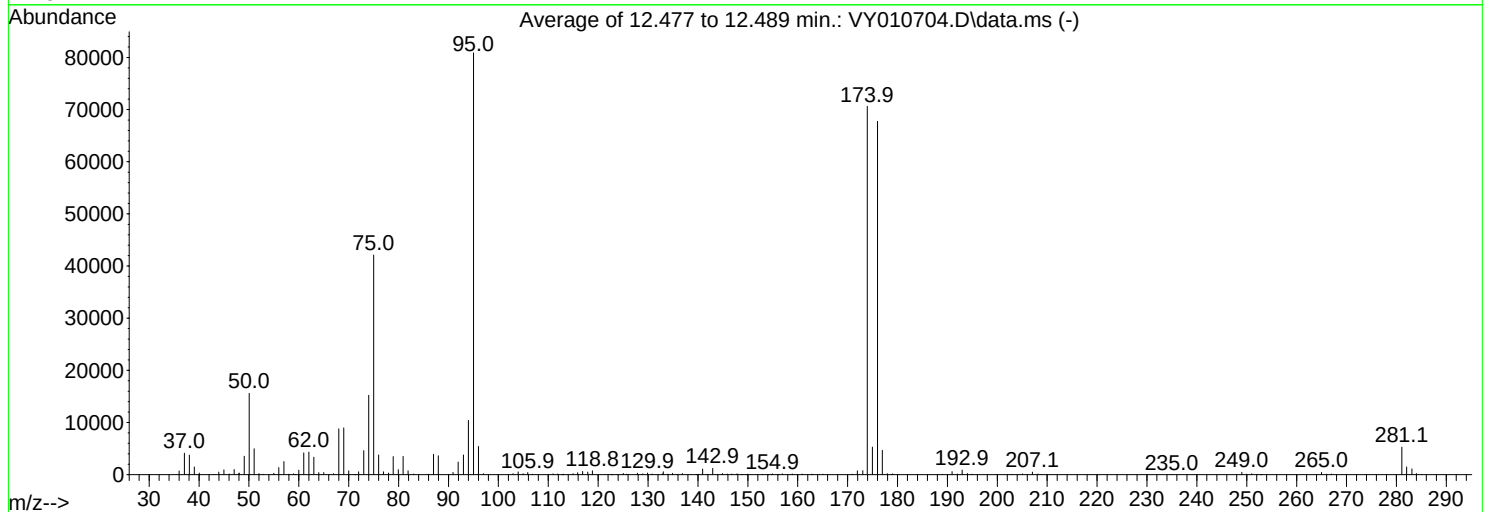


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY092822\  
 Data File : VY010704.D  
 Acq On : 28 Sep 2022 09:31  
 Operator : KP/MD  
 Sample : BFB  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y091922S.M  
 Title : SW846 8260  
 Last Update : Tue Sep 20 01:02:44 2022

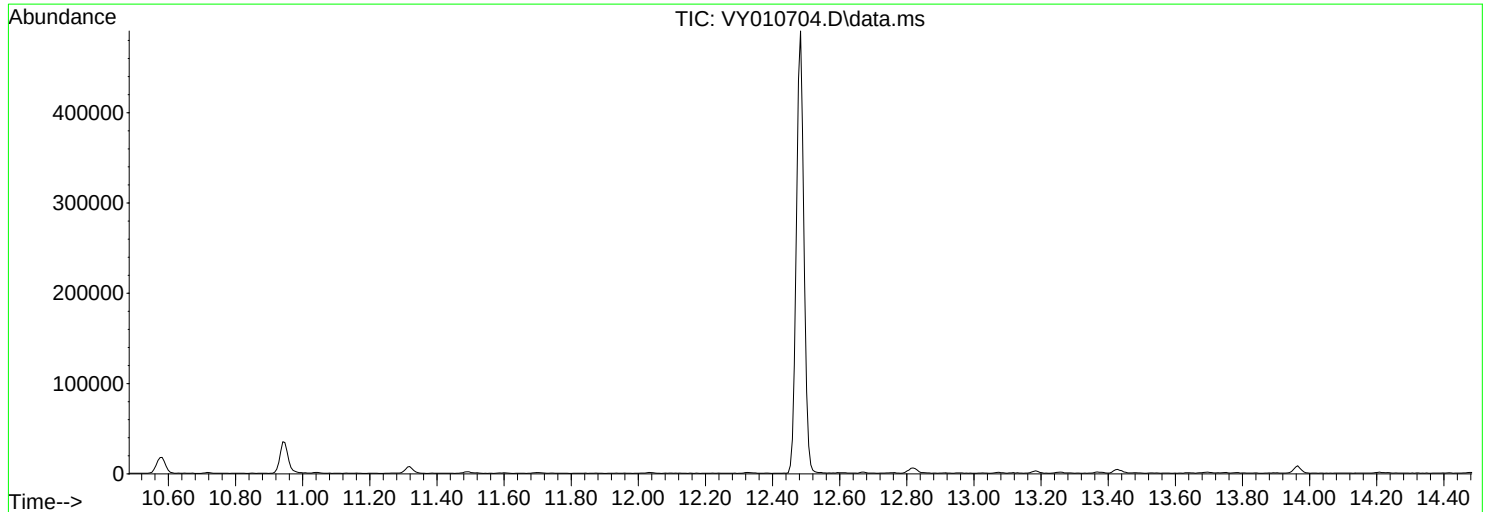

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.3         | 15596      | PASS                |
| 75             | 95              | 30              | 60              | 52.1         | 42136      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 80883      | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 5404       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.1          | 762        | PASS                |
| 174            | 95              | 50              | 100             | 87.3         | 70616      | PASS                |
| 175            | 174             | 5               | 9               | 7.5          | 5267       | PASS                |
| 176            | 174             | 95              | 101             | 95.9         | 67733      | PASS                |
| 177            | 176             | 5               | 9               | 6.9          | 4665       | PASS                |