

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100522\
 Data File : VY010816.D
 Acq On : 05 Oct 2022 13:45
 Operator : KP/MD
 Sample : N4947-01
 Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 CL-02-093022

Quant Time: Oct 05 14:15:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100322S.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 04 07:26:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	256186	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	441261	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	379741	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	163472	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	131176	50.515	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	101.040%
35) Dibromofluoromethane	7.710	113	138371	47.240	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	94.480%
50) Toluene-d8	10.179	98	435974	43.522	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	87.040%
62) 4-Bromofluorobenzene	12.477	95	158516	39.750	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	79.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY100522\
Data File : VY010816.D
Acq On : 05 Oct 2022 13:45
Operator : KP/MD
Sample : N4947-01
Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
CL-02-093022

Quant Time: Oct 05 14:15:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100322S.M
Quant Title : SW846 8260
QLast Update : Tue Oct 04 07:26:22 2022
Response via : Initial Calibration




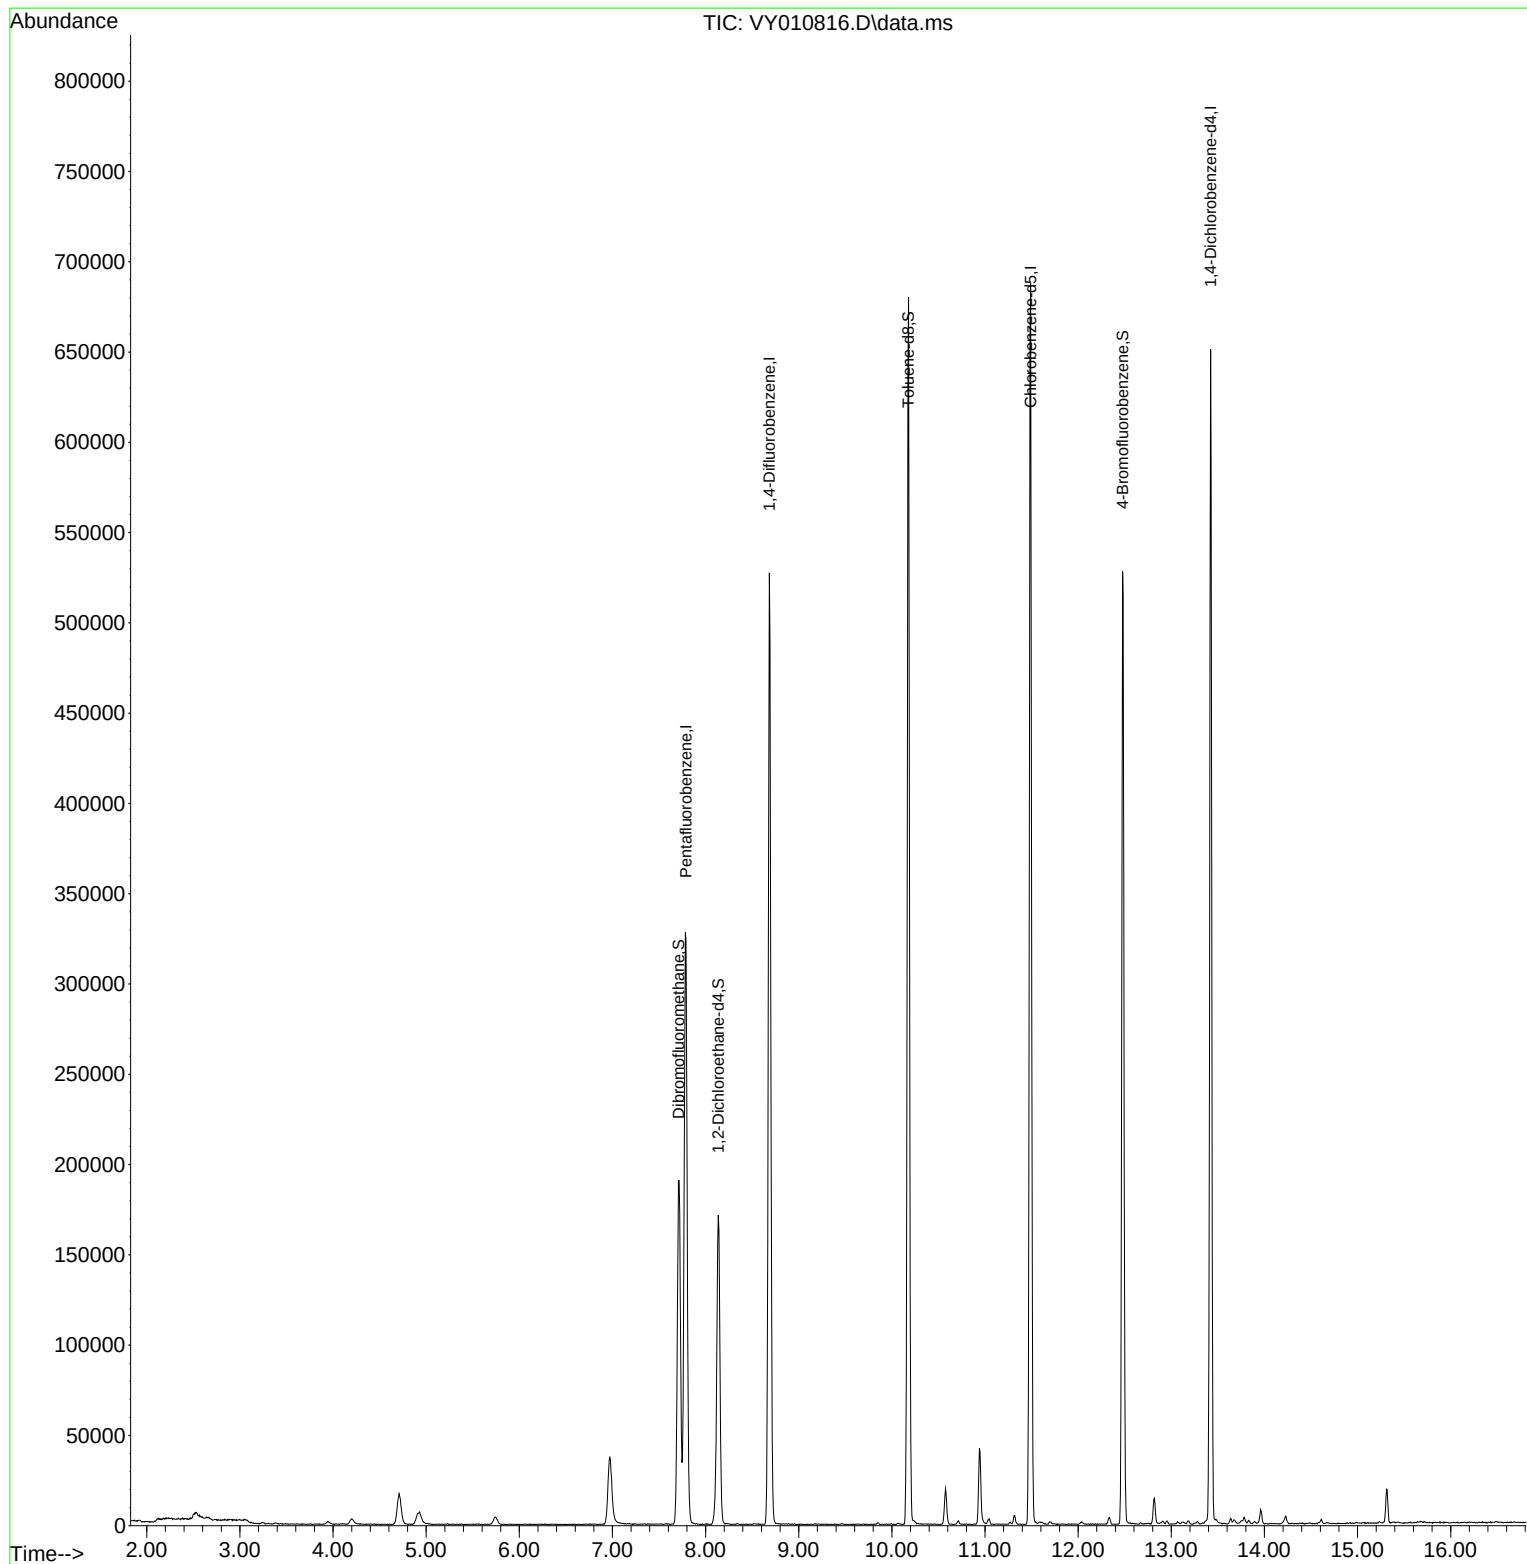


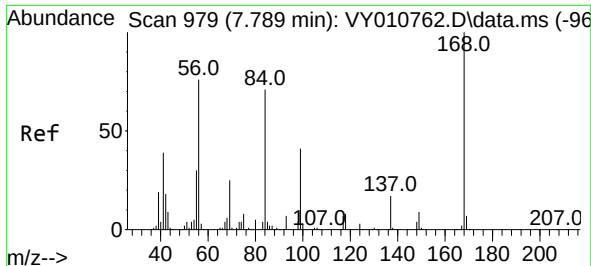

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY010816.D
Acq: 05 Oct 2022 13:45




Instrument :
MSVOA_Y
ClientSampleId :
CL-02-093022


Tgt Ion:168 Resp: 256186
Ion Ratio Lower Upper
168 100
99 53.9 46.9 70.3

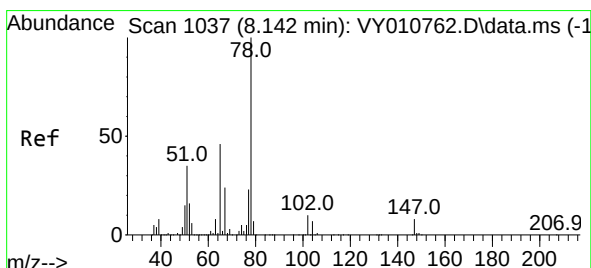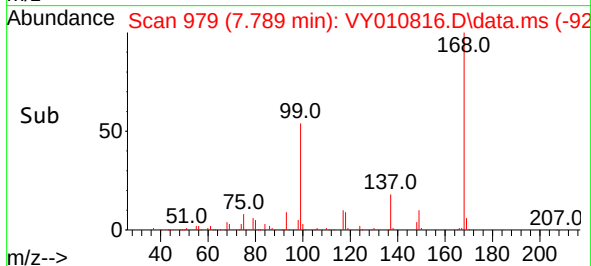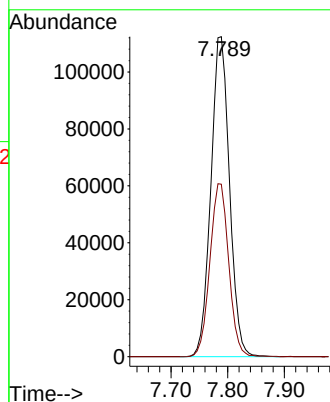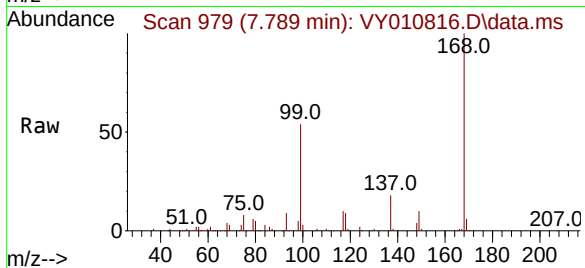

#33
1,2-Dichloroethane-d4
Concen: 50.515 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.001 min
Lab File: VY010816.D
Acq: 05 Oct 2022 13:45

Tgt Ion: 65 Resp: 131176
Ion Ratio Lower Upper
65 100
67 52.9 0.0 99.4

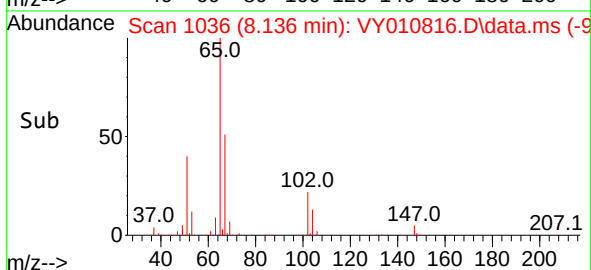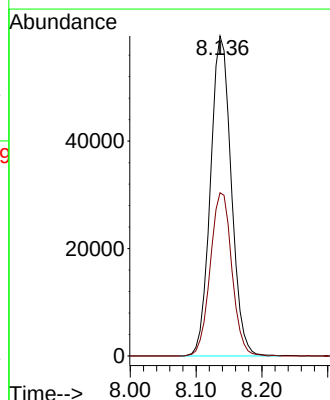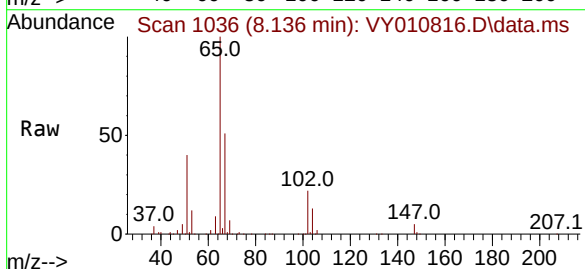

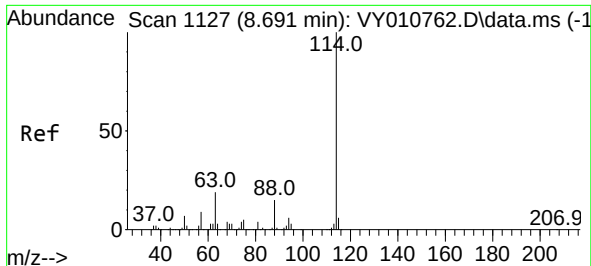

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY010816.D

Acq: 05 Oct 2022 13:45

Instrument :

MSVOA_Y

ClientSampleId :

CL-02-093022





Tgt Ion:114 Resp: 441261

Ion Ratio Lower Upper

114 100

63 20.0 0.0 43.2

88 15.0 0.0 31.8

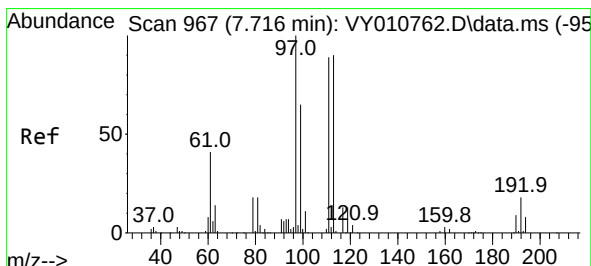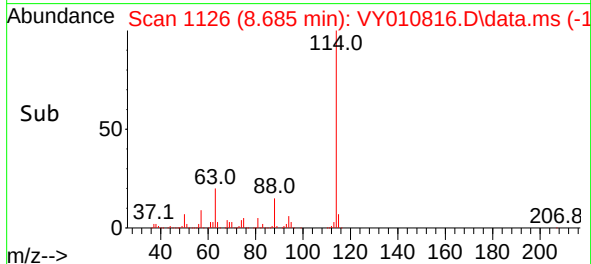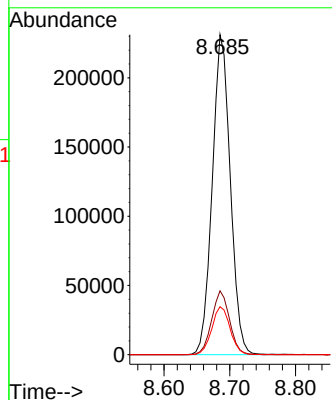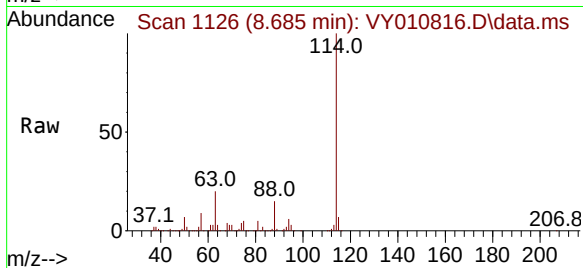

#35

Dibromofluoromethane

Concen: 47.240 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.000 min

Lab File: VY010816.D

Acq: 05 Oct 2022 13:45




Tgt Ion:113 Resp: 138371


Ion Ratio Lower Upper

113 100

111 103.5 82.6 124.0

192 19.4 17.6 26.4


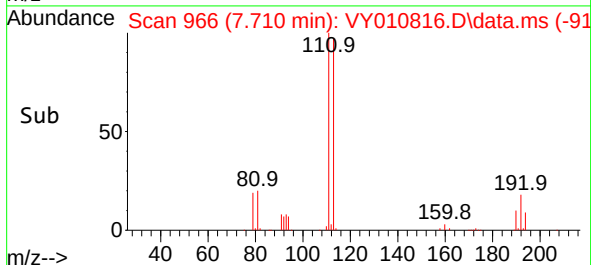
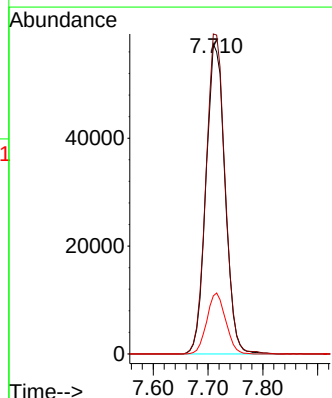
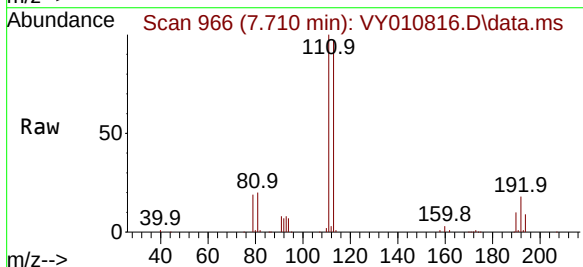


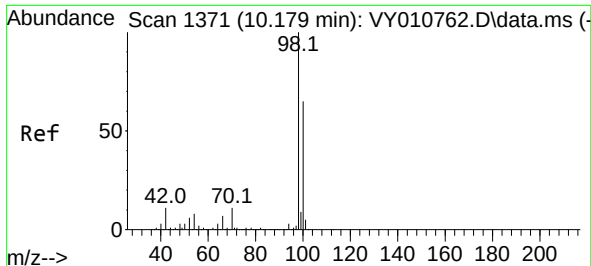

#50
Toluene-d8
Concen: 43.522 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY010816.D
Acq: 05 Oct 2022 13:45




Instrument :
MSVOA_Y
ClientSampleId :
CL-02-093022


Tgt Ion: 98 Resp: 435974
Ion Ratio Lower Upper
98 100
100 64.6 50.2 75.2

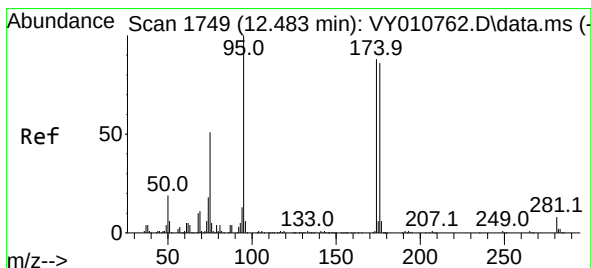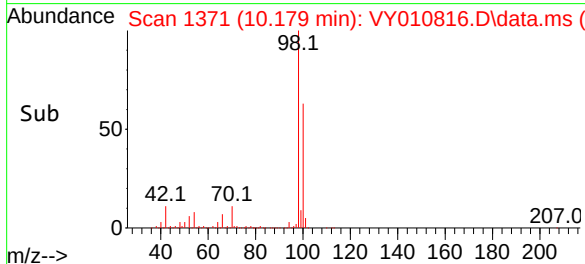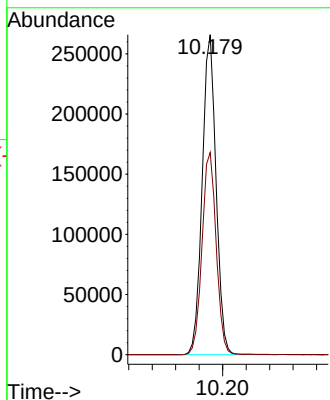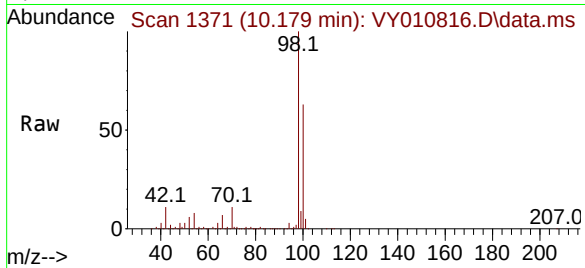

#62
4-Bromofluorobenzene
Concen: 39.750 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY010816.D
Acq: 05 Oct 2022 13:45

Tgt Ion: 95 Resp: 158516
Ion Ratio Lower Upper
95 100
174 84.0 0.0 177.0
176 80.8 0.0 175.8


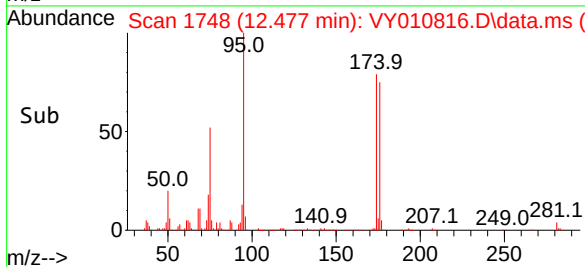
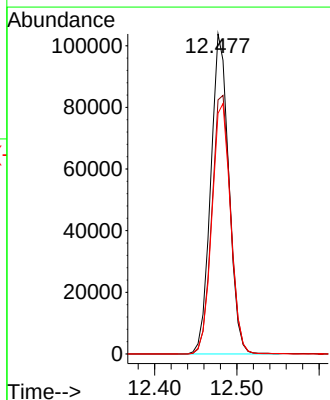
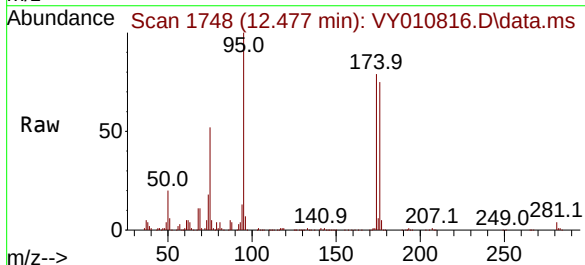


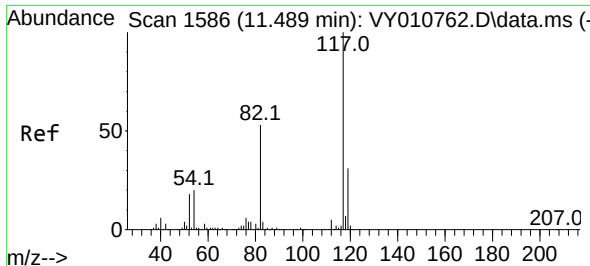

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. -0.001 min
Lab File: VY010816.D
Acq: 05 Oct 2022 13:45

Instrument :
MSVOA_Y
ClientSampleId :
CL-02-093022

Tgt Ion:117 Resp: 379741
Ion Ratio Lower Upper
117 100
82 53.5 43.0 64.4
119 31.9 25.4 38.0

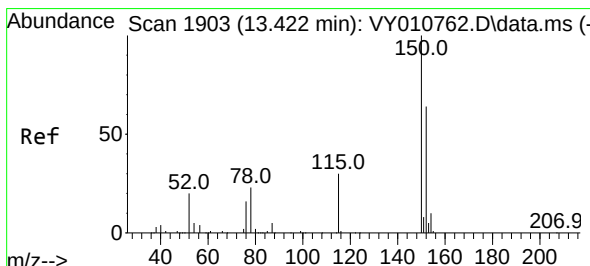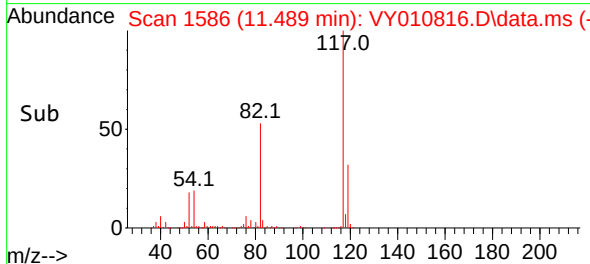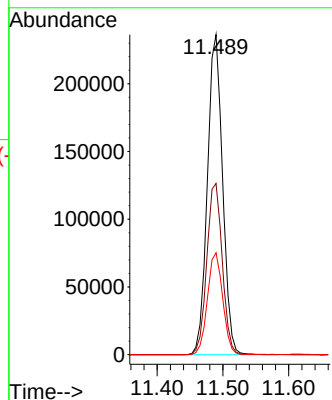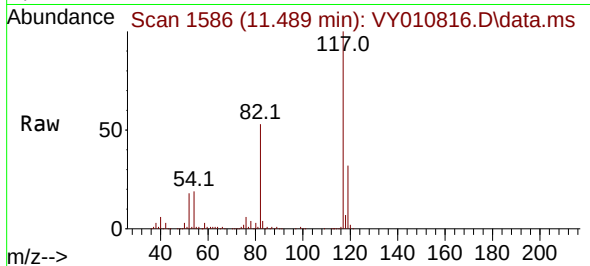

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY010816.D
Acq: 05 Oct 2022 13:45

Tgt Ion:152 Resp: 163472
Ion Ratio Lower Upper
152 100
115 58.6 28.2 84.7
150 158.0 0.0 347.6

