
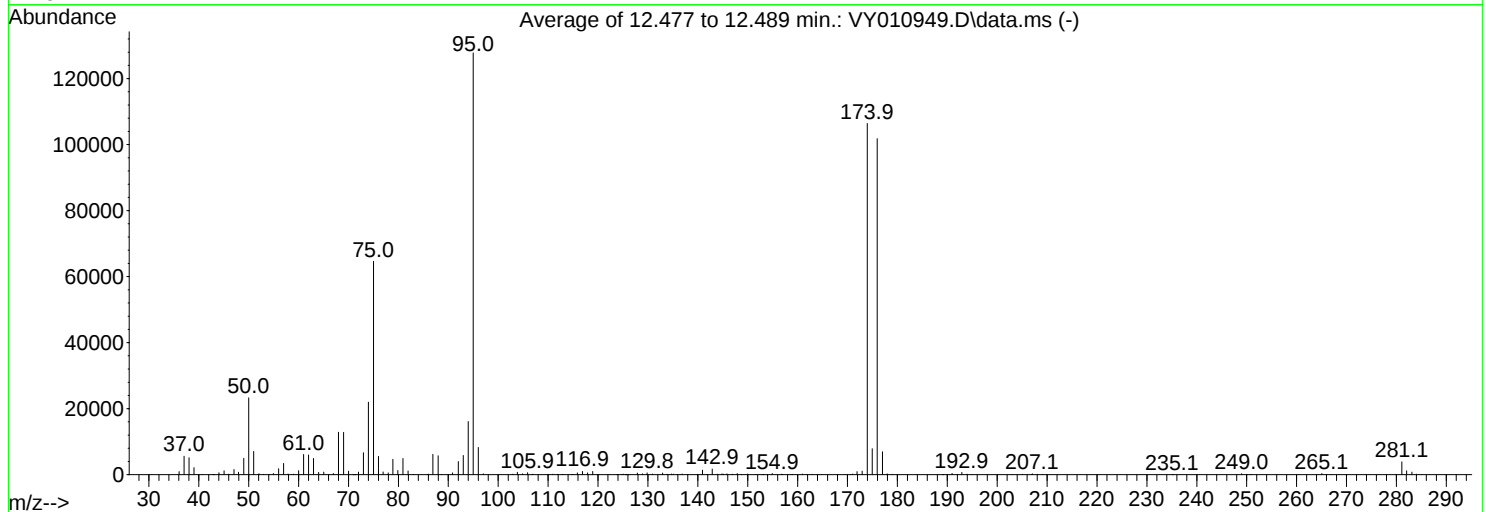


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY101322\
 Data File : VY010949.D
 Acq On : 13 Oct 2022 09:45
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100322S.M
 Title : SW846 8260
 Last Update : Tue Oct 04 07:26:22 2022

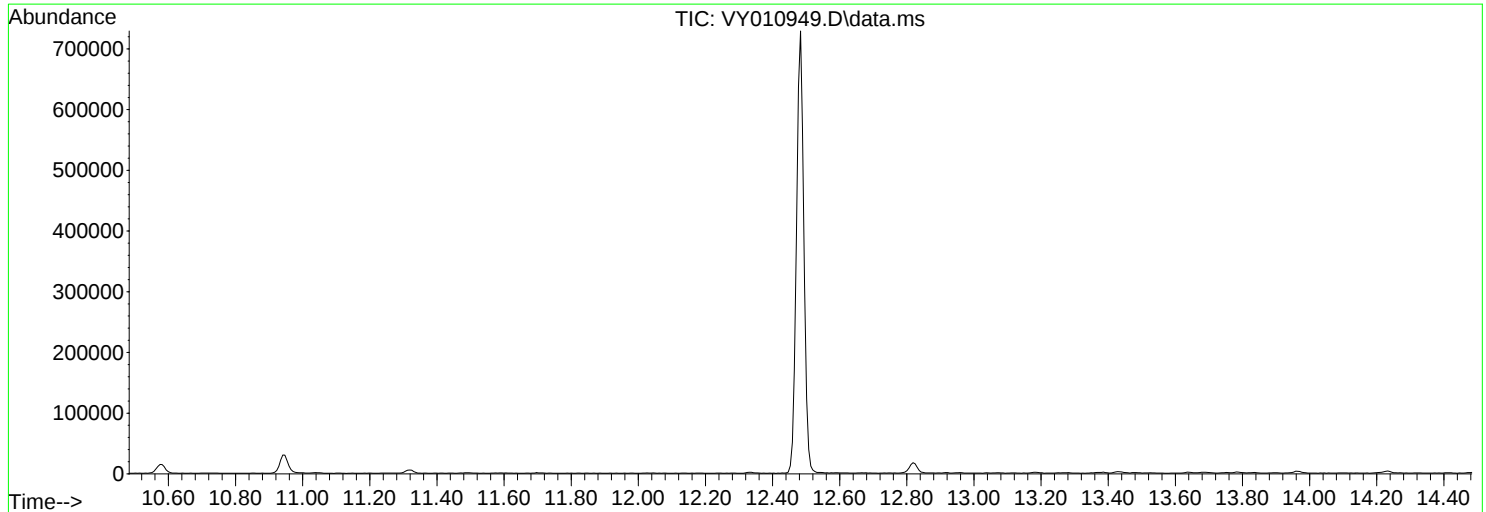

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	23283	PASS
75	95	30	60	50.6	64619	PASS
95	95	100	100	100.0	127816	PASS
96	95	5	9	6.4	8232	PASS
173	174	0.00	2	1.0	1076	PASS
174	95	50	100	83.2	106403	PASS
175	174	5	9	7.4	7846	PASS
176	174	95	101	95.7	101795	PASS
177	176	5	9	6.8	6935	PASS