


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv101719\
Data File : VY000333.D
Acq On : 17 Oct 2019 09:34
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y101119S.M
Title : SW846 8260
Last Update : Thu Oct 17 02:03:07 2019

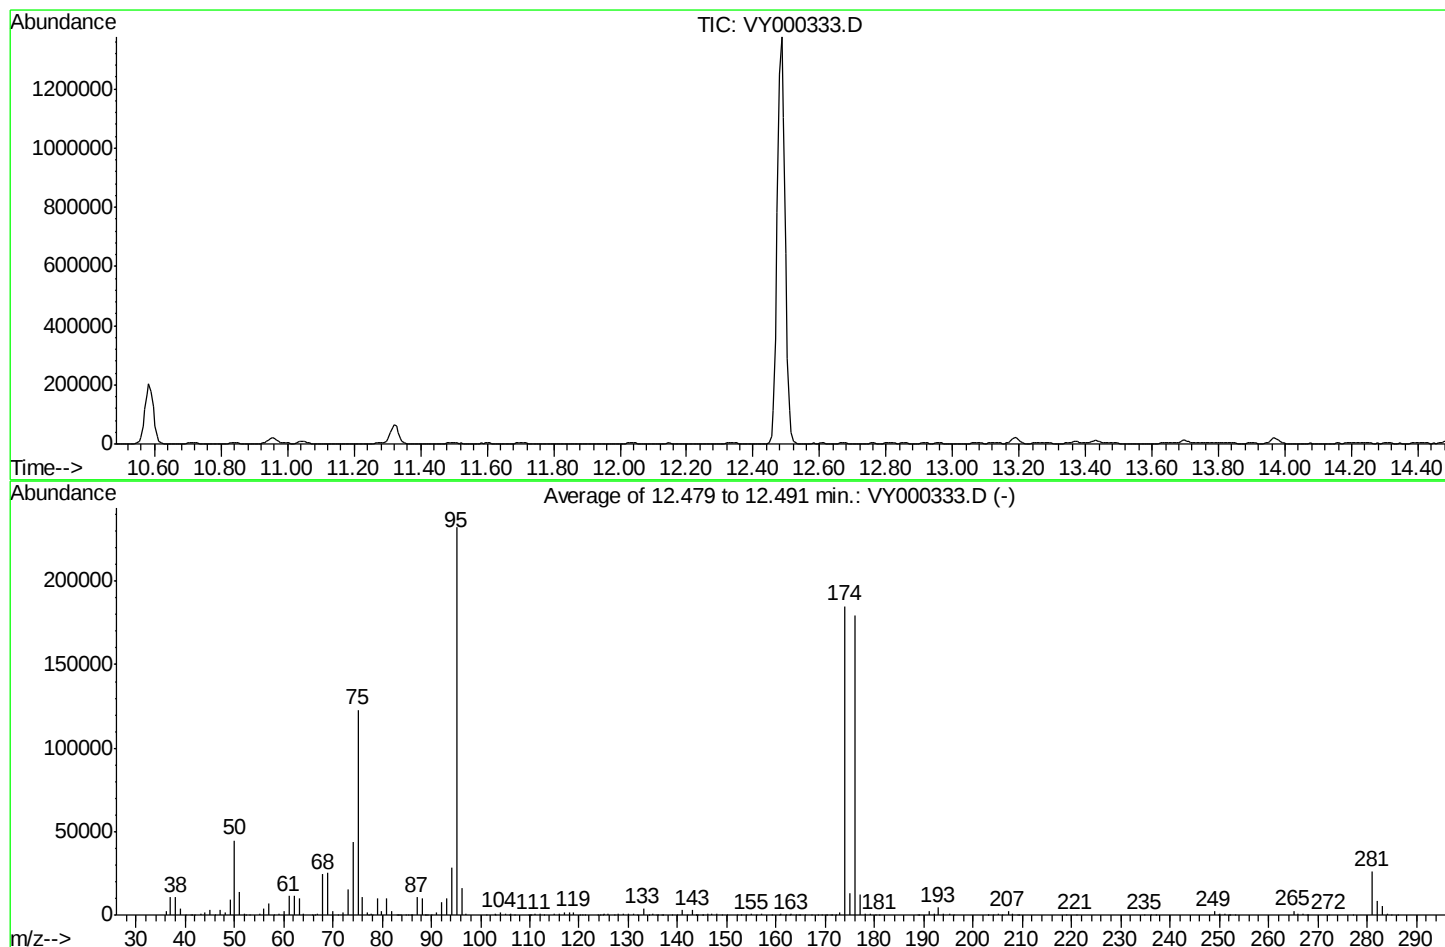

AutoFind: Scans 1762, 1763, 1764; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	44752	PASS
75	95	30	60	53.0	123085	PASS
95	95	100	100	100.0	232320	PASS
96	95	5	9	6.8	15807	PASS
173	174	0.00	2	0.8	1562	PASS
174	95	50	100	79.6	184874	PASS
175	174	5	9	7.0	12972	PASS
176	174	95	101	97.1	179605	PASS
177	176	5	9	6.9	12316	PASS