

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY102122\
 Data File : VY011043.D
 Acq On : 21 Oct 2022 12:29
 Operator : KP/MD
 Sample : N5217-03
 Misc : 5.07g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-B1-3.5-4.0

Quant Time: Oct 22 01:22:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101722S.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 18 01:42:42 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	364518	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	606452	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	507991	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	213993	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	214498	63.882	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 127.760%			
35) Dibromofluoromethane	7.716	113	220266	65.840	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 131.680%			
50) Toluene-d8	10.179	98	792655	62.598	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 125.200%			
62) 4-Bromofluorobenzene	12.477	95	268834	60.584	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 121.160%			
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	4.924	59	7025	Below Cal	#	80
16) Acetone	3.942	43	4619	4.737	ug/l	91
18) Methyl Acetate	4.479	43	251	Below Cal	#	56
20) Methylene Chloride	4.710	84	17943	Below Cal	#	81
25) 2-Butanone	6.984	43	3078	2.082	ug/l	93
28) Bromochloromethane	7.338	49	22	3.529	ug/l	# 16
31) Cyclohexane	7.783	56	9727	1.514	ug/l	# 1
36) 1,1-Dichloropropene	7.783	75	27347	4.844	ug/l	# 50
38) Carbon Tetrachloride	7.789	117	35659	6.119	ug/l	# 15
39) Methylcyclohexane	9.185	83	26737	3.954	ug/l	91
51) 4-Methyl-2-Pentanone	10.179	43	19840	6.370	ug/l	95
55) 1,1,2-Trichloroethane	10.618	97	74520	22.036	ug/l	# 19
56) Ethyl methacrylate	10.520	69	36345	8.092	ug/l	# 23
58) 2-Chloroethyl Vinyl ether	9.782	63	295	17.084	ug/l	# 48
59) 2-Hexanone	10.801	43	27813	13.001	ug/l	# 35
67) Ethyl Benzene	11.593	91	20762	1.125	ug/l	96
68) m/p-Xylenes	11.697	106	21518	3.032	ug/l	98
69) o-Xylene	12.026	106	26966	4.001	ug/l	97
73) Isopropylbenzene	12.331	105	22812	1.467	ug/l	95
74) N-amyl acetate	12.124	43	54669	13.859	ug/l	# 47
75) 1,1,2,2-Tetrachloroethane	12.556	83	14758	4.523	ug/l	# 67
76) 1,2,3-Trichloropropane	12.477	75	126649	52.130	ug/l	# 100
78) n-propylbenzene	12.672	91	23394	1.237	ug/l	93
80) 1,3,5-Trimethylbenzene	12.812	105	82341	6.348	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.477	75	126649	112.116	ug/l	# 9
84) 1,2,4-Trimethylbenzene	13.117	105	144537	11.300	ug/l	97
85) sec-Butylbenzene	13.251	105	32820	1.947	ug/l	80
86) p-Isopropyltoluene	13.367	119	22001	1.573	ug/l	95
90) Hexachloroethane	13.971	117	3312	1.200	ug/l	# 9
95) Naphthalene	15.233	128	446350	56.514	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 22 01:22:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y101722S.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 01:42:42 2022
Response via : Initial Calibration







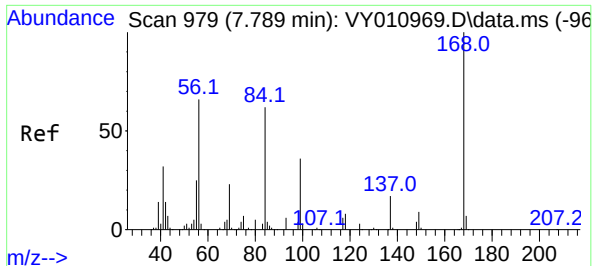

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion:168 Resp: 364518
Ion Ratio Lower Upper
168 100
99 55.1 46.9 70.3

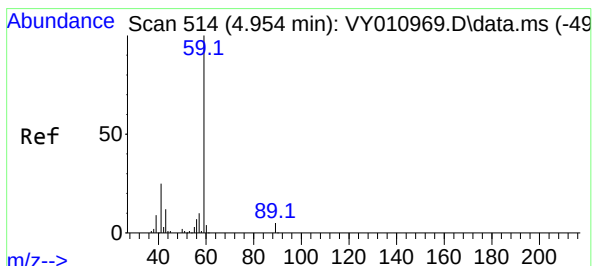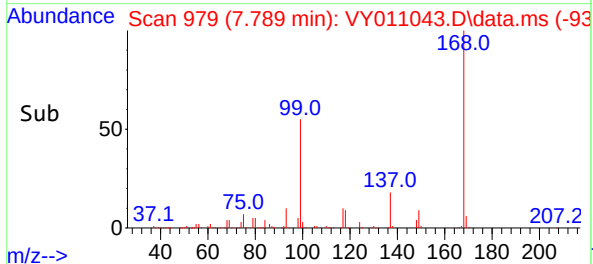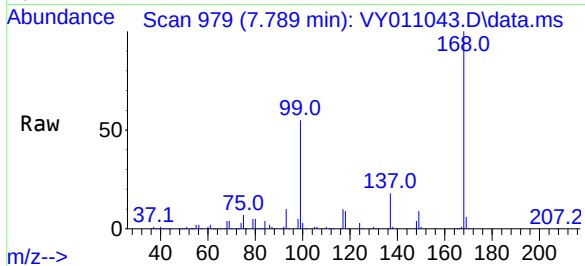

#11
Tert butyl alcohol
Concen: Below Cal
RT: 4.924 min Scan# 509
Delta R.T. -0.030 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion: 59 Resp: 7025
Ion Ratio Lower Upper
59 100
57 1.0 6.4 9.6#

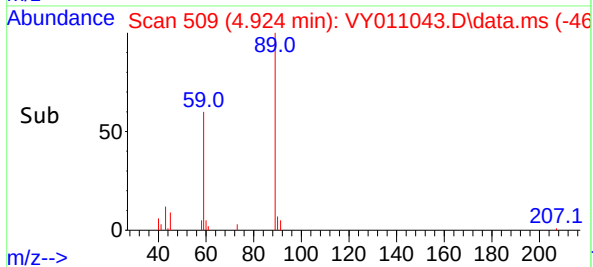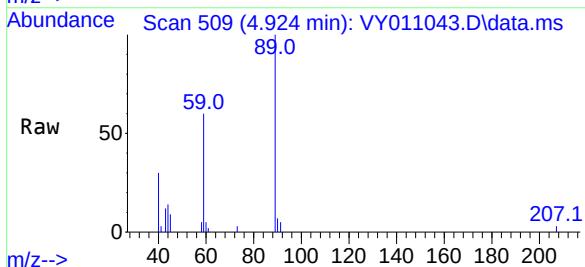



#16

Acetone

Concen: 4.737 ug/l

RT: 3.942 min Scan# 34

Delta R.T. 0.000 min

Lab File: VY011043.D

Acq: 21 Oct 2022 12:29

Instrument :

MSVOA_Y

ClientSampleId :





SB-B1-3.5-4.0

Tgt Ion: 43 Resp: 4619

Ion Ratio Lower Upper

43 100

58 32.4 22.0 33.0

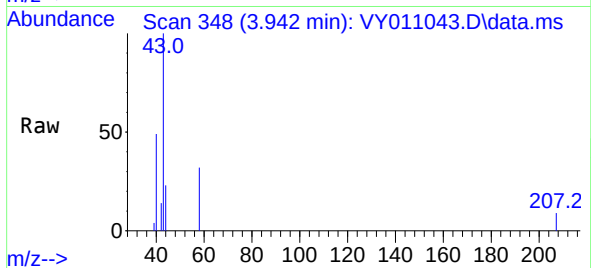

#18

Methyl Acetate

Concen: Below Cal

RT: 4.479 min Scan# 436

Delta R.T. 0.006 min

Lab File: VY011043.D




Acq: 21 Oct 2022 12:29


Tgt Ion: 43 Resp: 251

Ion Ratio Lower Upper

43 100

74 0.0 16.6 24.8#


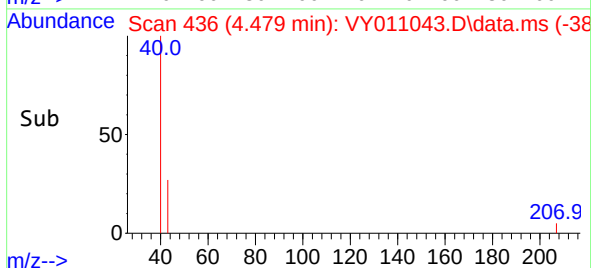
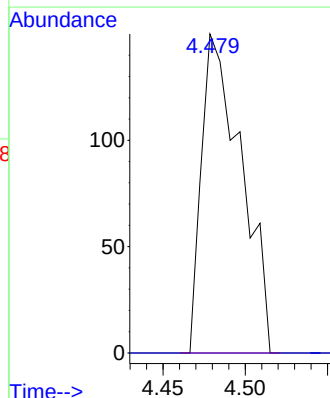





#20
Methylene Chloride
Concen: Below Cal
RT: 4.710 min Scan# 41
Delta R.T. 0.000 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion: 84 Resp: 17943
Ion Ratio Lower Upper
84 100
49 115.1 114.4 171.6
51 32.1 35.3 52.9#
86 57.7 53.7 80.5



#25
2-Butanone
Concen: 2.082 ug/l
RT: 6.984 min Scan# 847
Delta R.T. 0.006 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion: 43 Resp: 3078
Ion Ratio Lower Upper
43 100
72 18.9 17.7 26.5

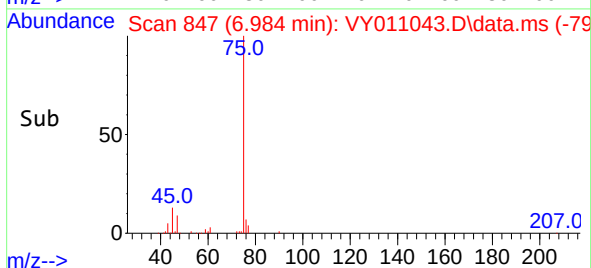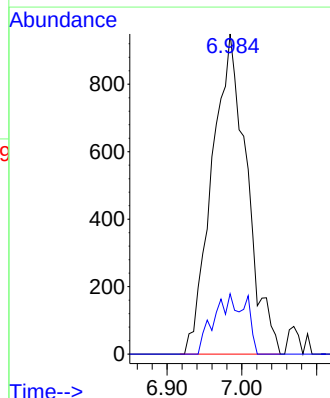



#28

Bromochloromethane

Concen: 3.529 ug/l

RT: 7.338 min Scan# 904

Delta R.T. 0.006 min

Lab File: VY011043.D

Acq: 21 Oct 2022 12:29

Instrument :

MSVOA_Y

ClientSampleId :

SB-B1-3.5-4.0





Tgt Ion: 49 Resp: 22

Ion Ratio Lower Upper

49 100

129 0.0 0.0 2.2

130 0.0 55.4 83.0#

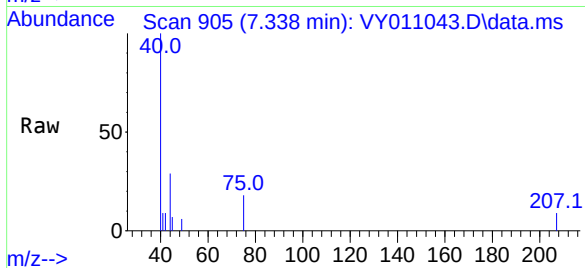

#31

Cyclohexane

Concen: 1.514 ug/l

RT: 7.783 min Scan# 978

Delta R.T. -0.000 min

Lab File: VY011043.D

Acq: 21 Oct 2022 12:29




Tgt Ion: 56 Resp: 9727


Ion Ratio Lower Upper

56 100

69 141.6 26.7 40.1#

84 141.5 67.2 100.8#

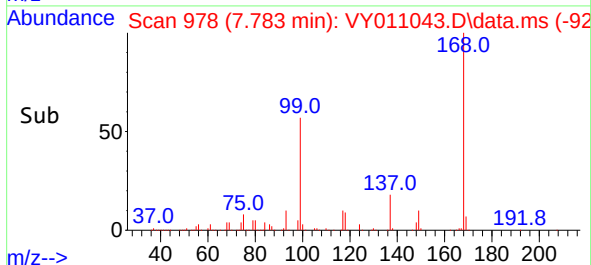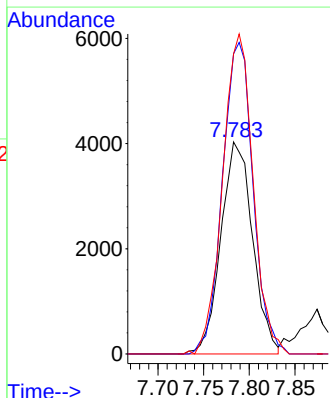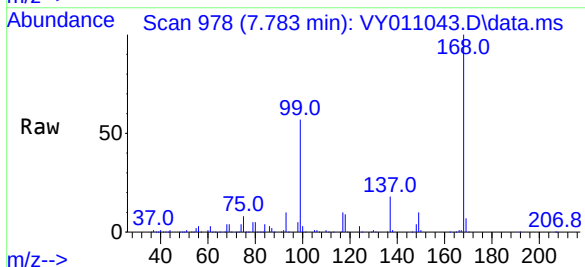

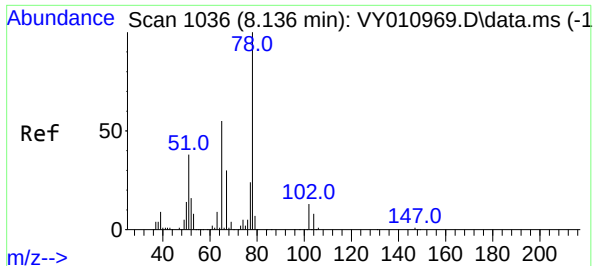

#33

1,2-Dichloroethane-d4

Concen: 63.882 ug/l

RT: 8.143 min Scan# 1103

Delta R.T. 0.007 min

Lab File: VY011043.D

Acq: 21 Oct 2022 12:29

Instrument :

MSVOA_Y

ClientSampleId :





SB-B1-3.5-4.0

Tgt Ion: 65 Resp: 214498

Ion Ratio Lower Upper

65 100

67 54.3 0.0 99.4

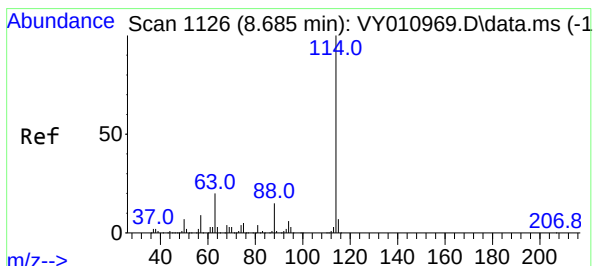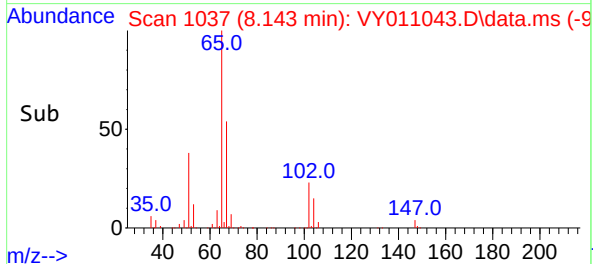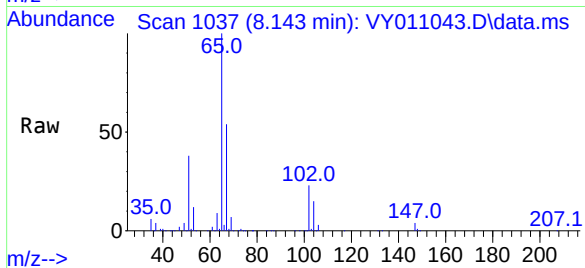

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY011043.D

Acq: 21 Oct 2022 12:29




Tgt Ion:114 Resp: 606452


Ion Ratio Lower Upper

114 100

63 18.9 0.0 43.2

88 15.2 0.0 31.8


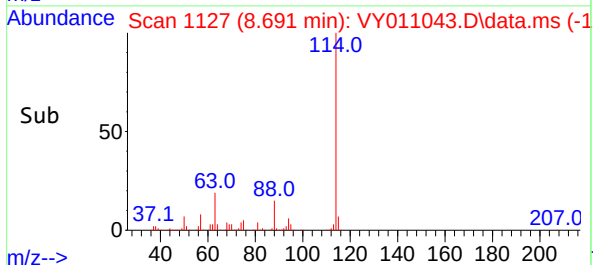
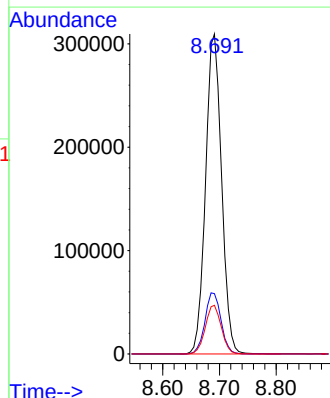
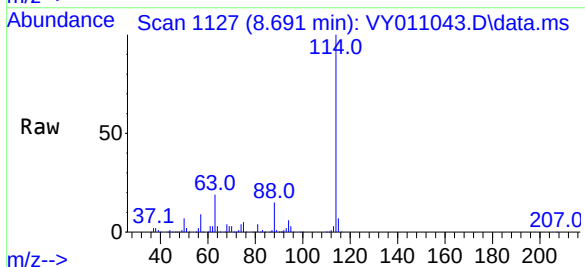




#35
Dibromofluoromethane
Concen: 65.840 ug/l
RT: 7.716 min Scan# 90
Delta R.T. 0.006 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion:113 Resp: 220266
Ion Ratio Lower Upper
113 100
111 102.1 82.6 124.0
192 19.5 17.6 26.4

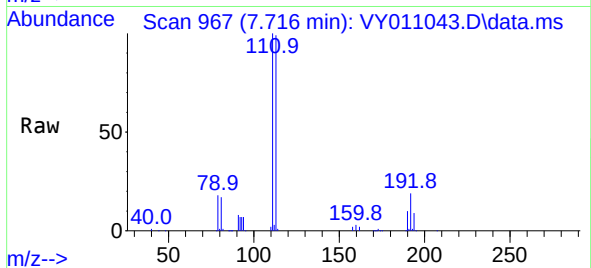

#36
1,1-Dichloropropene
Concen: 4.844 ug/l
RT: 7.783 min Scan# 978
Delta R.T. -0.134 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion: 75 Resp: 27347
Ion Ratio Lower Upper
75 100
110 8.5 17.1 51.2#
77 0.1 24.4 36.6#


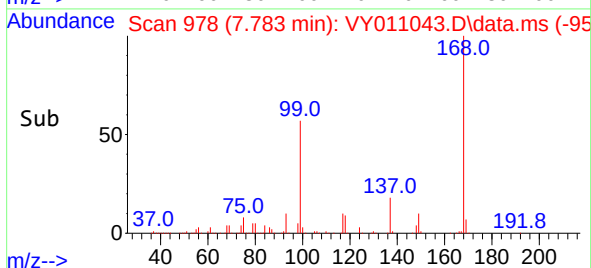
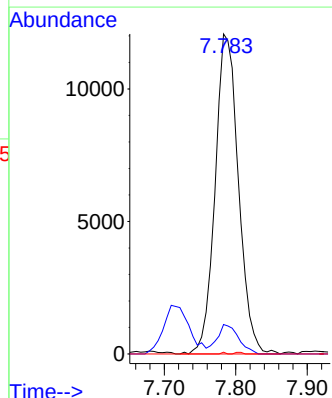



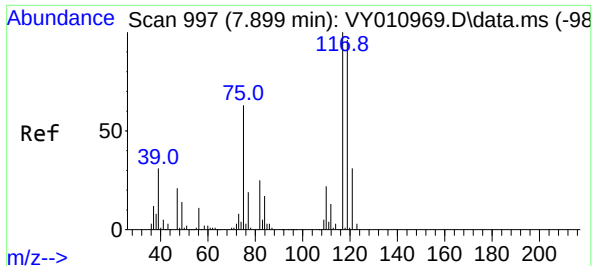

#38
Carbon Tetrachloride
Concen: 6.119 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.110 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion:117 Resp: 35659
Ion Ratio Lower Upper
117 100
119 4.3 77.9 116.9#
121 0.0 24.8 37.2#

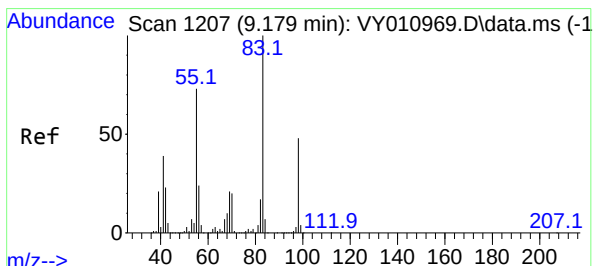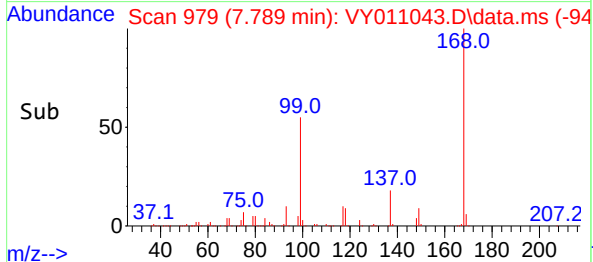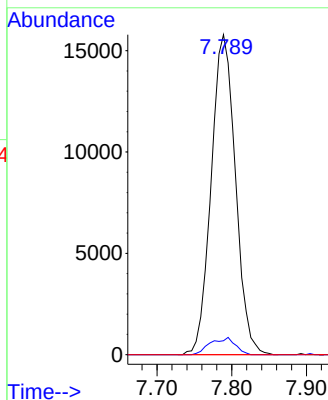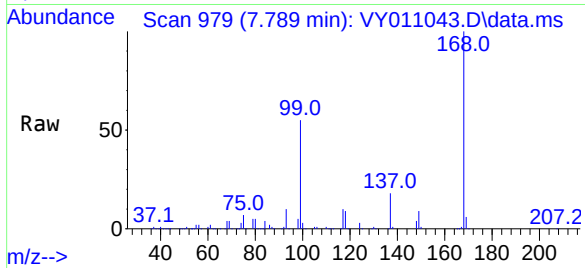

#39
Methylcyclohexane
Concen: 3.954 ug/l
RT: 9.185 min Scan# 1208
Delta R.T. 0.006 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion: 83 Resp: 26737
Ion Ratio Lower Upper
83 100
55 71.7 66.5 99.7
98 48.3 37.9 56.9


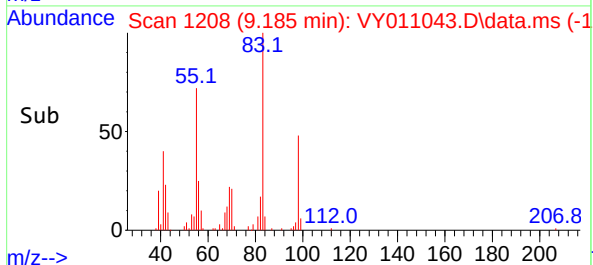
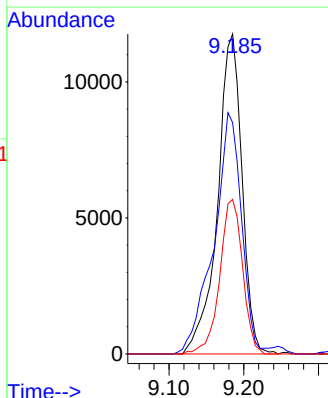
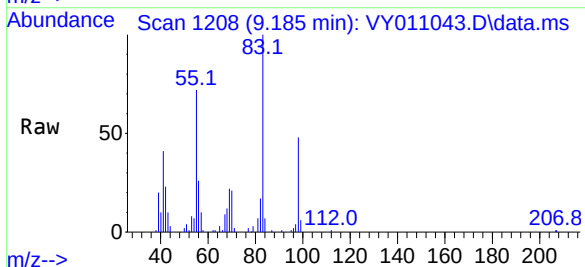




#50
Toluene-d8
Concen: 62.598 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion: 98 Resp: 792655
Ion Ratio Lower Upper
98 100
100 64.1 50.2 75.2

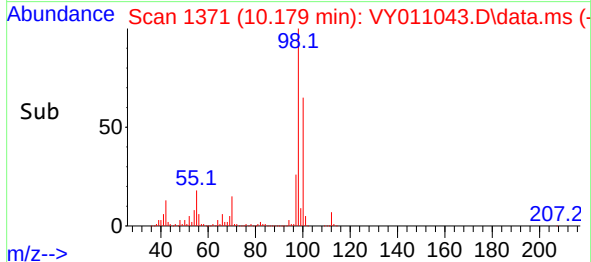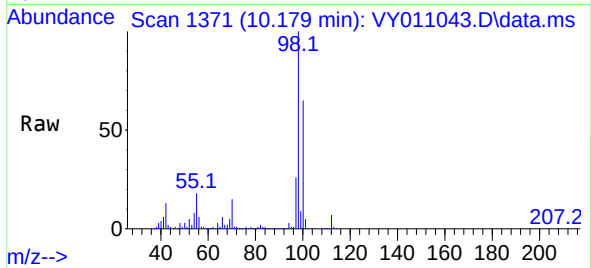

#51
4-Methyl-2-Pentanone
Concen: 6.370 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.110 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion: 43 Resp: 19840
Ion Ratio Lower Upper
43 100
58 32.2 28.1 42.1


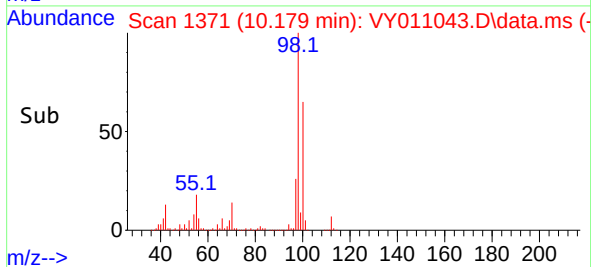

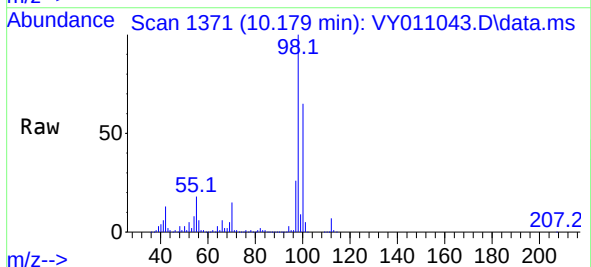




#55
1,1,2-Trichloroethane
Concen: 22.036 ug/l
RT: 10.618 min Scan# 1443
Delta R.T. -0.024 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion:	97	Resp:	74520
Ion	Ratio	Lower	Upper
97	100		
83	8.4	69.8	104.8#
85	1.4	44.3	66.5#
99	0.3	49.8	74.6#

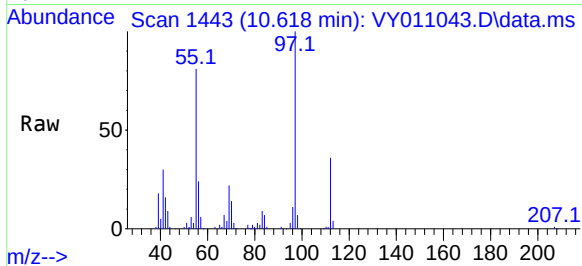

#56
Ethyl methacrylate
Concen: 8.092 ug/l
RT: 10.520 min Scan# 1427
Delta R.T. 0.012 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion:	69	Resp:	36345
Ion	Ratio	Lower	Upper
69	100		
41	159.9	63.4	95.0#
39	78.6	35.8	53.8#


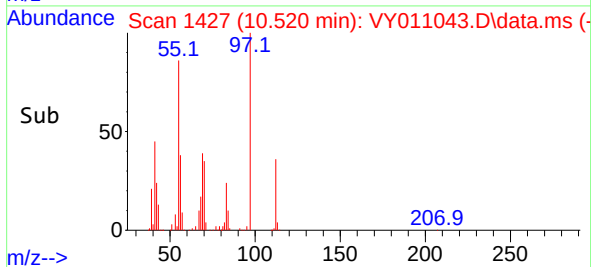

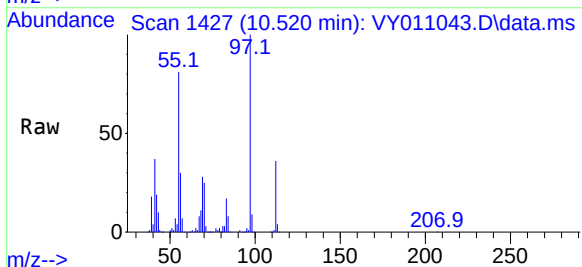


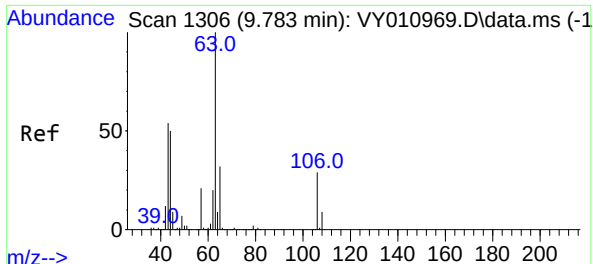

#58
2-Chloroethyl Vinyl ether
Concen: 17.084 ug/l
RT: 9.782 min Scan# 11
Delta R.T. -0.001 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion: 63 Resp: 295
Ion Ratio Lower Upper
63 100
106 0.0 21.5 32.3#

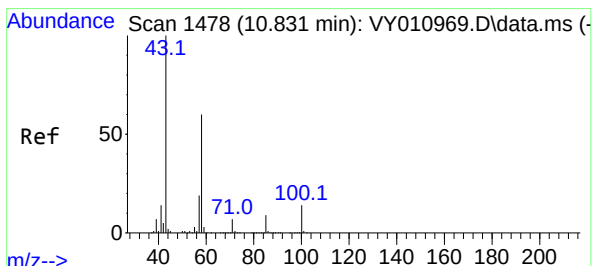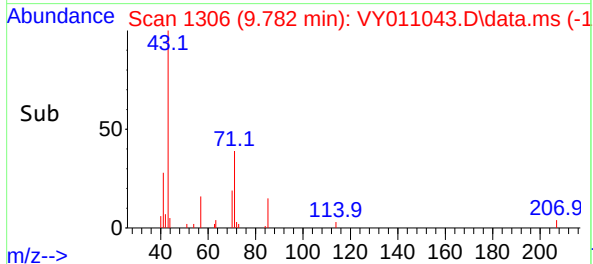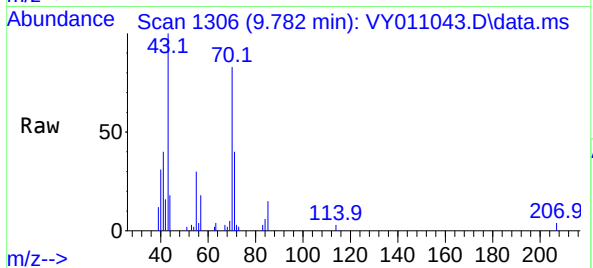

#59
2-Hexanone
Concen: 13.001 ug/l
RT: 10.801 min Scan# 1473
Delta R.T. -0.030 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion: 43 Resp: 27813
Ion Ratio Lower Upper
43 100
58 4.8 24.4 73.4#


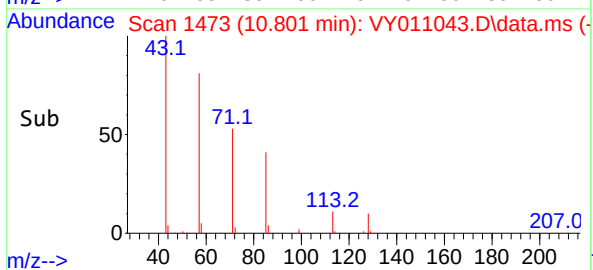

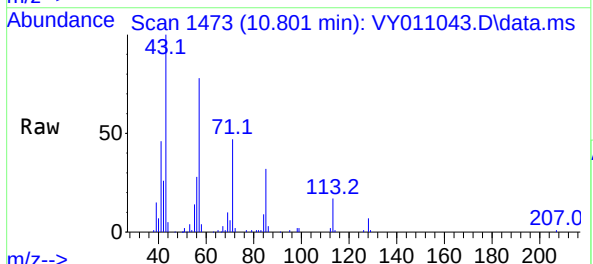




#62
4-Bromofluorobenzene
Concen: 60.584 ug/l
RT: 12.477 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion: 95 Resp: 268834
Ion Ratio Lower Upper
95 100
174 77.6 0.0 177.0
176 75.8 0.0 175.8

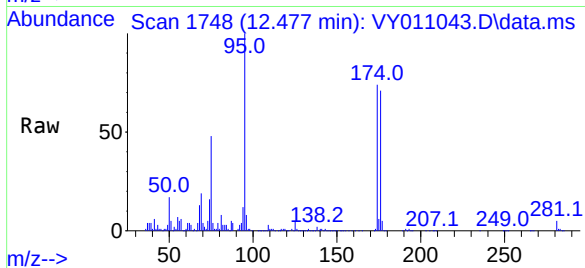

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.001 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion: 117 Resp: 507991
Ion Ratio Lower Upper
117 100
82 55.4 43.0 64.4
119 32.2 25.4 38.0


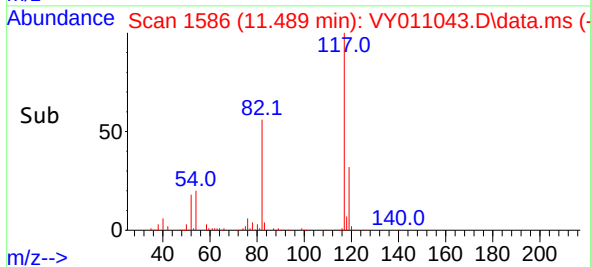

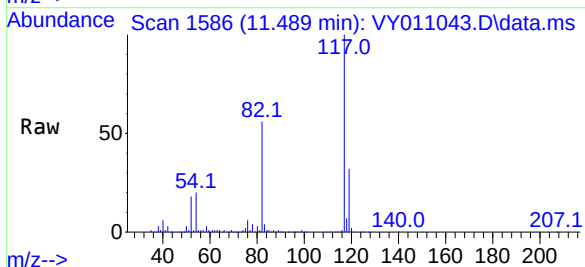




#67
Ethyl Benzene
Concen: 1.125 ug/l
RT: 11.593 min Scan# 1603
Delta R.T. 0.000 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion: 91 Resp: 20762
Ion Ratio Lower Upper
91 100
106 28.2 24.5 36.7

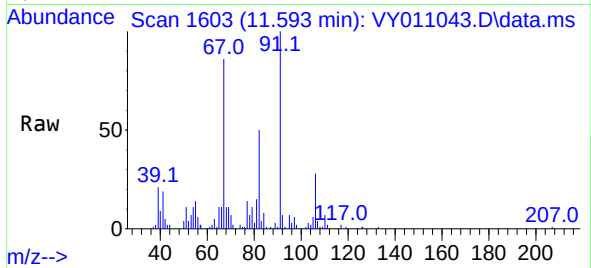

#68
m/p-Xylenes
Concen: 3.032 ug/l
RT: 11.697 min Scan# 1620
Delta R.T. -0.006 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion: 106 Resp: 21518
Ion Ratio Lower Upper
106 100
91 211.5 166.6 249.8


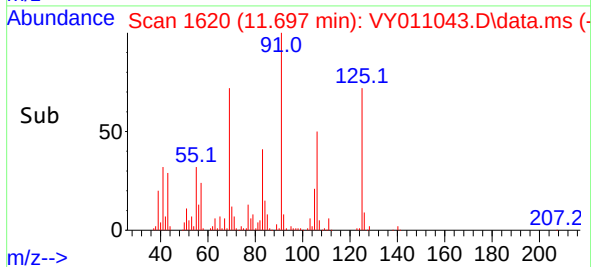

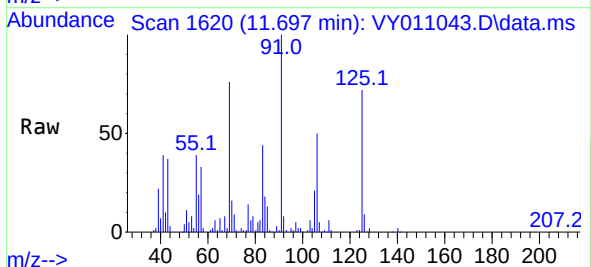




#69
o-Xylene
Concen: 4.001 ug/l
RT: 12.026 min Scan# 1
Delta R.T. -0.000 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion:106 Resp: 26966
Ion Ratio Lower Upper
106 100
91 225.7 110.3 331.0

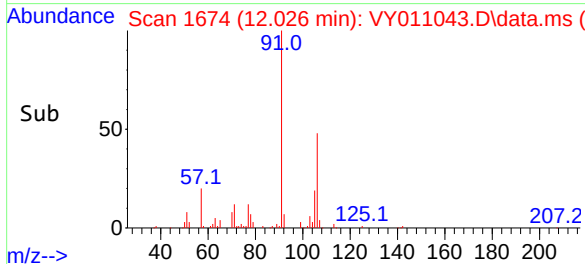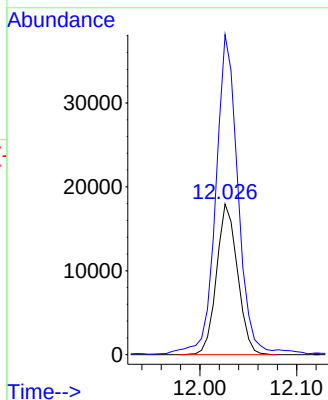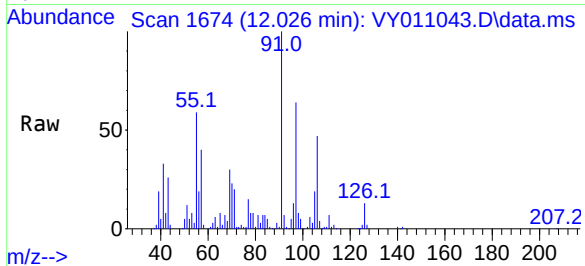

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion:152 Resp: 213993
Ion Ratio Lower Upper
152 100
115 58.4 28.2 84.7
150 152.5 0.0 347.6


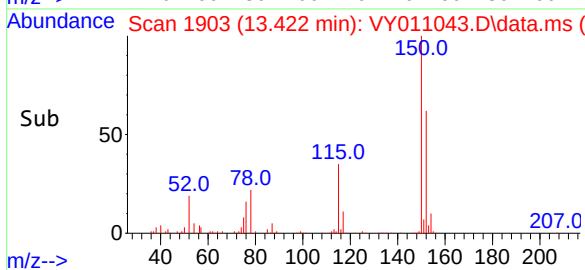
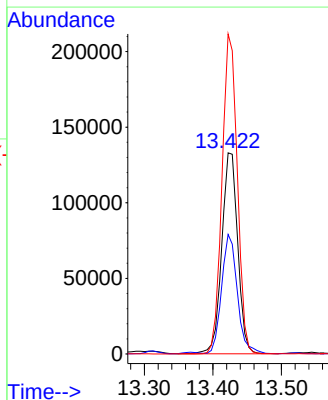
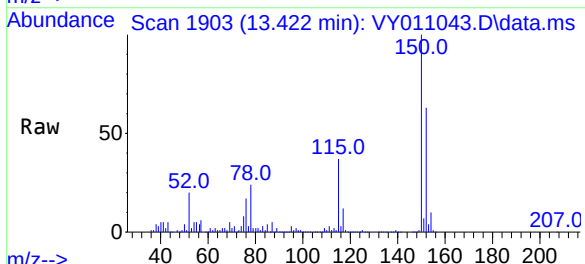




#73
Isopropylbenzene
Concen: 1.467 ug/l
RT: 12.331 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion:105 Resp: 22812
Ion Ratio Lower Upper
105 100
120 24.4 13.4 40.2

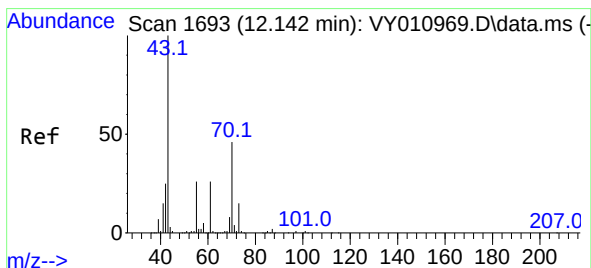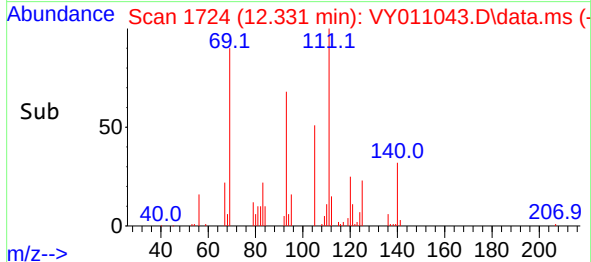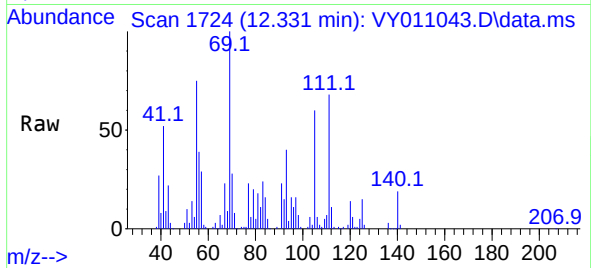

#74
N-ethyl acetate
Concen: 13.859 ug/l
RT: 12.124 min Scan# 1690
Delta R.T. -0.018 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion: 43 Resp: 54669
Ion Ratio Lower Upper
43 100
70 0.0 28.7 43.1#
55 0.0 17.3 25.9#
61 0.0 17.0 25.6#


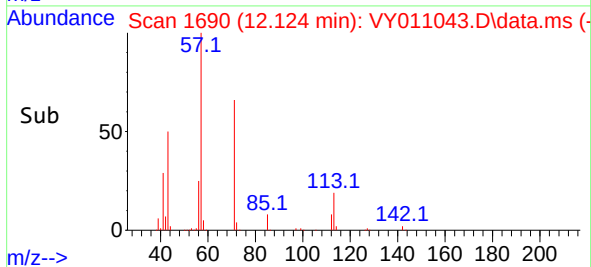

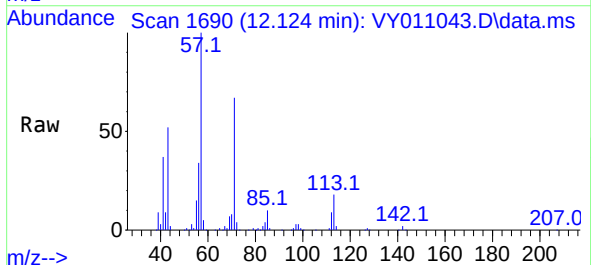




#75
1,1,2-Tetrachloroethane
Concen: 4.523 ug/l
RT: 12.556 min Scan# 1761
Delta R.T. -0.025 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion: 83 Resp: 14758
Ion Ratio Lower Upper
83 100
131 0.0 5.6 16.8#
85 37.7 32.3 96.8

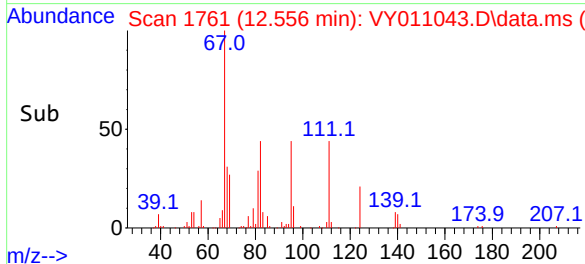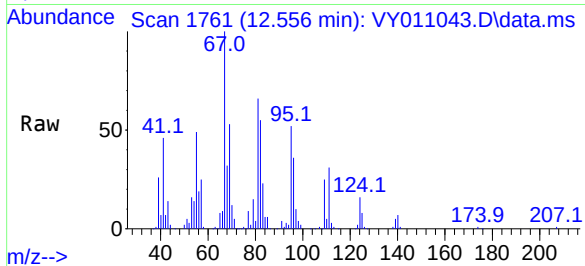

#76
1,2,3-Trichloropropane
Concen: 52.130 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.153 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion: 75 Resp: 126649
Ion Ratio Lower Upper
75 100
77 2.5 0.0 0.0#


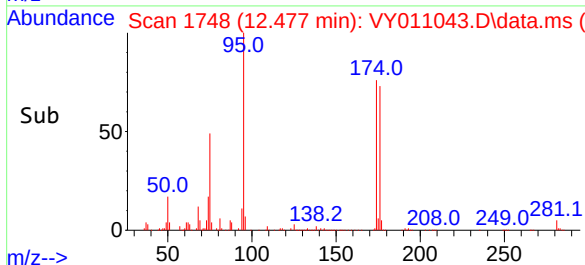
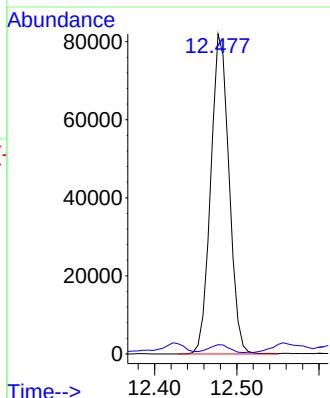
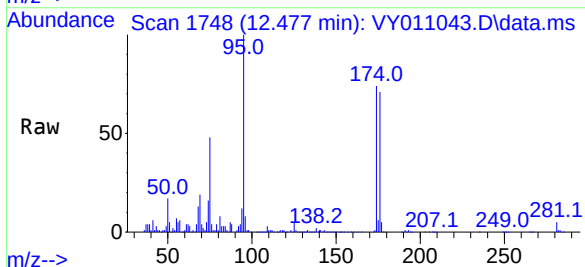




#78
n-propylbenzene
Concen: 1.237 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. 0.000 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion: 91 Resp: 23394
Ion Ratio Lower Upper
91 100
120 19.1 11.3 33.9

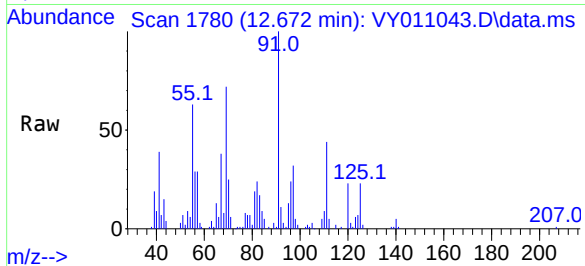

#80
1,3,5-Trimethylbenzene
Concen: 6.348 ug/l
RT: 12.812 min Scan# 1803
Delta R.T. 0.000 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion: 105 Resp: 82341
Ion Ratio Lower Upper
105 100
120 48.8 24.4 73.4


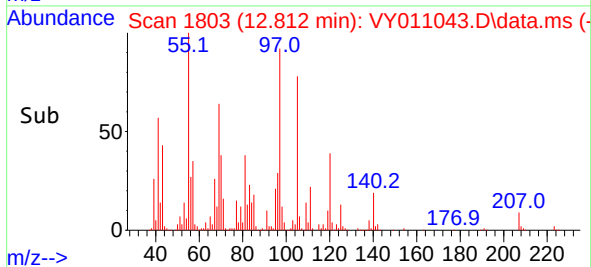

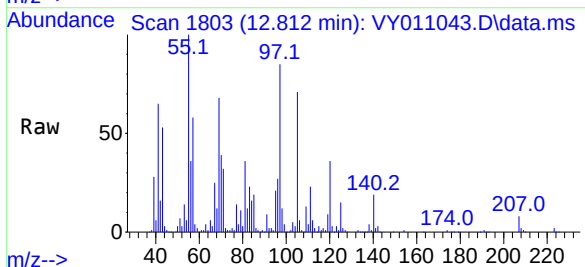




#81
trans-1,4-Dichloro-2-butene
Concen: 112.116 ug/l
RT: 12.477 min Scan# 11
Delta R.T. 0.097 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29




Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0


Tgt Ion: 75 Resp: 126649
Ion Ratio Lower Upper
75 100
53 2.5 85.3 127.9#
89 0.0 37.0 55.4#

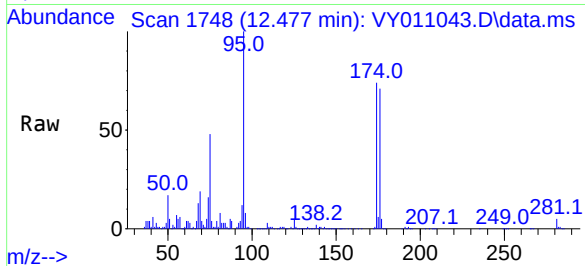

#84
1,2,4-Trimethylbenzene
Concen: 11.300 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion:105 Resp: 144537
Ion Ratio Lower Upper
105 100
120 46.3 22.3 66.9


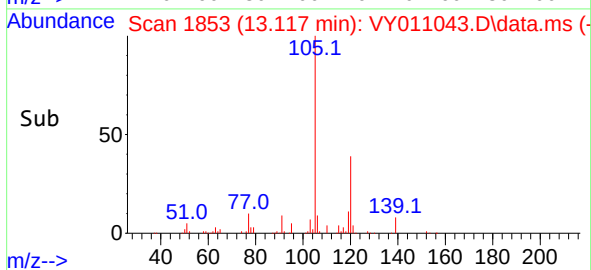

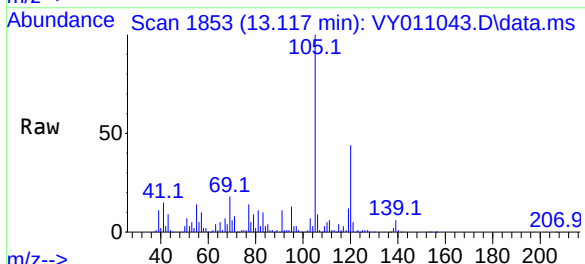




#85
 sec-Butylbenzene
 Concen: 1.947 ug/l
 RT: 13.251 min Scan# 1875
 Delta R.T. 0.000 min
 Lab File: VY011043.D
 Acq: 21 Oct 2022 12:29




Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-B1-3.5-4.0


Tgt Ion:105 Resp: 32820
 Ion Ratio Lower Upper
 105 100
 134 29.7 10.2 30.4

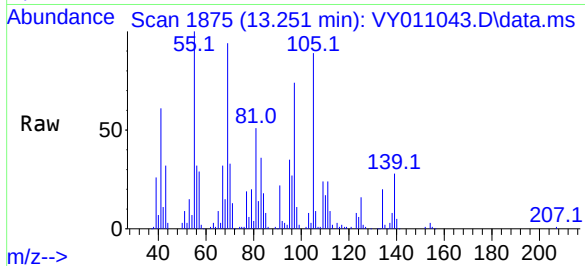

#86
 p-Isopropyltoluene
 Concen: 1.573 ug/l
 RT: 13.367 min Scan# 1894
 Delta R.T. 0.000 min
 Lab File: VY011043.D
 Acq: 21 Oct 2022 12:29

Tgt Ion:119 Resp: 22001
 Ion Ratio Lower Upper
 119 100
 134 25.7 13.2 39.5
 91 20.3 12.4 37.2


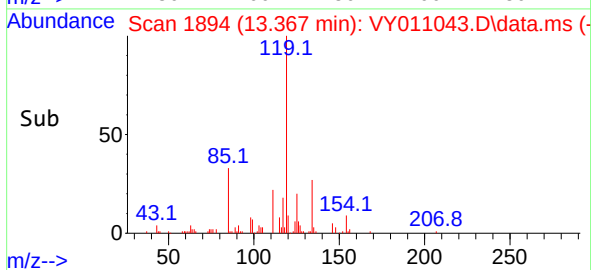

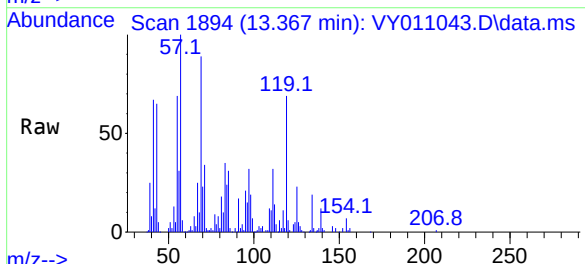




#90
Hexachloroethane
Concen: 1.200 ug/l
RT: 13.971 min Scan# 1993
Delta R.T. 0.012 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Instrument :
MSVOA_Y
ClientSampleId :
SB-B1-3.5-4.0

Tgt Ion:117 Resp: 3312
Ion Ratio Lower Upper
117 100
201 2.0 43.0 128.8#

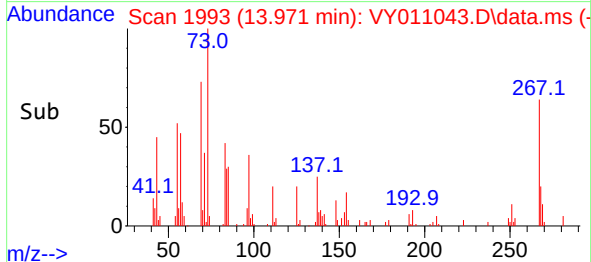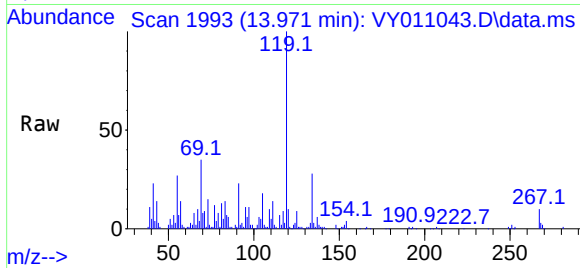

#95
Naphthalene
Concen: 56.514 ug/l
RT: 15.233 min Scan# 2200
Delta R.T. -0.000 min
Lab File: VY011043.D
Acq: 21 Oct 2022 12:29

Tgt Ion:128 Resp: 446350
Ion Ratio Lower Upper
128 100
127 12.9 11.0 16.4
129 10.9 8.4 12.6

