

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY102819\
 Data File : VY000458.D
 Acq On : 28 Oct 2019 16:34
 Operator : SY/MD
 Sample : K5576-06
 Misc : 4.19G/5ML/MSVOA Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 CSA-2-1-6-2

Quant Time: Oct 29 10:33:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y101119S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 17 02:03:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	192065	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.70	114	326598	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	272337	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	99274	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.15	65	111817	55.19	ug/l	0.00
Spiked Amount			Recovery	=	110.38%	
35) Dibromofluoromethane	7.74	113	98294	49.89	ug/l	0.00
Spiked Amount			Recovery	=	99.78%	
50) Toluene-d8	10.18	98	378366	49.93	ug/l	0.00
Spiked Amount			Recovery	=	99.86%	
62) 4-Bromofluorobenzene	12.48	95	108043	37.53	ug/l	0.00
Spiked Amount			Recovery	=	75.06%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY102819\
Data File : VY000458.D
Acq On : 28 Oct 2019 16:34
Operator : SY/MD
Sample : K5576-06
Misc : 4.19G/5ML/MSVOA Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
CSA-2-1-6-2

Quant Time: Oct 29 10:33:04 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y101119S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 17 02:03:07 2019
Response via : Initial Calibration

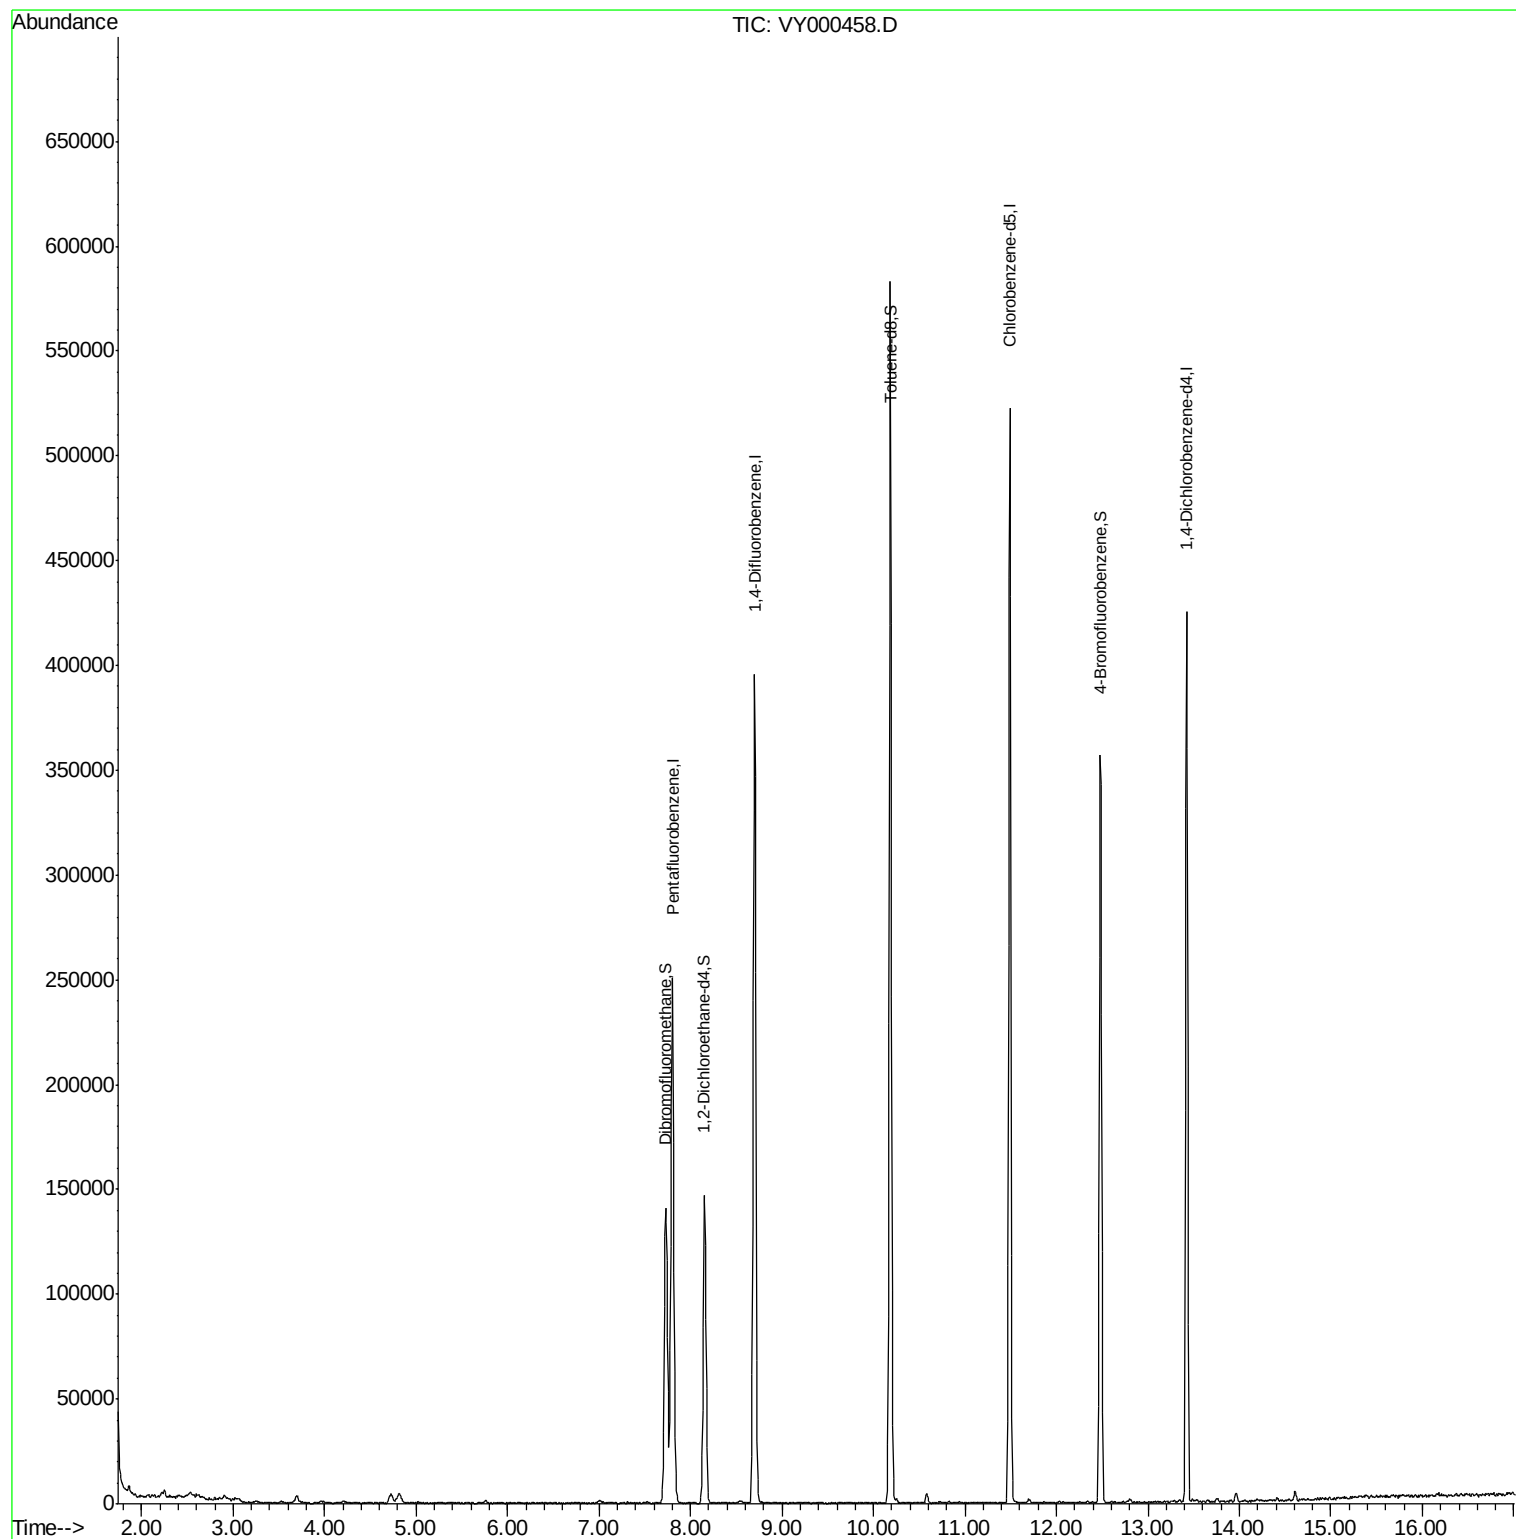

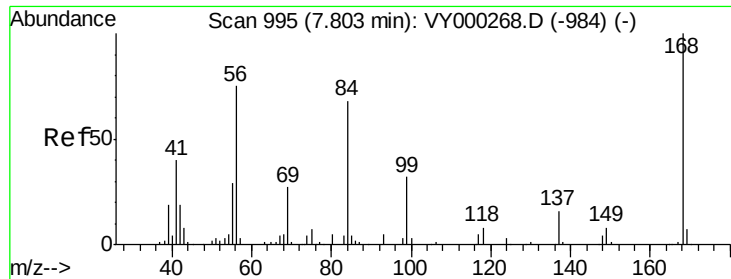

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 995

Delta R.T. -0.00 min

Lab File: VY000458.D

Acq: 28 Oct 2019 16:34

Instrument :

MSVOA_Y

ClientSampleId :


CSA-2-1-6-2

Tot Ion:168 Resp: 192065

Ion Ratio Lower Upper

168 100

99 55.3 46.6 69.8

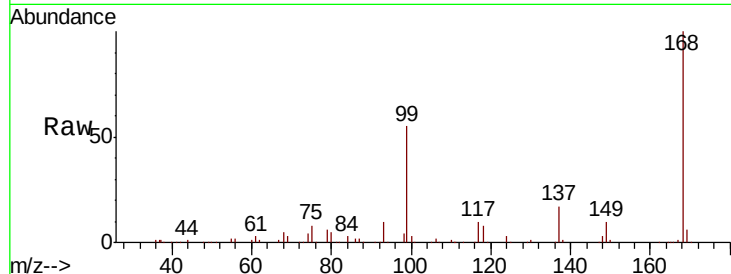

Abundance Ion 167.90 (167.60 to 168.60): VY000458.D (-946) (-)

Ion 98.90 (98.60 to 99.60): VY000458.D (-946) (-)

7.80

80000

60000



40000

20000

0

7.70 7.80 7.90

Time-->

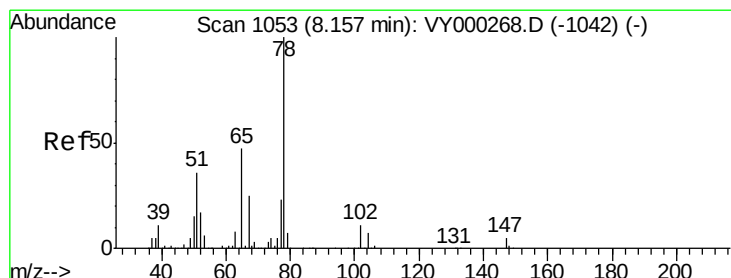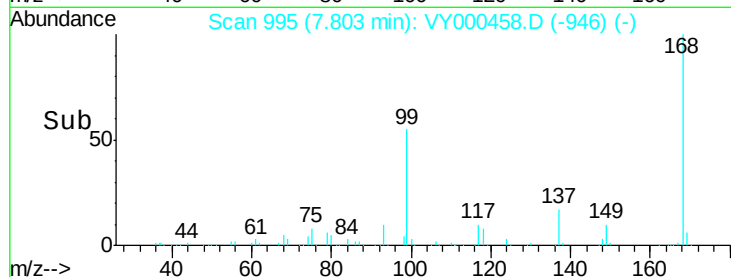

#33

1,2-Dichloroethane-d4

Concen: 55.191 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. -0.01 min

Lab File: VY000458.D


Acq: 28 Oct 2019 16:34

Tgt Ion: 65 Resp: 111817

Ion Ratio Lower Upper

65 100

67 53.1 0.0 109.4

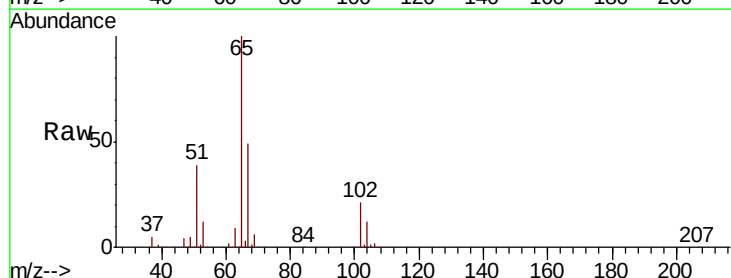

Abundance Ion 64.90 (64.60 to 65.60): VY000458.D (-1004) (-)

Ion 66.90 (66.60 to 67.60): VY000458.D (-1004) (-)

8.15

60000

50000

40000

30000


20000


10000

0

8.10 8.20

Time-->

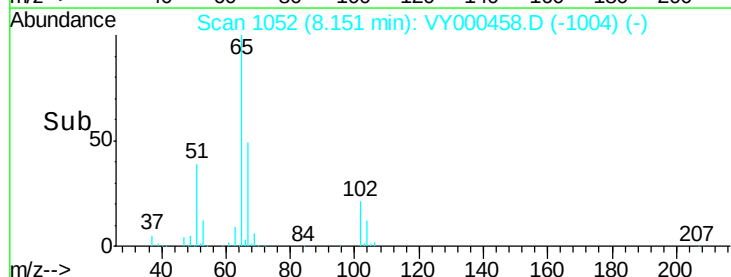


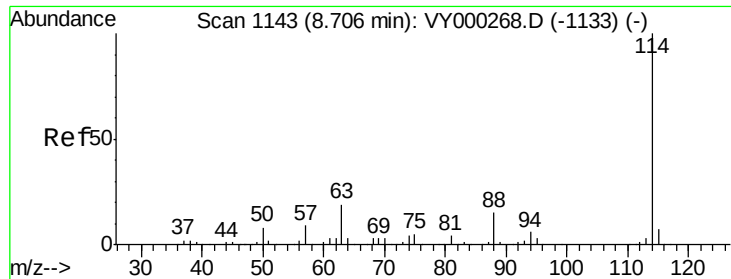




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.70 min Scan# 1142
Delta R.T. -0.01 min
Lab File: VY000458.D
Acq: 28 Oct 2019 16:34

Instrument :
MSVOA_Y
ClientSampleId :
CSA-2-1-6-2

Tot Ion:114 Resp: 326598
Ion Ratio Lower Upper
114 100
63 20.0 0.0 37.2
88 14.2 0.0 30.2

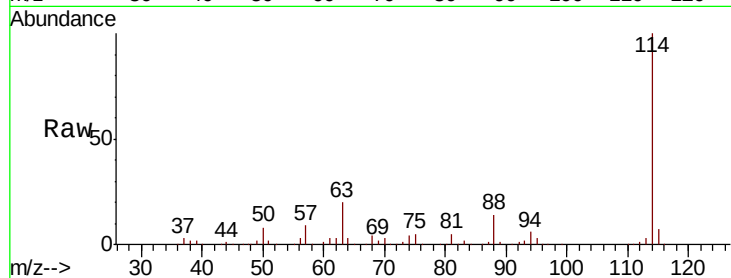


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VY0
Ion 87.90 (87.60 to 88.60): VY0

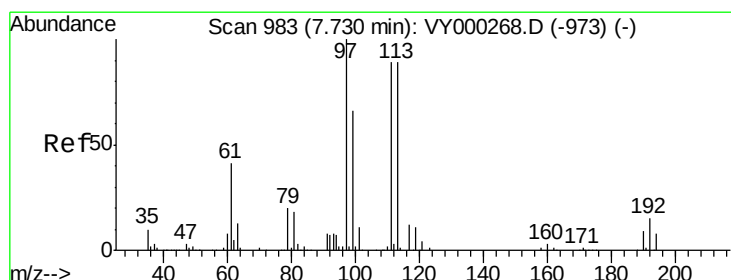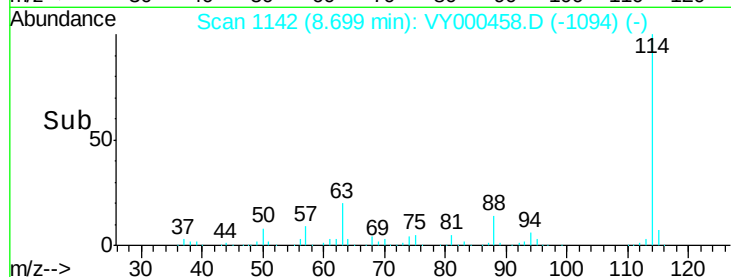
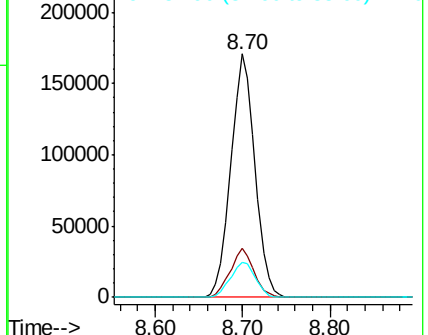



#35
Dibromofluoromethane
Concen: 49.894 ug/l
RT: 7.74 min Scan# 984
Delta R.T. 0.01 min
Lab File: VY000458.D
Acq: 28 Oct 2019 16:34

Tgt Ion:113 Resp: 98294
Ion Ratio Lower Upper
113 100
111 102.6 81.6 122.4
192 19.2 15.3 22.9

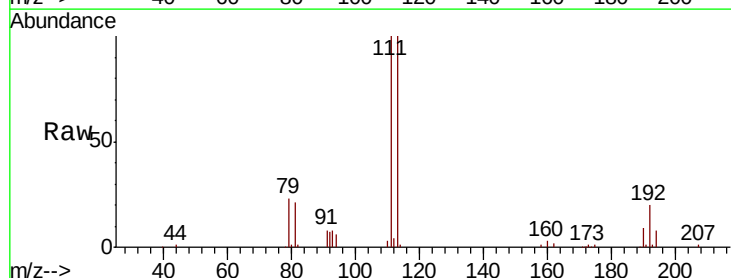

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

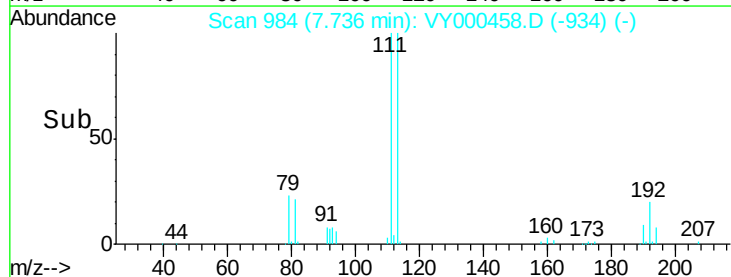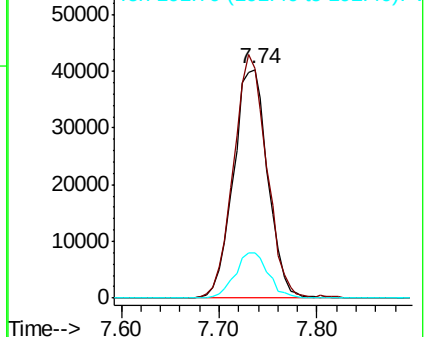

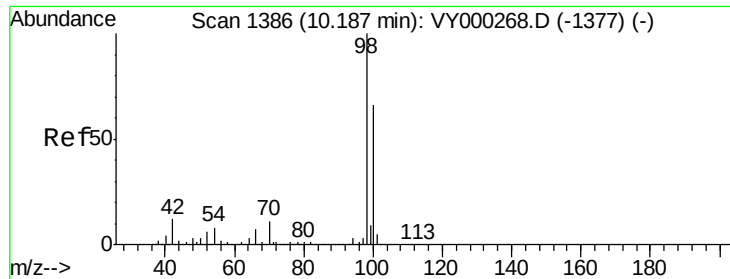

#50

Toluene-d8

Concen: 49.927 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. -0.01 min

Lab File: VY000458.D

Acq: 28 Oct 2019 16:34

Instrument :

MSVOA_Y

ClientSampleId :





CSA-2-1-6-2

Tot Ion: 98 Resp: 378366

Ion Ratio Lower Upper

98 100

100 65.0 52.8 79.2

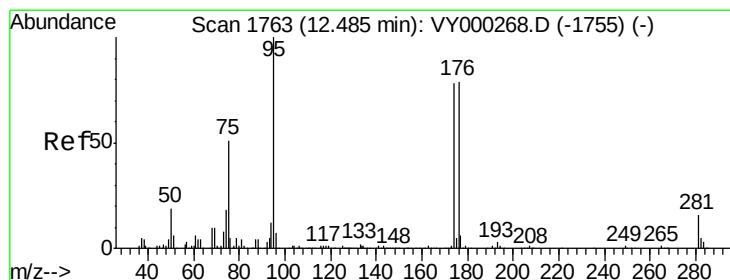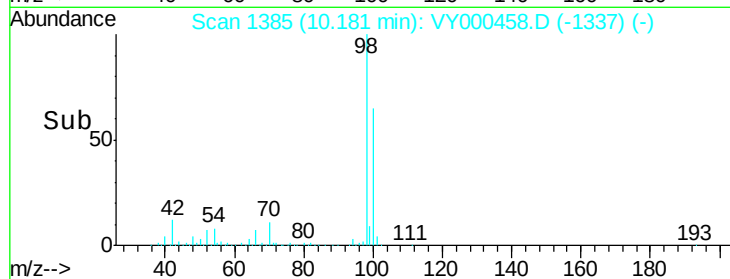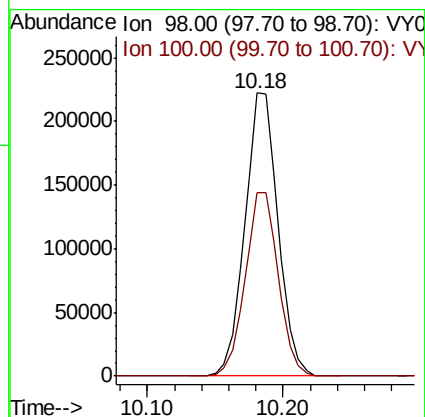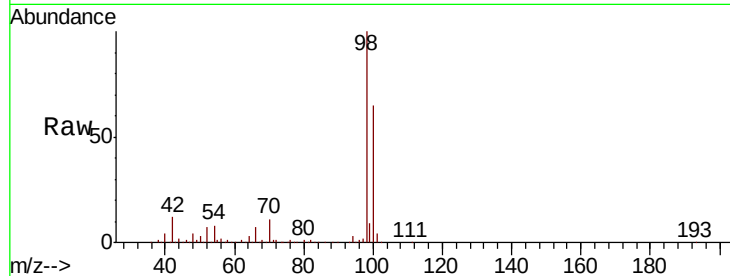

#62

4-Bromofluorobenzene

Concen: 37.527 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.01 min

Lab File: VY000458.D

Acq: 28 Oct 2019 16:34




Tgt Ion: 95 Resp: 108043


Ion Ratio Lower Upper

95 100

174 83.4 0.0 159.6

176 77.9 0.0 153.8


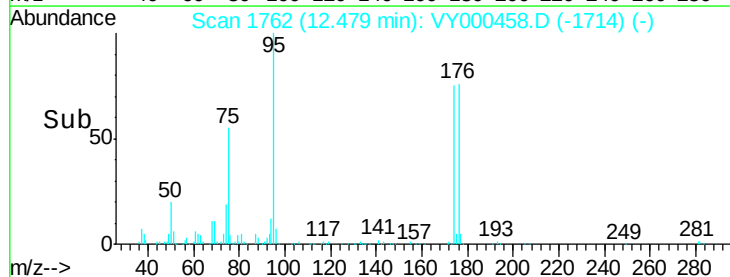
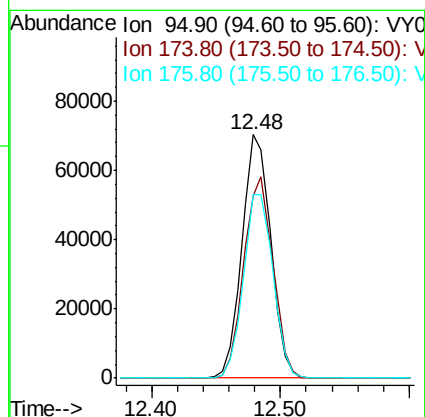
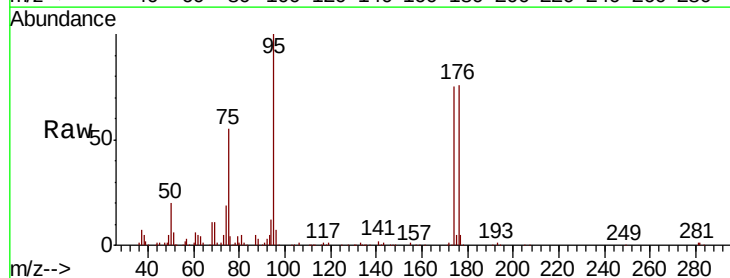


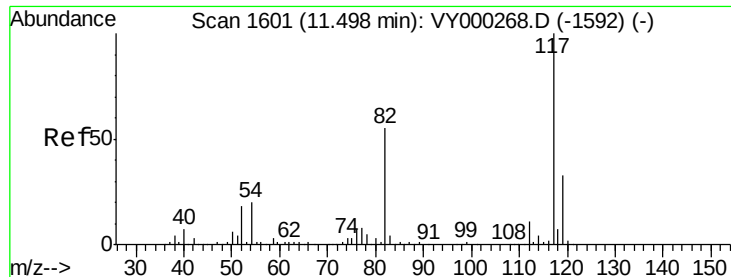

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. -0.01 min
Lab File: VY000458.D
Acq: 28 Oct 2019 16:34

Instrument :
MSVOA_Y
ClientSampleId :
CSA-2-1-6-2

Tot Ion:117 Resp: 272337
Ion Ratio Lower Upper
117 100
82 54.1 43.7 65.5
119 32.5 26.6 39.8

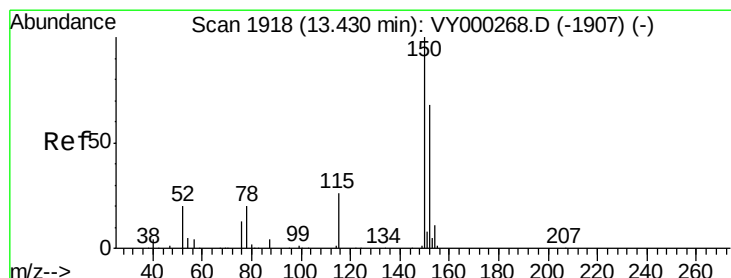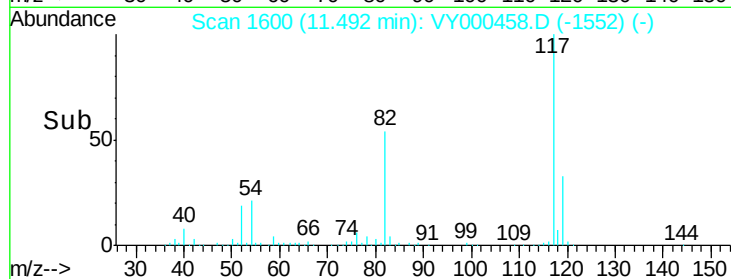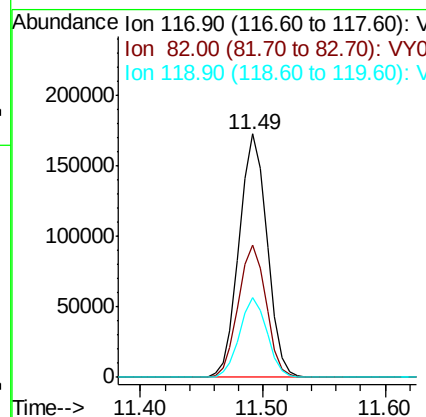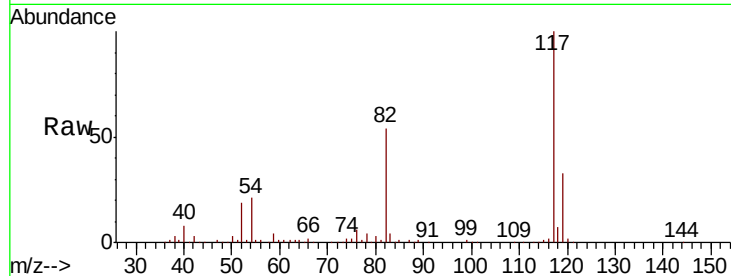

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. -0.01 min
Lab File: VY000458.D
Acq: 28 Oct 2019 16:34

Tgt Ion:152 Resp: 99274
Ion Ratio Lower Upper
152 100
115 58.1 29.3 88.0
150 157.3 0.0 348.4

