

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY103019\
 Data File : VY000486.D
 Acq On : 30 Oct 2019 11:46
 Operator : SY/MD
 Sample : VSTDICCC050
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050

Quant Time: Oct 30 13:14:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 30 13:10:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	235849	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.70	114	393846	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	351650	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	180128	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	132608	54.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.66%	
35) Dibromofluoromethane	7.73	113	119252	51.58	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.16%	
50) Toluene-d8	10.18	98	486211	55.42	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.84%	
62) 4-Bromofluorobenzene	12.48	95	173211	51.86	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.72%	

Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.90	85	121045	52.137	ug/l	100
3) Chloromethane	2.11	50	160758	50.264	ug/l	100
4) Vinyl Chloride	2.25	62	150339	50.620	ug/l	100
5) Bromomethane	2.65	94	85083	47.773	ug/l	100
6) Chloroethane	2.79	64	92015	49.503	ug/l	100
7) Trichlorofluoromethane	3.13	101	199041	49.625	ug/l	100
8) Diethyl Ether	3.54	74	71445	50.131	ug/l	100
9) 1,1,2-Trichlorotrifluoroet	3.90	101	118835	49.007	ug/l	100
10) Methyl Iodide	4.10	142	152870	53.449	ug/l	100
11) Tert butyl alcohol	4.97	59	54474	229.277	ug/l	100
12) 1,1-Dichloroethene	3.88	96	122792	52.122	ug/l	100
13) Acrolein	3.73	56	51142	247.118	ug/l	100
14) Allyl chloride	4.49	41	193830	50.598	ug/l	100
15) Acrylonitrile	5.18	53	180698	247.509	ug/l	100
16) Acetone	3.95	43	183753	273.160	ug/l	100
17) Carbon Disulfide	4.19	76	372580	50.142	ug/l	100
18) Methyl Acetate	4.48	43	97869	46.791	ug/l	100
19) Methyl tert-butyl Ether	5.22	73	326426	49.834	ug/l	100
20) Methylene Chloride	4.72	84	132363	45.921	ug/l	100
21) trans-1,2-Dichloroethene	5.22	96	133941	50.290	ug/l	100
22) Diisopropyl ether	6.13	45	418465	50.258	ug/l	100
23) Vinyl Acetate	6.07	43	1328359	252.729	ug/l	100
24) 1,1-Dichloroethane	6.03	63	223726	49.598	ug/l	100
25) 2-Butanone	7.00	43	276528	257.577	ug/l	100
26) 2,2-Dichloropropane	6.99	77	199669	48.437	ug/l	100
27) cis-1,2-Dichloroethene	7.00	96	145948	50.114	ug/l	100
28) Bromochloromethane	7.35	49	110556	60.681	ug/l	100
29) Tetrahydrofuran	7.36	42	162664	247.672	ug/l	100
30) Chloroform	7.52	83	226775	49.697	ug/l	100
31) Cyclohexane	7.79	56	229783	48.637	ug/l	100
32) 1,1,1-Trichloroethane	7.71	97	203517	50.044	ug/l	100
36) 1,1-Dichloropropene	7.93	75	182216	48.940	ug/l	100
37) Ethyl Acetate	7.09	43	105072	47.533	ug/l	100
38) Carbon Tetrachloride	7.91	117	179414	50.079	ug/l	100

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY103019\
 Data File : VY000486.D
 Acq On : 30 Oct 2019 11:46
 Operator : SY/MD
 Sample : VSTDICCC050
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050

Quant Time: Oct 30 13:14:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 30 13:10:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
39) Methylcyclohexane	9.19	83	243567	50.636	ug/l	100
40) Benzene	8.17	78	540512	49.517	ug/l	100
41) Methacrylonitrile	7.36	41	145906	118.362	ug/l #	58
42) 1,2-Dichloroethane	8.25	62	154855	50.018	ug/l	100
43) Isopropyl Acetate	8.28	43	202563	48.782	ug/l	100
44) Trichloroethene	8.94	130	140927	48.966	ug/l	100
45) 1,2-Dichloropropane	9.22	63	133136	49.557	ug/l	100
46) Dibromomethane	9.31	93	73327	49.629	ug/l	100
47) Bromodichloromethane	9.50	83	178537	50.926	ug/l	100
48) Methyl methacrylate	9.30	41	88676	48.876	ug/l	100
49) 1,4-Dioxane	9.31	88	20112	1011.421	ug/l	100
51) 4-Methyl-2-Pentanone	10.08	43	552496	250.254	ug/l	100
52) Toluene	10.25	92	343583	49.786	ug/l	100
53) t-1,3-Dichloropropene	10.47	75	194313	51.873	ug/l	100
54) cis-1,3-Dichloropropene	9.93	75	217516	50.687	ug/l	100
55) 1,1,2-Trichloroethane	10.64	97	106269	49.728	ug/l	100
56) Ethyl methacrylate	10.51	69	157852	52.116	ug/l	100
57) 1,3-Dichloropropane	10.79	76	188277	50.338	ug/l	100
58) 2-Chloroethyl Vinyl ether	9.79	63	357888	261.361	ug/l	100
59) 2-Hexanone	10.83	43	419447	260.761	ug/l	100
60) Dibromochloromethane	10.99	129	124511	50.867	ug/l	100
61) 1,2-Dibromoethane	11.09	107	104883	51.044	ug/l	100
64) Tetrachloroethene	10.72	164	145269	49.960	ug/l	100
65) Chlorobenzene	11.52	112	354761	49.759	ug/l	100
66) 1,1,1,2-Tetrachloroethane	11.59	131	127398	51.523	ug/l	100
67) Ethyl Benzene	11.59	91	671001	51.137	ug/l	100
68) m/p-Xylenes	11.70	106	525346	103.443	ug/l	100
69) o-Xylene	12.03	106	239644	50.208	ug/l	100
70) Styrene	12.04	104	422935	51.747	ug/l	100
71) Bromoform	12.20	173	74550	52.419	ug/l #	100
73) Isopropylbenzene	12.33	105	657764	49.408	ug/l	100
74) N-amyl acetate	12.14	43	193147	50.658	ug/l	100
75) 1,1,2,2-Tetrachloroethane	12.58	83	128257	48.657	ug/l	100
76) 1,2,3-Trichloropropane	12.63	75	176200	52.895	ug/l #	100
77) Bromobenzene	12.61	156	147496	48.857	ug/l	100
78) n-propylbenzene	12.67	91	800882	49.859	ug/l	100
79) 2-Chlorotoluene	12.75	91	438155	49.134	ug/l	100
80) 1,3,5-Trimethylbenzene	12.81	105	555804	50.128	ug/l	100
81) trans-1,4-Dichloro-2-buten	12.38	75	46647	50.994	ug/l	100
82) 4-Chlorotoluene	12.85	91	461212	49.895	ug/l	100
83) tert-Butylbenzene	13.07	119	474186	50.088	ug/l	100
84) 1,2,4-Trimethylbenzene	13.12	105	563077	51.006	ug/l	100
85) sec-Butylbenzene	13.25	105	687953	51.006	ug/l	100
86) p-Isopropyltoluene	13.37	119	608478	50.618	ug/l	100
87) 1,3-Dichlorobenzene	13.36	146	293020	49.554	ug/l	100
88) 1,4-Dichlorobenzene	13.44	146	294382	49.820	ug/l	100
89) n-Butylbenzene	13.69	91	602363	50.805	ug/l	100
90) Hexachloroethane	13.96	117	113379	51.018	ug/l	100
91) 1,2-Dichlorobenzene	13.74	146	268230	49.995	ug/l	100
92) 1,2-Dibromo-3-Chloropropan	14.36	75	22605	48.456	ug/l	100

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY103019\
Data File : VY000486.D
Acq On : 30 Oct 2019 11:46
Operator : SY/MD
Sample : VSTDICCC050
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050

Quant Time: Oct 30 13:14:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 30 13:10:11 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
93) 1,2,4-Trichlorobenzene	15.00	180	176036	48.188	ug/l	100
94) Hexachlorobutadiene	15.11	225	94955	50.425	ug/l	100
95) Naphthalene	15.23	128	398957	49.196	ug/l	100
96) 1,2,3-Trichlorobenzene	15.42	180	163343	49.839	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY103019\
 Data File : VY000486.D
 Acq On : 30 Oct 2019 11:46
 Operator : SY/MD
 Sample : VSTDICCC050
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050

Quant Time: Oct 30 13:14:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 30 13:10:11 2019
 Response via : Initial Calibration





#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 995

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :


VSTDICCC050

Tgt Ion:168 Resp: 235849

Ion Ratio Lower Upper

168 100

99 57.1 45.7 68.5



Abundance Ion 167.90 (167.60 to 168.60): VY000486.D (-985) (-)

Ion 98.90 (98.60 to 99.60): VY000486.D (-985) (-)

7.80

120000

100000

80000



60000

40000

20000

0

Time-->



#2

Dichlorodifluoromethane

Concen: 52.137 ug/l

RT: 1.90 min Scan# 27

Delta R.T. 0.00 min

Lab File: VY000486.D


Acq: 30 Oct 2019 11:46

Tgt Ion: 85 Resp: 121045

Ion Ratio Lower Upper

85 100

87 31.8 15.9 47.7



Abundance Ion 84.90 (84.60 to 85.60): VY000486.D (-20) (-)

Ion 86.90 (86.60 to 87.60): VY000486.D (-20) (-)

1.90

80000


60000


40000

20000

0

Time-->





#3

Chloromethane

Concen: 50.264 ug/l

RT: 2.11 min Scan# 61

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampled :





VSTDICCC050

Tgt Ion: 50 Resp: 160758

Ion Ratio Lower Upper

50 100

52 31.5 25.2 37.8



#4

Vinyl Chloride

Concen: 50.620 ug/l

RT: 2.25 min Scan# 84

Delta R.T. 0.00 min

Lab File: VY000486.D




Acq: 30 Oct 2019 11:46


Tgt Ion: 62 Resp: 150339

Ion Ratio Lower Upper

62 100

64 31.5 25.2 37.8





#5

Bromomethane

Concen: 47.773 ug/l

RT: 2.65 min Scan# 149

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :





VSTDICCC050

Tgt Ion: 94 Resp: 85083

Ion Ratio Lower Upper

94 100

96 89.0 71.2 106.8



#6

Chloroethane

Concen: 49.503 ug/l

RT: 2.79 min Scan# 173

Delta R.T. 0.00 min

Lab File: VY000486.D




Acq: 30 Oct 2019 11:46


Tgt Ion: 64 Resp: 92015

Ion Ratio Lower Upper

64 100

66 33.3 26.6 40.0









#7

Trichlorofluoromethane
 Concen: 49.625 ug/l
 RT: 3.13 min Scan# 228
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050




Tgt Ion: 101 Resp: 199041
 Ion Ratio Lower Upper
 101 100
 103 63.1 50.5 75.7




#8

Diethyl Ether
 Concen: 50.131 ug/l
 RT: 3.54 min Scan# 295
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Tgt Ion: 74 Resp: 71445
 Ion Ratio Lower Upper
 74 100
 45 90.9 45.5 136.4





#9

1,1,2-Trichlorotrifluoroethane

Concen: 49.007 ug/l

RT: 3.90 min Scan# 355

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050


Tgt Ion:101 Resp: 118835

Ion Ratio Lower Upper

101 100

85 45.9 36.7 55.1




151 80.4 64.3 96.5



Abundance Ion 100.90 (100.60 to 101.60): V

Ion 84.90 (84.60 to 85.60): VY0

Ion 150.80 (150.50 to 151.50): V



#10

Methyl Iodide

Concen: 53.449 ug/l

RT: 4.10 min Scan# 387

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46


Tgt Ion:142 Resp: 152870

Ion Ratio Lower Upper

142 100

127 42.1 33.7 50.5



141 13.6 10.9 16.3




Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V









#11

Tert butyl alcohol
 Concen: 229.277 ug/l
 RT: 4.97 min Scan# 530
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050




Tgt Ion: 59 Resp: 54474
 Ion Ratio Lower Upper
 59 100
 57 10.7 8.6 12.8




#12

1,1-Dichloroethene
 Concen: 52.122 ug/l
 RT: 3.88 min Scan# 351
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Tgt Ion: 96 Resp: 122792
 Ion Ratio Lower Upper
 96 100
 61 149.0 119.2 178.8
 98 60.8 48.6 73.0





#13

Acrolein

Concen: 247.118 ug/l

RT: 3.73 min Scan# 327

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :





VSTDICCC050

Tgt Ion: 56 Resp: 51142

Ion Ratio Lower Upper

56 100

55 71.3 57.0 85.6



#14

Allyl chloride

Concen: 50.598 ug/l

RT: 4.49 min Scan# 451

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46




Tgt Ion: 41 Resp: 193830


Ion Ratio Lower Upper

41 100

39 67.0 53.6 80.4

76 37.2 29.8 44.6





#15

Acrylonitrile

Concen: 247.509 ug/l

RT: 5.18 min Scan# 564

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050


Tgt Ion: 53 Resp: 180698

Ion Ratio Lower Upper

53 100

52 81.1 64.9 97.3




51 34.5 27.6 41.4



Abundance Ion 53.00 (52.70 to 53.70): VY0

Ion 52.00 (51.70 to 52.70): VY0

Ion 51.00 (50.70 to 51.70): VY0



#16

Acetone

Concen: 273.160 ug/l

RT: 3.95 min Scan# 363

Delta R.T. 0.00 min

Lab File: VY000486.D


Acq: 30 Oct 2019 11:46

Tgt Ion: 43 Resp: 183753

Ion Ratio Lower Upper



43 100


58 32.2 25.8 38.6



Abundance Ion 43.00 (42.70 to 43.70): VY0

Ion 58.00 (57.70 to 58.70): VY0









#17
Carbon Disulfide
Concen: 50.142 ug/l
RT: 4.19 min Scan# 403
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46




Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050


Tgt Ion: 76 Resp: 372580
Ion Ratio Lower Upper
76 100
78 9.4 7.5 11.3



#18
Methyl Acetate
Concen: 46.791 ug/l
RT: 4.48 min Scan# 450
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion: 43 Resp: 97869
Ion Ratio Lower Upper
43 100
74 24.0 19.2 28.8









#19

Methyl tert-butyl Ether
 Concen: 49.834 ug/l
 RT: 5.22 min Scan# 572
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050




Tgt Ion: 73 Resp: 326426
 Ion Ratio Lower Upper
 73 100
 57 21.7 17.4 26.0




#20

Methylene Chloride
 Concen: 45.921 ug/l
 RT: 4.72 min Scan# 489
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Tgt Ion: 84 Resp: 132363
 Ion Ratio Lower Upper
 84 100
 49 125.3 100.2 150.4
 51 37.0 29.6 44.4
 86 60.4 48.3 72.5





#21

trans-1,2-Dichloroethene

Concen: 50.290 ug/l

RT: 5.22 min Scan# 572

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050


Tgt Ion: 96 Resp: 133941

Ion Ratio Lower Upper




96 100

61 133.3 106.6 160.0

98 63.3 50.6 76.0



Abundance Ion 95.90 (95.60 to 96.60): VY0
Ion 60.90 (60.60 to 61.60): VY0
Ion 97.90 (97.60 to 98.60): VY0



#22

Diisopropyl ether

Concen: 50.258 ug/l

RT: 6.13 min Scan# 720

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Tgt Ion: 45 Resp: 418465


Ion Ratio Lower Upper

45 100



43 62.5 50.0 75.0


87 27.0 21.6 32.4

59 11.9 9.5 14.3



Abundance Ion 45.00 (44.70 to 45.70): VY0
Ion 43.00 (42.70 to 43.70): VY0
Ion 87.00 (86.70 to 87.70): VY0
Ion 59.00 (58.70 to 59.70): VY0









#23
 Vinyl Acetate
 Concen: 252.729 ug/l
 RT: 6.07 min Scan# 711
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46




Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050


Tgt Ion: 43 Resp: 1328359
 Ion Ratio Lower Upper
 43 100
 86 9.7 7.8 11.6



#24
 1,1-Dichloroethane
 Concen: 49.598 ug/l
 RT: 6.03 min Scan# 704
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Tgt Ion: 63 Resp: 223726
 Ion Ratio Lower Upper
 63 100
 98 7.1 3.5 10.6
 100 4.7 2.4 7.1









#25
2-Butanone
Concen: 257.577 ug/l
RT: 7.00 min Scan# 863
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46




Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050


Tgt Ion: 43 Resp: 276528
Ion Ratio Lower Upper
43 100
72 26.1 20.9 31.3



#26
2,2-Dichloropropane
Concen: 48.437 ug/l
RT: 6.99 min Scan# 862
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion: 77 Resp: 199669
Ion Ratio Lower Upper
77 100
97 23.6 11.8 35.4









#27

cis-1,2-Dichloroethene
Concen: 50.114 ug/l
RT: 7.00 min Scan# 863
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050




Tgt Ion: 96 Resp: 145948
Ion Ratio Lower Upper
96 100
61 143.5 0.0 287.0
98 64.7 0.0 129.4




#28

Bromochloromethane
Concen: 60.681 ug/l
RT: 7.35 min Scan# 920
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion: 49 Resp: 110556
Ion Ratio Lower Upper
49 100
129 1.8 0.0 3.6
130 74.2 59.4 89.0









#29
Tetrahydrofuran
Concen: 247.672 ug/l
RT: 7.36 min Scan# 922
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050

Tgt Ion: 42 Resp: 162664
Ion Ratio Lower Upper
42 100
72 42.5 34.0 51.0
71 38.5 30.8 46.2




Abundance Ion 42.00 (41.70 to 42.70): VY0
Ion 72.00 (71.70 to 72.70): VY0
Ion 71.00 (70.70 to 71.70): VY0






#30
Chloroform
Concen: 49.697 ug/l
RT: 7.52 min Scan# 948
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion: 83 Resp: 226775
Ion Ratio Lower Upper
83 100
85 66.2 53.0 79.4



Abundance Ion 82.90 (82.60 to 83.60): VY0
Ion 84.90 (84.60 to 85.60): VY0









#31
Cyclohexane
Concen: 48.637 ug/l
RT: 7.79 min Scan# 993
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050

Tgt Ion: 56 Resp: 229783
Ion Ratio Lower Upper
56 100
69 31.3 25.0 37.6
84 89.3 71.4 107.2




Abundance Ion 56.00 (55.70 to 56.70): VY0
Ion 69.00 (68.70 to 69.70): VY0
Ion 84.00 (83.70 to 84.70): VY0






#32
1,1,1-Trichloroethane
Concen: 50.044 ug/l
RT: 7.71 min Scan# 980
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion: 97 Resp: 203517
Ion Ratio Lower Upper
97 100
99 63.6 50.9 76.3
61 43.6 34.9 52.3



Abundance Ion 96.90 (96.60 to 97.60): VY0
Ion 98.90 (98.60 to 99.60): VY0
Ion 60.90 (60.60 to 61.60): VY0





#33

1,2-Dichloroethane-d4

Concen: 54.331 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :


VSTDICCC050

Tgt Ion: 65 Resp: 132608

Ion Ratio Lower Upper




65 100

67 53.6 0.0 107.2



Abundance Ion 64.90 (64.60 to 65.60): VY0

Ion 66.90 (66.60 to 67.60): VY0



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.70 min Scan# 1142

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46


Tgt Ion: 114 Resp: 393846

Ion Ratio Lower Upper

114 100

63 19.0 0.0 38.0



88 14.3 0.0 28.6




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0









#35
 Dibromofluoromethane
 Concen: 51.577 ug/l
 RT: 7.73 min Scan# 983
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46




Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050


Tgt Ion: 113 Resp: 119252
 Ion Ratio Lower Upper
 113 100
 111 102.1 81.7 122.5
 192 18.7 15.0 22.4



#36
 1,1-Dichloropropene
 Concen: 48.940 ug/l
 RT: 7.93 min Scan# 1015
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Tgt Ion: 75 Resp: 182216
 Ion Ratio Lower Upper
 75 100
 110 36.1 18.1 54.1
 77 31.3 25.0 37.6









#37
Ethyl Acetate
Concen: 47.533 ug/l
RT: 7.09 min Scan# 878
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46




Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050


Tgt Ion: 43 Resp: 105072
Ion Ratio Lower Upper
43 100
61 12.7 10.2 15.2
70 9.8 7.8 11.8



#38
Carbon Tetrachloride
Concen: 50.079 ug/l
RT: 7.91 min Scan# 1013
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion: 117 Resp: 179414
Ion Ratio Lower Upper
117 100
119 97.5 78.0 117.0
121 33.3 26.6 40.0









#39
Methylcyclohexane
Concen: 50.636 ug/l
RT: 9.19 min Scan# 1222
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050

Tgt Ion: 83 Resp: 243567
Ion Ratio Lower Upper
83 100
55 71.9 57.5 86.3
98 47.5 38.0 57.0




Abundance Ion 83.00 (82.70 to 83.70): VY0
Ion 55.00 (54.70 to 55.70): VY0
Ion 98.00 (97.70 to 98.70): VY0






#40
Benzene
Concen: 49.517 ug/l
RT: 8.17 min Scan# 1055
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion: 78 Resp: 540512
Ion Ratio Lower Upper
78 100
77 23.3 18.6 28.0



Abundance Ion 78.00 (77.70 to 78.70): VY0
Ion 77.00 (76.70 to 77.70): VY0





#41

Methacrylonitrile

Concen: 118.362 ug/l

RT: 7.36 min Scan# 922

Delta R.T. 0.01 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050

Tgt Ion: 41 Resp: 145906


Ion Ratio Lower Upper

41 100

39 46.7 68.2 102.4#

67 0.0 0.0 0.0

52 0.0 0.0 0.0






Abundance Ion 41.00 (40.70 to 41.70): VY0

Ion 39.00 (38.70 to 39.70): VY0

Ion 67.00 (66.70 to 67.70): VY0

Ion 52.00 (51.70 to 52.70): VY0



#42

1,2-Dichloroethane

Concen: 50.018 ug/l

RT: 8.25 min Scan# 1068

Delta R.T. 0.00 min

Lab File: VY000486.D


Acq: 30 Oct 2019 11:46

Tgt Ion: 62 Resp: 154855

Ion Ratio Lower Upper



62 100


98 9.6 0.0 19.2



Abundance Ion 61.90 (61.60 to 62.60): VY0

Ion 97.90 (97.60 to 98.60): VY0





#43

Isopropyl Acetate

Concen: 48.782 ug/l

RT: 8.28 min Scan# 1074

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050


Tgt Ion: 43 Resp: 202563

Ion Ratio Lower Upper

43 100

61 28.7 23.0 34.4

87 13.1 10.5 15.7



Abundance Ion 43.00 (42.70 to 43.70): VY000486.D (-1062) (-)

Ion 61.00 (60.70 to 61.70): VY000486.D (-1062) (-)

Ion 87.00 (86.70 to 87.70): VY000486.D (-1062) (-)

8.28



100000

50000

0

8.20 8.30 8.40

Time-->



#44

Trichloroethene

Concen: 48.966 ug/l

RT: 8.94 min Scan# 1182

Delta R.T. 0.00 min

Lab File: VY000486.D


Acq: 30 Oct 2019 11:46

Tgt Ion: 130 Resp: 140927

Ion Ratio Lower Upper

130 100

95 101.6 0.0 203.2



Abundance Ion 129.80 (129.50 to 130.50): VY000486.D (-1173) (-)

Ion 94.90 (94.60 to 95.60): VY000486.D (-1173) (-)

8.94

80000

60000


40000


20000

0

8.85 8.90 8.95 9.00 9.05

Time-->









#45
 1,2-Dichloropropane
 Concen: 49.557 ug/l
 RT: 9.22 min Scan# 1228
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46




Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050


Tgt Ion: 63 Resp: 133136
 Ion Ratio Lower Upper
 63 100
 65 33.7 27.0 40.4



#46
 Dibromomethane
 Concen: 49.629 ug/l
 RT: 9.31 min Scan# 1242
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Tgt Ion: 93 Resp: 73327
 Ion Ratio Lower Upper
 93 100
 95 83.0 66.4 99.6
 174 96.4 77.1 115.7









#47
Bromodichloromethane
Concen: 50.926 ug/l
RT: 9.50 min Scan# 1274
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46




Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050


Tgt Ion: 83 Resp: 178537
Ion Ratio Lower Upper
83 100
85 64.8 51.8 77.8
127 8.4 6.7 10.1



#48
Methyl methacrylate
Concen: 48.876 ug/l
RT: 9.30 min Scan# 1240
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion: 41 Resp: 88676
Ion Ratio Lower Upper
41 100
69 90.6 72.5 108.7
39 59.8 47.8 71.8





#49

1,4-Dioxane

Concen: 1011.421 ug/l

RT: 9.31 min Scan# 1242

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050


Tgt Ion: 88 Resp: 20112

Ion Ratio Lower Upper




88 100

43 31.4 25.1 37.7

58 63.2 50.6 75.8



Abundance Ion 88.00 (87.70 to 88.70): VY0
Ion 43.00 (42.70 to 43.70): VY0
Ion 58.00 (57.70 to 58.70): VY0



#50

Toluene-d8

Concen: 55.419 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. 0.00 min

Lab File: VY000486.D


Acq: 30 Oct 2019 11:46

Tgt Ion: 98 Resp: 486211



Ion Ratio Lower Upper


98 100

100 66.1 52.9 79.3



Abundance Ion 98.00 (97.70 to 98.70): VY0
Ion 100.00 (99.70 to 100.70): VY0





#51

4-Methyl-2-Pentanone

Concen: 250.254 ug/l

RT: 10.08 min Scan# 1368

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :


VSTDICCC050

Tgt Ion: 43 Resp: 552496

Ion Ratio Lower Upper




43 100

58 37.8 30.2 45.4



Abundance Ion 43.00 (42.70 to 43.70): VY000486.D (-1359) (-)

Ion 58.00 (57.70 to 58.70): VY000486.D (-1359) (-)



#52

Toluene

Concen: 49.786 ug/l

RT: 10.25 min Scan# 1396

Delta R.T. 0.00 min

Lab File: VY000486.D


Acq: 30 Oct 2019 11:46

Tgt Ion: 92 Resp: 343583

Ion Ratio Lower Upper



92 100


91 170.4 136.3 204.5



Abundance Ion 92.00 (91.70 to 92.70): VY000486.D (-1387) (-)

Ion 91.00 (90.70 to 91.70): VY000486.D (-1387) (-)









#53
t-1,3-Dichloropropene
Concen: 51.873 ug/l
RT: 10.47 min Scan# 1432
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46




Instrument :
MSVOA_Y
ClientSampled :
VSTDICCC050


Tgt Ion: 75 Resp: 194313
Ion Ratio Lower Upper
75 100
77 30.8 24.6 37.0



#54
cis-1,3-Dichloropropene
Concen: 50.687 ug/l
RT: 9.93 min Scan# 1344
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion: 75 Resp: 217516
Ion Ratio Lower Upper
75 100
77 30.6 24.5 36.7
39 44.3 35.4 53.2









#55
 1,1,2-Trichloroethane
 Concen: 49.728 ug/l
 RT: 10.64 min Scan# 1461
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050

Tgt Ion: 97 Resp: 106269




Ion	Ratio	Lower	Upper
97	100		
83	87.8	70.2	105.4
85	58.6	46.9	70.3
99	65.7	52.6	78.8




#56
 Ethyl methacrylate
 Concen: 52.116 ug/l
 RT: 10.51 min Scan# 1439
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Tgt Ion: 69 Resp: 157852

Ion	Ratio	Lower	Upper
69	100		
41	66.6	53.3	79.9
39	35.0	28.0	42.0





#57

1,3-Dichloropropane

Concen: 50.338 ug/l

RT: 10.79 min Scan# 1485

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :





VSTDICCC050

Tgt Ion: 76 Resp: 188277

Ion Ratio Lower Upper

76 100

78 31.5 25.2 37.8



#58

2-Chloroethyl Vinyl ether

Concen: 261.361 ug/l

RT: 9.79 min Scan# 1321

Delta R.T. 0.00 min

Lab File: VY000486.D




Acq: 30 Oct 2019 11:46


Tgt Ion: 63 Resp: 357888

Ion Ratio Lower Upper

63 100

106 28.2 22.6 33.8









#59
2-Hexanone
Concen: 260.761 ug/l
RT: 10.83 min Scan# 1492
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46




Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050


Tgt Ion: 43 Resp: 419447
Ion Ratio Lower Upper
43 100
58 54.2 27.1 81.3



#60
Dibromochloromethane
Concen: 50.867 ug/l
RT: 10.99 min Scan# 1517
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion: 129 Resp: 124511
Ion Ratio Lower Upper
129 100
127 78.1 39.1 117.2





#61

1,2-Dibromoethane

Concen: 51.044 ug/l

RT: 11.09 min Scan# 1534

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :


VSTDICCC050

Tgt Ion: 107 Resp: 104883

Ion Ratio Lower Upper




107 100

109 92.0 73.6 110.4



Abundance Ion 106.90 (106.60 to 107.60): V

Ion 108.80 (108.50 to 109.50): V



#62

4-Bromofluorobenzene

Concen: 51.860 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46


Tgt Ion: 95 Resp: 173211

Ion Ratio Lower Upper

95 100

174 80.8 0.0 161.6



176 78.9 0.0 157.8




Abundance Ion 94.90 (94.60 to 95.60): VY0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V




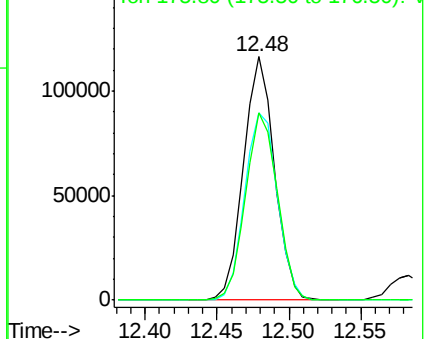




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46




Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050


Tgt Ion:117 Resp: 351650
Ion Ratio Lower Upper
117 100
82 51.0 40.8 61.2
119 32.7 26.2 39.2

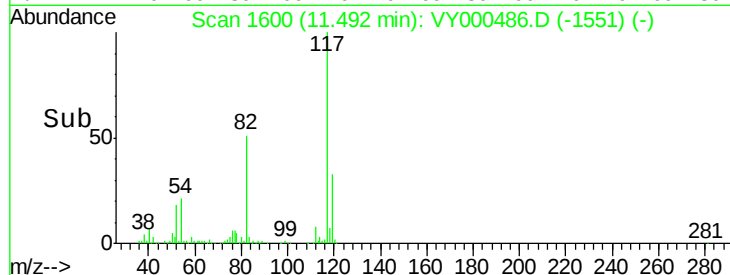

#64
Tetrachloroethene
Concen: 49.960 ug/l
RT: 10.72 min Scan# 1473
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion:164 Resp: 145269
Ion Ratio Lower Upper
164 100
166 128.4 102.7 154.1
129 91.5 73.2 109.8
131 92.7 74.2 111.2



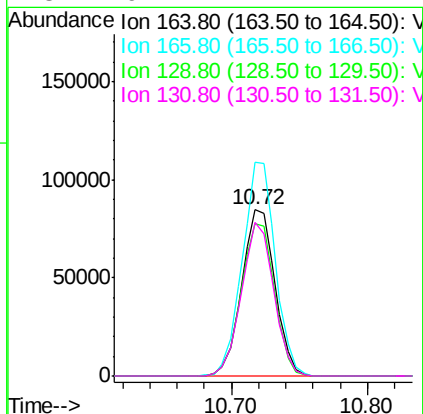





#65
Chlorobenzene
Concen: 49.759 ug/l
RT: 11.52 min Scan# 1604
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46




Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050


Tgt Ion:112 Resp: 354761
Ion Ratio Lower Upper
112 100
114 31.6 25.3 37.9

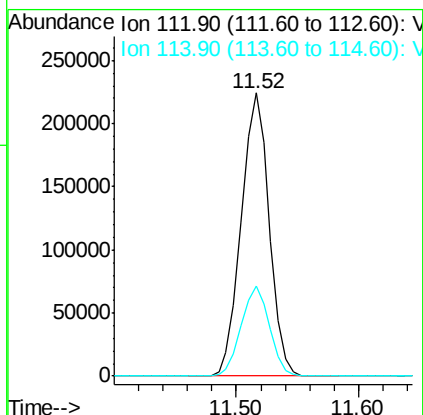

#66
1,1,1,2-Tetrachloroethane
Concen: 51.523 ug/l
RT: 11.59 min Scan# 1616
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion:131 Resp: 127398
Ion Ratio Lower Upper
131 100
133 95.9 47.9 143.8
119 66.2 33.1 99.3


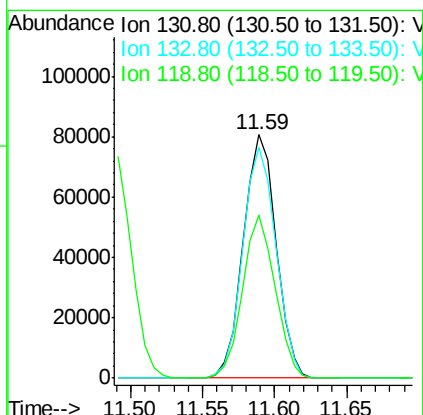






#67
Ethyl Benzene
Concen: 51.137 ug/l
RT: 11.59 min Scan# 1616
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46




Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050


Tgt Ion: 91 Resp: 671001
Ion Ratio Lower Upper
91 100
106 31.7 25.4 38.0

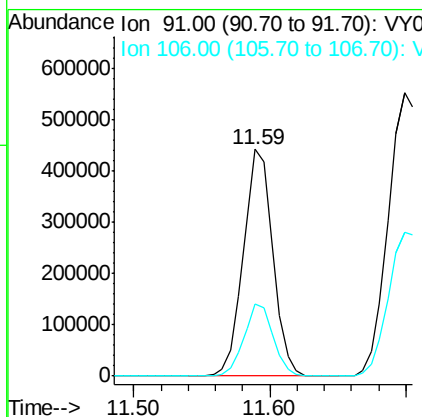

#68
m/p-Xylenes
Concen: 103.443 ug/l
RT: 11.70 min Scan# 1634
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion: 106 Resp: 525346
Ion Ratio Lower Upper
106 100
91 194.9 155.9 233.9



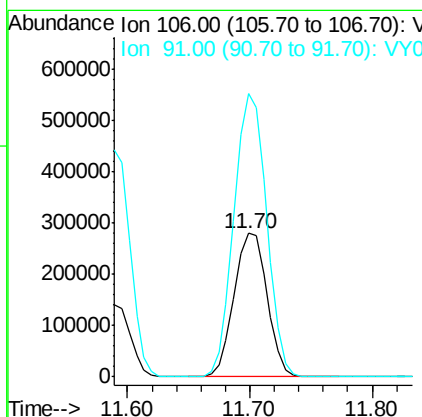





#69
o-Xylene
Concen: 50.208 ug/l
RT: 12.03 min Scan# 1688
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46




Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050


Tgt Ion:106 Resp: 239644
Ion Ratio Lower Upper
106 100
91 213.1 106.5 319.6



#70
Styrene
Concen: 51.747 ug/l
RT: 12.04 min Scan# 1690
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion:104 Resp: 422935
Ion Ratio Lower Upper
104 100
78 48.7 39.0 58.4
103 53.1 42.5 63.7





#71

Bromoform

Concen: 52.419 ug/l

RT: 12.20 min Scan# 1717

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050


Tgt Ion:173 Resp: 74550

Ion Ratio Lower Upper

173 100

175 48.8 24.4 73.2




254 0.1 0.1 0.1#



Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

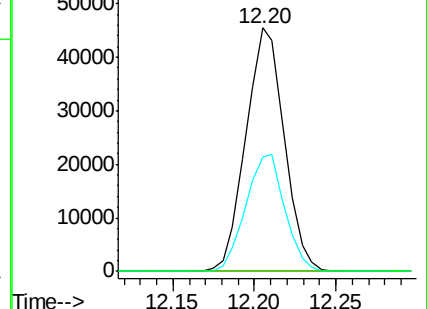

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.42 min Scan# 1917

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46


Tgt Ion:152 Resp: 180128

Ion Ratio Lower Upper

152 100

115 58.3 29.1 87.4



150 174.4 0.0 348.8




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

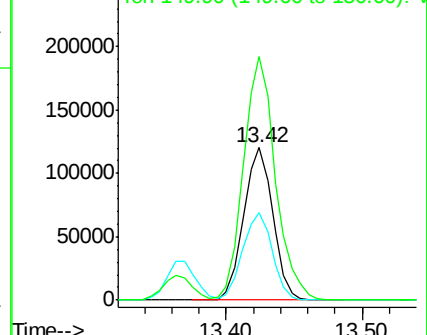



#73

Isopropylbenzene

Concen: 49.408 ug/l

RT: 12.33 min Scan# 1737

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :


VSTDICCC050

Tgt Ion: 105 Resp: 657764

Ion Ratio Lower Upper




105 100

120 26.9 13.5 40.4



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

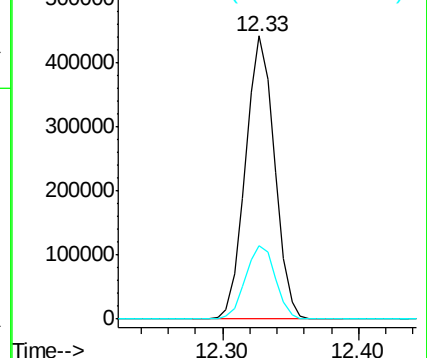

#74

N-ethyl acetate

Concen: 50.658 ug/l

RT: 12.14 min Scan# 1707

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Tgt Ion: 43 Resp: 193147


Ion Ratio Lower Upper

43 100

70 41.4 33.1 49.7

55 22.5 18.0 27.0

61 23.9 19.1 28.7






Abundance Ion 43.00 (42.70 to 43.70): VY0

Ion 70.00 (69.70 to 70.70): VY0

Ion 55.00 (54.70 to 55.70): VY0

Ion 61.00 (60.70 to 61.70): VY0

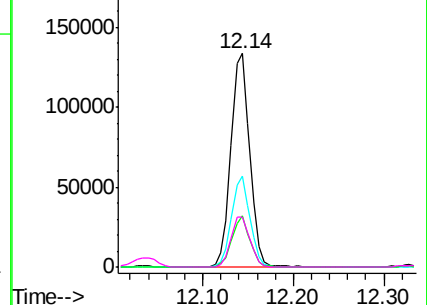



#75

1,1,2,2-Tetrachloroethane

Concen: 48.657 ug/l

RT: 12.58 min Scan# 1779

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050





Tgt Ion: 83 Resp: 128257

Ion Ratio Lower Upper

83 100

131 9.9 5.0 14.9

85 64.6 32.3 96.9

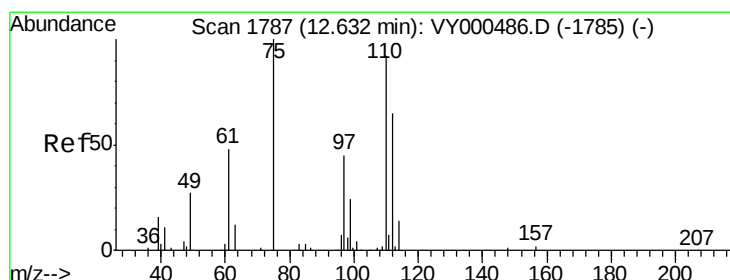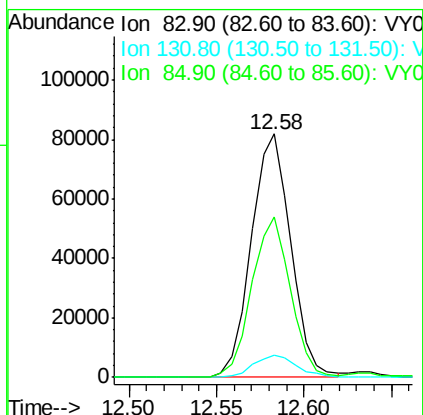

#76

1,2,3-Trichloropropane

Concen: 52.895 ug/l

RT: 12.63 min Scan# 1787

Delta R.T. 0.00 min

Lab File: VY000486.D




Acq: 30 Oct 2019 11:46


Tgt Ion: 75 Resp: 176200

Ion Ratio Lower Upper

75 100

77 0.0 0.0 0.0





#77

Bromobenzene

Concen: 48.857 ug/l

RT: 12.61 min Scan# 1783

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050


Tgt Ion:156 Resp: 147496

Ion Ratio Lower Upper

156 100

77 196.3 98.2 294.4




158 99.3 49.6 149.0



Abundance Ion 155.80 (155.50 to 156.50): V

Ion 77.00 (76.70 to 77.70): VY0

Ion 157.80 (157.50 to 158.50): V

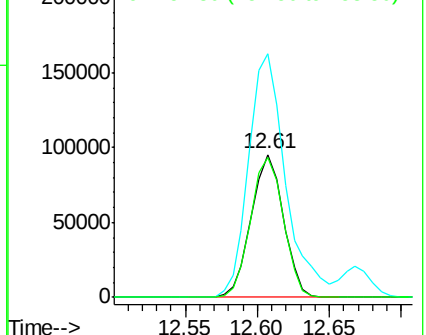

#78

n-propylbenzene

Concen: 49.859 ug/l

RT: 12.67 min Scan# 1793

Delta R.T. 0.00 min

Lab File: VY000486.D


Acq: 30 Oct 2019 11:46

Tgt Ion: 91 Resp: 800882

Ion Ratio Lower Upper



91 100


120 22.7 11.4 34.1



Abundance Ion 91.00 (90.70 to 91.70): VY0

Ion 120.00 (119.70 to 120.70): V




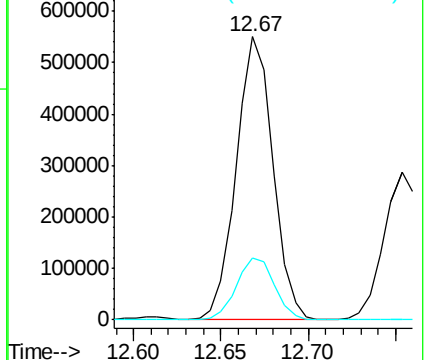




#79
 2-Chlorotoluene
 Concen: 49.134 ug/l
 RT: 12.75 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46




Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050


Tgt Ion: 91 Resp: 438155
 Ion Ratio Lower Upper
 91 100
 126 35.4 17.7 53.1



#80
 1,3,5-Trimethylbenzene
 Concen: 50.128 ug/l
 RT: 12.81 min Scan# 1816
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Tgt Ion: 105 Resp: 555804
 Ion Ratio Lower Upper
 105 100
 120 49.9 24.9 74.8





#81

trans-1,4-Dichloro-2-butene

Concen: 50.994 ug/l

RT: 12.38 min Scan# 1745

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050





Tgt Ion: 75 Resp: 46647

Ion Ratio Lower Upper

75 100

53 91.5 73.2 109.8

89 44.9 35.9 53.9

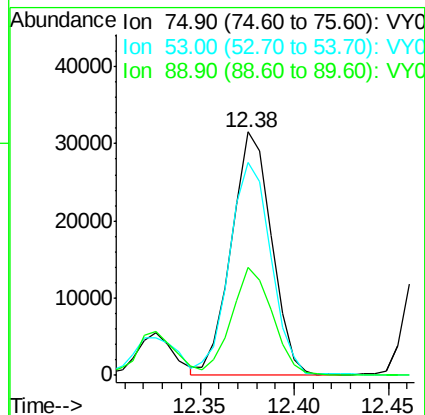

#82

4-Chlorotoluene

Concen: 49.895 ug/l

RT: 12.85 min Scan# 1823

Delta R.T. 0.00 min

Lab File: VY000486.D




Acq: 30 Oct 2019 11:46


Tgt Ion: 91 Resp: 461212

Ion Ratio Lower Upper

91 100

126 35.3 17.6 52.9



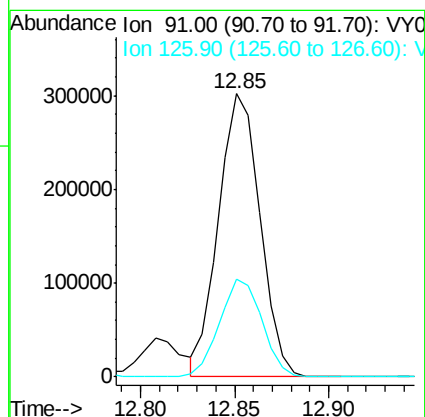





#83
tert-Butylbenzene
Concen: 50.088 ug/l
RT: 13.07 min Scan# 1859
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46




Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050


Tgt Ion:119 Resp: 474186
Ion Ratio Lower Upper
119 100
91 64.2 32.1 96.3
134 26.3 13.2 39.5



#84
1,2,4-Trimethylbenzene
Concen: 51.006 ug/l
RT: 13.12 min Scan# 1867
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion:105 Resp: 563077
Ion Ratio Lower Upper
105 100
120 46.6 23.3 69.9





#85

sec-Butylbenzene

Concen: 51.006 ug/l

RT: 13.25 min Scan# 1889

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :


VSTDICCC050

Tgt Ion:105 Resp: 687953

Ion Ratio Lower Upper




105 100

134 20.1 10.1 30.1



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 134.00 (133.70 to 134.70): V



#86

p-Isopropyltoluene

Concen: 50.618 ug/l

RT: 13.37 min Scan# 1908

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46


Tgt Ion:119 Resp: 608478

Ion Ratio Lower Upper

119 100

134 27.2 13.6 40.8



91 24.1 12.0 36.1




Abundance Ion 119.00 (118.70 to 119.70): V

Ion 134.00 (133.70 to 134.70): V

Ion 91.00 (90.70 to 91.70): VY0





#87

1,3-Dichlorobenzene

Concen: 49.554 ug/l

RT: 13.36 min Scan# 1907

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050


Tgt Ion:146 Resp: 293020

Ion Ratio Lower Upper




146 100

111 40.5 20.3 60.8

148 63.0 31.5 94.5



Abundance Ion 145.90 (145.60 to 146.60): V
Ion 110.90 (110.60 to 111.60): V
Ion 147.90 (147.60 to 148.60): V



#88

1,4-Dichlorobenzene

Concen: 49.820 ug/l

RT: 13.44 min Scan# 1920

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46


Tgt Ion:146 Resp: 294382

Ion Ratio Lower Upper



146 100


111 39.3 19.7 59.0

148 63.8 31.9 95.7



Abundance Ion 145.90 (145.60 to 146.60): V
Ion 110.90 (110.60 to 111.60): V
Ion 147.90 (147.60 to 148.60): V





#89

n-Butylbenzene

Concen: 50.805 ug/l

RT: 13.69 min Scan# 1961

Delta R.T. 0.00 min

Lab File: VY000486.D

Acq: 30 Oct 2019 11:46

Instrument :

MSVOA_Y

ClientSampleId :

VSTDICCC050


Tgt Ion: 91 Resp: 602363

Ion Ratio Lower Upper

91 100

92 53.5 26.8 80.3




134 25.8 12.9 38.7



Abundance Ion 91.00 (90.70 to 91.70): VY000486.D (-1953) (-)

Ion 92.00 (91.70 to 92.70): VY000486.D (-1953) (-)

Ion 134.00 (133.70 to 134.70): VY000486.D (-1953) (-)



#90

Hexachloroethane

Concen: 51.018 ug/l

RT: 13.96 min Scan# 2005

Delta R.T. 0.00 min

Lab File: VY000486.D


Acq: 30 Oct 2019 11:46

Tgt Ion: 117 Resp: 113379

Ion Ratio Lower Upper



117 100


201 71.5 35.8 107.3



Abundance Ion 116.80 (116.50 to 117.50): VY000486.D (-1996) (-)

Ion 200.70 (200.40 to 201.40): VY000486.D (-1996) (-)









#91
 1,2-Dichlorobenzene
 Concen: 49.995 ug/l
 RT: 13.74 min Scan# 1968
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46




Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050


Tgt Ion: 146 Resp: 268230
 Ion Ratio Lower Upper
 146 100
 111 41.0 20.5 61.5
 148 63.4 31.7 95.1



#92
 1,2-Dibromo-3-Chloropropane
 Concen: 48.456 ug/l
 RT: 14.36 min Scan# 2070
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Tgt Ion: 75 Resp: 22605
 Ion Ratio Lower Upper
 75 100
 155 84.7 42.4 127.1
 157 110.2 55.1 165.3









#93
 1,2,4-Trichlorobenzene
 Concen: 48.188 ug/l
 RT: 15.00 min Scan# 2176
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Instrument :
 MSVOA_Y
 ClientSampleId :
 VSTDICCC050

Tgt Ion:180 Resp: 176036
 Ion Ratio Lower Upper
 180 100
 182 95.6 47.8 143.4
 145 31.9 16.0 47.9




Abundance Ion 179.80 (179.50 to 180.50): V
 Ion 181.80 (181.50 to 182.50): V
 Ion 144.80 (144.50 to 145.50): V






#94
 Hexachlorobutadiene
 Concen: 50.425 ug/l
 RT: 15.11 min Scan# 2193
 Delta R.T. 0.00 min
 Lab File: VY000486.D
 Acq: 30 Oct 2019 11:46

Tgt Ion:225 Resp: 94955
 Ion Ratio Lower Upper
 225 100
 223 62.5 31.3 93.8
 227 64.7 32.4 97.0



Abundance Ion 224.70 (224.40 to 225.40): V
 Ion 222.70 (222.40 to 223.40): V
 Ion 226.70 (226.40 to 227.40): V









#95
Naphthalene
Concen: 49.196 ug/l
RT: 15.23 min Scan# 2214
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Instrument :
MSVOA_Y
ClientSampleId :
VSTDICCC050

Tgt Ion:128 Resp: 398957
Ion Ratio Lower Upper
128 100
127 12.2 9.8 14.6
129 10.9 8.7 13.1



#96
1,2,3-Trichlorobenzene
Concen: 49.839 ug/l
RT: 15.42 min Scan# 2244
Delta R.T. 0.00 min
Lab File: VY000486.D
Acq: 30 Oct 2019 11:46

Tgt Ion:180 Resp: 163343
Ion Ratio Lower Upper
180 100
182 94.9 47.4 142.3
145 31.3 15.7 47.0

