

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY103019\
 Data File : VY000490.D
 Acq On : 30 Oct 2019 14:00
 Operator : SY/MD
 Sample : VY1030SBL01
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1030SBL01

Quant Time: Oct 31 02:30:27 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 30 13:30:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	228009	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	395987	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	345001	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	154112	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.15	65	135325	57.35	ug/l	0.00
Spiked Amount	50.000		Recovery	=	114.70%	
35) Dibromofluoromethane	7.73	113	117317	50.47	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.94%	
50) Toluene-d8	10.18	98	463105	52.50	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.00%	
62) 4-Bromofluorobenzene	12.48	95	155327	46.25	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.50%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_Y\DATA\VY103019\
Data File : VY000490.D
Acq On : 30 Oct 2019 14:00
Operator : SY/MD
Sample : VY1030SBL01
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1030SBL01

Quant Time: Oct 31 02:30:27 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 30 13:30:53 2019
Response via : Initial Calibration

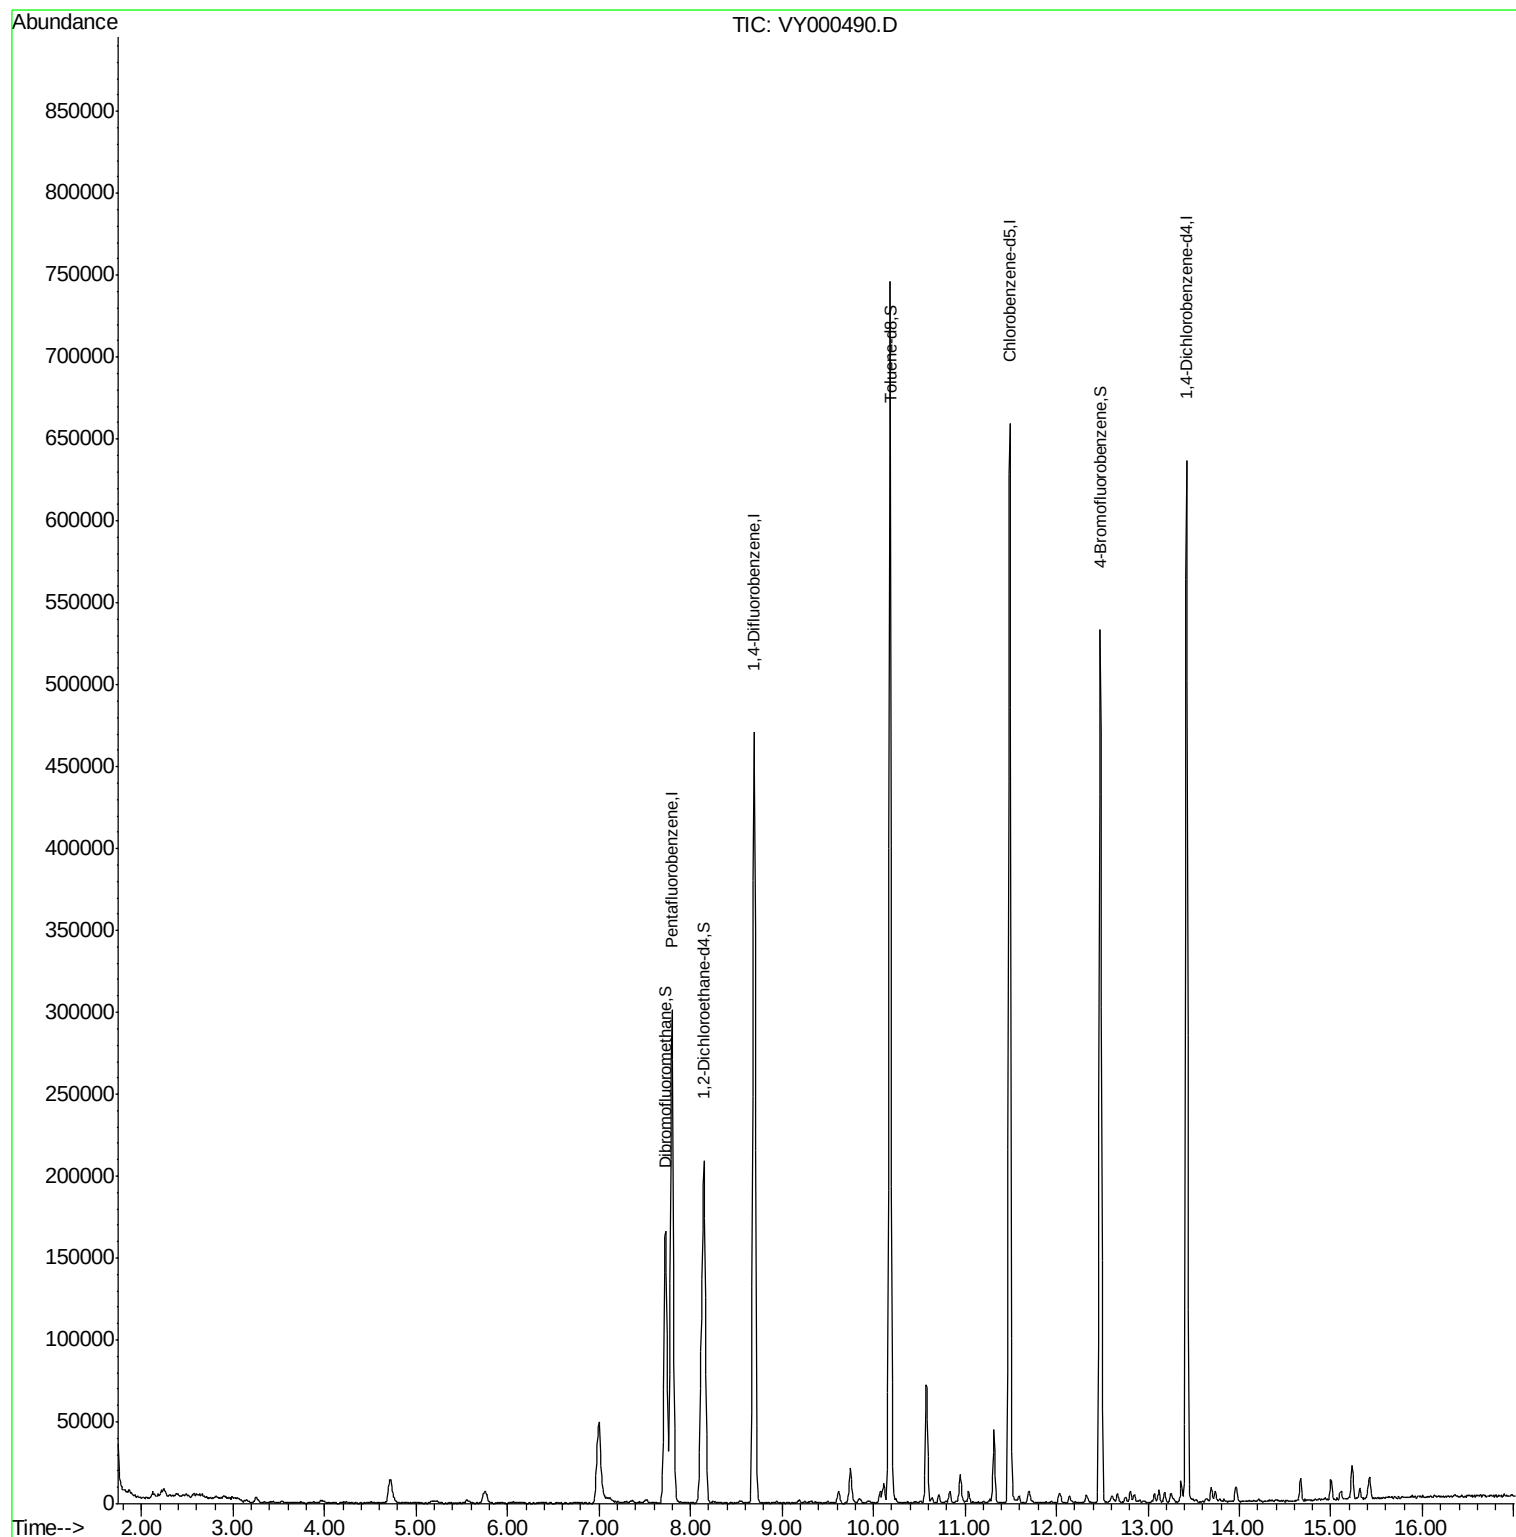

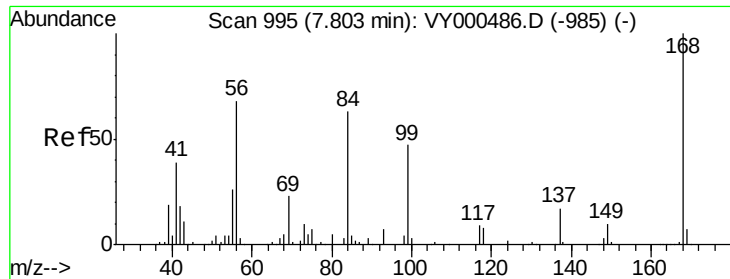

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. -0.01 min

Lab File: VY000490.D

Acq: 30 Oct 2019 14:00

Instrument :

MSVOA_Y

ClientSampleId :


VY1030SBL01

Tgt Ion:168 Resp: 228009

Ion Ratio Lower Upper

168 100

99 54.5 45.7 68.5

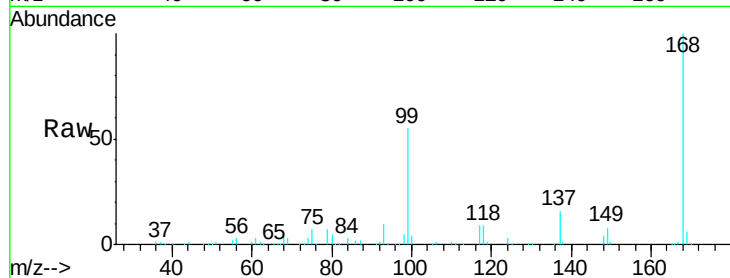

Abundance Ion 167.90 (167.60 to 168.60): VY000486.D (-985) (-)

Ion 98.90 (98.60 to 99.60): VY000486.D (-985) (-)

7.80

120000

100000

80000



60000

40000

20000

0

Time-->

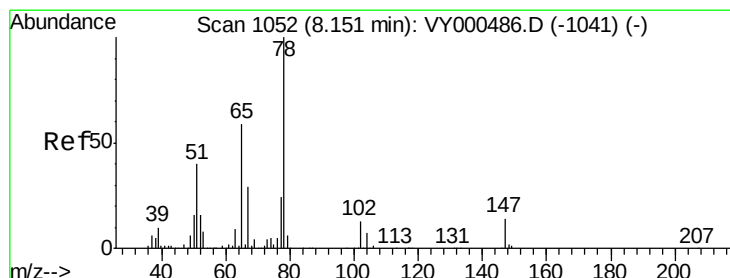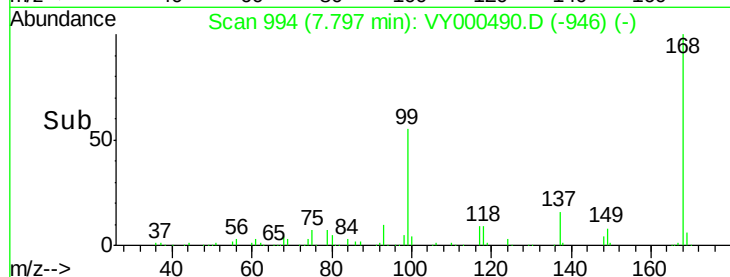

#33

1,2-Dichloroethane-d4

Concen: 57.351 ug/l

RT: 8.15 min Scan# 1052

Delta R.T. -0.00 min

Lab File: VY000490.D


Acq: 30 Oct 2019 14:00

Tgt Ion: 65 Resp: 135325

Ion Ratio Lower Upper

65 100

67 54.6 0.0 107.2

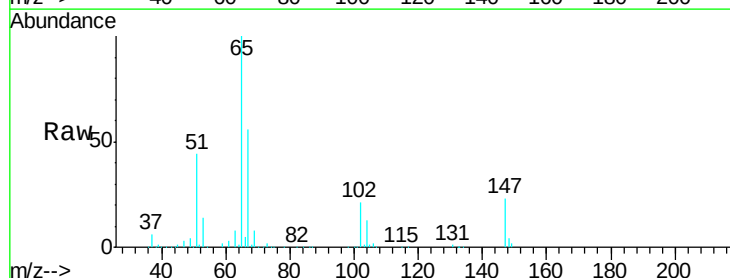

Abundance Ion 64.90 (64.60 to 65.60): VY000486.D (-1041) (-)

Ion 66.90 (66.60 to 67.60): VY000486.D (-1041) (-)

8.15


60000


40000

20000

0

Time-->

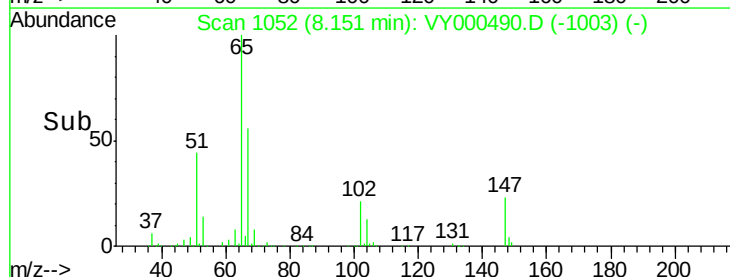

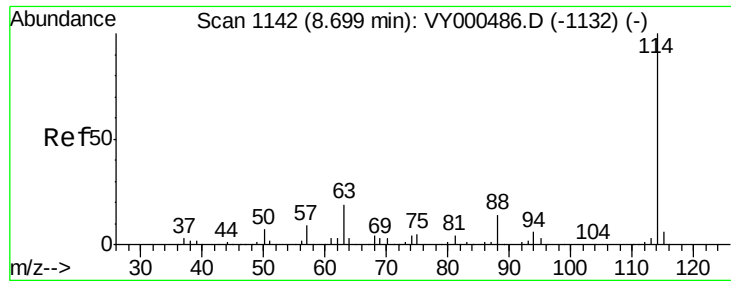

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.69 min Scan# 1141

Delta R.T. -0.01 min

Lab File: VY000490.D

Acq: 30 Oct 2019 14:00

Instrument :

MSVOA_Y

ClientSampleId :

VY1030SBL01


Tgt Ion:114 Resp: 395987

Ion Ratio Lower Upper

114 100

63 20.9 0.0 38.0




88 15.1 0.0 28.6

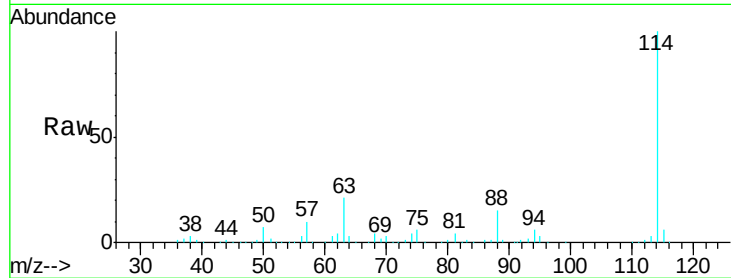

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VY0

Ion 87.90 (87.60 to 88.60): VY0

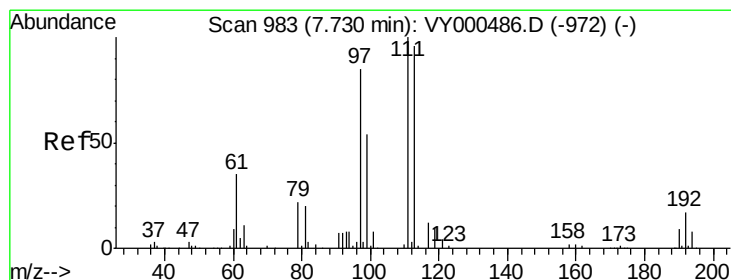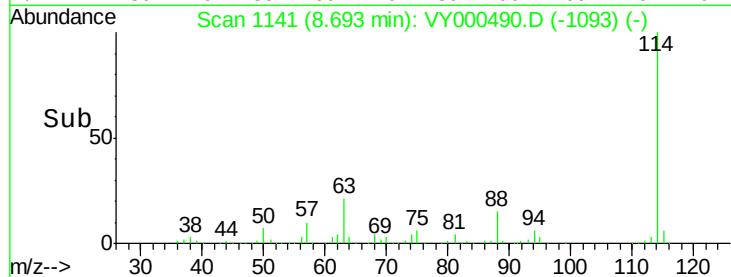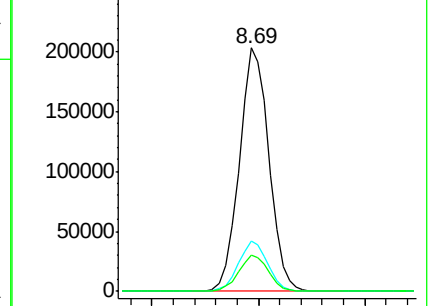

#35

Dibromofluoromethane

Concen: 50.465 ug/l

RT: 7.73 min Scan# 983

Delta R.T. -0.00 min

Lab File: VY000490.D

Acq: 30 Oct 2019 14:00


Tgt Ion:113 Resp: 117317

Ion Ratio Lower Upper

113 100

111 102.9 81.7 122.5



192 19.2 15.0 22.4

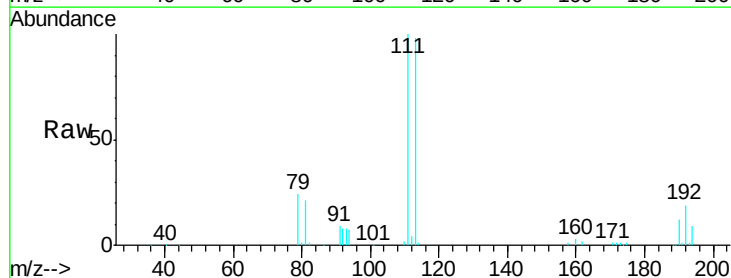


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

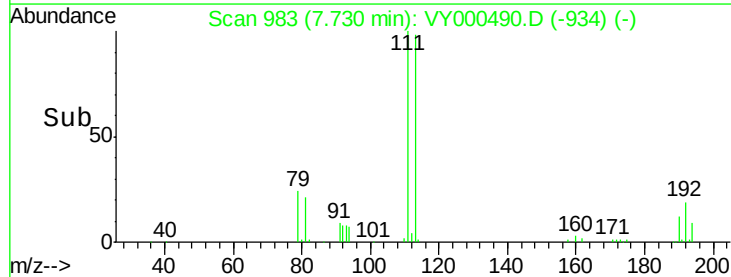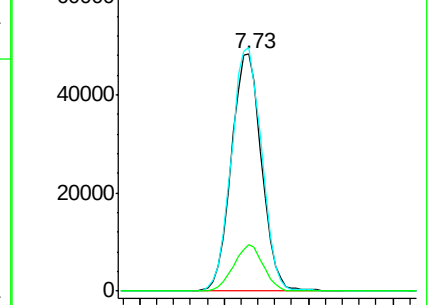

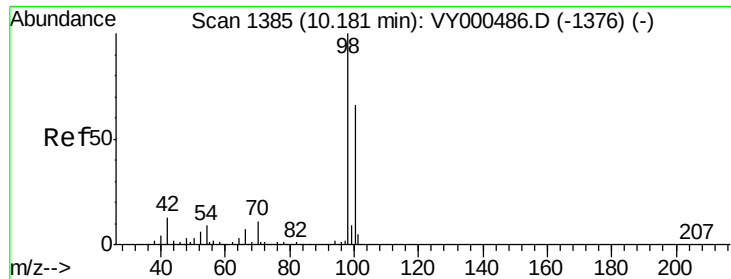

#50

Toluene-d8

Concen: 52.500 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. -0.00 min

Lab File: VY000490.D

Acq: 30 Oct 2019 14:00

Instrument :

MSVOA_Y

ClientSampleId :


VY1030SBL01

Tgt Ion: 98 Resp: 463105

Ion Ratio Lower Upper


98 100

100 66.3 52.9 79.3


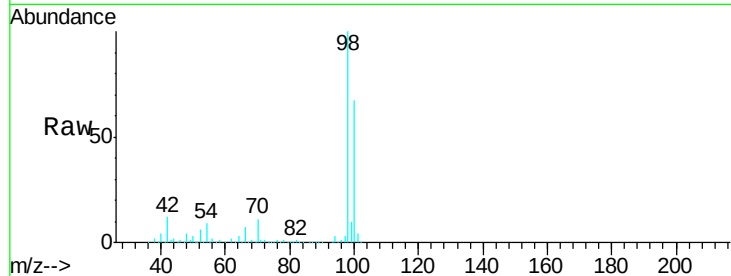


Abundance Ion 98.00 (97.70 to 98.70): VY0

Ion 100.00 (99.70 to 100.70): VY

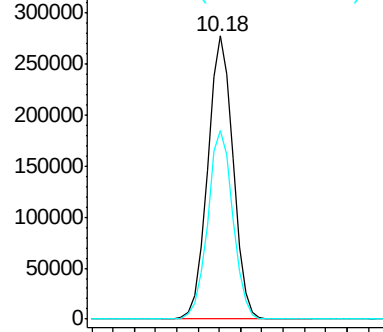

Time-->

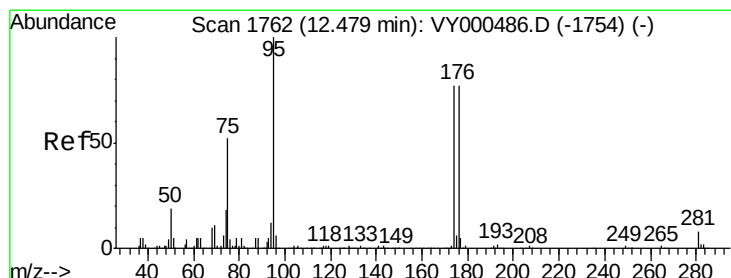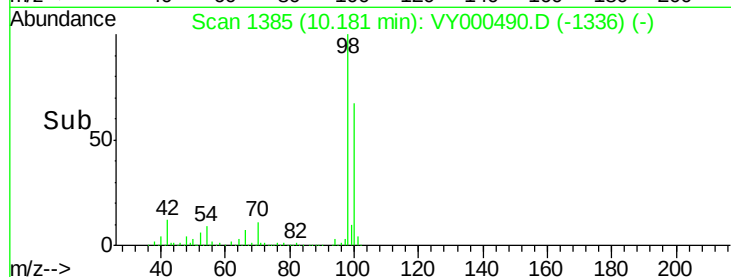

#62

4-Bromofluorobenzene

Concen: 46.254 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.00 min

Lab File: VY000490.D

Acq: 30 Oct 2019 14:00


Tgt Ion: 95 Resp: 155327

Ion Ratio Lower Upper

95 100

174 79.1 0.0 161.6


176 76.5 0.0 157.8

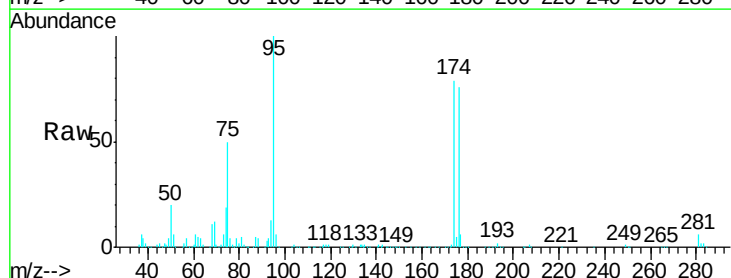


Abundance Ion 94.90 (94.60 to 95.60): VY0


Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

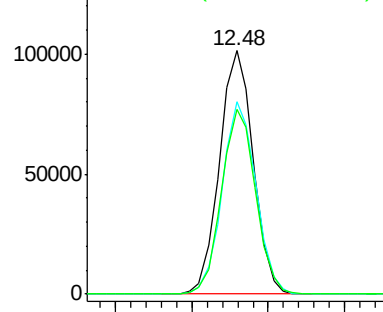

Time-->

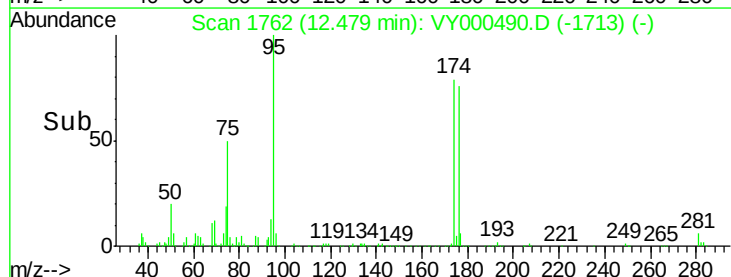


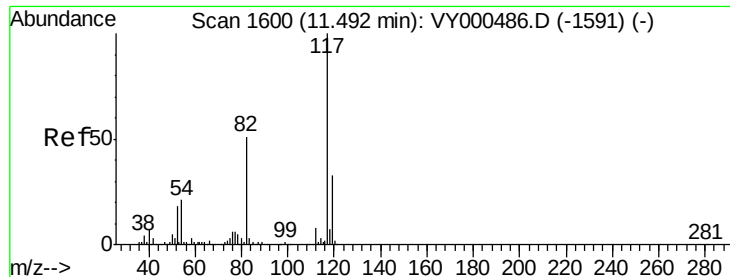




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1600
Delta R.T. -0.00 min
Lab File: VY000490.D
Acq: 30 Oct 2019 14:00

Instrument :
MSVOA_Y
ClientSampleId :
VY1030SBL01

Tgt Ion:117 Resp: 345001
Ion Ratio Lower Upper
117 100
82 54.0 40.8 61.2
119 30.9 26.2 39.2

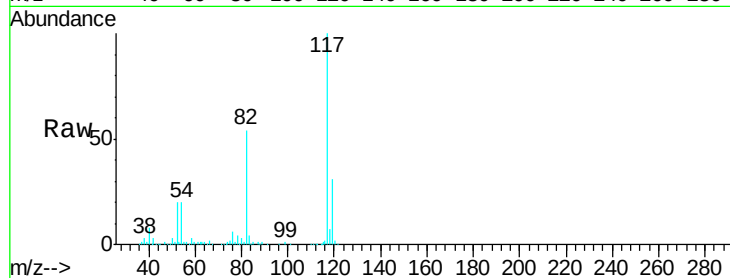


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VY0
Ion 118.90 (118.60 to 119.60): V

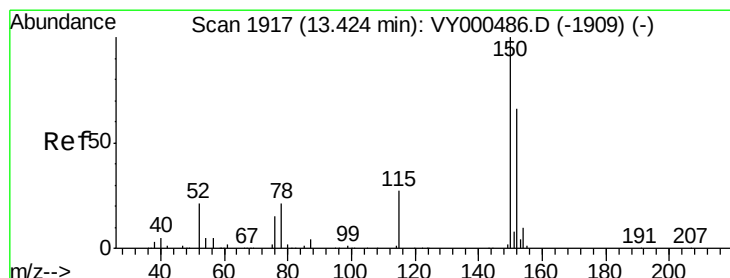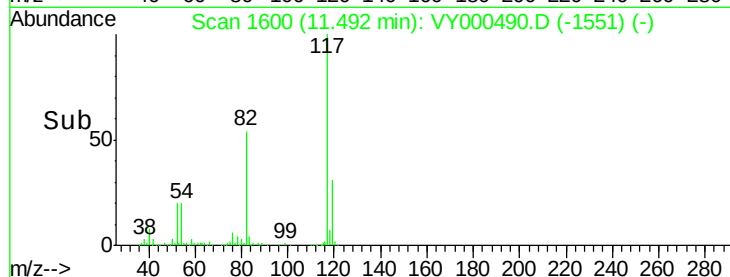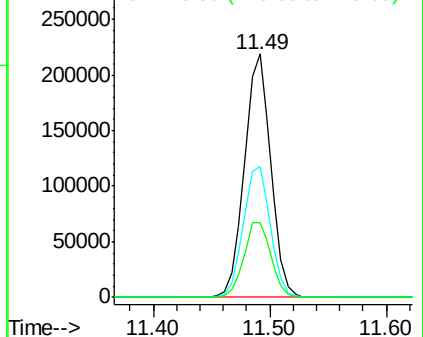

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. -0.00 min
Lab File: VY000490.D
Acq: 30 Oct 2019 14:00

Tgt Ion:152 Resp: 154112
Ion Ratio Lower Upper
152 100
115 57.5 29.1 87.4
150 157.7 0.0 348.8

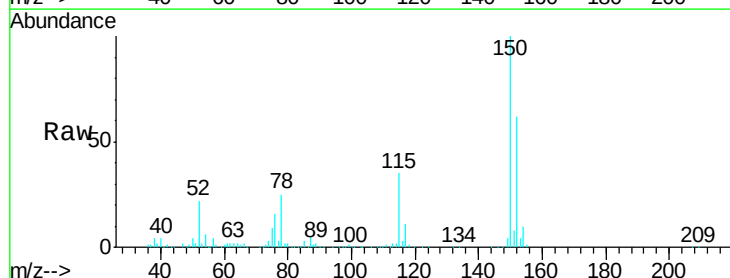

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

