


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\vy103119\
Data File : VY000496.D
Acq On : 31 Oct 2019 09:53
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y103019S.M
Title : SW846 8260
Last Update : Wed Oct 30 13:30:53 2019

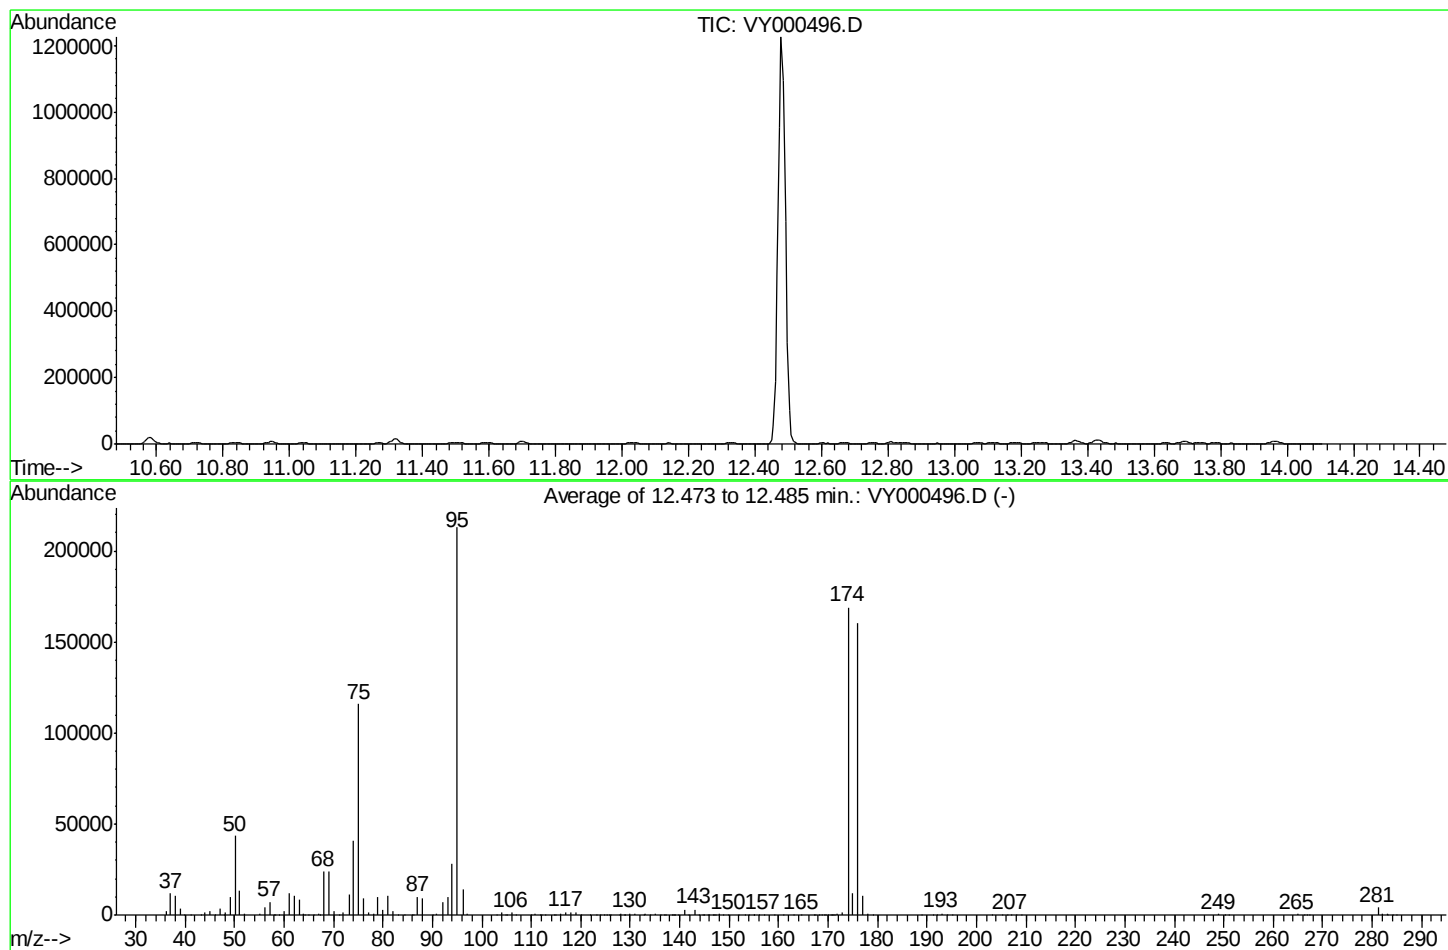

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	43317	PASS
75	95	30	60	54.4	115821	PASS
95	95	100	100	100.0	212885	PASS
96	95	5	9	6.5	13882	PASS
173	174	0.00	2	0.8	1293	PASS
174	95	50	100	79.4	169002	PASS
175	174	5	9	7.2	12106	PASS
176	174	95	101	94.9	160458	PASS
177	176	5	9	6.6	10515	PASS