

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110122\
 Data File : VY011241.D
 Acq On : 02 Nov 2022 00:00
 Operator : KP/MD
 Sample : N5336-02
 Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-01-16.5-17.0

Quant Time: Nov 02 01:45:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 01 11:56:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	176661	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	328563	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	309717	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	136015	50.000	ug/l	0.00


System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	123911	65.582	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	131.160%
35) Dibromofluoromethane	7.716	113	123177	58.350	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	116.700%
50) Toluene-d8	10.179	98	406489	49.595	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	99.200%
62) 4-Bromofluorobenzene	12.477	95	142530	50.092	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	100.180%

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 02 01:45:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 01 11:56:18 2022
Response via : Initial Calibration







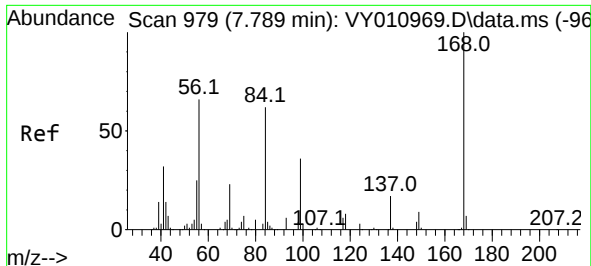

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY011241.D
Acq: 02 Nov 2022 00:00




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-16.5-17.0


Tgt Ion:168 Resp: 176661
Ion Ratio Lower Upper
168 100
99 53.4 46.9 70.3

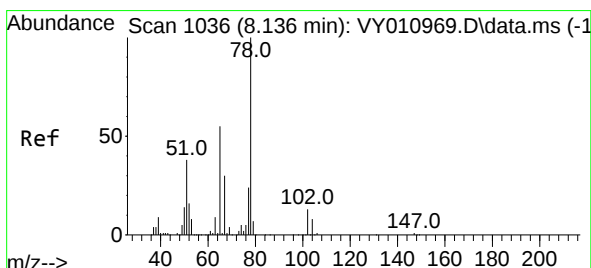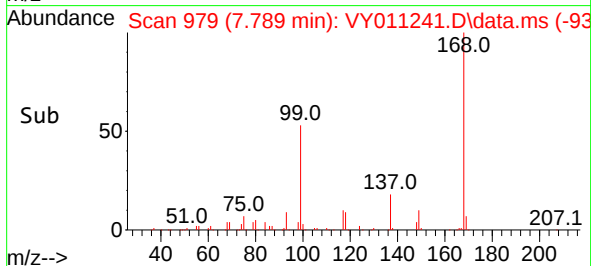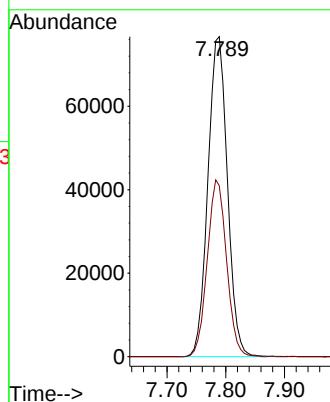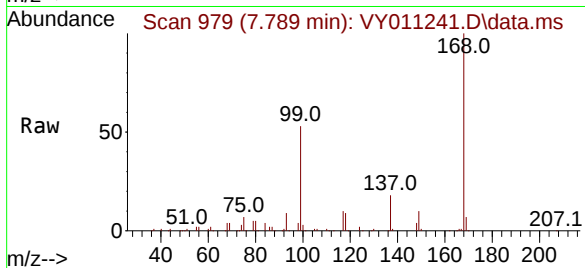

#33
1,2-Dichloroethane-d4
Concen: 65.582 ug/l
RT: 8.137 min Scan# 1036
Delta R.T. 0.001 min
Lab File: VY011241.D
Acq: 02 Nov 2022 00:00

Tgt Ion: 65 Resp: 123911
Ion Ratio Lower Upper
65 100
67 54.3 0.0 99.4

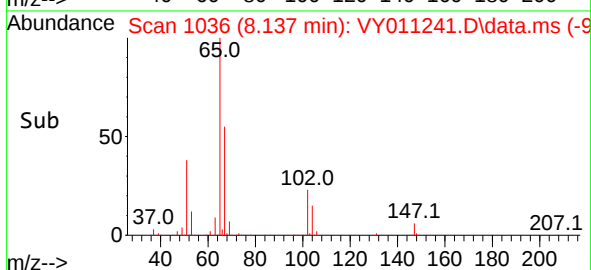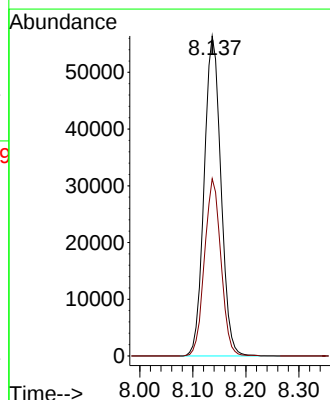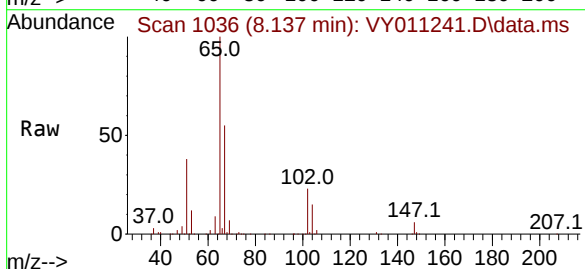

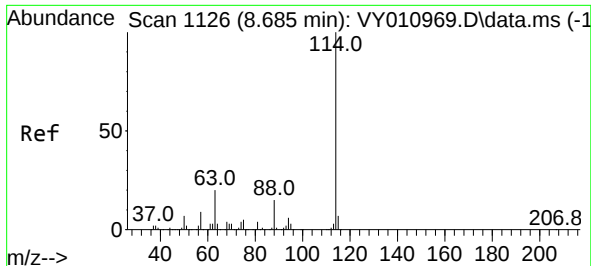

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY011241.D

Acq: 02 Nov 2022 00:00

Instrument :

MSVOA_Y

ClientSampleId :

SB-01-16.5-17.0





Tgt Ion:114 Resp: 328563

Ion Ratio Lower Upper

114 100

63 18.9 0.0 43.2

88 15.1 0.0 31.8

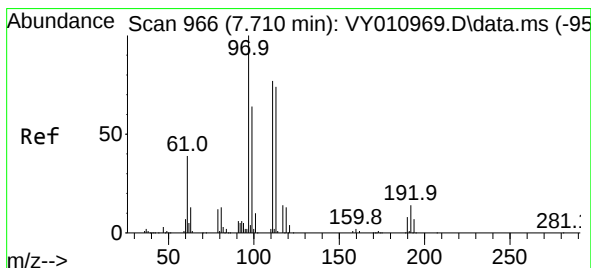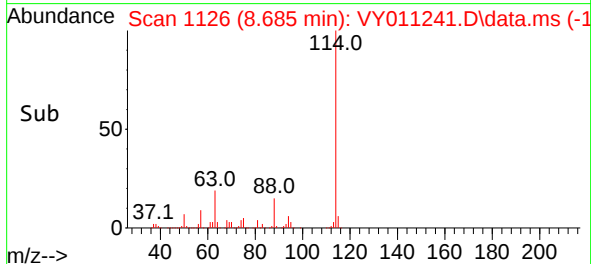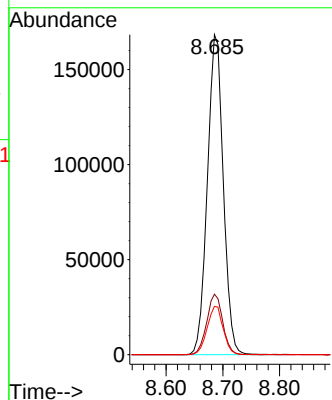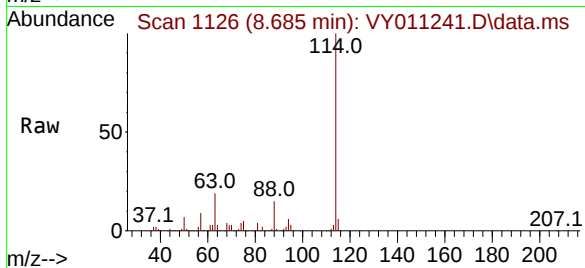

#35

Dibromofluoromethane

Concen: 58.350 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.006 min

Lab File: VY011241.D

Acq: 02 Nov 2022 00:00




Tgt Ion:113 Resp: 123177


Ion Ratio Lower Upper

113 100

111 102.4 82.6 124.0

192 19.2 17.6 26.4

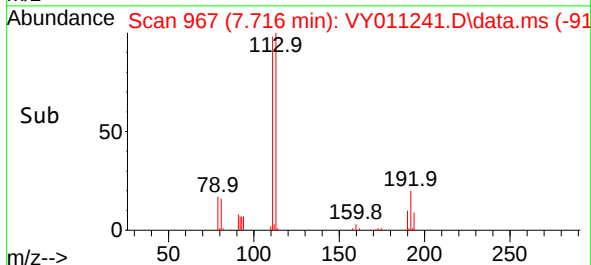
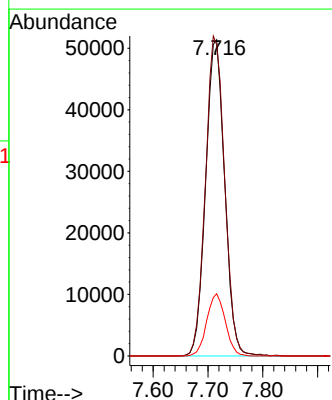
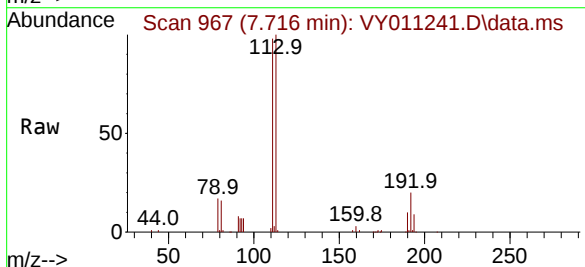


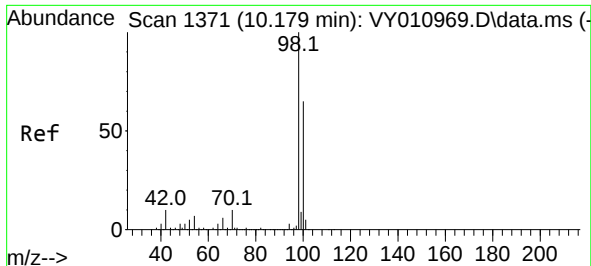

#50
Toluene-d8
Concen: 49.595 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY011241.D
Acq: 02 Nov 2022 00:00




Instrument :
MSVOA_Y
ClientSampleId :
SB-01-16.5-17.0


Tgt Ion: 98 Resp: 406489
Ion Ratio Lower Upper
98 100
100 64.7 50.2 75.2

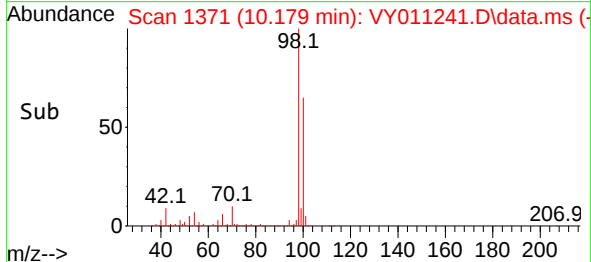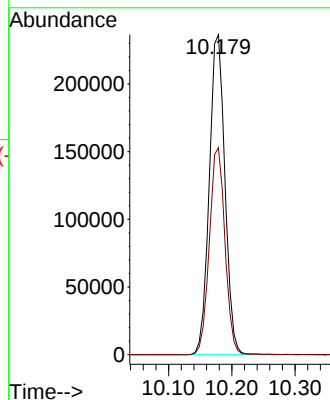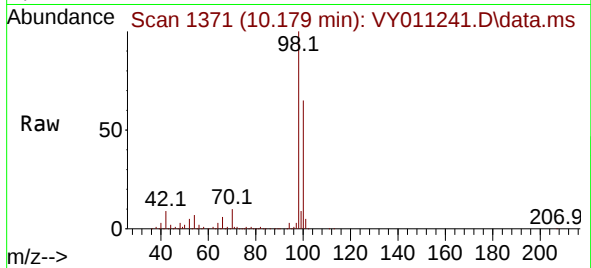

#62
4-Bromofluorobenzene
Concen: 50.092 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY011241.D
Acq: 02 Nov 2022 00:00

Tgt Ion: 95 Resp: 142530
Ion Ratio Lower Upper
95 100
174 82.7 0.0 177.0
176 80.3 0.0 175.8


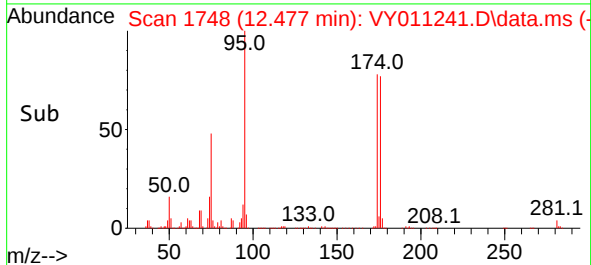
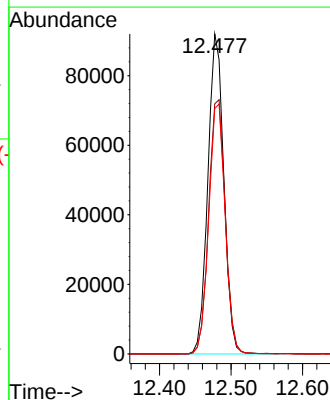
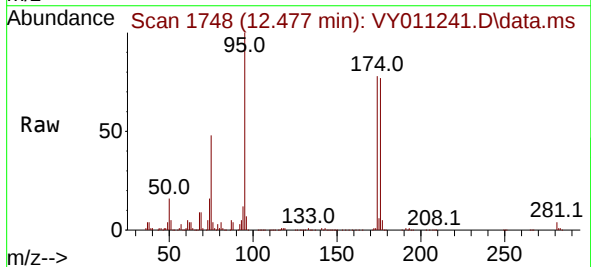


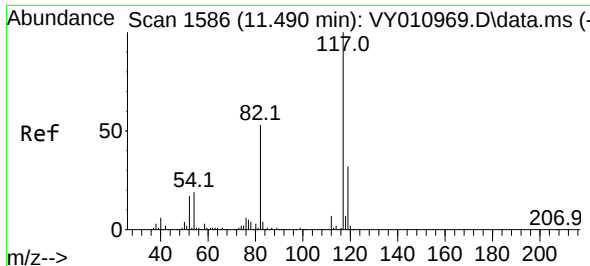

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY011241.D
Acq: 02 Nov 2022 00:00

Instrument :
MSVOA_Y
ClientSampleId :
SB-01-16.5-17.0

Tgt Ion:117 Resp: 309717
Ion Ratio Lower Upper
117 100
82 54.2 43.0 64.4
119 32.2 25.4 38.0

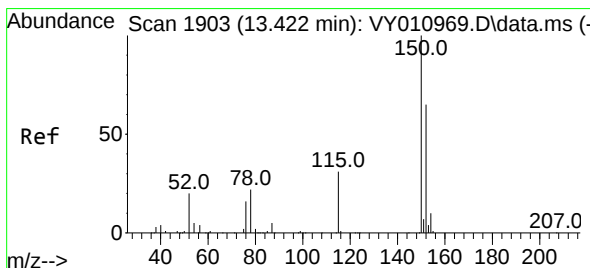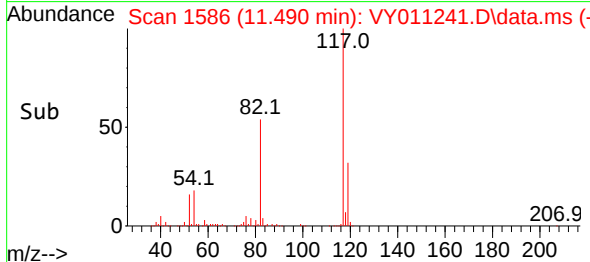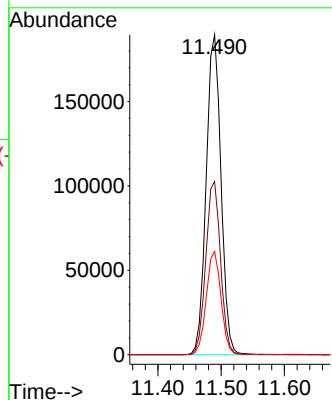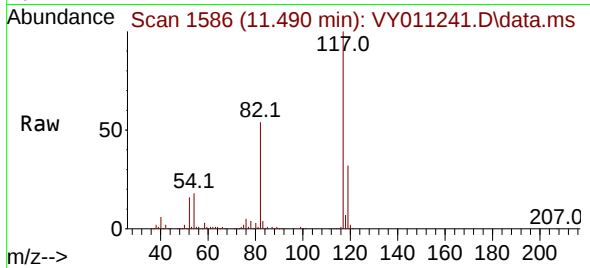

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY011241.D
Acq: 02 Nov 2022 00:00

Tgt Ion:152 Resp: 136015
Ion Ratio Lower Upper
152 100
115 58.2 28.2 84.7
150 157.2 0.0 347.6

