
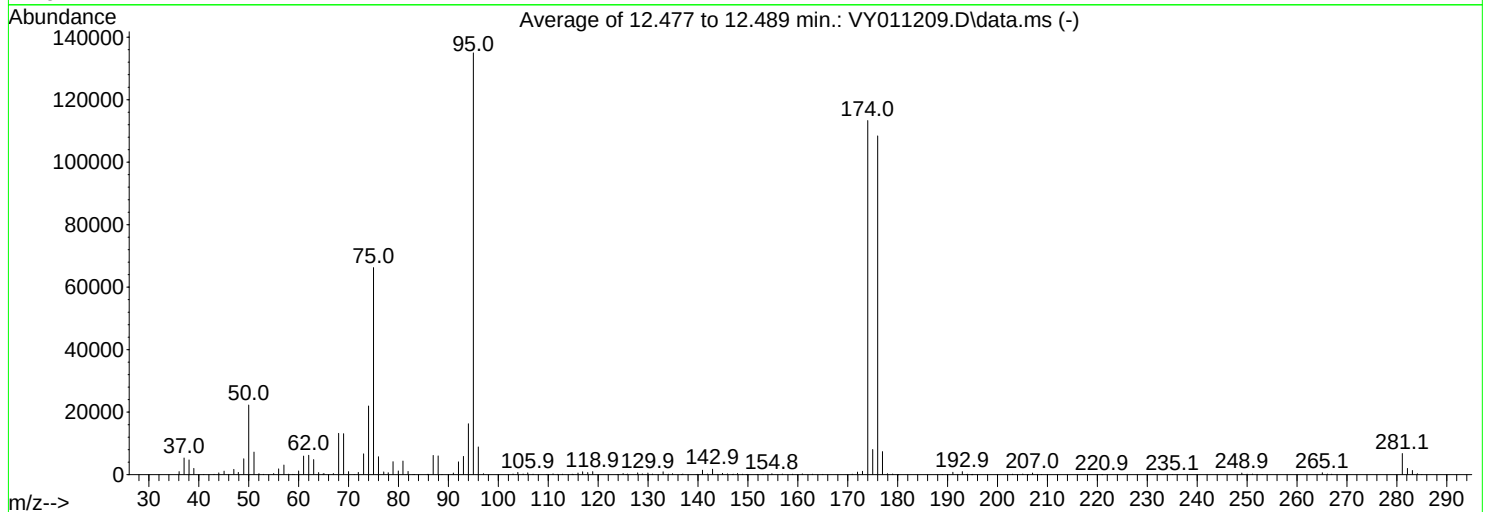


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110122\
Data File : VY011209.D
Acq On : 01 Nov 2022 08:37
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
Title : SW846 8260
Last Update : Tue Nov 01 11:56:18 2022

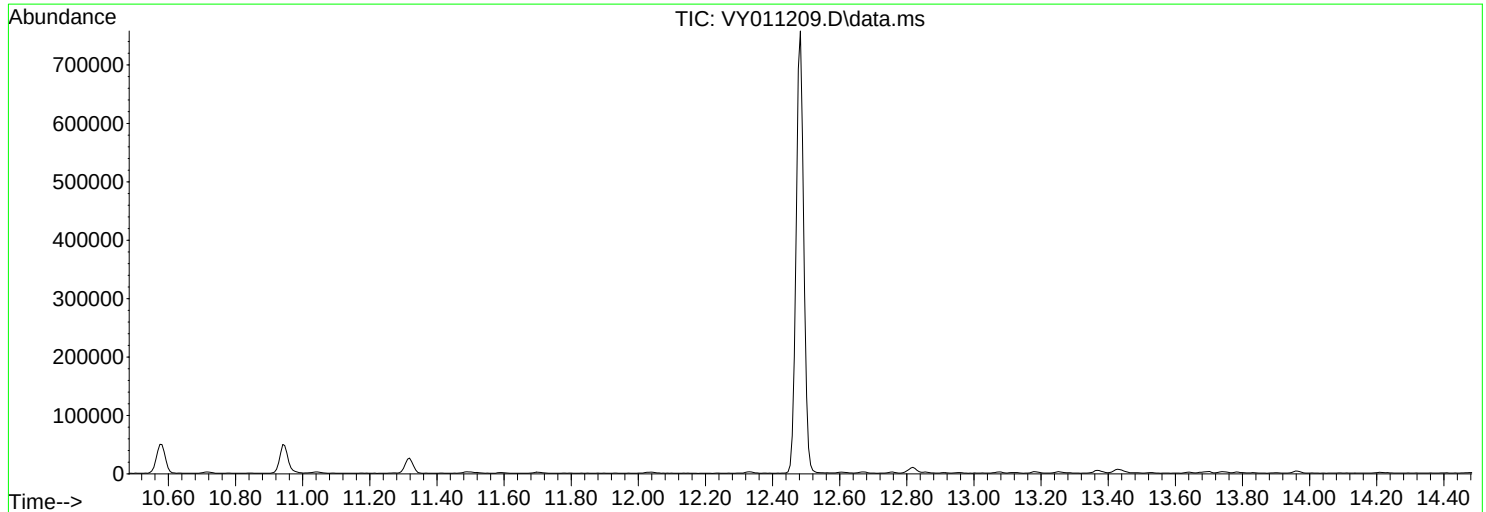

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	22299	PASS
75	95	30	60	49.1	66248	PASS
95	95	100	100	100.0	135000	PASS
96	95	5	9	6.6	8876	PASS
173	174	0.00	2	0.9	1065	PASS
174	95	50	100	84.0	113341	PASS
175	174	5	9	7.1	8018	PASS
176	174	95	101	95.6	108392	PASS
177	176	5	9	6.8	7363	PASS