
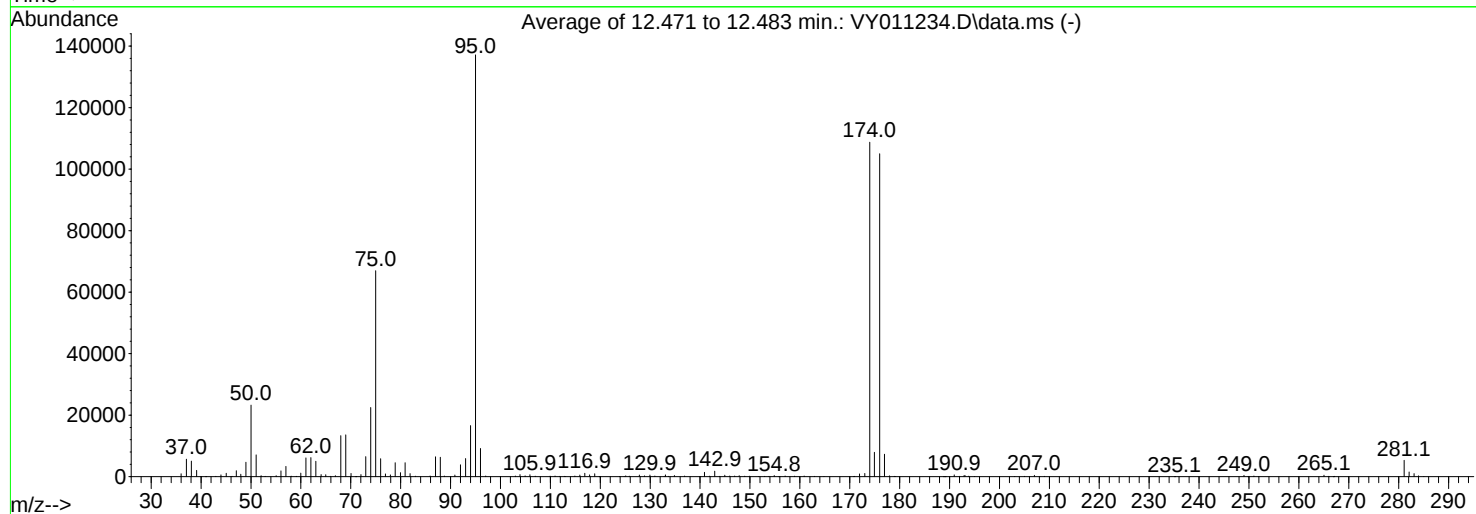


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110122\
Data File : VY011234.D
Acq On : 01 Nov 2022 20:14
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
Title : SW846 8260
Last Update : Tue Nov 01 11:56:18 2022

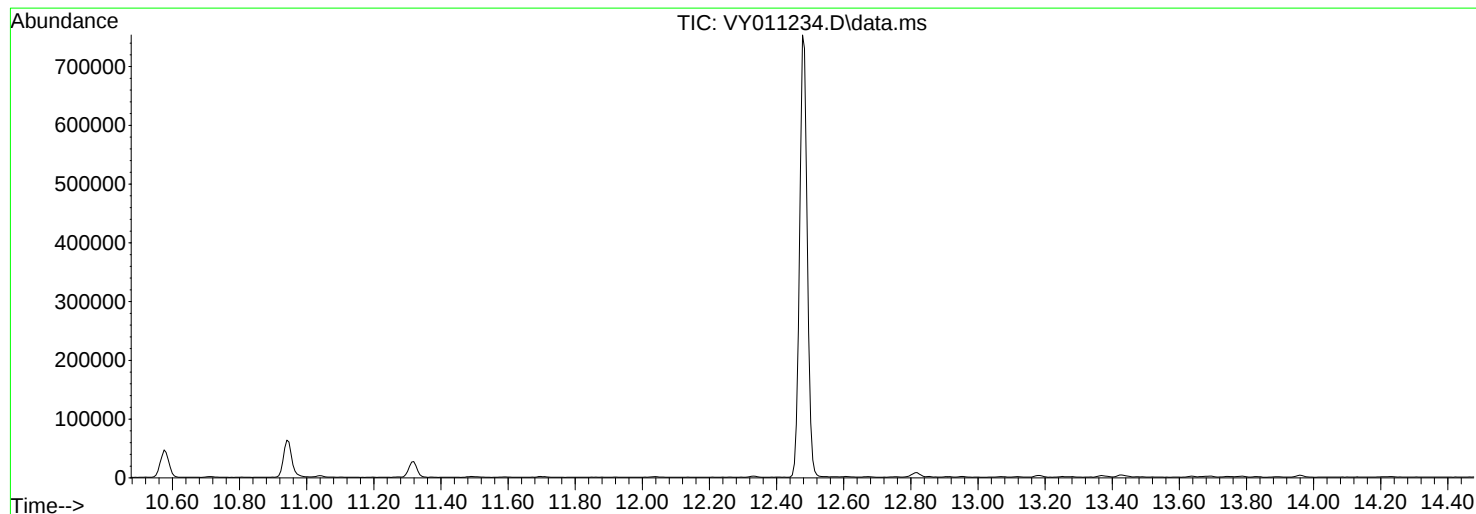

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	23248	PASS
75	95	30	60	48.8	66981	PASS
95	95	100	100	100.0	137168	PASS
96	95	5	9	6.7	9185	PASS
173	174	0.00	2	0.9	1025	PASS
174	95	50	100	79.3	108728	PASS
175	174	5	9	7.3	7924	PASS
176	174	95	101	96.5	104976	PASS
177	176	5	9	6.9	7277	PASS