


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111022\
Data File : VY011377.D
Acq On : 10 Nov 2022 08:56
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111022S.M
Title : SW846 8260
Last Update : Thu Nov 10 17:47:26 2022

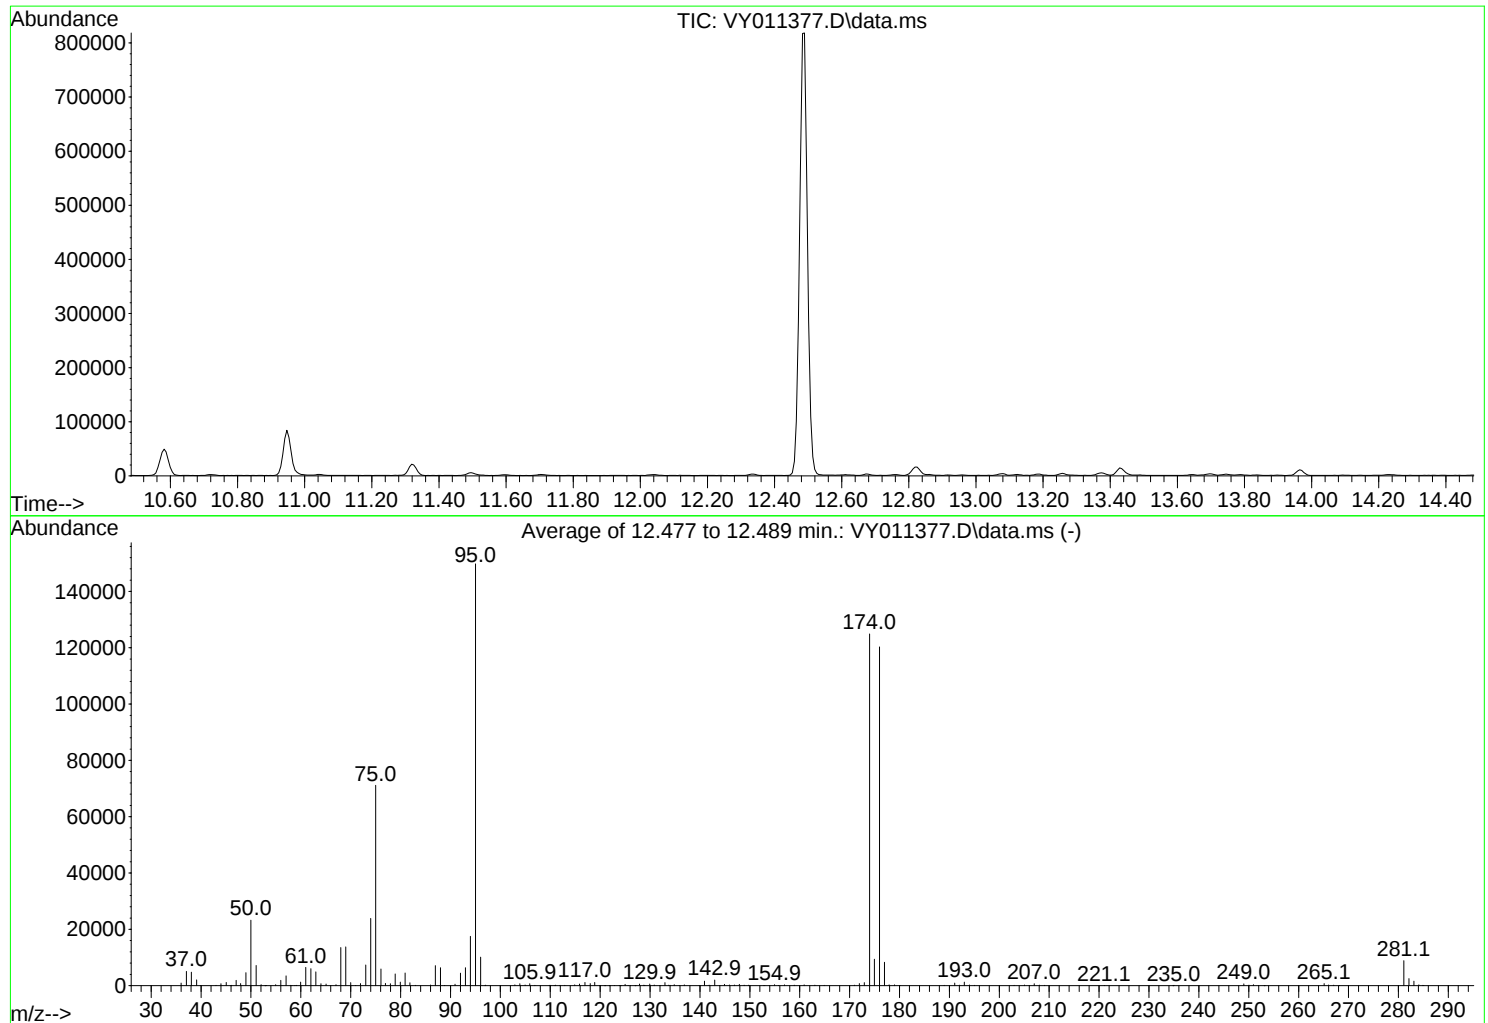

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.5	23216	PASS
75	95	30	60	47.5	71123	PASS
95	95	100	100	100.0	149792	PASS
96	95	5	9	6.7	10102	PASS
173	174	0.00	2	0.9	1099	PASS
174	95	50	100	83.4	124883	PASS
175	174	5	9	7.5	9402	PASS
176	174	95	101	96.3	120296	PASS
177	176	5	9	6.9	8280	PASS