

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121222\
 Data File : VY011763.D
 Acq On : 12 Dec 2022 12:10
 Operator : KP/MD
 Sample : N5947-01
 Misc : 6.21g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 NYE-SOIL-1208

Quant Time: Dec 12 12:25:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120922S.M
 Quant Title : SW846 8260
 QLast Update : Sat Dec 10 04:19:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	166376	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	272236	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	240405	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	106287	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	68625	61.553	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	123.100%
35) Dibromofluoromethane	7.716	113	68745	57.413	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	114.820%
50) Toluene-d8	10.179	98	204071	51.684	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	103.360%
62) 4-Bromofluorobenzene	12.483	95	77310	48.879	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	97.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121222\
Data File : VY011763.D
Acq On : 12 Dec 2022 12:10
Operator : KP/MD
Sample : N5947-01
Misc : 6.21g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
NYE-SOIL-1208

Quant Time: Dec 12 12:25:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120922S.M
Quant Title : SW846 8260
QLast Update : Sat Dec 10 04:19:59 2022
Response via : Initial Calibration




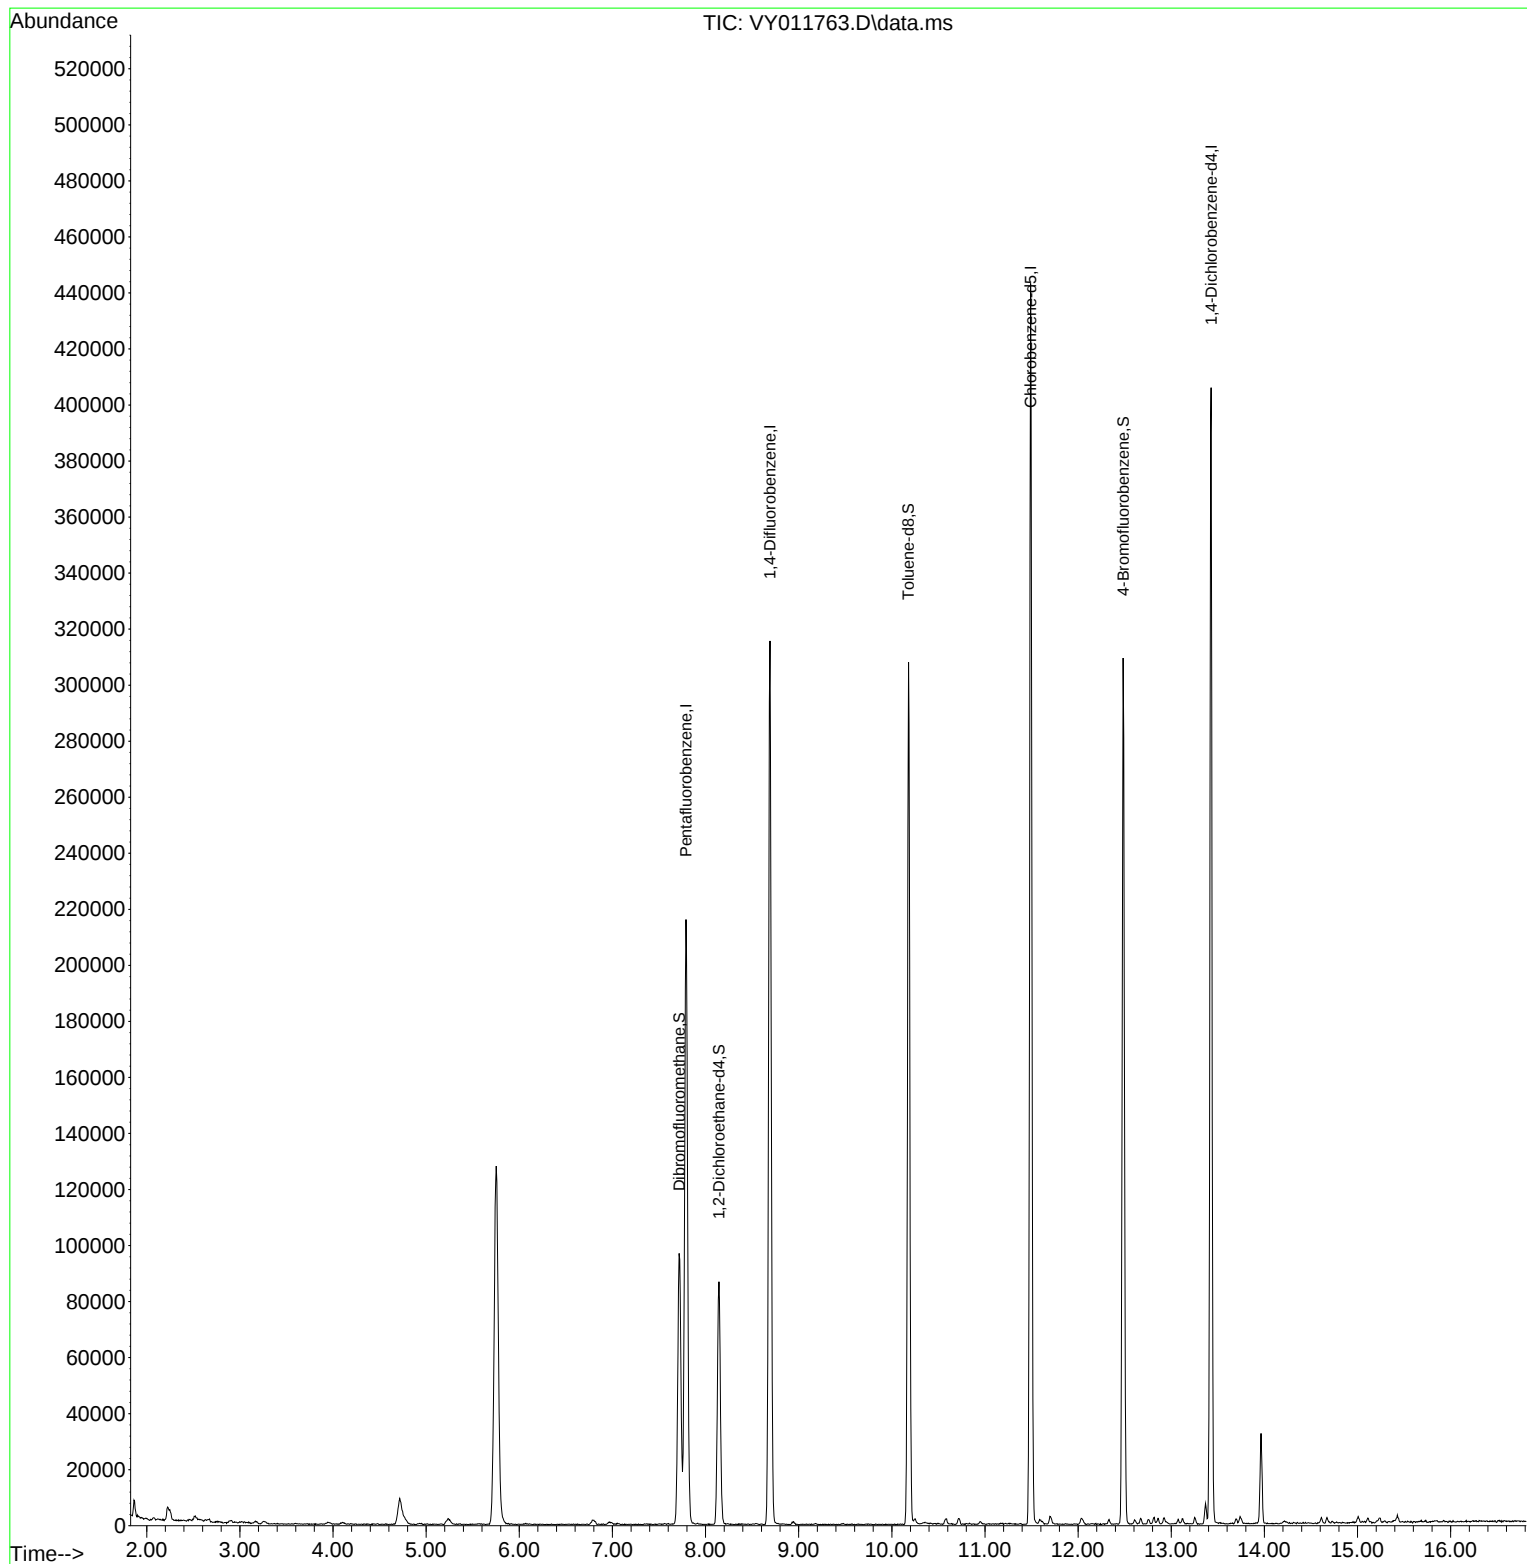


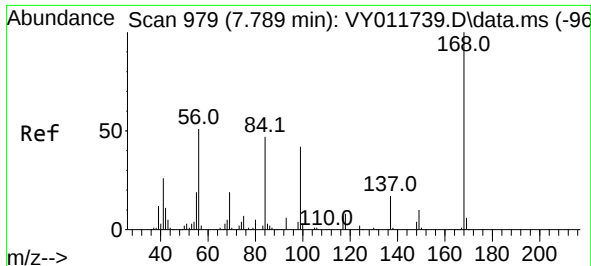

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY011763.D
Acq: 12 Dec 2022 12:10




Instrument :
MSVOA_Y
ClientSampleId :
NYE-SOIL-1208


Tgt Ion:168 Resp: 166376
Ion Ratio Lower Upper
168 100
99 56.0 44.0 66.0

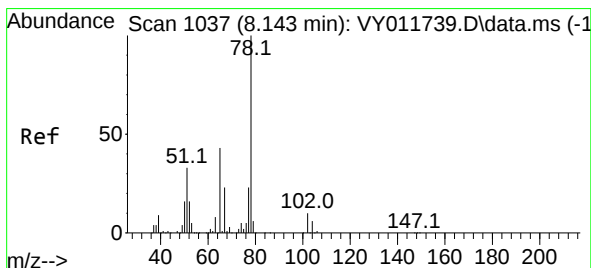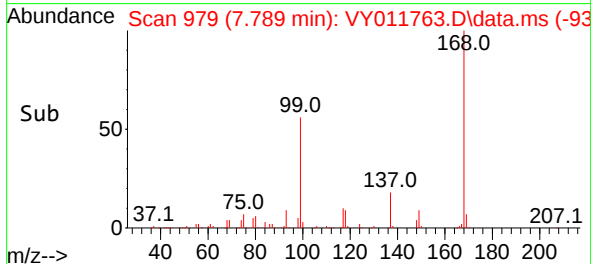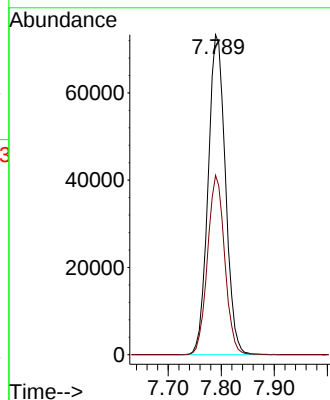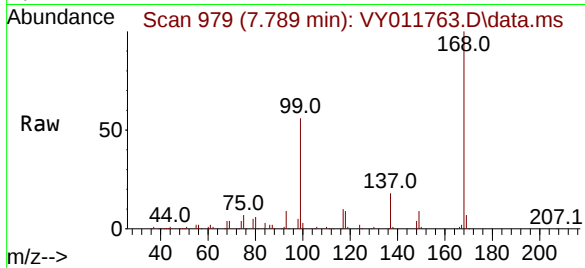

#33
1,2-Dichloroethane-d4
Concen: 61.553 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY011763.D
Acq: 12 Dec 2022 12:10

Tgt Ion: 65 Resp: 68625
Ion Ratio Lower Upper
65 100
67 52.4 0.0 103.2

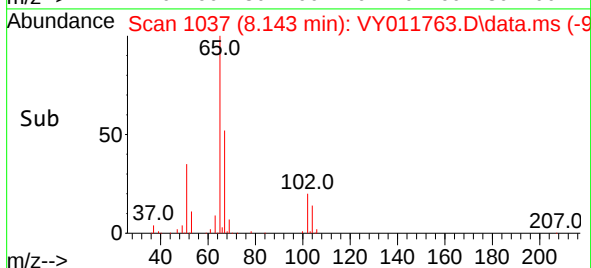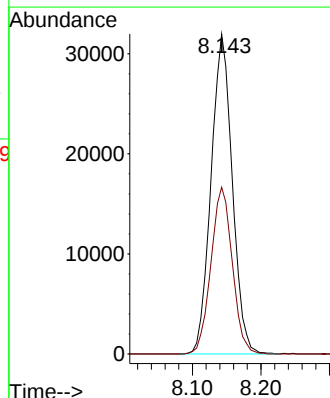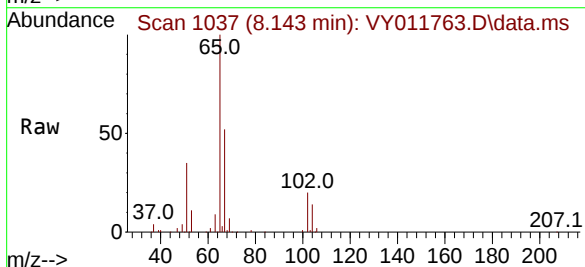

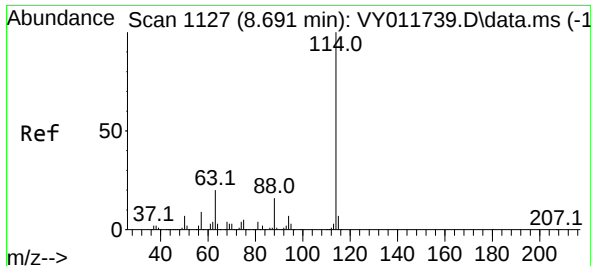

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY011763.D

Acq: 12 Dec 2022 12:10

Instrument :

MSVOA_Y

ClientSampleId :

NYE-SOIL-1208





Tgt Ion:114 Resp: 272236

Ion Ratio Lower Upper

114 100

63 19.1 0.0 39.6

88 14.7 0.0 32.2

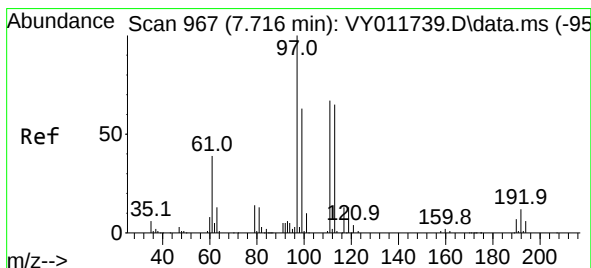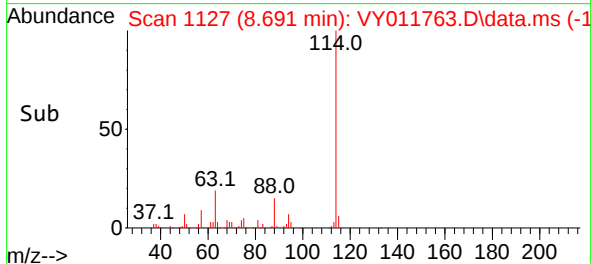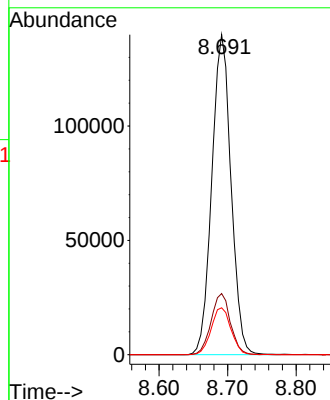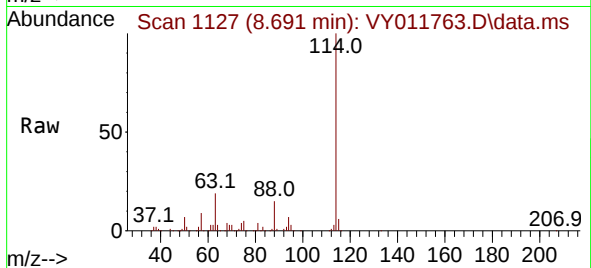

#35

Dibromofluoromethane

Concen: 57.413 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY011763.D

Acq: 12 Dec 2022 12:10




Tgt Ion:113 Resp: 68745


Ion Ratio Lower Upper

113 100

111 103.7 83.0 124.4

192 20.4 16.0 24.0

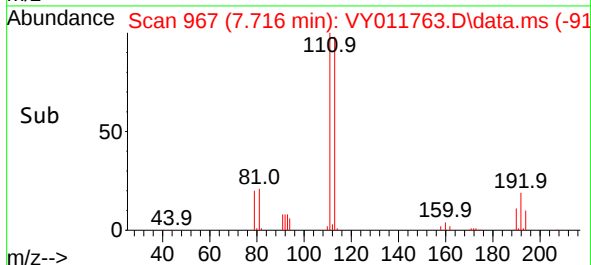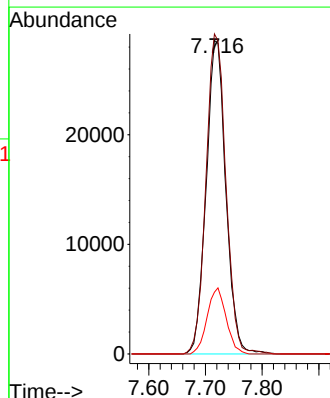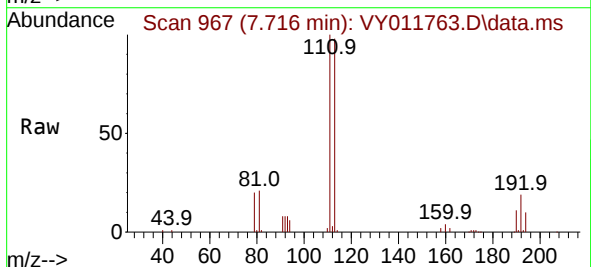

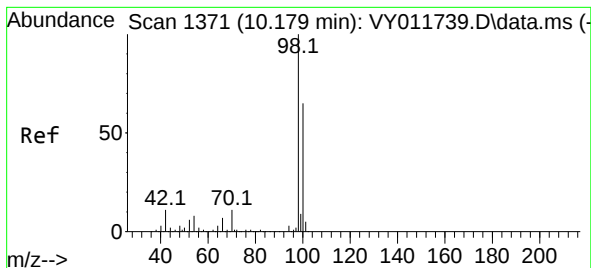

#50

Toluene-d8

Concen: 51.684 ug/l

RT: 10.179 min Scan# 1371

Delta R.T. -0.000 min

Lab File: VY011763.D

Acq: 12 Dec 2022 12:10

Instrument :

MSVOA_Y

ClientSampleId :





NYE-SOIL-1208

Tgt Ion: 98 Resp: 204071

Ion Ratio Lower Upper

98 100

100 64.3 51.9 77.9

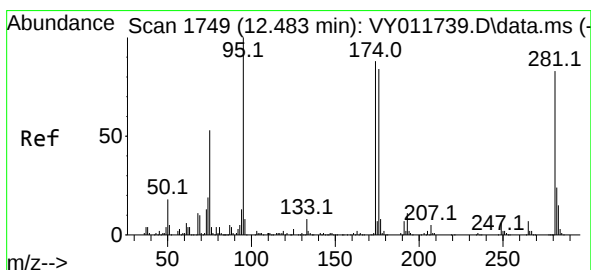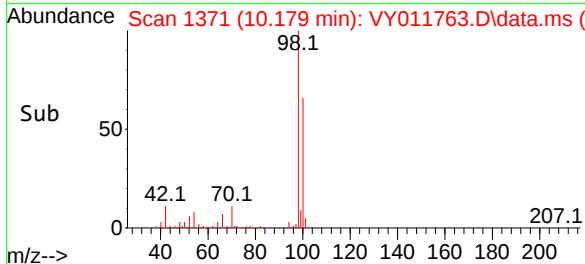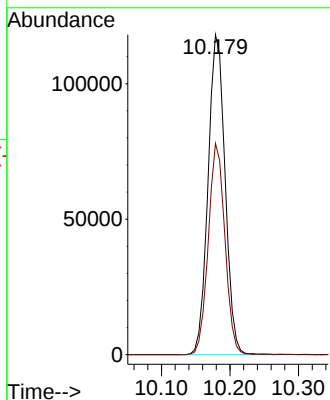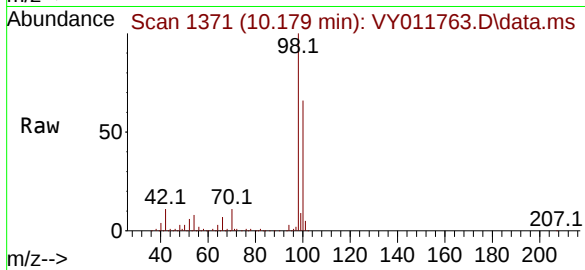

#62

4-Bromofluorobenzene

Concen: 48.879 ug/l

RT: 12.483 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VY011763.D

Acq: 12 Dec 2022 12:10




Tgt Ion: 95 Resp: 77310


Ion Ratio Lower Upper

95 100

174 87.9 0.0 172.0

176 85.4 0.0 167.6

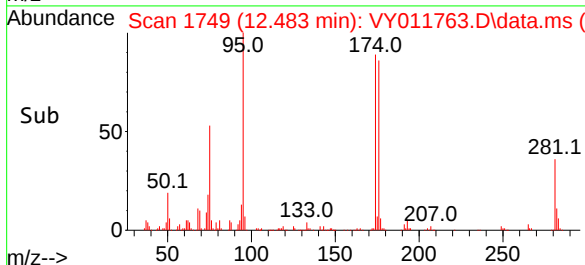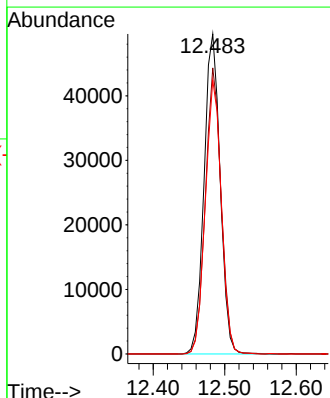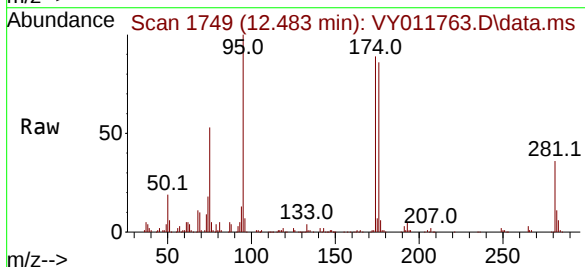

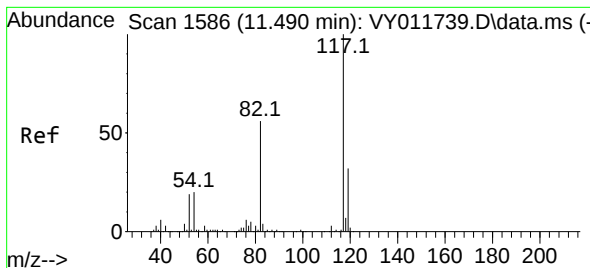

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY011763.D

Acq: 12 Dec 2022 12:10

Instrument :

MSVOA_Y

ClientSampleId :

NYE-SOIL-1208





Tgt Ion:117 Resp: 240405

Ion Ratio Lower Upper

117 100

82 55.1 44.8 67.2

119 32.4 25.4 38.2

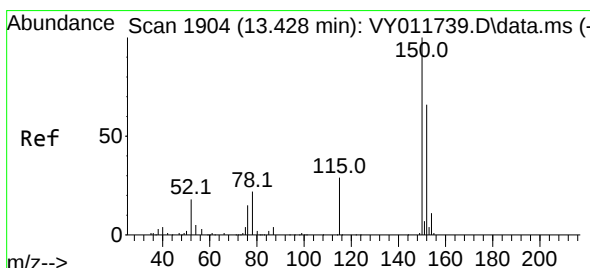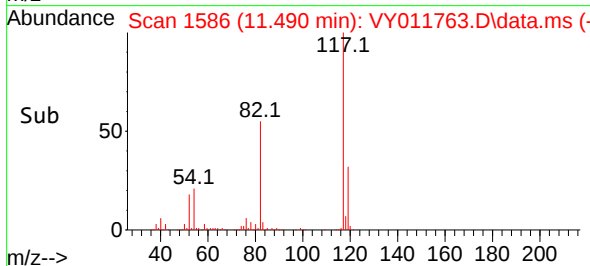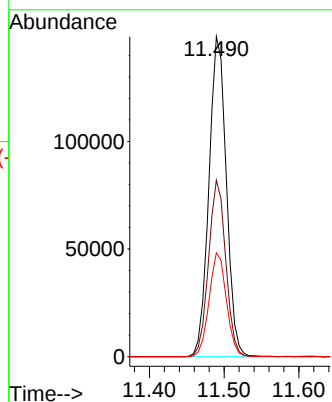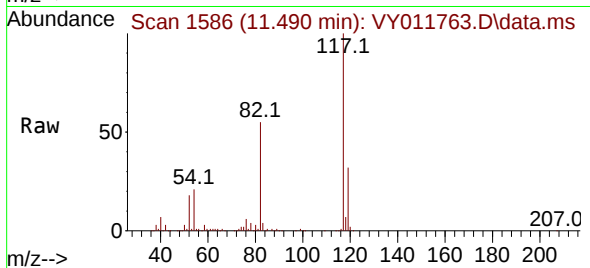

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY011763.D

Acq: 12 Dec 2022 12:10

Tgt Ion:152 Resp: 106287

Ion Ratio Lower Upper

152 100

115 57.7 29.1 87.3

150 157.1 0.0 342.6

