

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121520\
 Data File : VY003775.D
 Acq On : 15 Dec 2020 15:42
 Operator : SY/MD
 Sample : VY1215SBL01
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1215SBL01

Quant Time: Dec 16 05:04:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y121520S.M
 Quant Title : Sw846 8260
 QLast Update : Wed Dec 16 05:00:50 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	235807	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	380362	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	332155	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	154176	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	125437	42.89	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	85.78%		
35) Dibromofluoromethane	7.728	113	113558	41.27	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	82.54%		
50) Toluene-d8	10.179	98	448560	41.18	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery =	82.36%		
62) 4-Bromofluorobenzene	12.483	95	144807	38.69	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery =	77.38%		


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121520\
Data File : VY003775.D
Acq On : 15 Dec 2020 15:42
Operator : SY/MD
Sample : VY1215SBL01
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1215SBL01

Quant Time: Dec 16 05:04:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y121520S.M
Quant Title : SW846 8260
QLast Update : Wed Dec 16 05:00:50 2020
Response via : Initial Calibration




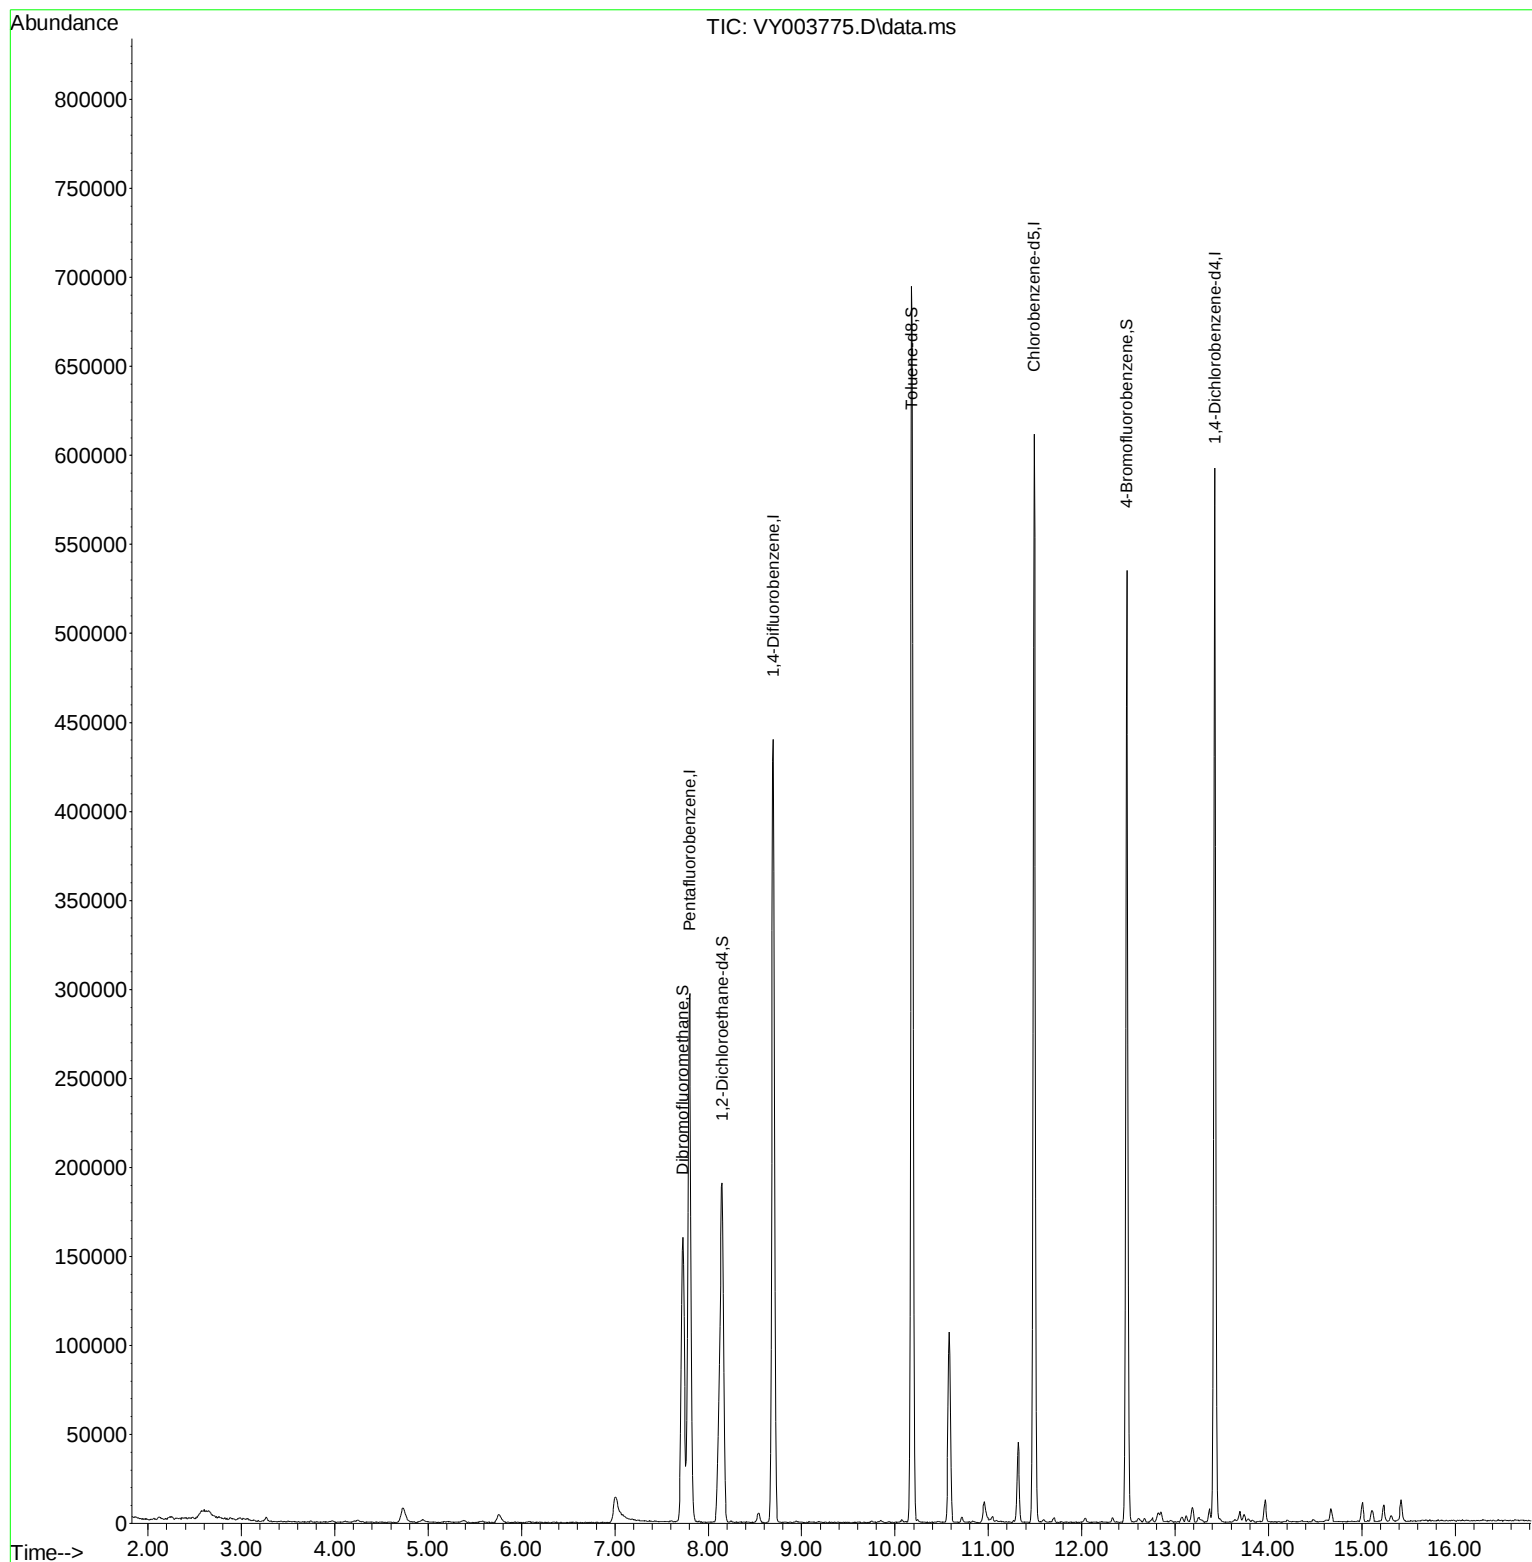


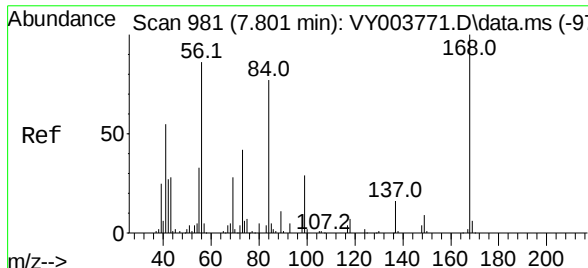

Pentafluorobenzene
 Concen: 50.00 ug/l
 RT: 7.801 min Scan# 981
 Delta R.T. 0.000 min
 Lab File: VY003775.D
 Acq: 15 Dec 2020 15:42




Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1215SBL01

Tgt Ion:168 Resp: 235807
 Ion Ratio Lower Upper
 168 100
 99 50.4 41.9 62.9

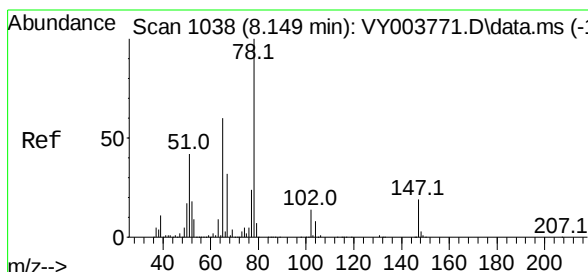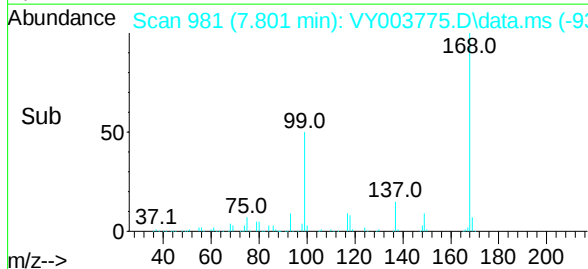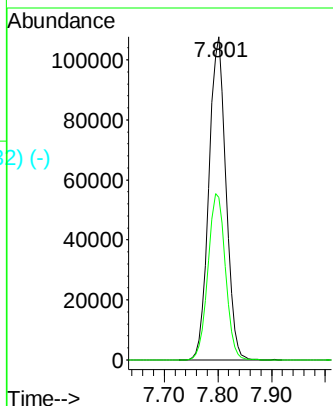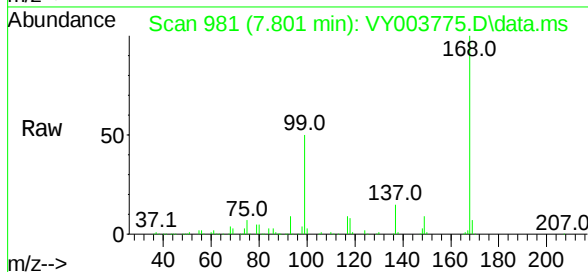


1,2-Dichloroethane-d4
 Concen: 42.89 ug/l
 RT: 8.149 min Scan# 1038
 Delta R.T. -0.000 min
 Lab File: VY003775.D
 Acq: 15 Dec 2020 15:42

Tgt Ion: 65 Resp: 125437
 Ion Ratio Lower Upper
 65 100
 67 53.3 0.0 107.6

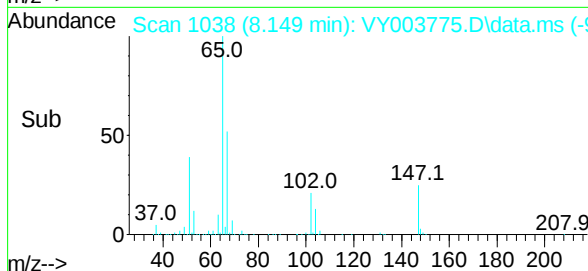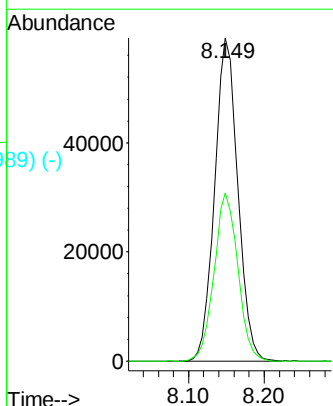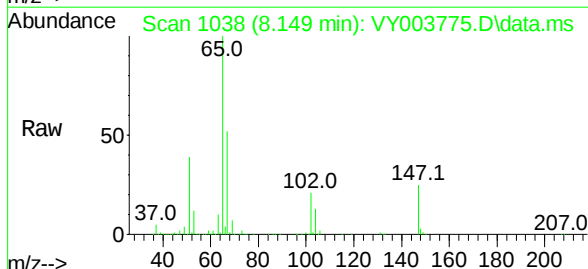



Abundance Scan 1128 (8.697 min): VY003771.D\data.ms (-1116)

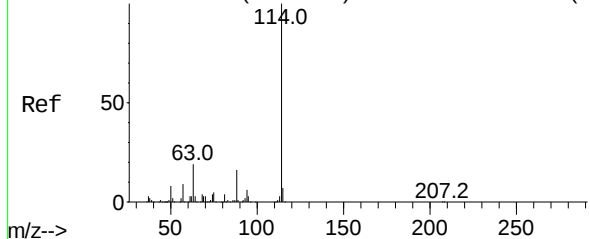


1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY003775.D
Acq: 15 Dec 2020 15:42

Instrument :
MSVOA_Y
ClientSampleId :
VY1215SBL01


Tgt Ion	Ratio	Lower	Upper
114	100		
63	19.6	0.0	38.4
88	14.8	0.0	31.8

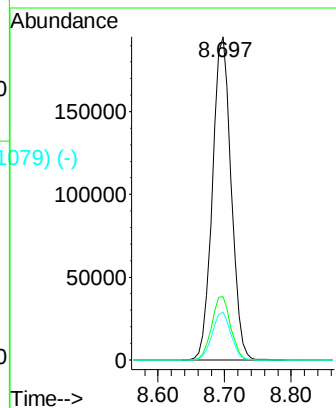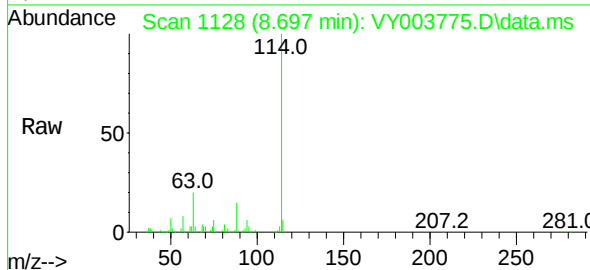

Abundance Scan 1128 (8.697 min): VY003775.D\data.ms (-1079) (-)


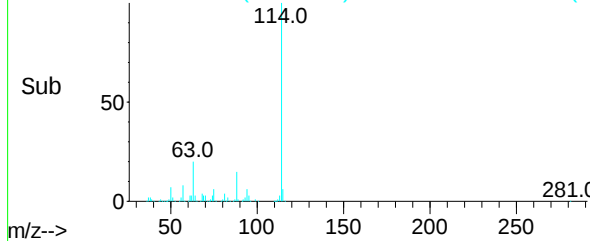


Abundance Scan 969 (7.728 min): VY003771.D\data.ms (-958)

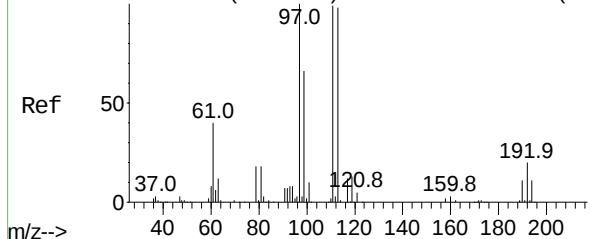



Dibromofluoromethane
Concen: 41.27 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY003775.D
Acq: 15 Dec 2020 15:42

Tgt Ion	Ratio	Lower	Upper
113	100		
111	101.2	82.2	123.2
192	21.0	16.7	25.1

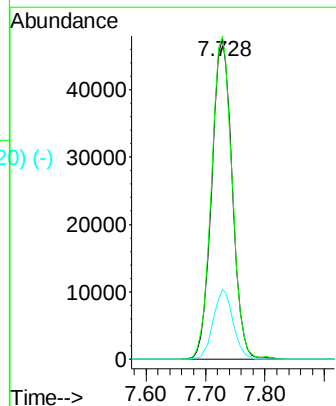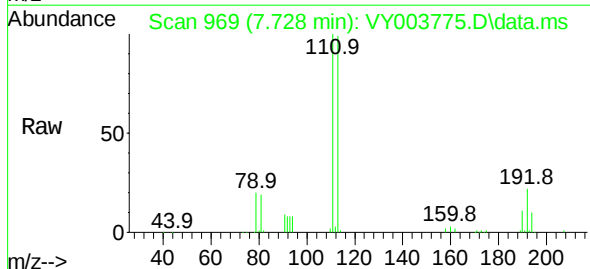

Abundance Scan 969 (7.728 min): VY003775.D\data.ms (-920) (-)




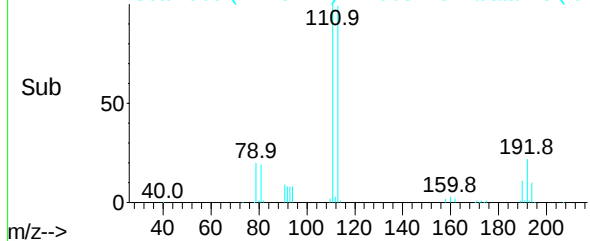


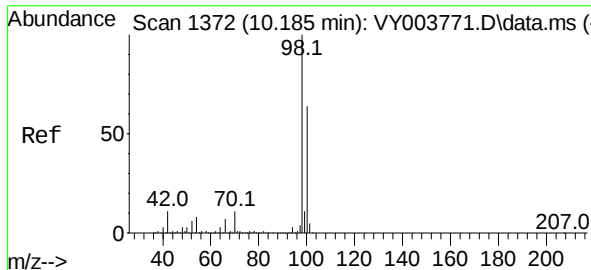

Scan 1372 (10.185 min): VY003771.D\data.ms (-1359) (-)
 Toluene-d8
 Concen: 41.18 ug/l
 RT: 10.179 min Scan# 1371
 Delta R.T. -0.006 min
 Lab File: VY003775.D
 Acq: 15 Dec 2020 15:42




Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1215SBL01


Tgt Ion: 98 Resp: 448560
 Ion Ratio Lower Upper
 98 100
 100 64.6 51.6 77.4

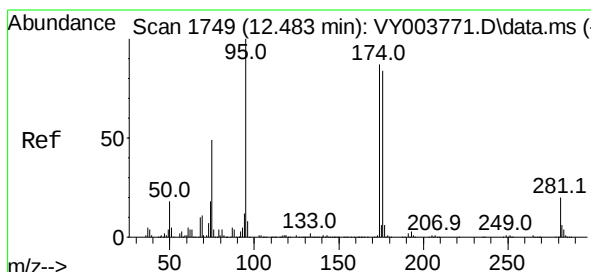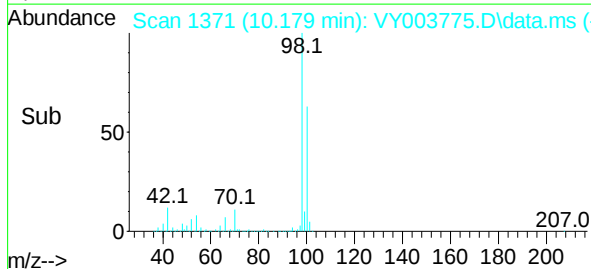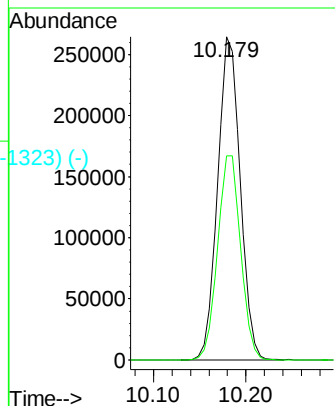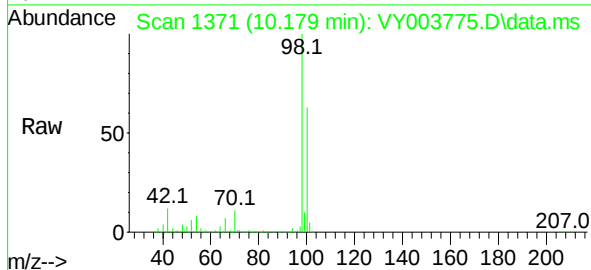

Scan 1749 (12.483 min): VY003771.D\data.ms (-1702) (-)
 4-Bromofluorobenzene
 Concen: 38.69 ug/l
 RT: 12.483 min Scan# 1749
 Delta R.T. -0.000 min
 Lab File: VY003775.D
 Acq: 15 Dec 2020 15:42

Tgt Ion: 95 Resp: 144807
 Ion Ratio Lower Upper
 95 100
 174 85.4 0.0 170.8
 176 82.9 0.0 165.0


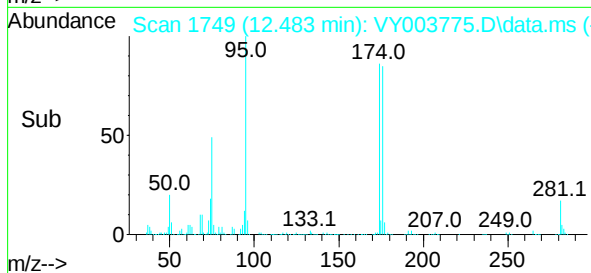
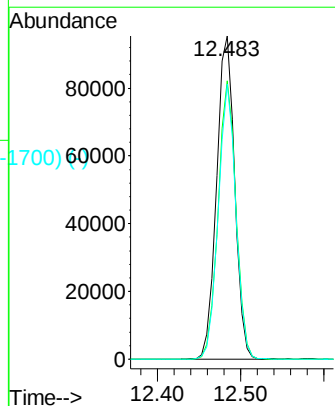
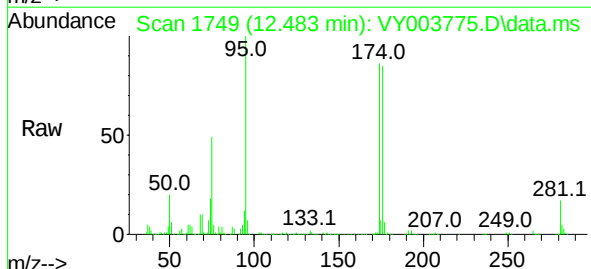


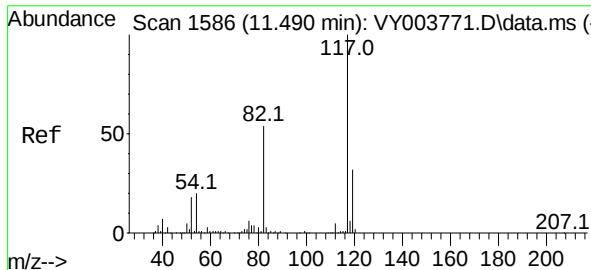

Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.000 min
Lab File: VY003775.D
Acq: 15 Dec 2020 15:42

Instrument :
MSVOA_Y
ClientSampleId :
VY1215SBL01

Tgt Ion:	117	Resp:	332155
Ion	Ratio	Lower	Upper
117	100		
82	55.3	43.0	64.6
119	32.7	25.7	38.5

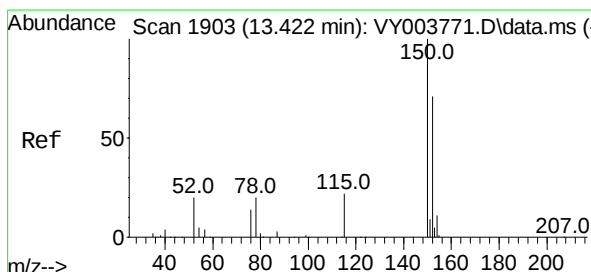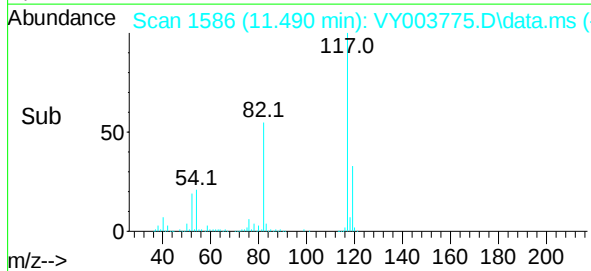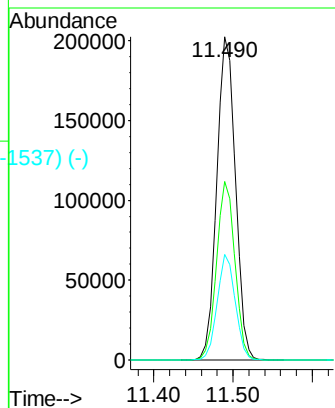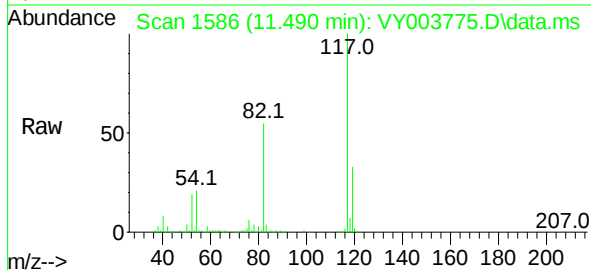

1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY003775.D
Acq: 15 Dec 2020 15:42

Tgt Ion:	152	Resp:	154176
Ion	Ratio	Lower	Upper
152	100		
115	56.4	28.0	83.9
150	156.8	0.0	347.6

