

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121522\
 Data File : VY011882.D
 Acq On : 15 Dec 2022 19:08
 Operator : KP/MD
 Sample : N6038-05
 Misc : 6.33g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 RB-31-(1-3)

Quant Time: Dec 16 00:16:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120922S.M
 Quant Title : SW846 8260
 QLast Update : Sat Dec 10 04:19:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	241565	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	403148	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	320188	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	105624	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	90359	55.327	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.660%
35) Dibromofluoromethane	7.716	113	101752	57.382	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	114.760%
50) Toluene-d8	10.179	98	264512	44.283	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	88.560%
62) 4-Bromofluorobenzene	12.483	95	101066	42.560	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	85.120%
Target Compounds						
20) Methylene Chloride	4.716	84	28393	7.045	ug/l	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121522\
Data File : VY011882.D
Acq On : 15 Dec 2022 19:08
Operator : KP/MD
Sample : N6038-05
Misc : 6.33g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
RB-31-(1-3)

Quant Time: Dec 16 00:16:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120922S.M
Quant Title : SW846 8260
QLast Update : Sat Dec 10 04:19:59 2022
Response via : Initial Calibration




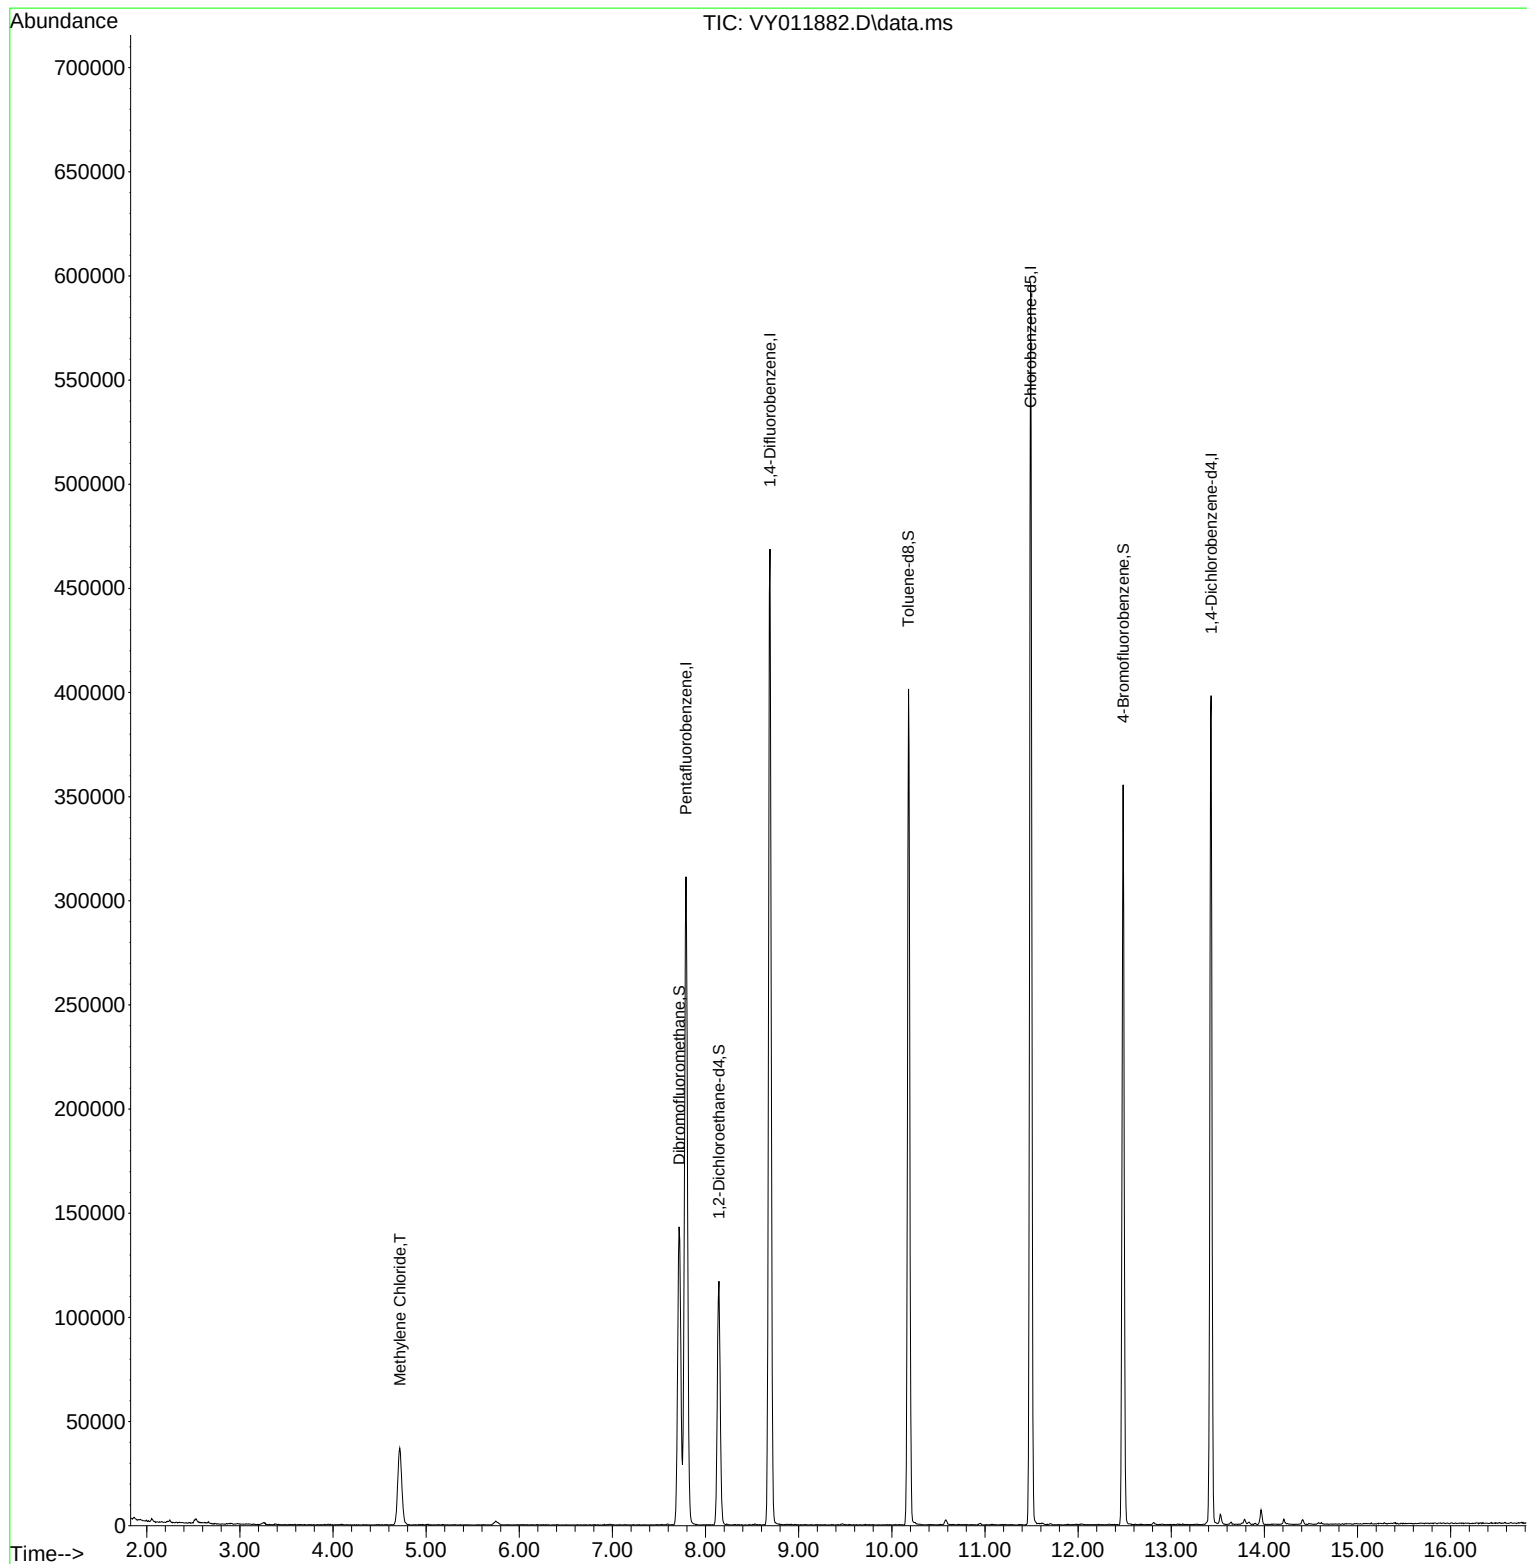


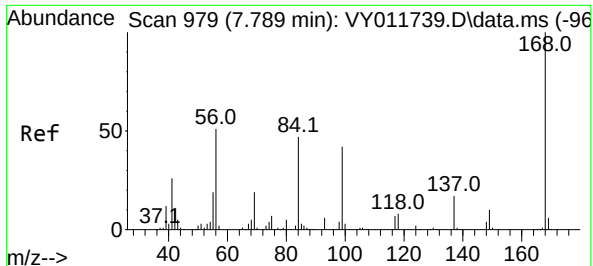

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY011882.D
Acq: 15 Dec 2022 19:08




Instrument :
MSVOA_Y
ClientSampleId :
RB-31-(1-3)


Tgt Ion:168 Resp: 241565
Ion Ratio Lower Upper
168 100
99 55.8 44.0 66.0

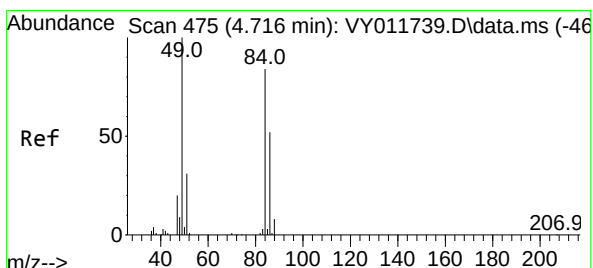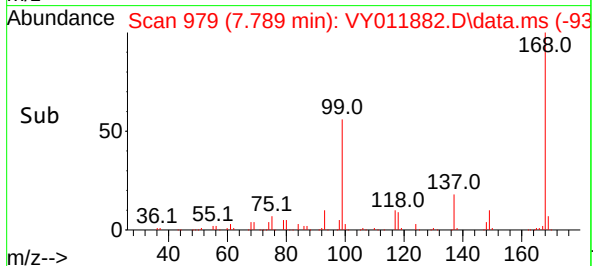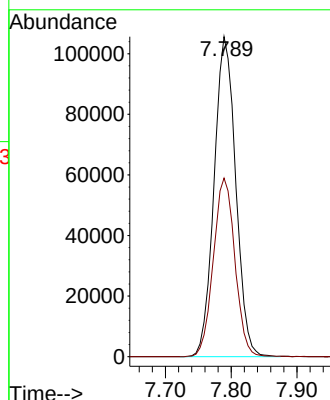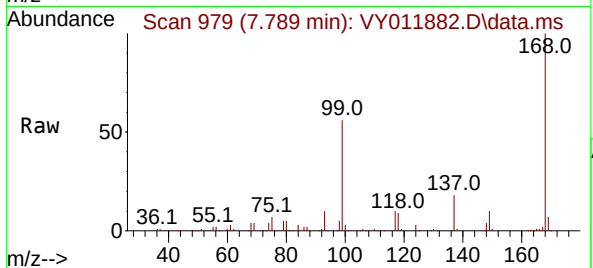

#20
Methylene Chloride
Concen: 7.045 ug/l
RT: 4.716 min Scan# 475
Delta R.T. 0.000 min
Lab File: VY011882.D
Acq: 15 Dec 2022 19:08

Tgt Ion: 84 Resp: 28393
Ion Ratio Lower Upper
84 100
49 110.9 95.4 143.2
51 33.7 29.9 44.9
86 63.4 49.6 74.4

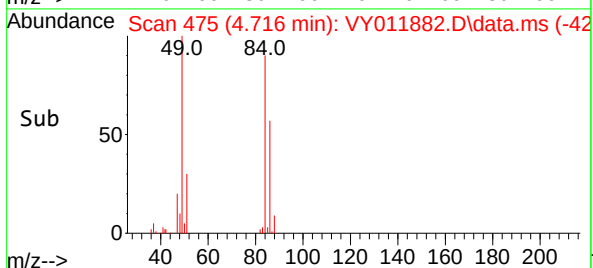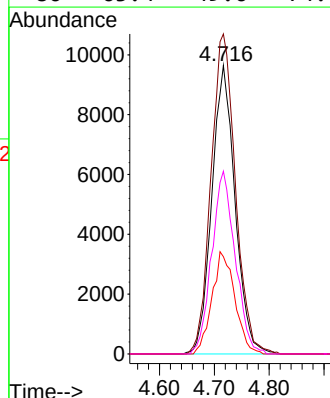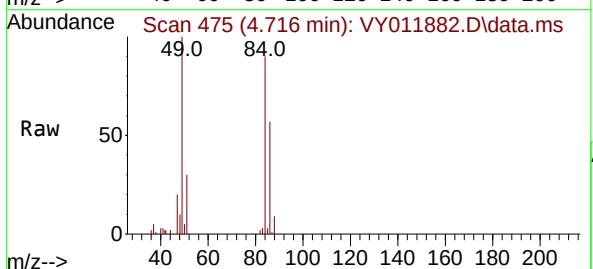

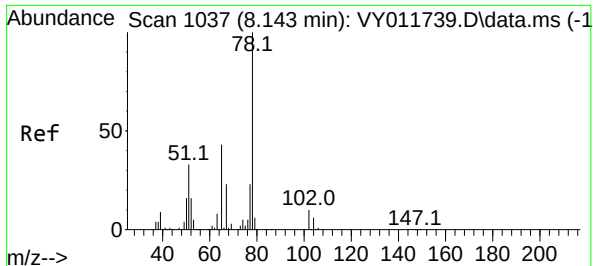

#33

1,2-Dichloroethane-d4

Concen: 55.327 ug/l

RT: 8.143 min Scan# 1

Delta R.T. -0.000 min

Lab File: VY011882.D

Acq: 15 Dec 2022 19:08

Instrument :

MSVOA_Y

ClientSampleId :





RB-31-(1-3)

Tgt Ion: 65 Resp: 90359

Ion Ratio Lower Upper

65 100

67 53.5 0.0 103.2

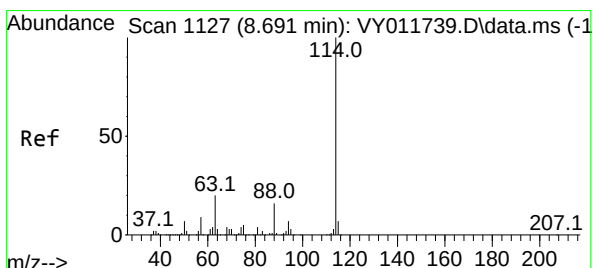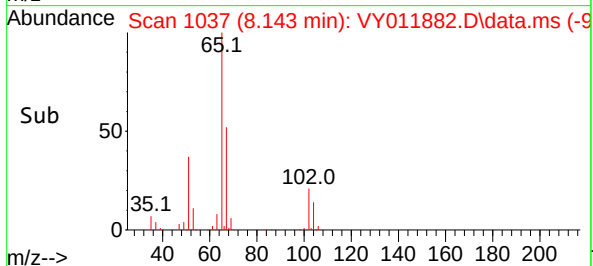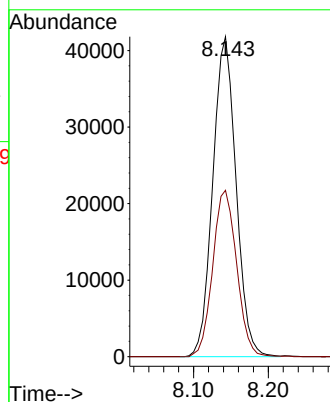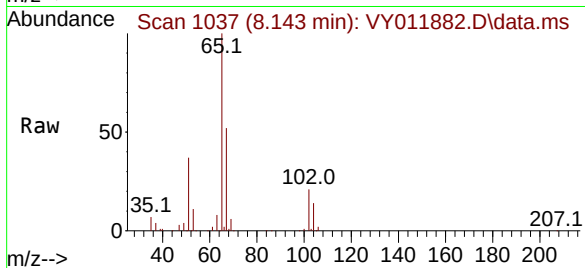

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY011882.D

Acq: 15 Dec 2022 19:08




Tgt Ion: 114 Resp: 403148


Ion Ratio Lower Upper

114 100

63 19.4 0.0 39.6

88 15.0 0.0 32.2


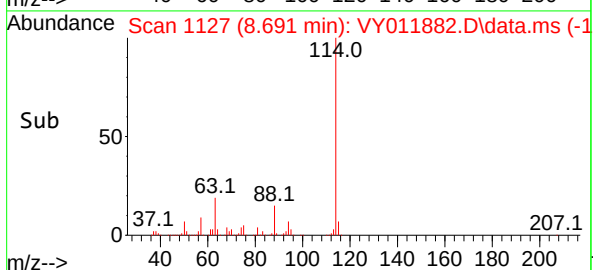
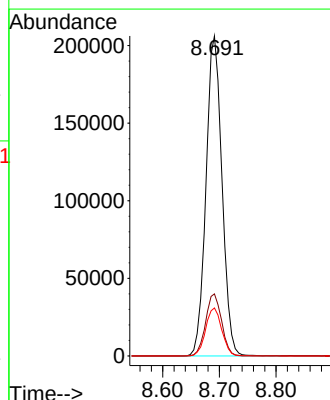
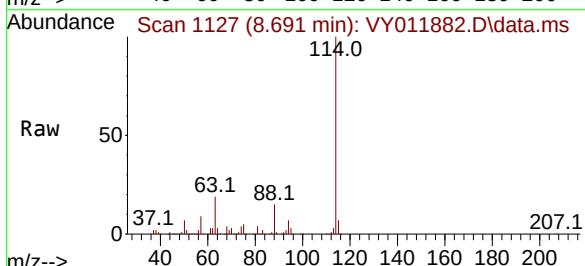


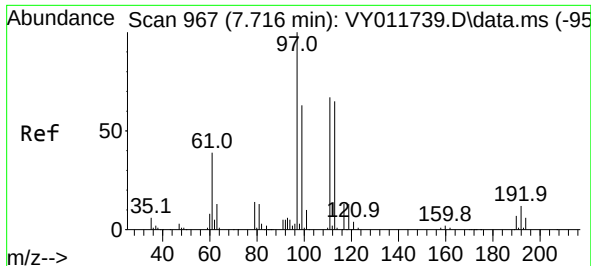

#35
Dibromofluoromethane
Concen: 57.382 ug/l
RT: 7.716 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY011882.D
Acq: 15 Dec 2022 19:08




Instrument :
MSVOA_Y
ClientSampleId :
RB-31-(1-3)


Tgt Ion:113 Resp: 101752
Ion Ratio Lower Upper
113 100
111 103.2 83.0 124.4
192 20.9 16.0 24.0

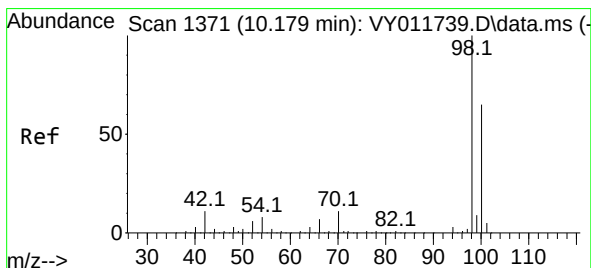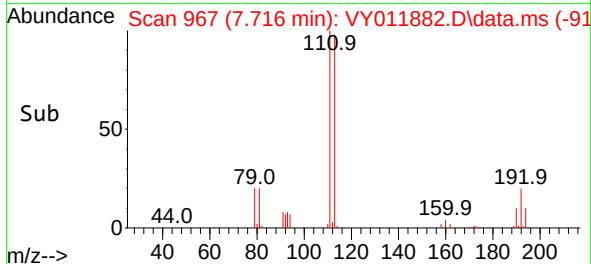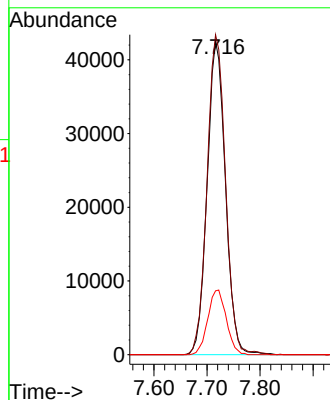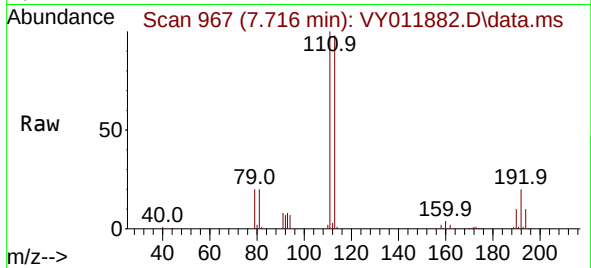

#50
Toluene-d8
Concen: 44.283 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY011882.D
Acq: 15 Dec 2022 19:08

Tgt Ion: 98 Resp: 264512
Ion Ratio Lower Upper
98 100
100 63.8 51.9 77.9


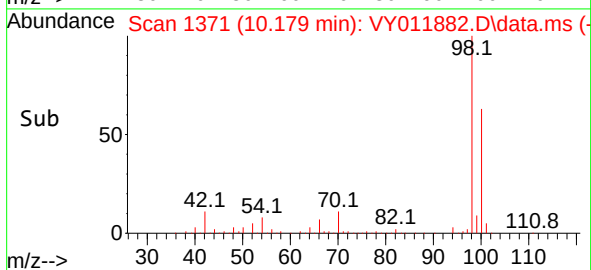
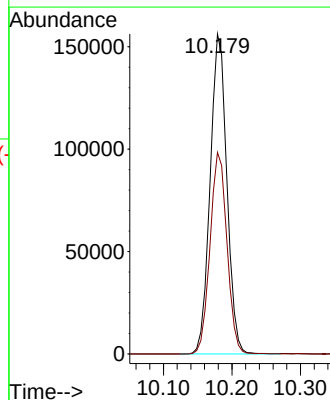
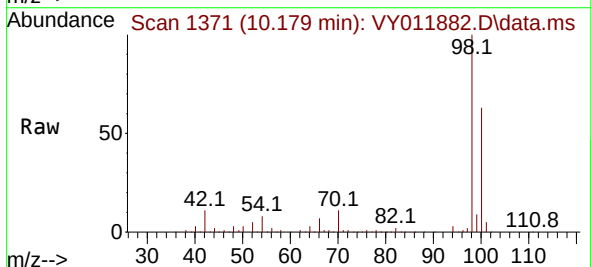


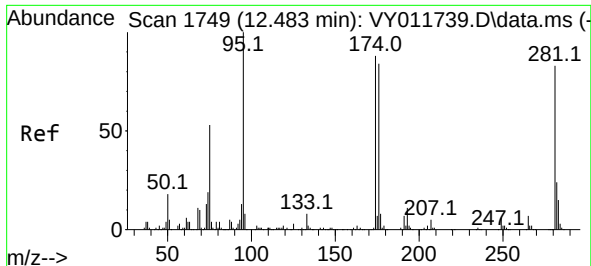

#62
4-Bromofluorobenzene
Concen: 42.560 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY011882.D
Acq: 15 Dec 2022 19:08




Instrument :
MSVOA_Y
ClientSampleId :
RB-31-(1-3)


Tgt Ion: 95 Resp: 101066
Ion Ratio Lower Upper
95 100
174 89.0 0.0 172.0
176 85.1 0.0 167.6

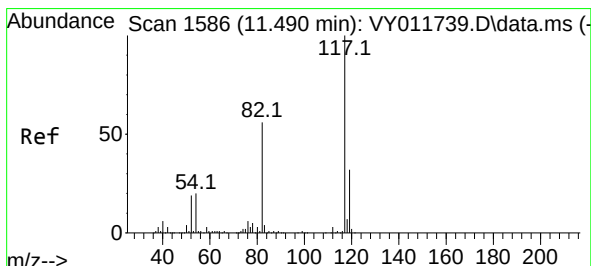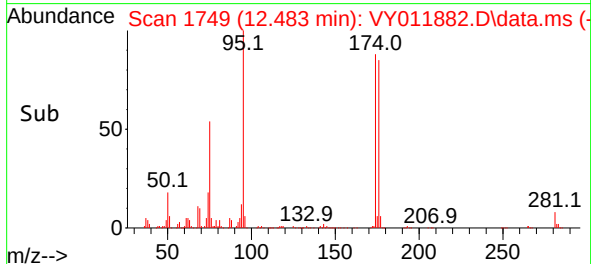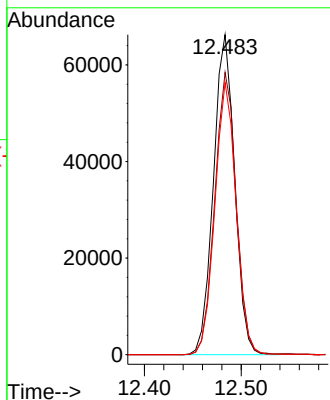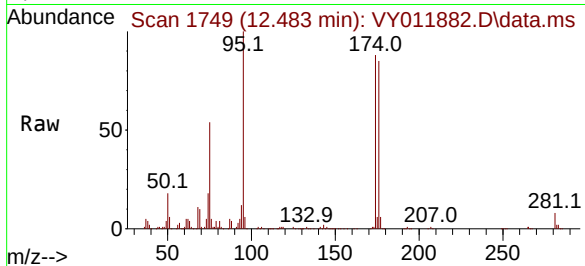

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. 0.000 min
Lab File: VY011882.D
Acq: 15 Dec 2022 19:08

Tgt Ion: 117 Resp: 320188
Ion Ratio Lower Upper
117 100
82 54.0 44.8 67.2
119 31.7 25.4 38.2

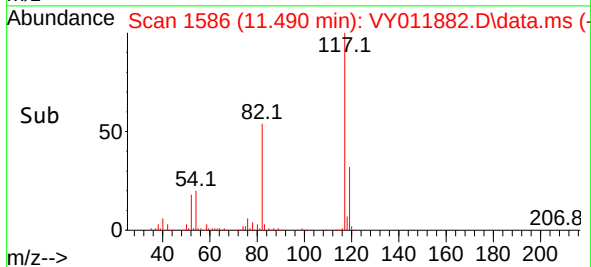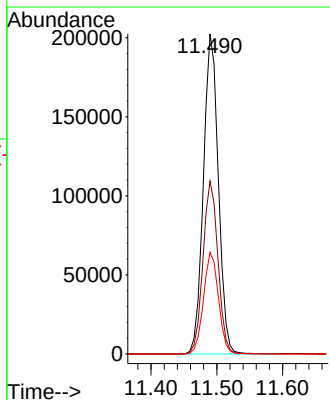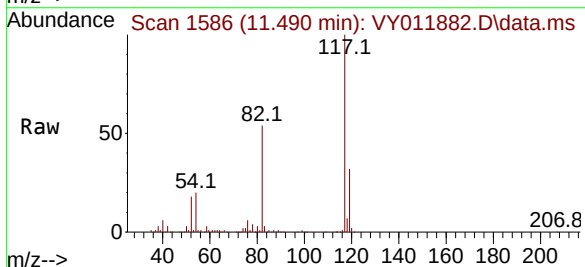

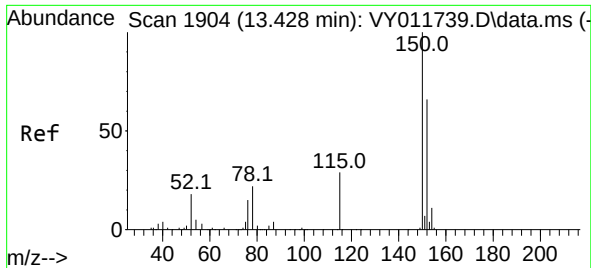

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY011882.D


Acq: 15 Dec 2022 19:08

Instrument :

MSVOA_Y

ClientSampleId :

RB-31-(1-3)

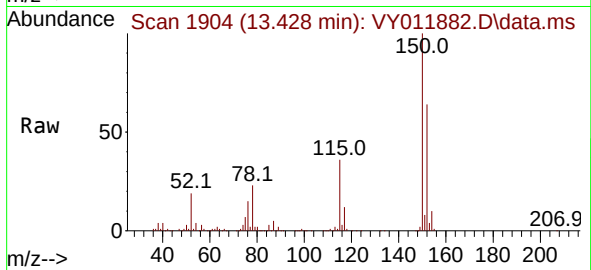

Tgt Ion:152 Resp: 105624

Ion Ratio Lower Upper

152 100

115 57.3 29.1 87.3

150 157.0 0.0 342.6

