

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY011422\
 Data File : VY007162.D
 Acq On : 14 Jan 2022 12:36
 Operator : SY/MD
 Sample : N1119-06
 Misc : 5.09g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Jan 14 13:46:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 14 05:48:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	58778	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	99929	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	74841	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	23183	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	29516	40.925	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	81.860%
35) Dibromofluoromethane	7.716	113	30053	44.476	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	88.960%
50) Toluene-d8	10.179	98	117995	47.791	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	95.580%
62) 4-Bromofluorobenzene	12.477	95	34052	38.772	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	77.540%

Target Compounds			Qvalue			
11) Tert butyl alcohol	4.930	59	268	Below Cal	#	73
16) Acetone	3.942	43	5473	29.240	ug/l #	85
25) 2-Butanone	6.972	43	1828	7.554	ug/l #	68
26) 2,2-Dichloropropane	6.972	77	1277	1.333	ug/l #	53
31) Cyclohexane	7.783	56	4350	3.568	ug/l #	73
36) 1,1-Dichloropropene	7.783	75	5671	5.255	ug/l #	49
38) Carbon Tetrachloride	7.789	117	6324	5.571	ug/l #	18
39) Methylcyclohexane	9.179	83	19989	15.170	ug/l	97
48) Methyl methacrylate	9.240	41	1162	2.371	ug/l #	26
51) 4-Methyl-2-Pentanone	10.179	43	2339	4.281	ug/l	100
55) 1,1,2-Trichloroethane	10.618	97	8029	13.674	ug/l #	22
56) Ethyl methacrylate	10.520	69	3857	4.663	ug/l #	1
59) 2-Hexanone	10.801	43	19151	51.643	ug/l #	27
64) Tetrachloroethene	10.715	164	817	1.514	ug/l #	83
67) Ethyl Benzene	11.587	91	5644	1.835	ug/l	93
68) m/p-Xylenes	11.697	106	2182	1.909	ug/l	95
73) Isopropylbenzene	12.331	105	12024	6.005	ug/l	97
74) N-amyl acetate	12.124	43	70501	131.668	ug/l #	54
75) 1,1,2,2-Tetrachloroethane	12.557	83	6573	16.881	ug/l #	60
76) 1,2,3-Trichloropropane	12.477	75	16747	63.352	ug/l #	100
78) n-propylbenzene	12.672	91	29411	11.849	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.477	75	16747	115.981	ug/l #	9
83) tert-Butylbenzene	13.069	119	2652	1.867	ug/l	89
84) 1,2,4-Trimethylbenzene	13.117	105	3166	1.943	ug/l	95
85) sec-Butylbenzene	13.251	105	39292	18.488	ug/l	85
86) p-Isopropyltoluene	13.367	119	2748	1.573	ug/l	97
89) n-Butylbenzene	13.697	91	37894	22.035	ug/l #	80
90) Hexachloroethane	13.971	117	6948	20.349	ug/l #	16
92) 1,2-Dibromo-3-Chloropr...	14.379	75	339	5.041	ug/l #	27
93) 1,2,4-Trichlorobenzene	15.001	180	1385	3.002	ug/l #	1
95) Naphthalene	15.233	128	1883	1.921	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.446	180	1221	3.102	ug/l #	13

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jan 14 13:46:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
Quant Title : SW846 8260
QLast Update : Fri Jan 14 05:48:29 2022
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:168 Resp: 58778
Ion Ratio Lower Upper
168 100
99 65.9 49.1 73.7

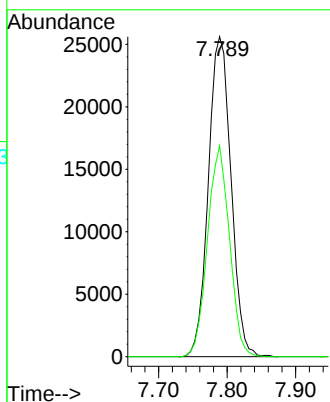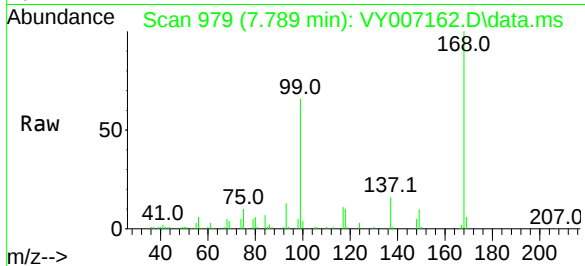

#16
Acetone
Concen: 29.240 ug/l
RT: 3.942 min Scan# 348
Delta R.T. -0.006 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Tgt Ion: 43 Resp: 5473
Ion Ratio Lower Upper
43 100
58 21.6 23.8 35.6#

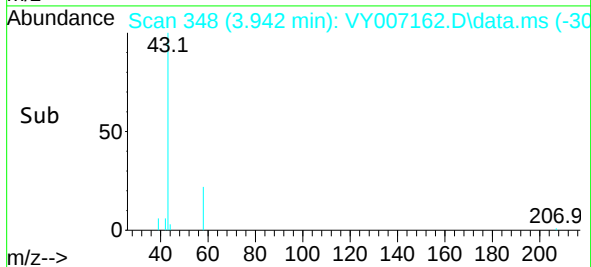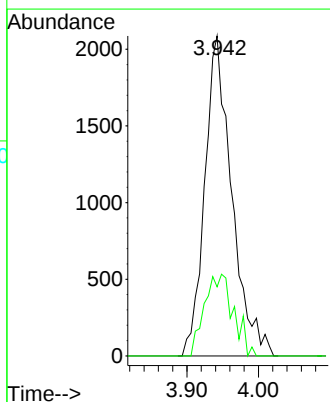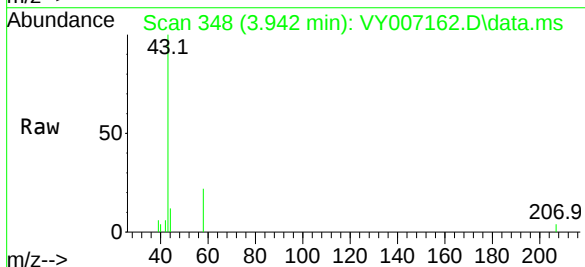



#25

2-Butanone

Concen: 7.554 ug/l

RT: 6.972 min Scan# 845

Delta R.T. -0.012 min


Lab File: VY007162.D

Acq: 14 Jan 2022 12:36

Instrument :

MSVOA_Y

ClientSampleId :



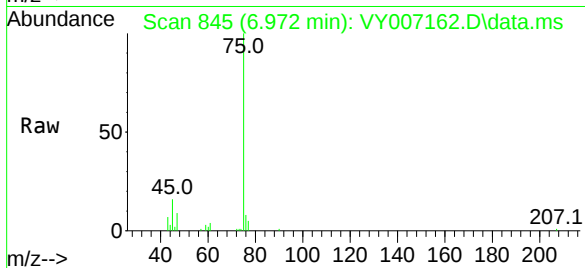


Tgt Ion: 43 Resp: 1828

Ion Ratio Lower Upper

43 100

72 10.9 21.9 32.9#

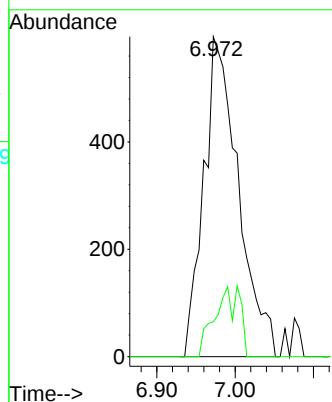

#26

2,2-Dichloropropane

Concen: 1.333 ug/l

RT: 6.972 min Scan# 845

Delta R.T. -0.012 min

Lab File: VY007162.D




Acq: 14 Jan 2022 12:36


Tgt Ion: 77 Resp: 1277

Ion Ratio Lower Upper

77 100


97 0.0 11.3 33.8#

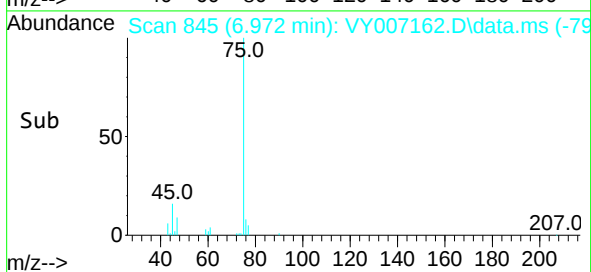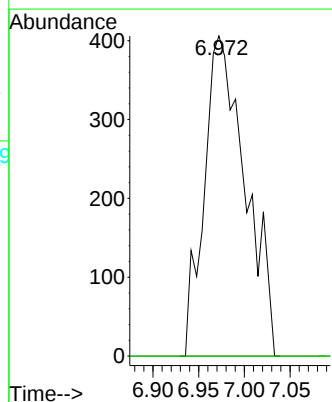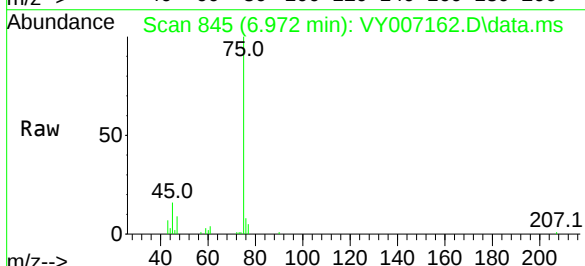






#31
Cyclohexane
Concen: 3.568 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Instrument :
MSVOA_Y
ClientSampleId :



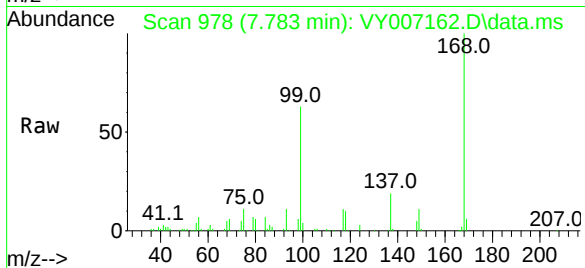



Tgt Ion: 56 Resp: 4350
Ion Ratio Lower Upper
56 100
69 77.9 27.2 40.8#
84 98.5 72.1 108.1

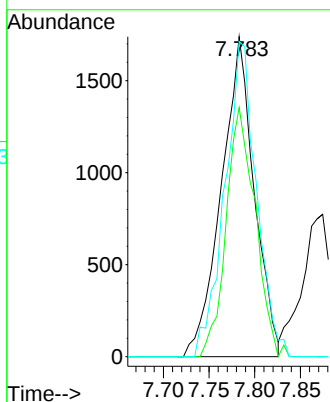

#33
1,2-Dichloroethane-d4
Concen: 40.925 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.001 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36


Tgt Ion: 65 Resp: 29516
Ion Ratio Lower Upper
65 100
67 50.6 0.0 105.6

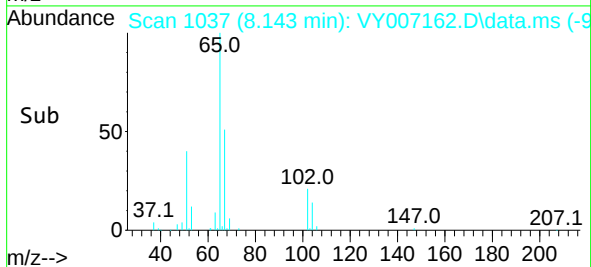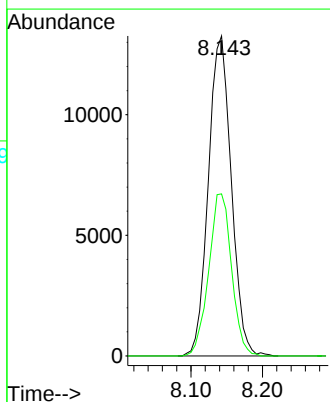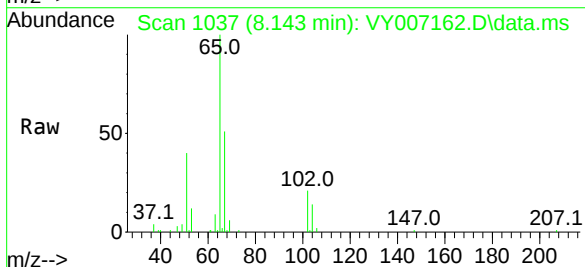






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.001 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion	Ratio	Lower	Upper
114	100		
63	19.7	0.0	39.2
88	16.7	0.0	31.0

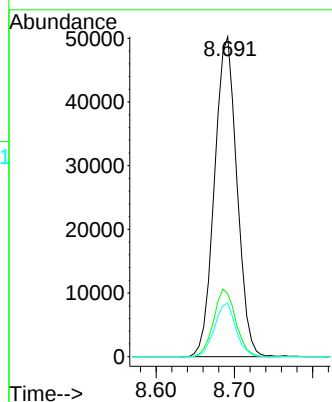

#35
Dibromofluoromethane
Concen: 44.476 ug/l
RT: 7.716 min Scan# 967
Delta R.T. 0.001 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36


Tgt Ion	Ratio	Lower	Upper
113	100		
111	105.6	82.2	123.4
192	16.9	14.2	21.4

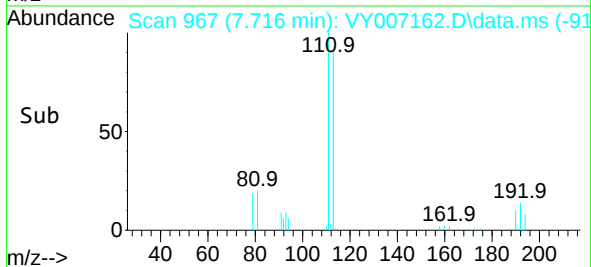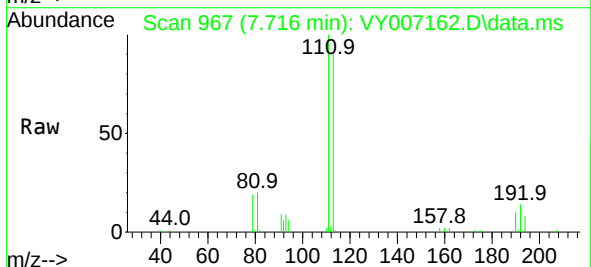



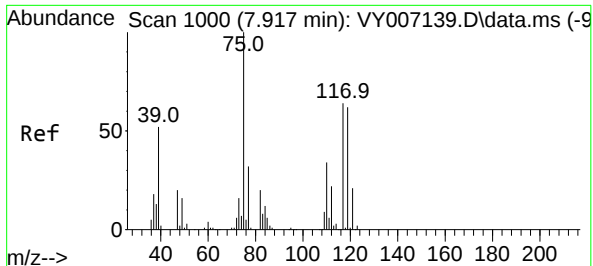


#36
1,1-Dichloropropene
Concen: 5.255 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.134 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Instrument :
MSVOA_Y
ClientSampleId :



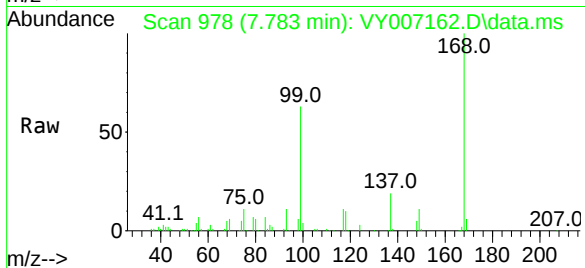



Tgt Ion: 75 Resp: 5671
Ion Ratio Lower Upper
75 100
110 7.8 17.3 51.9#
77 0.0 24.7 37.1#

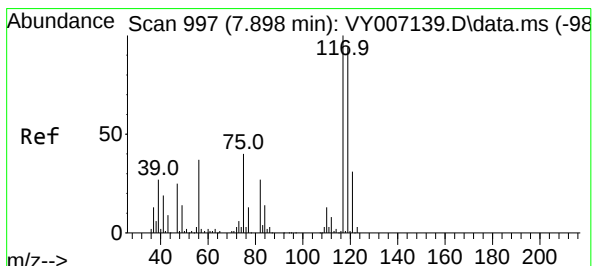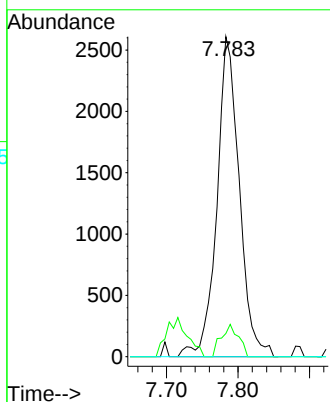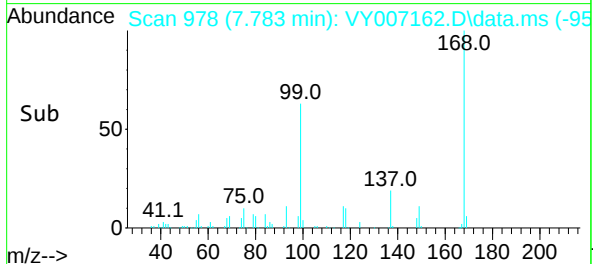

#38
Carbon Tetrachloride
Concen: 5.571 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.109 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Tgt Ion: 117 Resp: 6324
Ion Ratio Lower Upper
117 100
119 8.0 77.2 115.8#
121 0.0 24.2 36.2#

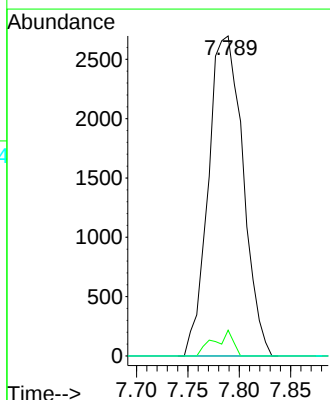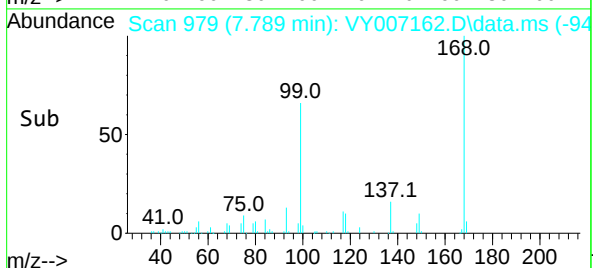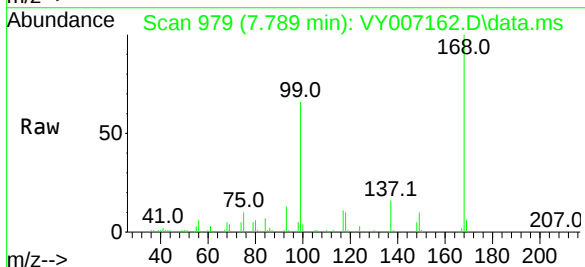



#39

Methylcyclohexane

Concen: 15.170 ug/l

RT: 9.179 min Scan# 11

Delta R.T. -0.006 min


Lab File: VY007162.D

Acq: 14 Jan 2022 12:36

Instrument :

MSVOA_Y

ClientSampleId :

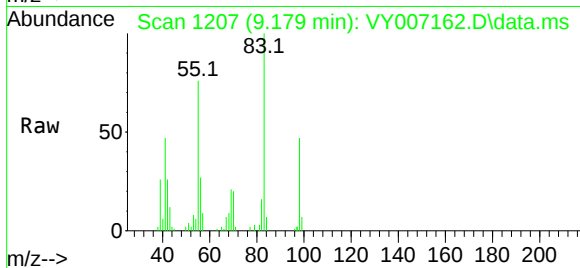




Tgt Ion: 83 Resp: 19989

Ion Ratio Lower Upper

83 100

55 75.7 58.8 88.2

98 46.7 38.7 58.1



#48

Methyl methacrylate

Concen: 2.371 ug/l

RT: 9.240 min Scan# 1217

Delta R.T. -0.054 min

Lab File: VY007162.D

Acq: 14 Jan 2022 12:36




Tgt Ion: 41 Resp: 1162


Ion Ratio Lower Upper

41 100

69 0.0 70.5 105.7#

39 25.8 43.8 65.8#


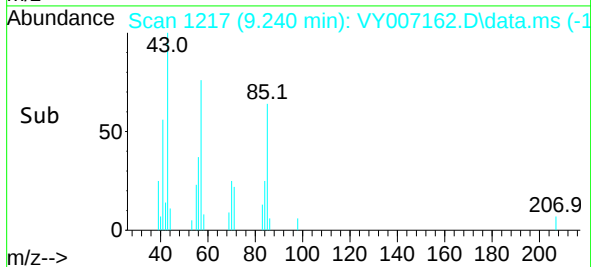

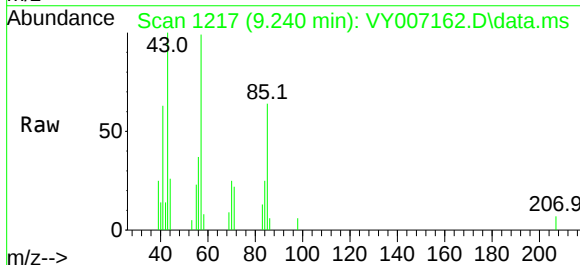




#50
Toluene-d8
Concen: 47.791 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.001 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 98 Resp: 117995
Ion Ratio Lower Upper
98 100
100 63.0 52.2 78.2

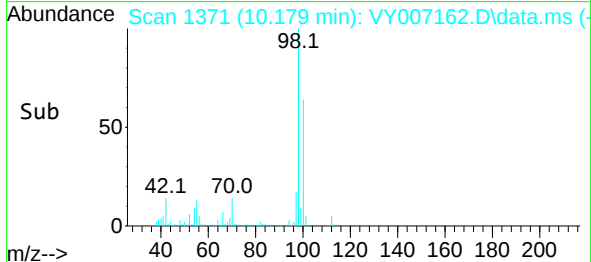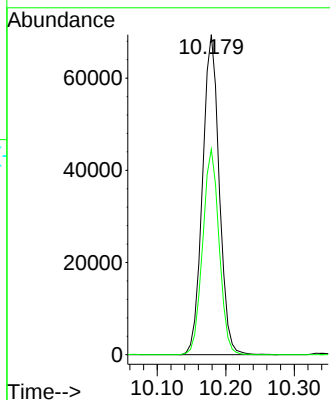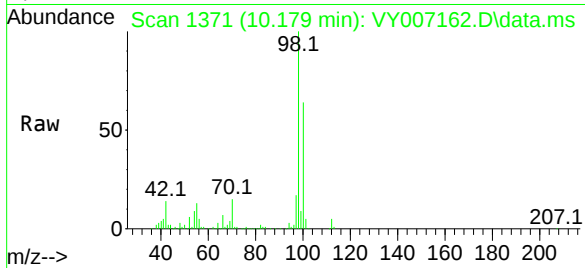

#51
4-Methyl-2-Pentanone
Concen: 4.281 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.110 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36


Tgt Ion: 43 Resp: 2339
Ion Ratio Lower Upper
43 100
58 41.0 32.8 49.2

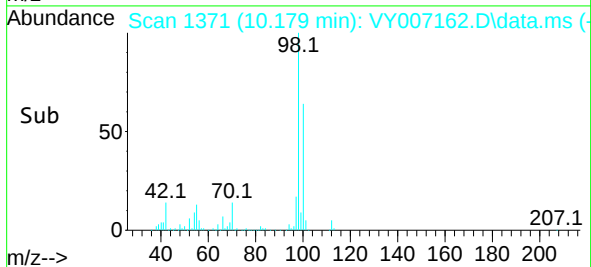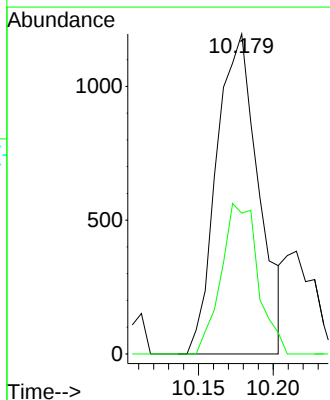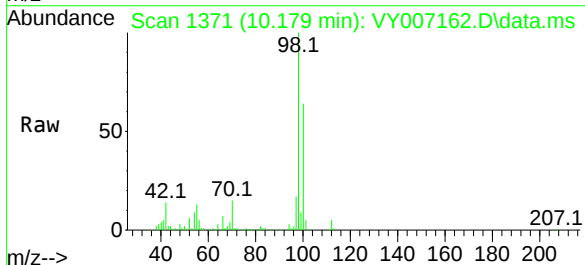






#55
1,1,2-Trichloroethane
Concen: 13.674 ug/l
RT: 10.618 min Scan# 1443
Delta R.T. -0.030 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Instrument :
MSVOA_Y
ClientSampleId :



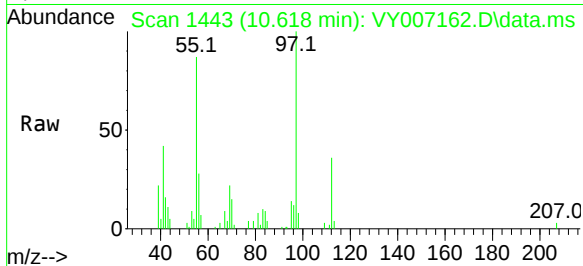



Tgt Ion: 97	Resp: 8029
Ion Ratio	Lower Upper
97 100	
83 10.1	67.0 100.4#
85 3.8	41.2 61.8#
99 0.0	50.7 76.1#

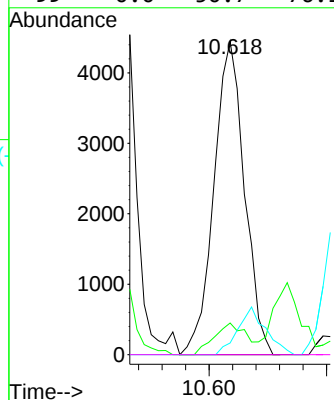

#56
Ethyl methacrylate
Concen: 4.663 ug/l
RT: 10.520 min Scan# 1427
Delta R.T. 0.013 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Tgt Ion: 69	Resp: 3857
Ion Ratio	Lower Upper
69 100	
41 201.9	49.4 74.0#
39 82.8	27.7 41.5#


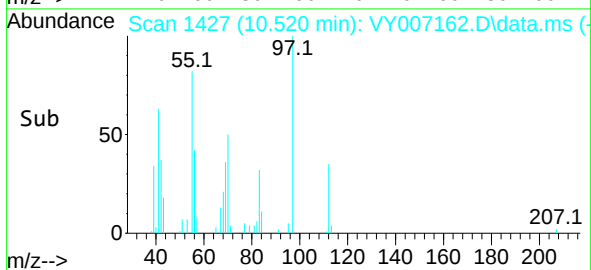
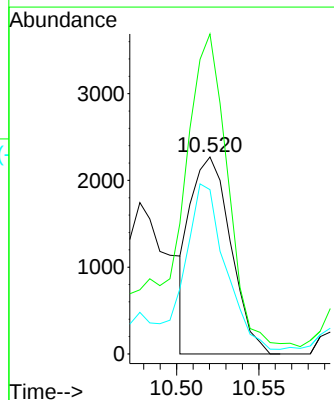
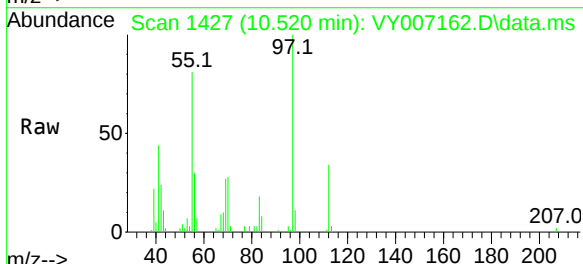




#59
2-Hexanone
Concen: 51.643 ug/l
RT: 10.801 min Scan# 1473
Delta R.T. -0.030 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 43 Resp: 19151
Ion Ratio Lower Upper
43 100
58 3.5 28.4 85.3#

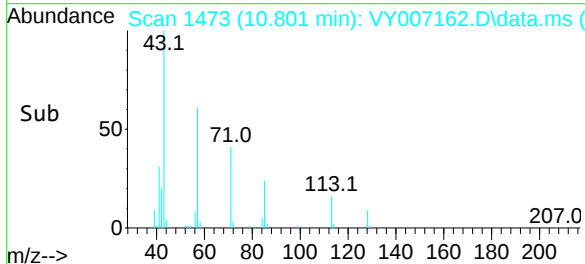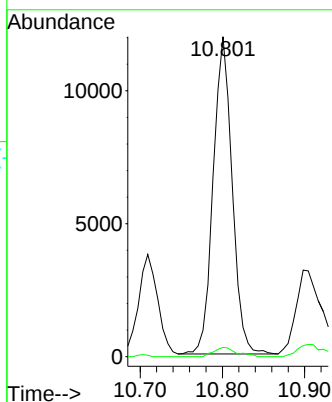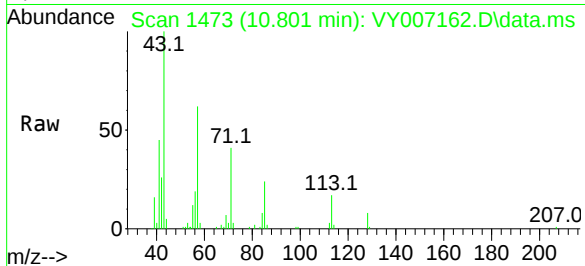

#62
4-Bromofluorobenzene
Concen: 38.772 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Tgt Ion: 95 Resp: 34052
Ion Ratio Lower Upper
95 100
174 63.8 0.0 148.4
176 62.6 0.0 146.6

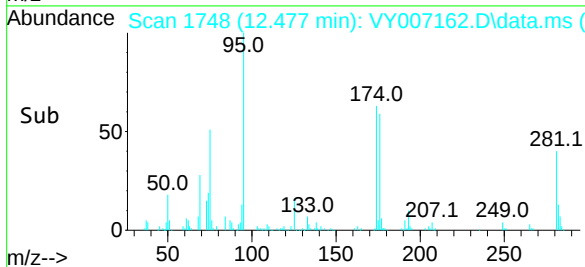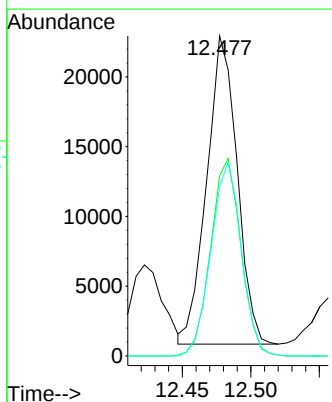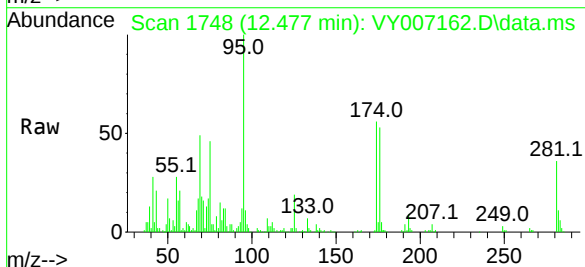



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 1

Delta R.T. 0.001 min

Lab File: VY007162.D





Acq: 14 Jan 2022 12:36

Instrument :

MSVOA_Y

ClientSampleId :

Tgt Ion:117	Resp:	74841
Ion Ratio	Lower	Upper
117	100	
82	56.5	45.4 68.0
119	31.3	26.4 39.6

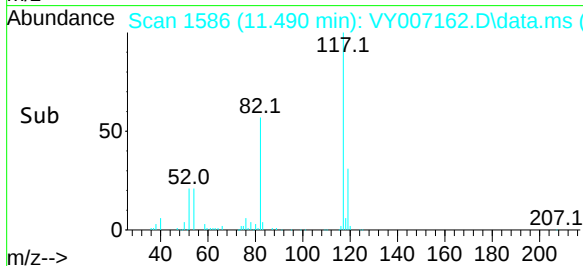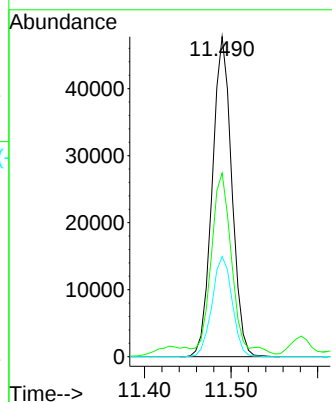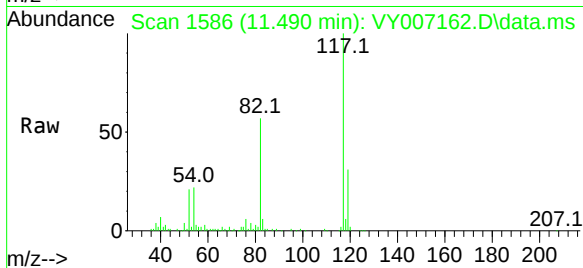

#64

Tetrachloroethene

Concen: 1.514 ug/l




RT: 10.715 min Scan# 1459


Delta R.T. -0.006 min

Lab File: VY007162.D

Acq: 14 Jan 2022 12:36

Tgt Ion:164	Resp:	817
Ion Ratio	Lower	Upper
164	100	
166	110.2	102.6 154.0
129	88.2	84.6 127.0
131	78.5	78.7 118.1#

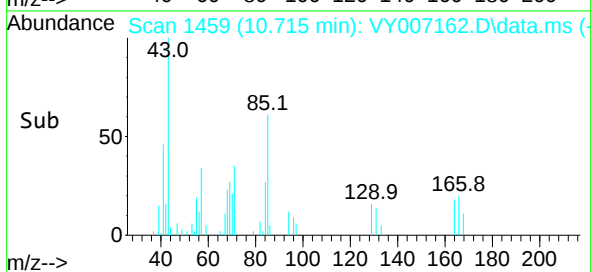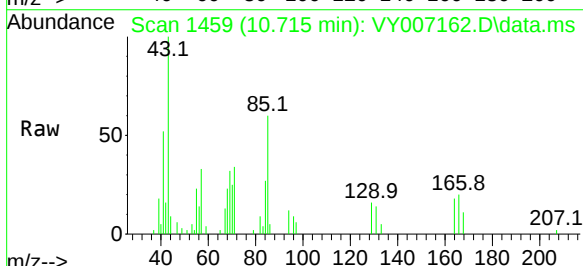



#67

Ethyl Benzene

Concen: 1.835 ug/l

RT: 11.587 min Scan# 1

Delta R.T. -0.006 min

Lab File: VY007162.D

Acq: 14 Jan 2022 12:36

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 91 Resp: 5644

Ion Ratio Lower Upper

91 100

106 26.4 23.9 35.9

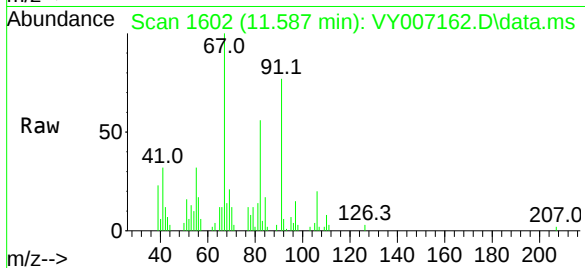

#68

m/p-Xylenes

Concen: 1.909 ug/l

RT: 11.697 min Scan# 1620

Delta R.T. -0.006 min

Lab File: VY007162.D




Acq: 14 Jan 2022 12:36


Tgt Ion:106 Resp: 2182

Ion Ratio Lower Upper

106 100

91 217.4 167.1 250.7

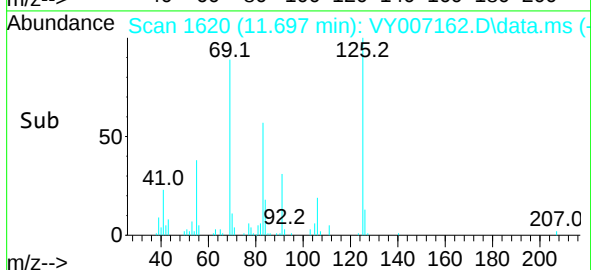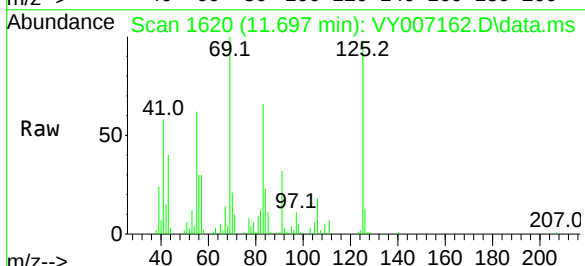



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1904

Delta R.T. -0.006 min

Lab File: VY007162.D

Acq: 14 Jan 2022 12:36

Instrument :

MSVOA_Y

ClientSampleId :





Tgt Ion:152 Resp: 23183

Ion Ratio Lower Upper

152 100

115 66.2 31.4 94.0

150 133.1 0.0 348.4

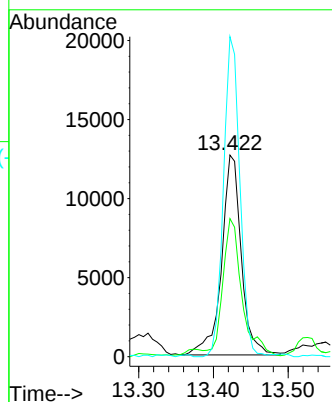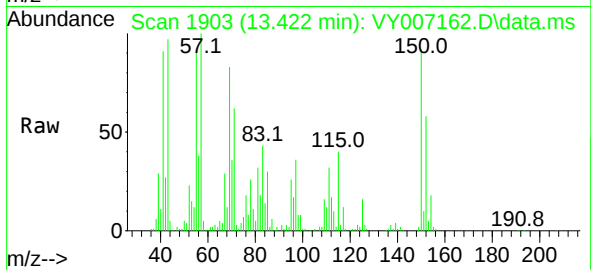

#73

Isopropylbenzene

Concen: 6.005 ug/l

RT: 12.331 min Scan# 1724

Delta R.T. 0.001 min

Lab File: VY007162.D




Acq: 14 Jan 2022 12:36


Tgt Ion:105 Resp: 12024

Ion Ratio Lower Upper

105 100


120 24.4 13.1 39.1

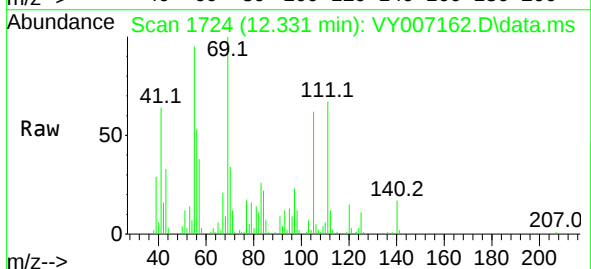



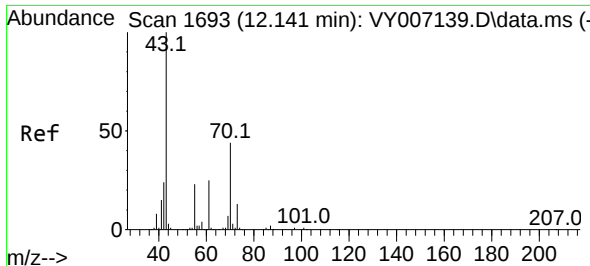


#74
N-amy1 acetate
Concen: 131.668 ug/l
RT: 12.124 min Scan# 1
Delta R.T. -0.018 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Instrument :
MSVOA_Y
ClientSampleId :



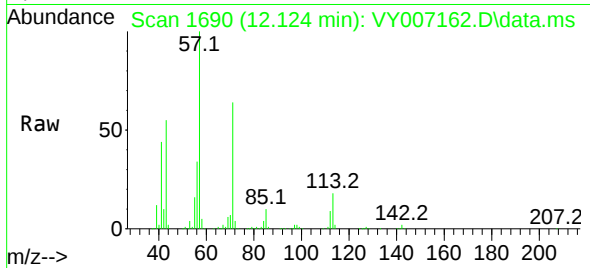



Tgt Ion: 43 Resp: 70501
Ion Ratio Lower Upper
43 100
70 8.8 36.2 54.4#
55 12.7 19.0 28.4#
61 0.0 20.4 30.6#

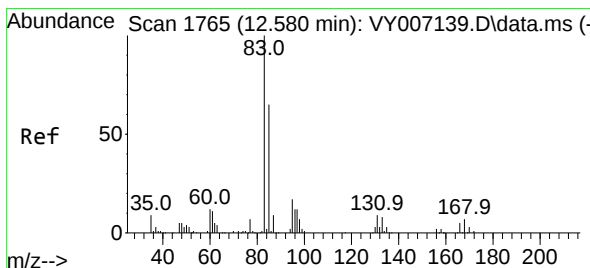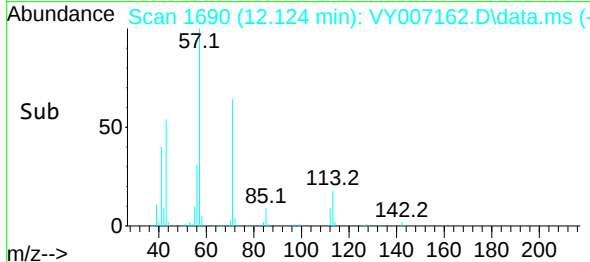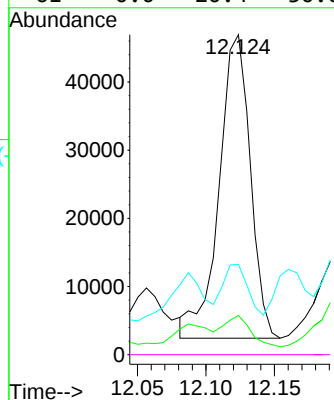

#75
1,1,2,2-Tetrachloroethane
Concen: 16.881 ug/l
RT: 12.557 min Scan# 1761
Delta R.T. -0.024 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Tgt Ion: 83 Resp: 6573
Ion Ratio Lower Upper
83 100
131 0.0 5.3 16.1#
85 97.4 32.4 97.2#


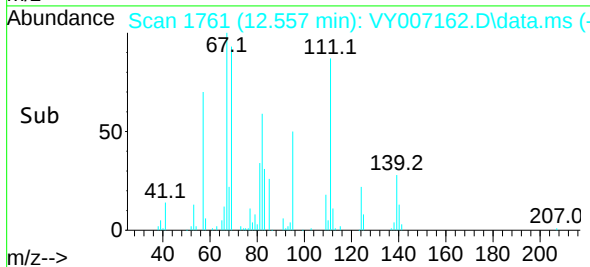
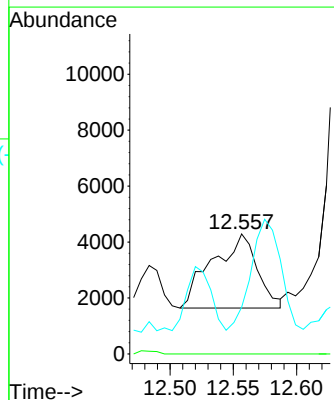
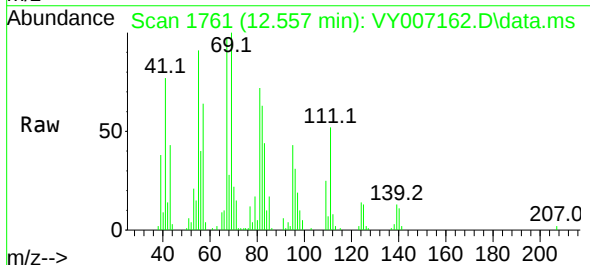




#76
1,2,3-Trichloropropane
Concen: 63.352 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.158 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 75 Resp: 16747
Ion Ratio Lower Upper
75 100
77 4.9 0.0 0.0#

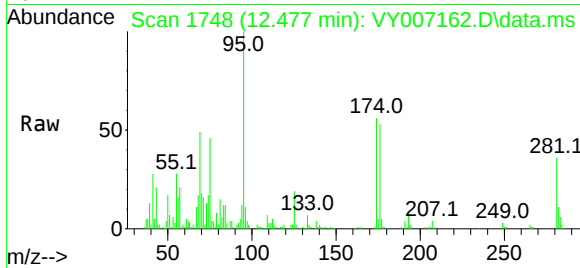

#78
n-propylbenzene
Concen: 11.849 ug/l
RT: 12.672 min Scan# 1780
Delta R.T. 0.001 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Tgt Ion: 91 Resp: 29411
Ion Ratio Lower Upper
91 100
120 20.2 11.2 33.5




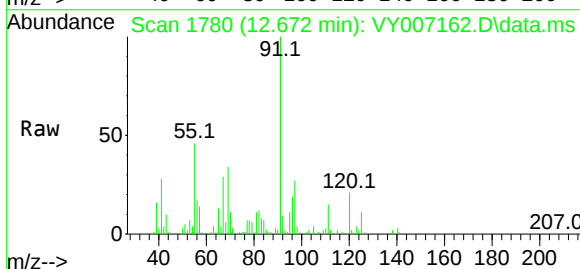




#81
 trans-1,4-Dichloro-2-butene
 Concen: 115.981 ug/l
 RT: 12.477 min Scan# 1732
 Delta R.T. 0.098 min
 Lab File: VY007162.D
 Acq: 14 Jan 2022 12:36




Instrument :
 MSVOA_Y
 ClientSampleId :


Tgt Ion: 75 Resp: 16747
 Ion Ratio Lower Upper
 75 100
 53 5.4 73.9 110.9#
 89 1.4 0.0 0.0#

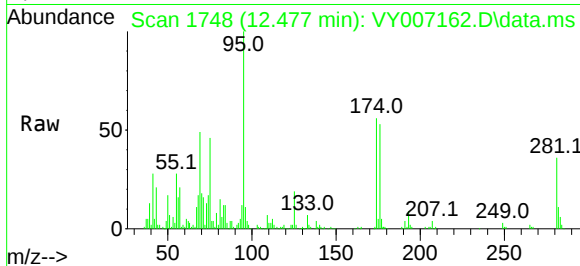

#83
 tert-Butylbenzene
 Concen: 1.867 ug/l
 RT: 13.069 min Scan# 1845
 Delta R.T. -0.006 min
 Lab File: VY007162.D
 Acq: 14 Jan 2022 12:36

Tgt Ion: 119 Resp: 2652
 Ion Ratio Lower Upper
 119 100
 91 78.7 33.1 99.5
 134 26.1 12.9 38.7

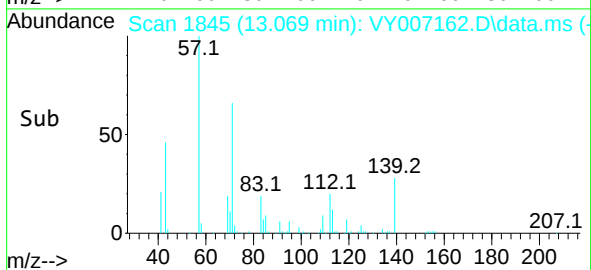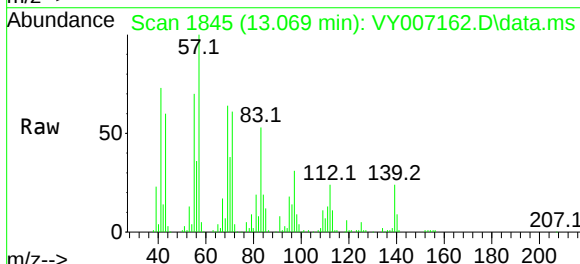



#84

1,2,4-Trimethylbenzene

Concen: 1.943 ug/l

RT: 13.117 min Scan# 1853

Delta R.T. -0.006 min

Lab File: VY007162.D

Acq: 14 Jan 2022 12:36

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion:105 Resp: 3166

Ion Ratio Lower Upper

105 100

120 40.1 21.6 64.6

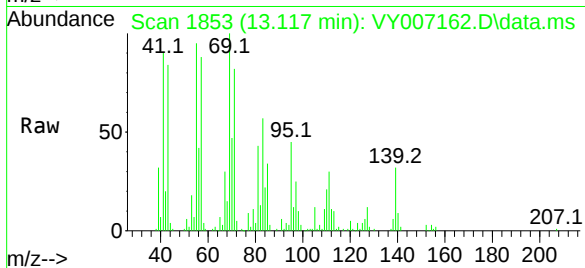

#85

sec-Butylbenzene

Concen: 18.488 ug/l

RT: 13.251 min Scan# 1875

Delta R.T. 0.001 min

Lab File: VY007162.D




Acq: 14 Jan 2022 12:36


Tgt Ion:105 Resp: 39292

Ion Ratio Lower Upper

105 100

134 26.9 9.9 29.7


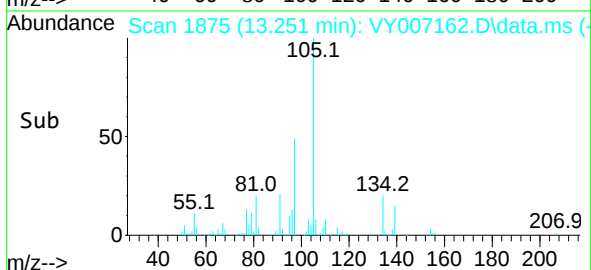

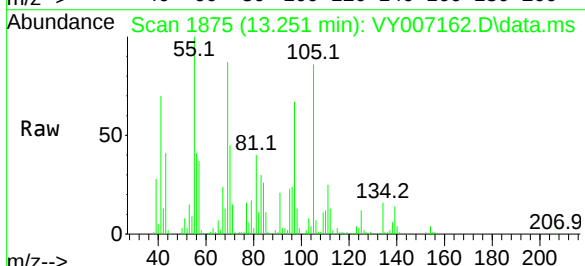


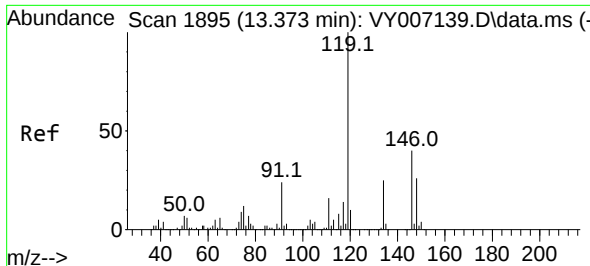

#86
p-Isopropyltoluene
Concen: 1.573 ug/l
RT: 13.367 min Scan# 1895
Delta R.T. -0.006 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:119 Resp: 2748
Ion Ratio Lower Upper
119 100
134 25.4 12.9 38.7
91 22.3 12.4 37.2

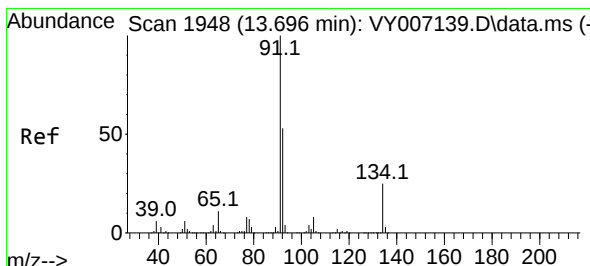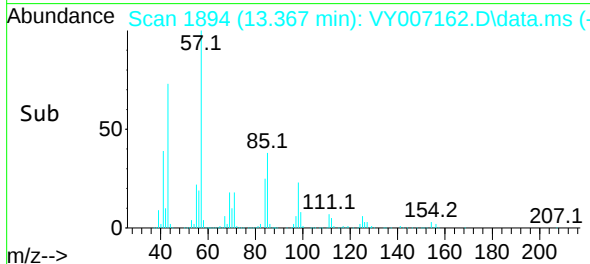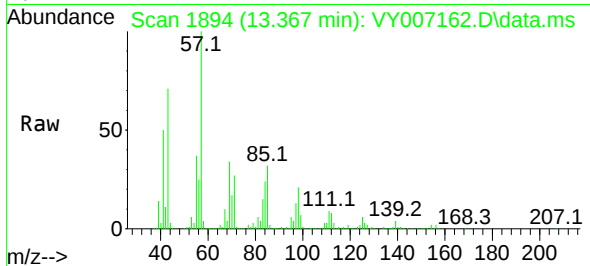

#89
n-Butylbenzene
Concen: 22.035 ug/l
RT: 13.697 min Scan# 1948
Delta R.T. 0.001 min
Lab File: VY007162.D
Acq: 14 Jan 2022 12:36

Tgt Ion: 91 Resp: 37894
Ion Ratio Lower Upper
91 100
92 46.6 26.9 80.6
134 45.7 12.6 37.6#

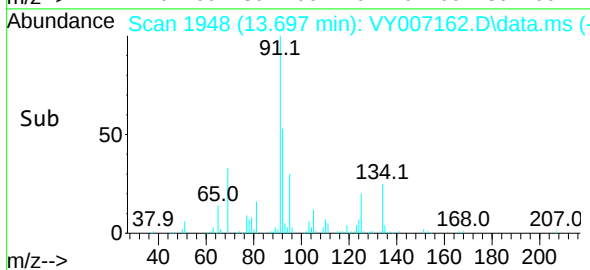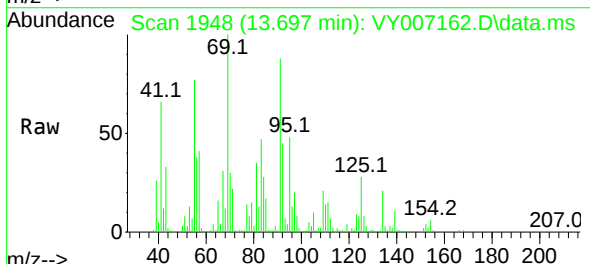



#90

Hexachloroethane

Concen: 20.349 ug/l

RT: 13.971 min Scan# 1993

Delta R.T. 0.013 min

Lab File: VY007162.D

Acq: 14 Jan 2022 12:36

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion:117 Resp: 6948

Ion Ratio Lower Upper

117 100

201 0.0 33.6 100.6#

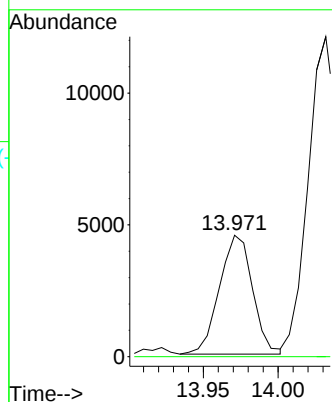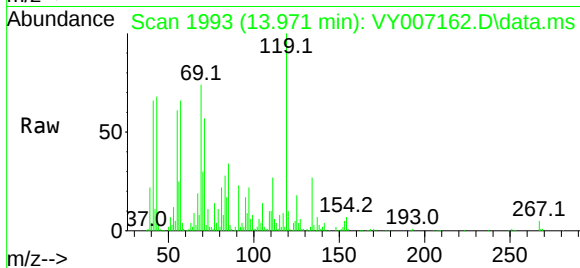

#92

1,2-Dibromo-3-Chloropropane

Concen: 5.041 ug/l

RT: 14.379 min Scan# 2060

Delta R.T. 0.025 min

Lab File: VY007162.D

Acq: 14 Jan 2022 12:36




Tgt Ion: 75 Resp: 339


Ion Ratio Lower Upper

75 100

155 48.1 40.1 120.2

157 0.0 51.7 155.2#

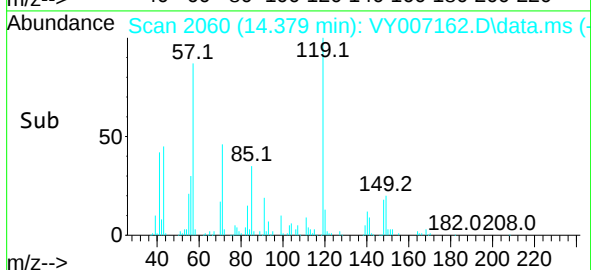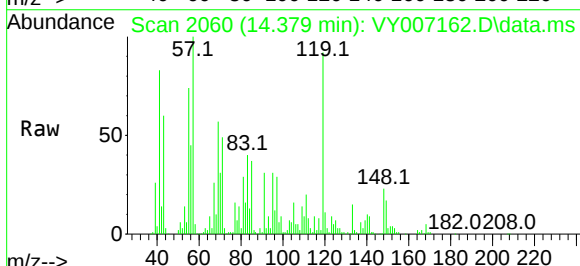



#93

1,2,4-Trichlorobenzene

Concen: 3.002 ug/l

RT: 15.001 min Scan# 21

Delta R.T. -0.006 min

Lab File: VY007162.D





Acq: 14 Jan 2022 12:36

Instrument :

MSVOA_Y

ClientSampleId :

Tgt Ion:180 Resp: 1385
 Ion Ratio Lower Upper
 180 100
 182 171.2 47.6 142.8#
 145 1838.0 16.4 49.1#

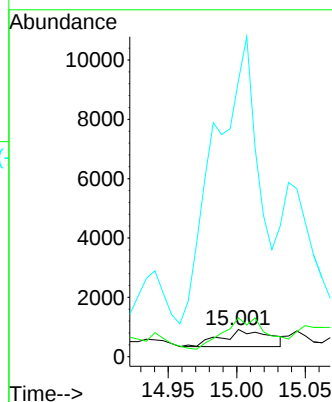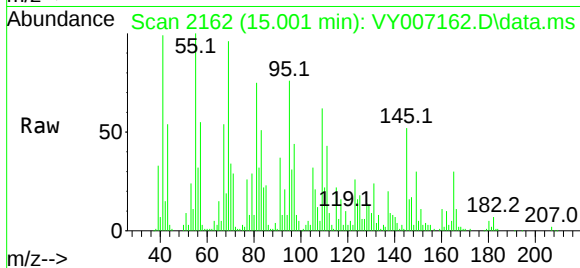

#95

Naphthalene

Concen: 1.921 ug/l




RT: 15.233 min Scan# 2200


Delta R.T. -0.006 min

Lab File: VY007162.D

Acq: 14 Jan 2022 12:36

Tgt Ion:128 Resp: 1883
 Ion Ratio Lower Upper
 128 100
 127 0.0 10.3 15.5#
 129 0.0 8.9 13.3#

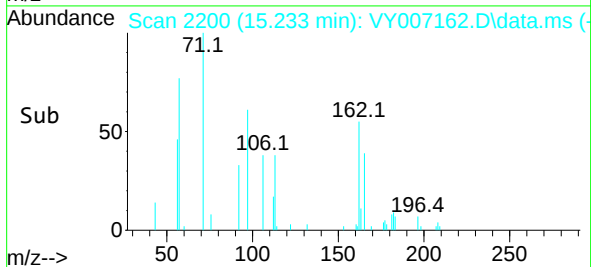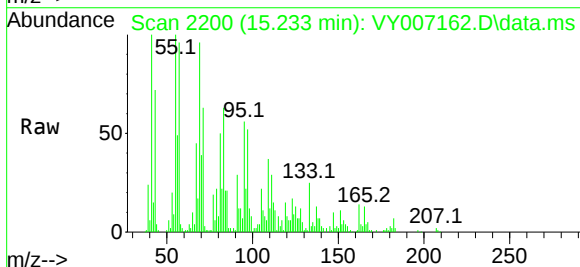



#96

1,2,3-Trichlorobenzene

Concen: 3.102 ug/l

RT: 15.446 min Scan# 21

Delta R.T. 0.025 min


Lab File: VY007162.D

Acq: 14 Jan 2022 12:36

Instrument :

MSVOA_Y

ClientSampleId :

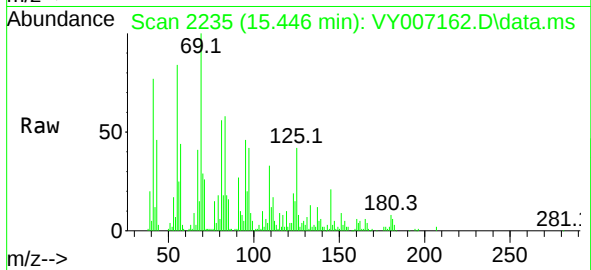

Tgt Ion:180 Resp: 1221

Ion Ratio Lower Upper

180 100

182 0.0 47.3 141.8#

145 0.0 17.2 51.5#

