

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY012122\
 Data File : VY007252.D
 Acq On : 21 Jan 2022 14:37
 Operator : SY/MD
 Sample : N1217-06
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Jan 22 00:23:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 14 05:48:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	14394	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	8.697	114	26657	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	24355	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	9028	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	9883	55.957	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	111.920%
35) Dibromofluoromethane	7.728	113	8830	48.987	ug/l	0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.980%
50) Toluene-d8	10.185	98	32148	48.811	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	97.620%
62) 4-Bromofluorobenzene	12.489	95	10776	45.996	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	92.000%

Target Compounds						Qvalue
3) Chloromethane	2.131	50	270	2.551	ug/l	92
5) Bromomethane	2.668	94	187	1.875	ug/l	88
11) Tert butyl alcohol	4.954	59	134	4.165	ug/l #	73
16) Acetone	3.954	43	35295	770.023	ug/l	97
20) Methylene Chloride	4.710	84	264	1.393	ug/l #	89
25) 2-Butanone	6.990	43	3693	62.317	ug/l	100
31) Cyclohexane	7.777	56	409	1.370	ug/l #	50
36) 1,1-Dichloropropene	7.795	75	1510	5.245	ug/l #	42
37) Ethyl Acetate	7.069	43	160	1.083	ug/l #	67
38) Carbon Tetrachloride	7.801	117	1560	5.152	ug/l #	12
48) Methyl methacrylate	9.148	41	376	2.876	ug/l #	40
51) 4-Methyl-2-Pentanone	10.075	43	9151	62.780	ug/l	98
52) Toluene	10.252	92	576	1.183	ug/l	98
59) 2-Hexanone	10.837	43	229	2.315	ug/l	87
67) Ethyl Benzene	11.593	91	1671	1.669	ug/l #	85
68) m/p-Xylenes	11.703	106	2636	7.087	ug/l	98
69) o-Xylene	12.032	106	1228	3.506	ug/l	95
74) N-amyl acetate	12.117	43	426	2.043	ug/l #	41
76) 1,2,3-Trichloropropane	12.483	75	5972	58.013	ug/l #	100
78) n-propylbenzene	12.678	91	1188	1.229	ug/l	99
80) 1,3,5-Trimethylbenzene	12.812	105	1579	2.466	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.483	75	5972	106.205	ug/l #	3
84) 1,2,4-Trimethylbenzene	13.123	105	5371	8.463	ug/l	94
87) 1,3-Dichlorobenzene	13.373	146	362	1.090	ug/l	77
88) 1,4-Dichlorobenzene	13.373	146	362	1.084	ug/l	77
89) n-Butylbenzene	13.696	91	1003	1.498	ug/l	91
90) Hexachloroethane	13.965	117	134	1.008	ug/l #	16
91) 1,2-Dichlorobenzene	13.751	146	346	1.171	ug/l	79
93) 1,2,4-Trichlorobenzene	15.013	180	518	2.883	ug/l	90
94) Hexachlorobutadiene	15.117	225	157	1.695	ug/l	84
95) Naphthalene	15.245	128	1383	3.624	ug/l #	93
96) 1,2,3-Trichlorobenzene	15.428	180	584	3.809	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Quant Time: Jan 22 00:23:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y011322S.M
Quant Title : SW846 8260
QLast Update : Fri Jan 14 05:48:29 2022
Response via : Initial Calibration








#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 91
Delta R.T. 0.012 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion:168 Resp: 14394
Ion Ratio Lower Upper
168 100
99 58.8 49.1 73.7

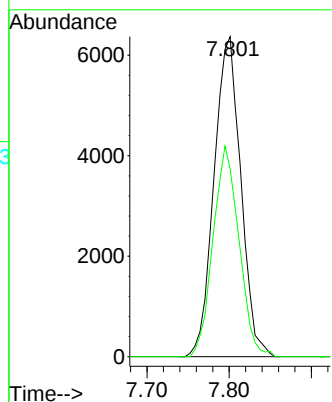

#3
Chloromethane
Concen: 2.551 ug/l
RT: 2.131 min Scan# 51
Delta R.T. 0.019 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Tgt Ion: 50 Resp: 270
Ion Ratio Lower Upper
50 100
52 29.5 27.1 40.7


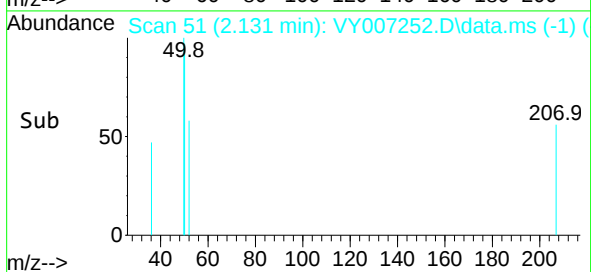
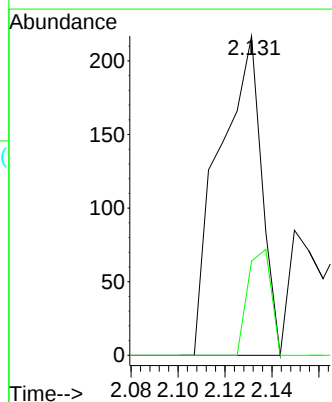



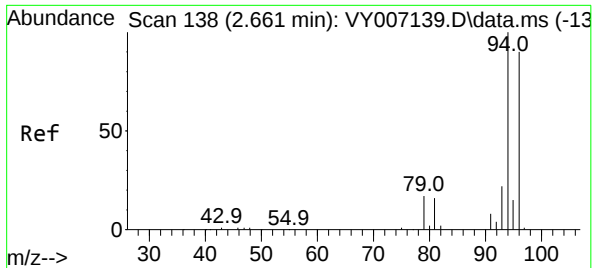

#5
Bromomethane
Concen: 1.875 ug/l
RT: 2.668 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 94 Resp: 187
Ion Ratio Lower Upper
94 100
96 82.6 75.8 113.6

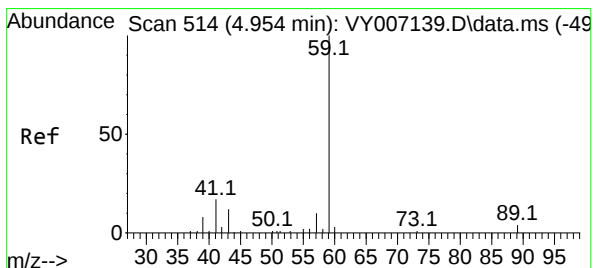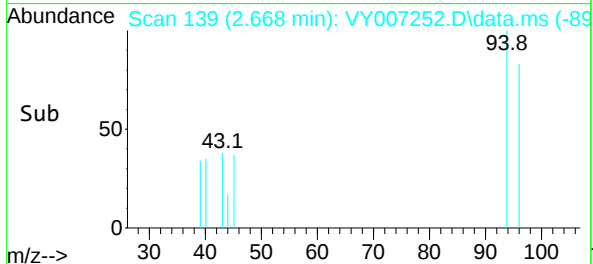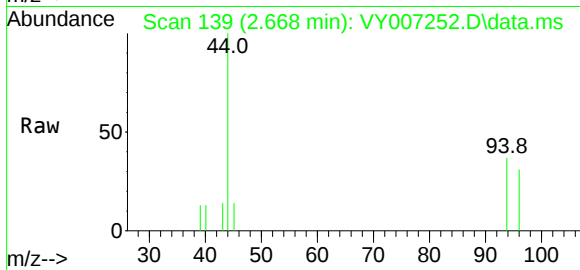

#11
Tert butyl alcohol
Concen: 4.165 ug/l
RT: 4.954 min Scan# 514
Delta R.T. -0.000 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37


Tgt Ion: 59 Resp: 134
Ion Ratio Lower Upper
59 100
57 0.0 8.1 12.1#

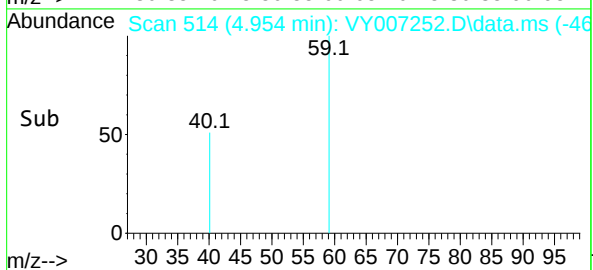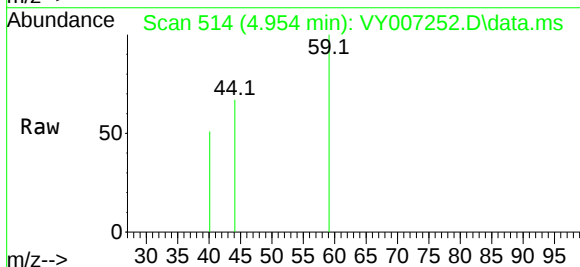






#16
Acetone
Concen: 770.023 ug/l
RT: 3.954 min Scan# 350
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion: 43 Resp: 35295
Ion Ratio Lower Upper
43 100
58 27.9 23.8 35.6

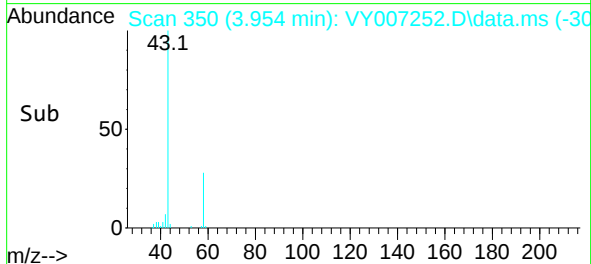

#20
Methylene Chloride
Concen: 1.393 ug/l
RT: 4.710 min Scan# 474
Delta R.T. 0.000 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37


Tgt Ion: 84 Resp: 264
Ion Ratio Lower Upper
84 100
49 110.6 92.6 139.0
51 31.9 28.6 42.8
86 42.0 50.1 75.1#

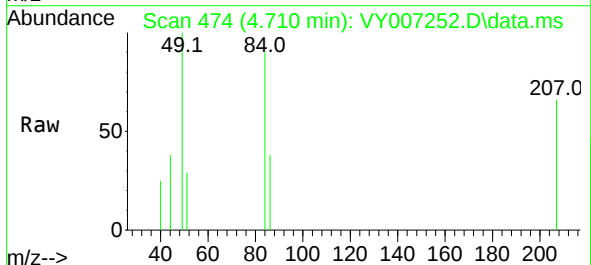






#25
2-Butanone
Concen: 62.317 ug/l
RT: 6.990 min Scan# 847
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion: 43 Resp: 3693
Ion Ratio Lower Upper
43 100
72 27.5 21.9 32.9

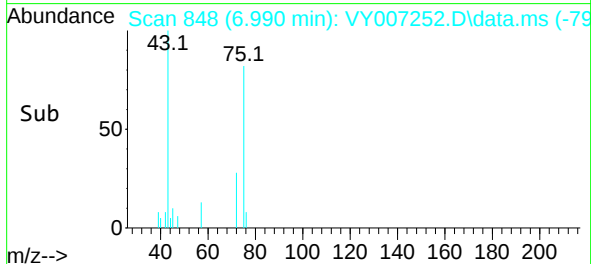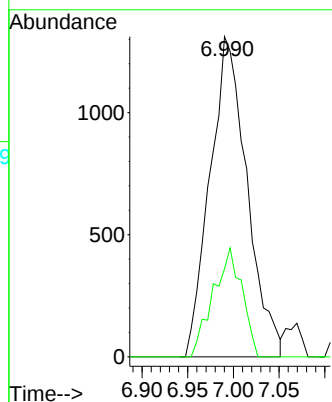

#31
Cyclohexane
Concen: 1.370 ug/l
RT: 7.777 min Scan# 977
Delta R.T. -0.012 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Tgt Ion: 56 Resp: 409
Ion Ratio Lower Upper
56 100
69 80.9 27.2 40.8#
84 54.7 72.1 108.1#


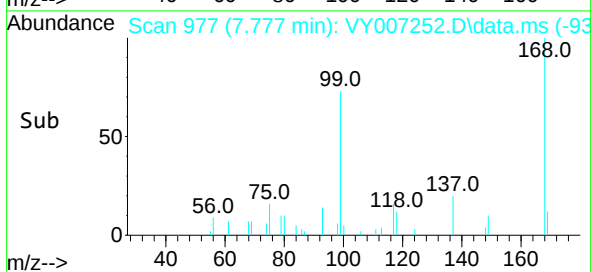
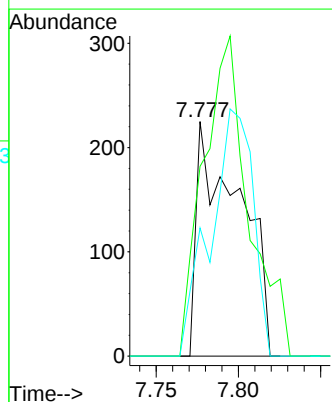





#33
1,2-Dichloroethane-d4
Concen: 55.957 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 65 Resp: 9883
Ion Ratio Lower Upper
65 100
67 53.8 0.0 105.6

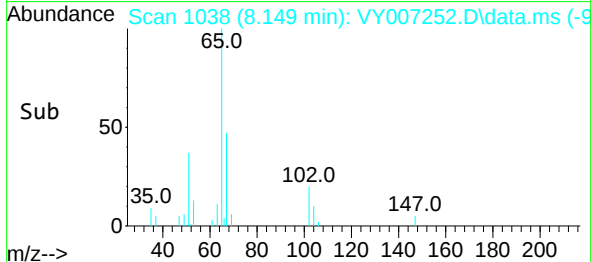

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37


Tgt Ion: 114 Resp: 26657
Ion Ratio Lower Upper
114 100
63 21.1 0.0 39.2
88 14.6 0.0 31.0

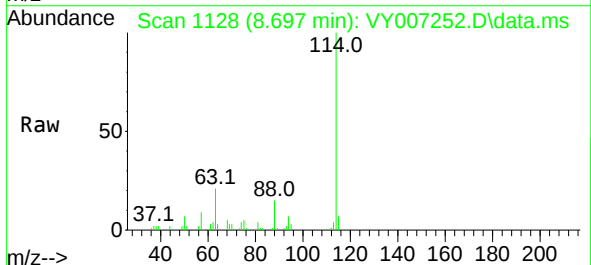






#35
Dibromofluoromethane
Concen: 48.987 ug/l
RT: 7.728 min Scan# 91
Delta R.T. 0.012 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion:113 Resp: 8830
Ion Ratio Lower Upper
113 100
111 103.5 82.2 123.4
192 18.6 14.2 21.4

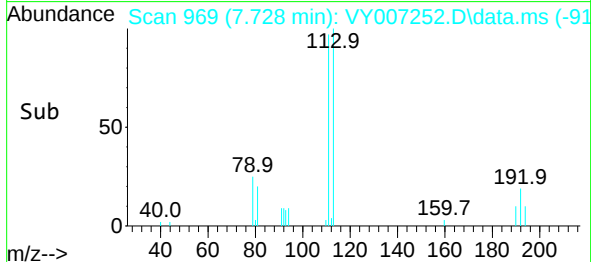

#36
1,1-Dichloropropene
Concen: 5.245 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.122 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Tgt Ion: 75 Resp: 1510
Ion Ratio Lower Upper
75 100
110 0.0 17.3 51.9#
77 0.0 24.7 37.1#

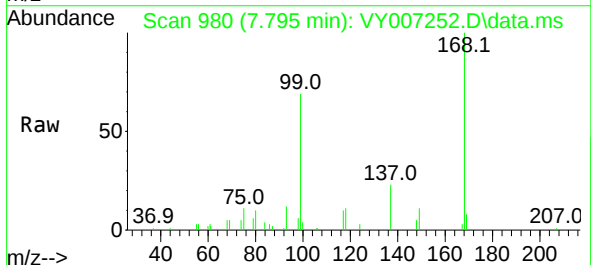



#37

Ethyl Acetate

Concen: 1.083 ug/l

RT: 7.069 min Scan# 80

Delta R.T. -0.006 min


Lab File: VY007252.D

Acq: 21 Jan 2022 14:37




Instrument :

MSVOA_Y

ClientSampleId :

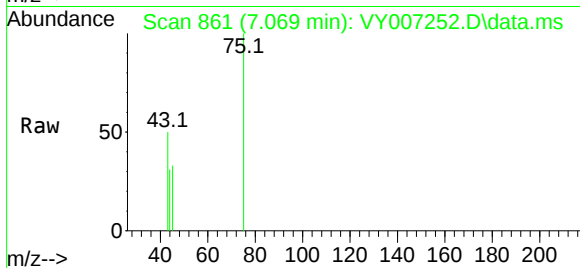

Tgt Ion:	43	Resp:	160
Ion	Ratio	Lower	Upper
43	100		
61	0.0	11.8	17.8#
70	0.0	9.0	13.4#

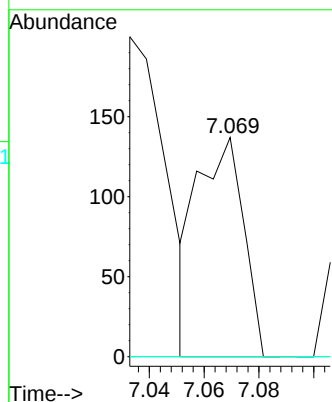

#38

Carbon Tetrachloride

Concen: 5.152 ug/l




RT: 7.801 min Scan# 981


Delta R.T. -0.097 min

Lab File: VY007252.D

Acq: 21 Jan 2022 14:37


Tgt Ion:	117	Resp:	1560
Ion	Ratio	Lower	Upper
117	100		
119	0.0	77.2	115.8#
121	0.0	24.2	36.2#

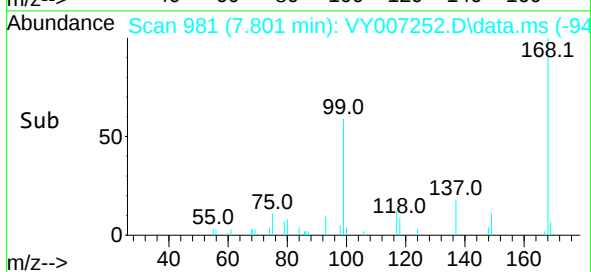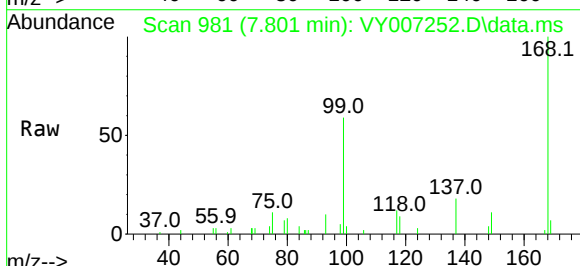






#48
Methyl methacrylate
Concen: 2.876 ug/l
RT: 9.148 min Scan# 11
Delta R.T. -0.146 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion: 41 Resp: 376
Ion Ratio Lower Upper
41 100
69 0.0 70.5 105.7#
39 51.1 43.8 65.8

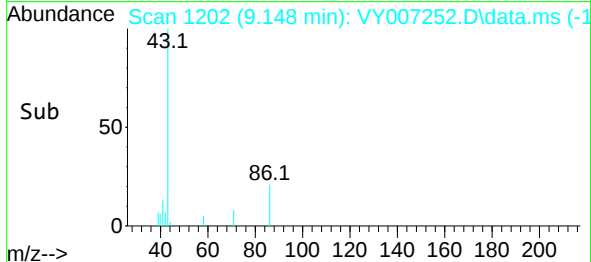

#50
Toluene-d8
Concen: 48.811 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Tgt Ion: 98 Resp: 32148
Ion Ratio Lower Upper
98 100
100 64.9 52.2 78.2




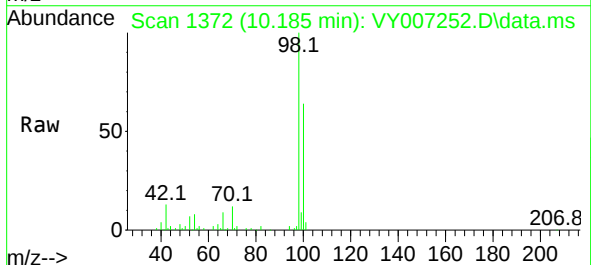




#51
4-Methyl-2-Pentanone
Concen: 62.780 ug/l
RT: 10.075 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 43 Resp: 9151
Ion Ratio Lower Upper
43 100
58 39.8 32.8 49.2

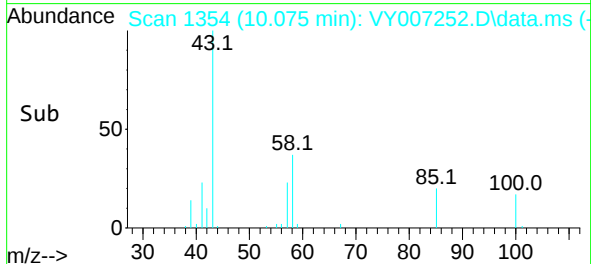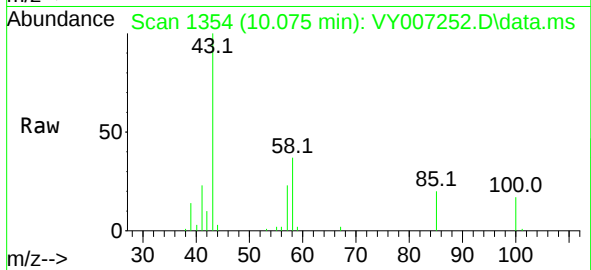

#52
Toluene
Concen: 1.183 ug/l
RT: 10.252 min Scan# 1383
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Tgt Ion: 92 Resp: 576
Ion Ratio Lower Upper
92 100
91 176.6 138.6 207.8


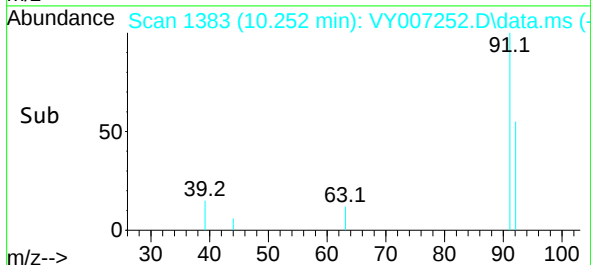






#59
2-Hexanone
Concen: 2.315 ug/l
RT: 10.837 min Scan# 1478
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 43 Resp: 229
Ion Ratio Lower Upper
43 100
58 66.4 28.4 85.3

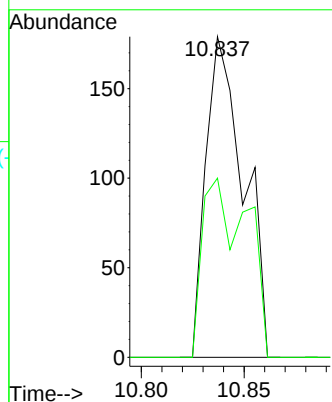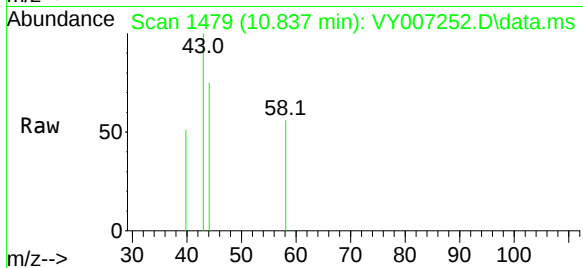

#62
4-Bromofluorobenzene
Concen: 45.996 ug/l
RT: 12.489 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Tgt Ion: 95 Resp: 10776
Ion Ratio Lower Upper
95 100
174 76.1 0.0 148.4
176 74.3 0.0 146.6

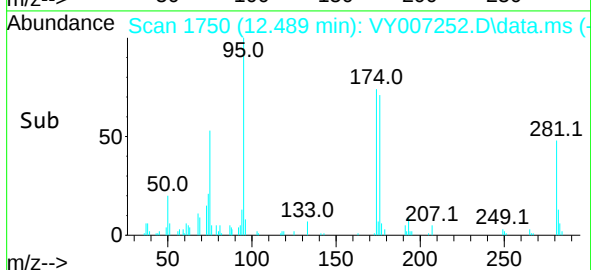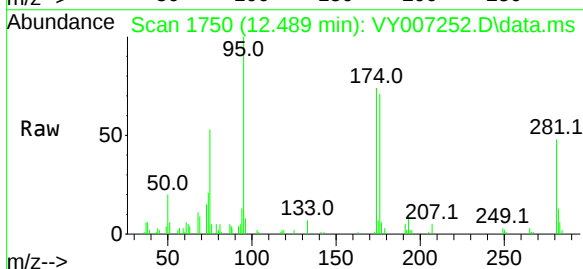



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.495 min Scan# 11

Delta R.T. 0.006 min


Lab File: VY007252.D

Acq: 21 Jan 2022 14:37




Instrument :

MSVOA_Y

ClientSampleId :

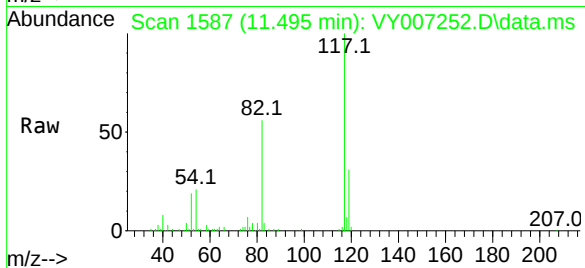

Tgt Ion:117	Resp:	24355
Ion	Ratio	Lower Upper
117	100	
82	55.8	45.4 68.0
119	31.3	26.4 39.6

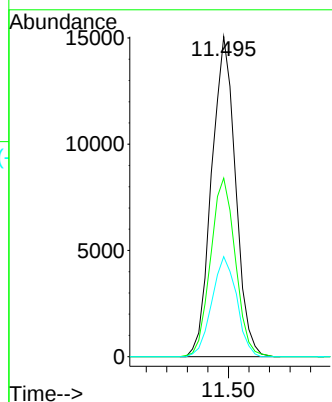

#67

Ethyl Benzene

Concen: 1.669 ug/l




RT: 11.593 min Scan# 1603


Delta R.T. 0.000 min

Lab File: VY007252.D

Acq: 21 Jan 2022 14:37

Tgt Ion: 91	Resp:	1671
Ion	Ratio	Lower Upper
91	100	
106	21.9	23.9 35.9#

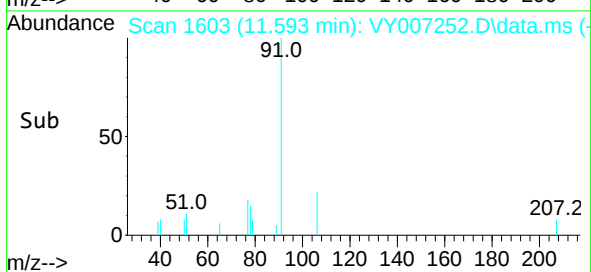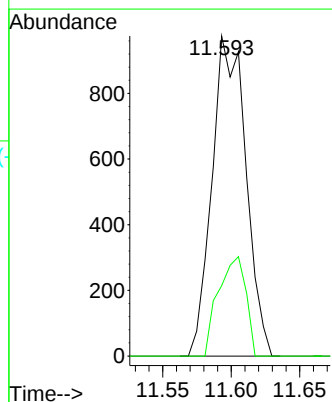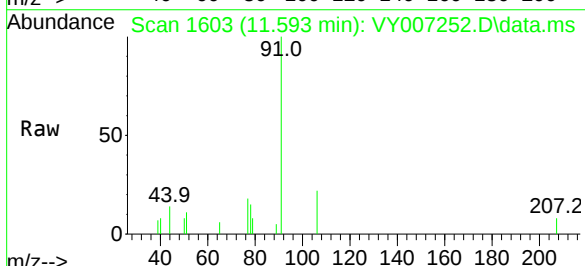



#68

m/p-Xylenes

Concen: 7.087 ug/l

RT: 11.703 min Scan# 1

Delta R.T. 0.000 min

Lab File: VY007252.D

Acq: 21 Jan 2022 14:37

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion:106 Resp: 2636

Ion Ratio Lower Upper

106 100

91 206.1 167.1 250.7

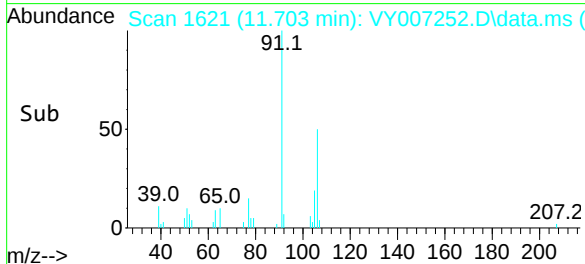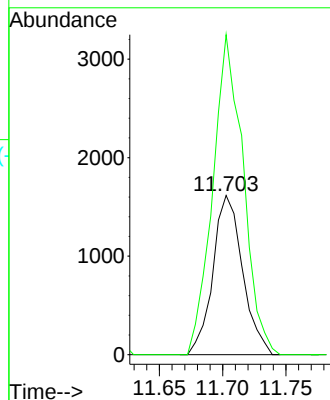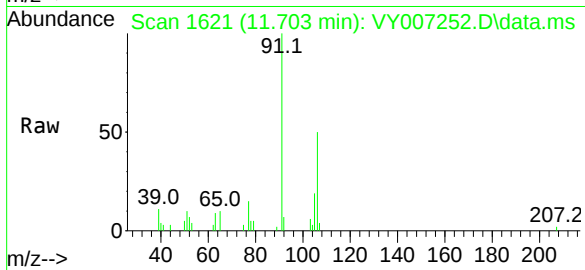

#69

o-Xylene

Concen: 3.506 ug/l

RT: 12.032 min Scan# 1675

Delta R.T. 0.000 min

Lab File: VY007252.D




Acq: 21 Jan 2022 14:37


Tgt Ion:106 Resp: 1228

Ion Ratio Lower Upper

106 100


91 227.4 109.9 329.6

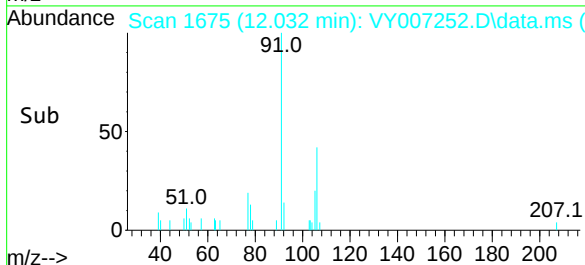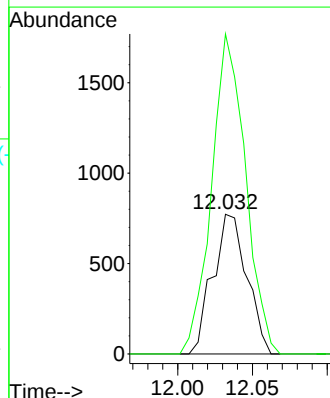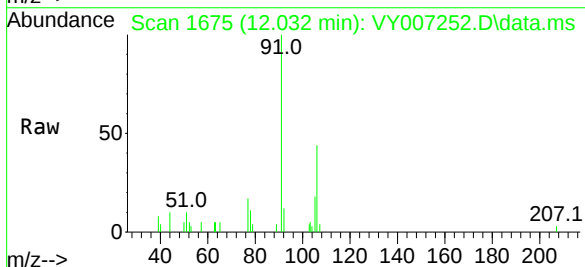



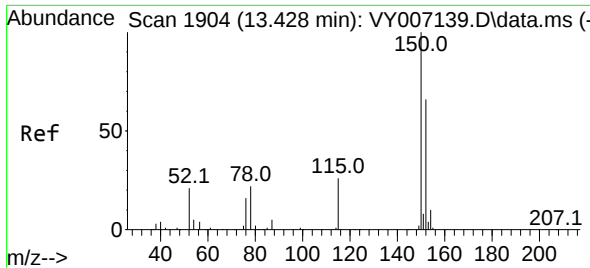


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37


Instrument :
MSVOA_Y
ClientSampleId :

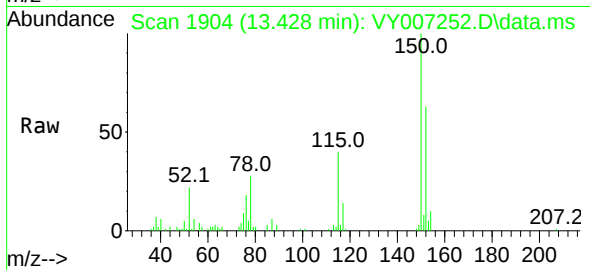



Tgt Ion:152 Resp: 9028
Ion Ratio Lower Upper
152 100
115 66.5 31.4 94.0
150 161.3 0.0 348.4

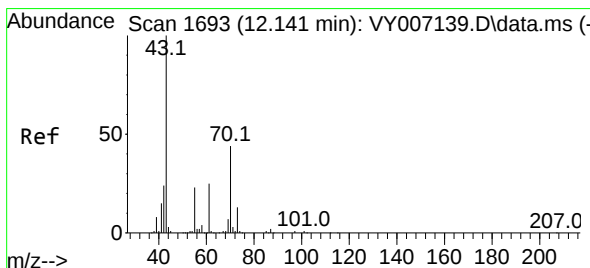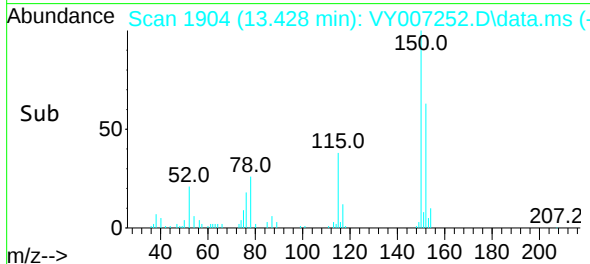


#74
N-ethyl acetate
Concen: 2.043 ug/l
RT: 12.117 min Scan# 1689
Delta R.T. -0.024 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

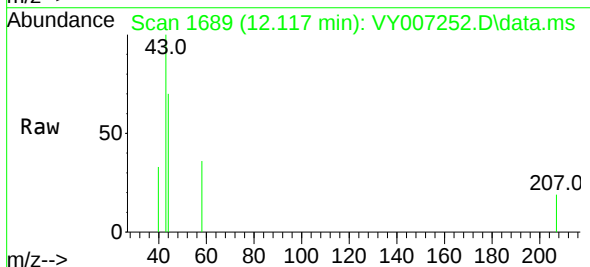

Tgt Ion: 43 Resp: 426
Ion Ratio Lower Upper
43 100
70 0.0 36.2 54.4#
55 0.0 19.0 28.4#
61 0.0 20.4 30.6#



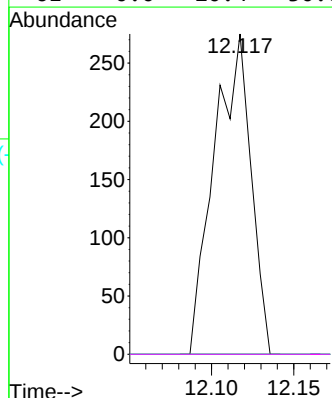
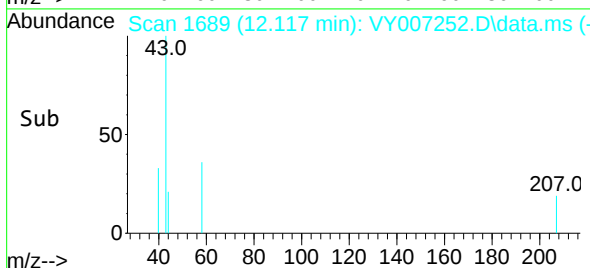




#76
1,2,3-Trichloropropane
Concen: 58.013 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.152 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 75 Resp: 5972
Ion Ratio Lower Upper
75 100
77 0.3 0.0 0.0#

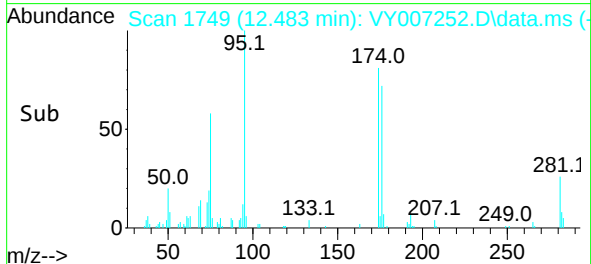

#78
n-propylbenzene
Concen: 1.229 ug/l
RT: 12.678 min Scan# 1781
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Tgt Ion: 91 Resp: 1188
Ion Ratio Lower Upper
91 100
120 21.7 11.2 33.5





#80

1,3,5-Trimethylbenzene

Concen: 2.466 ug/l

RT: 12.812 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VY007252.D

Acq: 21 Jan 2022 14:37

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion:105 Resp: 1579

Ion Ratio Lower Upper

105 100

120 49.3 23.7 71.1

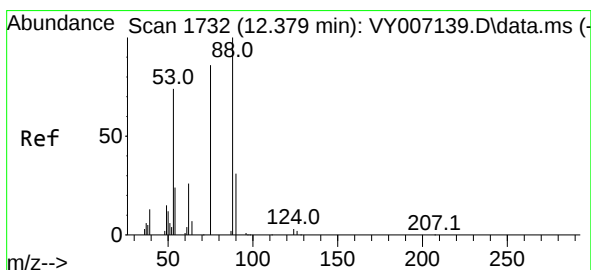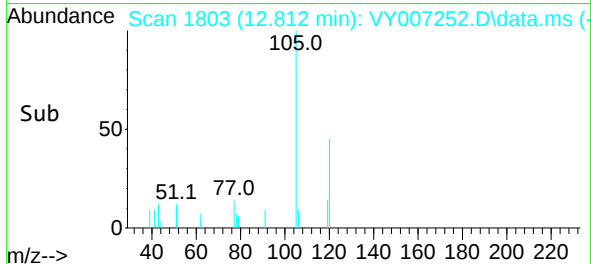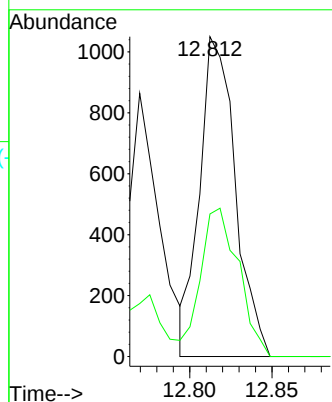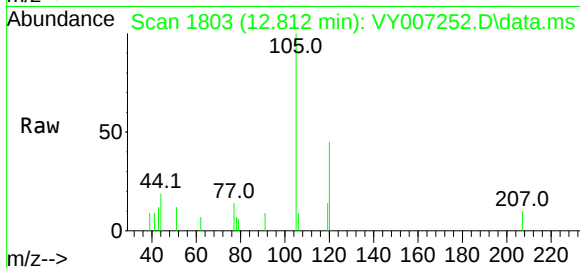

#81

trans-1,4-Dichloro-2-butene

Concen: 106.205 ug/l

RT: 12.483 min Scan# 1749

Delta R.T. 0.104 min

Lab File: VY007252.D

Acq: 21 Jan 2022 14:37




Tgt Ion: 75 Resp: 5972


Ion Ratio Lower Upper

75 100

53 0.0 73.9 110.9#

89 0.0 0.0 0.0




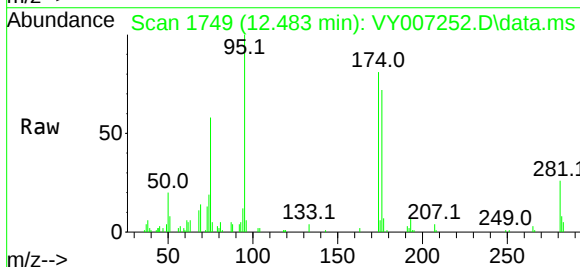




#84
1,2,4-Trimethylbenzene
Concen: 8.463 ug/l
RT: 13.123 min Scan# 1854
Delta R.T. 0.000 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:105 Resp: 5371
Ion Ratio Lower Upper
105 100
120 46.8 21.6 64.6

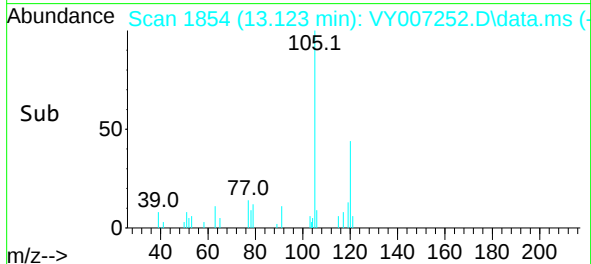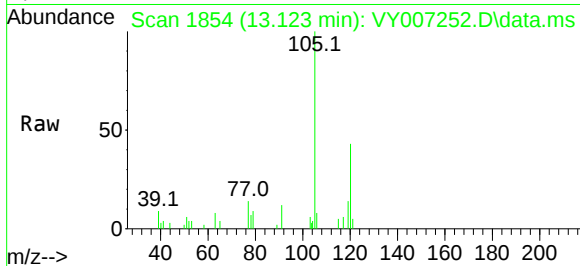

#87
1,3-Dichlorobenzene
Concen: 1.090 ug/l
RT: 13.373 min Scan# 1895
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37


Tgt Ion:146 Resp: 362
Ion Ratio Lower Upper
146 100
111 27.6 21.1 63.1
148 45.6 31.9 95.7








#88
1,4-Dichlorobenzene
Concen: 1.084 ug/l
RT: 13.373 min Scan# 11
Delta R.T. -0.073 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Instrument :
MSVOA_Y
ClientSampleId :







Tgt Ion:146 Resp: 362
Ion Ratio Lower Upper
146 100
111 27.6 20.7 62.1
148 45.6 32.0 96.2

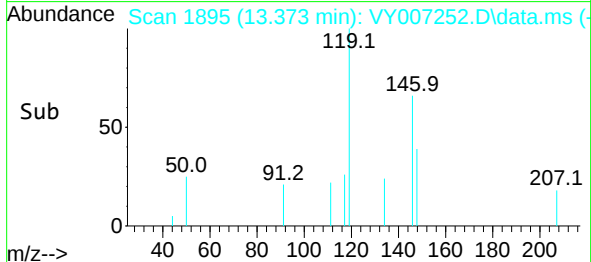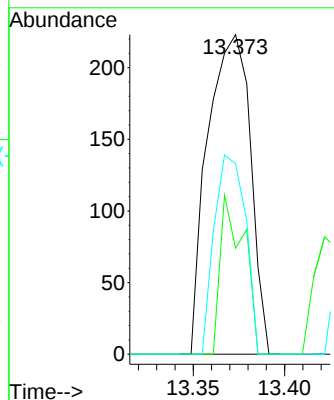

#89
n-Butylbenzene
Concen: 1.498 ug/l
RT: 13.696 min Scan# 1948
Delta R.T. 0.000 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Tgt Ion: 91 Resp: 1003
Ion Ratio Lower Upper
91 100
92 45.4 26.9 80.6
134 22.8 12.6 37.6



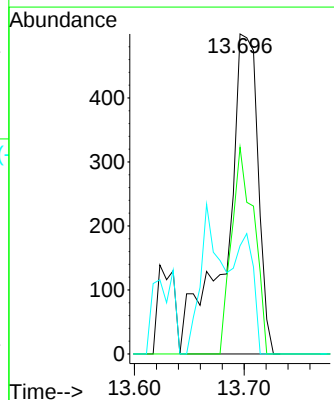
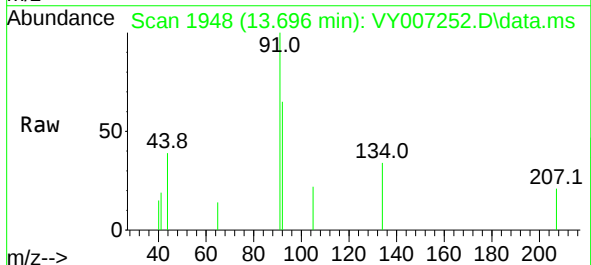




#90
Hexachloroethane
Concen: 1.008 ug/l
RT: 13.965 min Scan# 1991
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:117 Resp: 134
Ion Ratio Lower Upper
117 100
201 0.0 33.6 100.6#

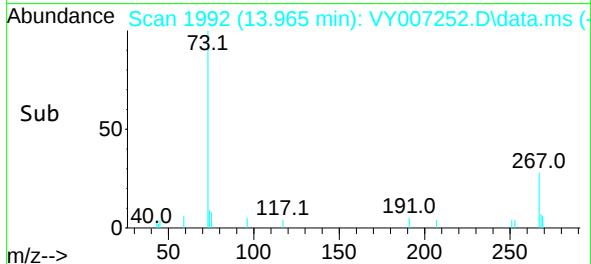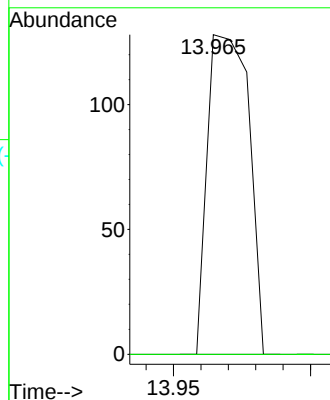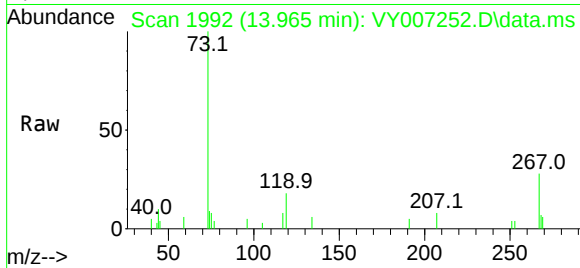

#91
1,2-Dichlorobenzene
Concen: 1.171 ug/l
RT: 13.751 min Scan# 1957
Delta R.T. 0.012 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Tgt Ion:146 Resp: 346
Ion Ratio Lower Upper
146 100
111 27.2 21.4 64.3
148 48.3 31.1 93.5

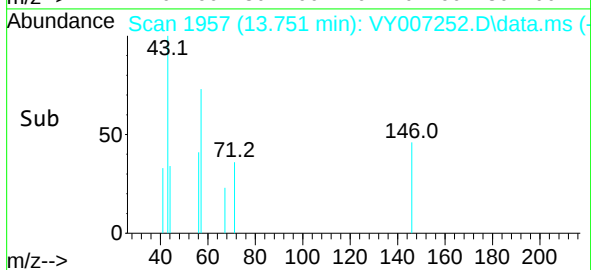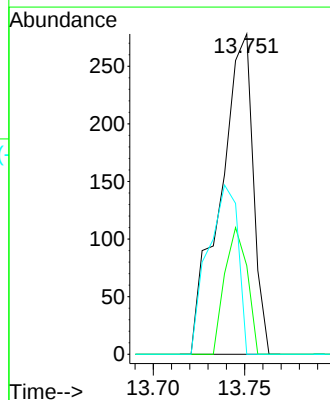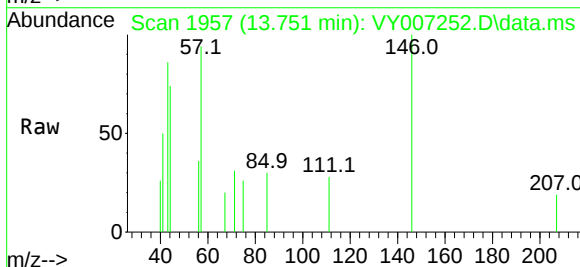



#93

1,2,4-Trichlorobenzene

Concen: 2.883 ug/l

RT: 15.013 min Scan# 2163

Delta R.T. 0.006 min

Lab File: VY007252.D

Acq: 21 Jan 2022 14:37

Instrument :

MSVOA_Y

ClientSampleId :





Tgt Ion:180 Resp: 518

Ion Ratio Lower Upper

180 100

182 84.6 47.6 142.8

145 28.0 16.4 49.1

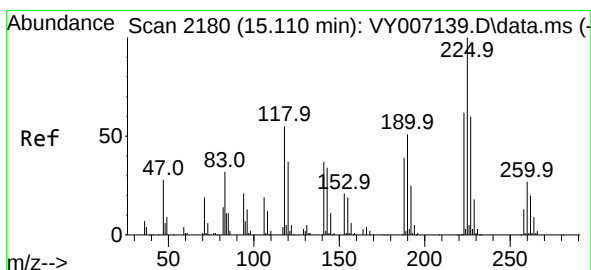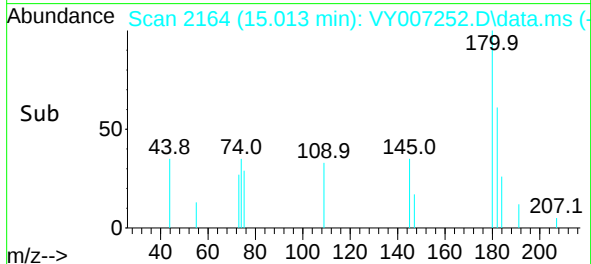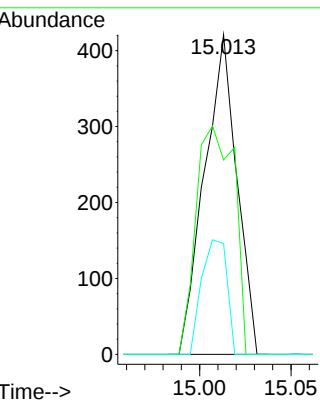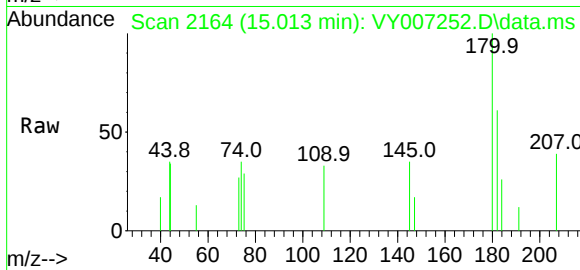

#94

Hexachlorobutadiene

Concen: 1.695 ug/l

RT: 15.117 min Scan# 2181

Delta R.T. 0.006 min

Lab File: VY007252.D

Acq: 21 Jan 2022 14:37




Tgt Ion:225 Resp: 157


Ion Ratio Lower Upper

225 100

223 88.5 32.6 97.8

227 61.8 32.0 96.2


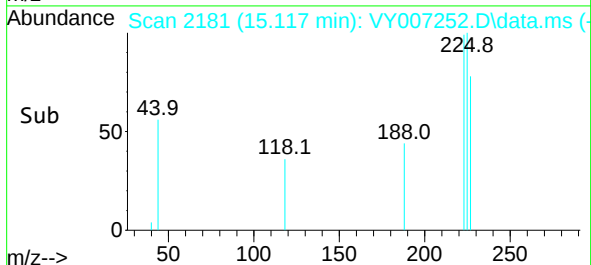
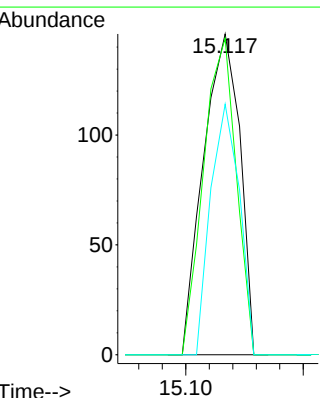
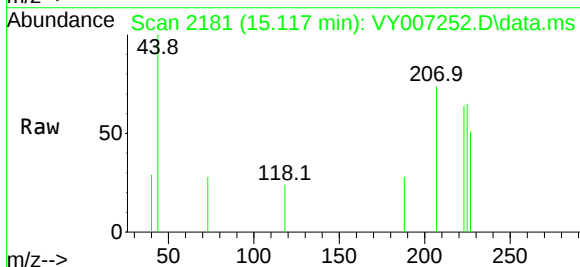




#95
Naphthalene
Concen: 3.624 ug/l
RT: 15.245 min Scan# 21
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Instrument :
MSVOA_Y
ClientSampleId :

Tgt Ion:128 Resp: 1383
Ion Ratio Lower Upper
128 100
127 12.4 10.3 15.5
129 5.6 8.9 13.3#

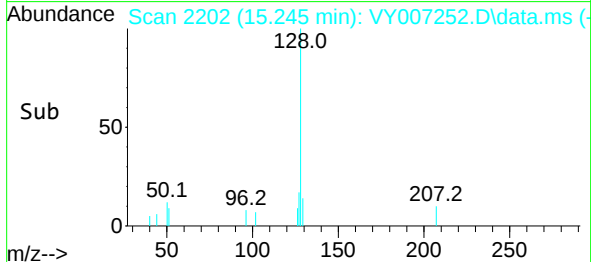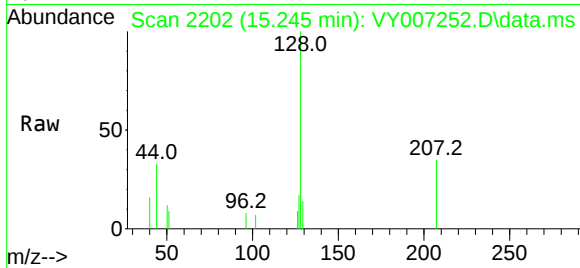

#96
1,2,3-Trichlorobenzene
Concen: 3.809 ug/l
RT: 15.428 min Scan# 2232
Delta R.T. 0.006 min
Lab File: VY007252.D
Acq: 21 Jan 2022 14:37

Tgt Ion:180 Resp: 584
Ion Ratio Lower Upper
180 100
182 95.5 47.3 141.8
145 30.5 17.2 51.5

