

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021122\
 Data File : VY007475.D
 Acq On : 11 Feb 2022 11:24
 Operator : SY/MD
 Sample : VY0211SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0211SBL01

Quant Time: Feb 12 02:51:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020222S.M
 Quant Title : SW846 8260
 QLast Update : Thu Feb 03 04:36:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.795	168	118160	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	221527	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	211250	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	86708	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	74508	54.820	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 109.640%	
35) Dibromofluoromethane	7.728	113	71571	50.313	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 100.620%	
50) Toluene-d8	10.185	98	267401	50.880	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 101.760%	
62) 4-Bromofluorobenzene	12.483	95	95774	53.617	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 107.240%	
Target Compounds						Qvalue
95) Naphthalene	15.233	128	10139	2.892	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY021122\
Data File : VY007475.D
Acq On : 11 Feb 2022 11:24
Operator : SY/MD
Sample : VY0211SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0211SBL01

Quant Time: Feb 12 02:51:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y020222S.M
Quant Title : SW846 8260
QLast Update : Thu Feb 03 04:36:48 2022
Response via : Initial Calibration




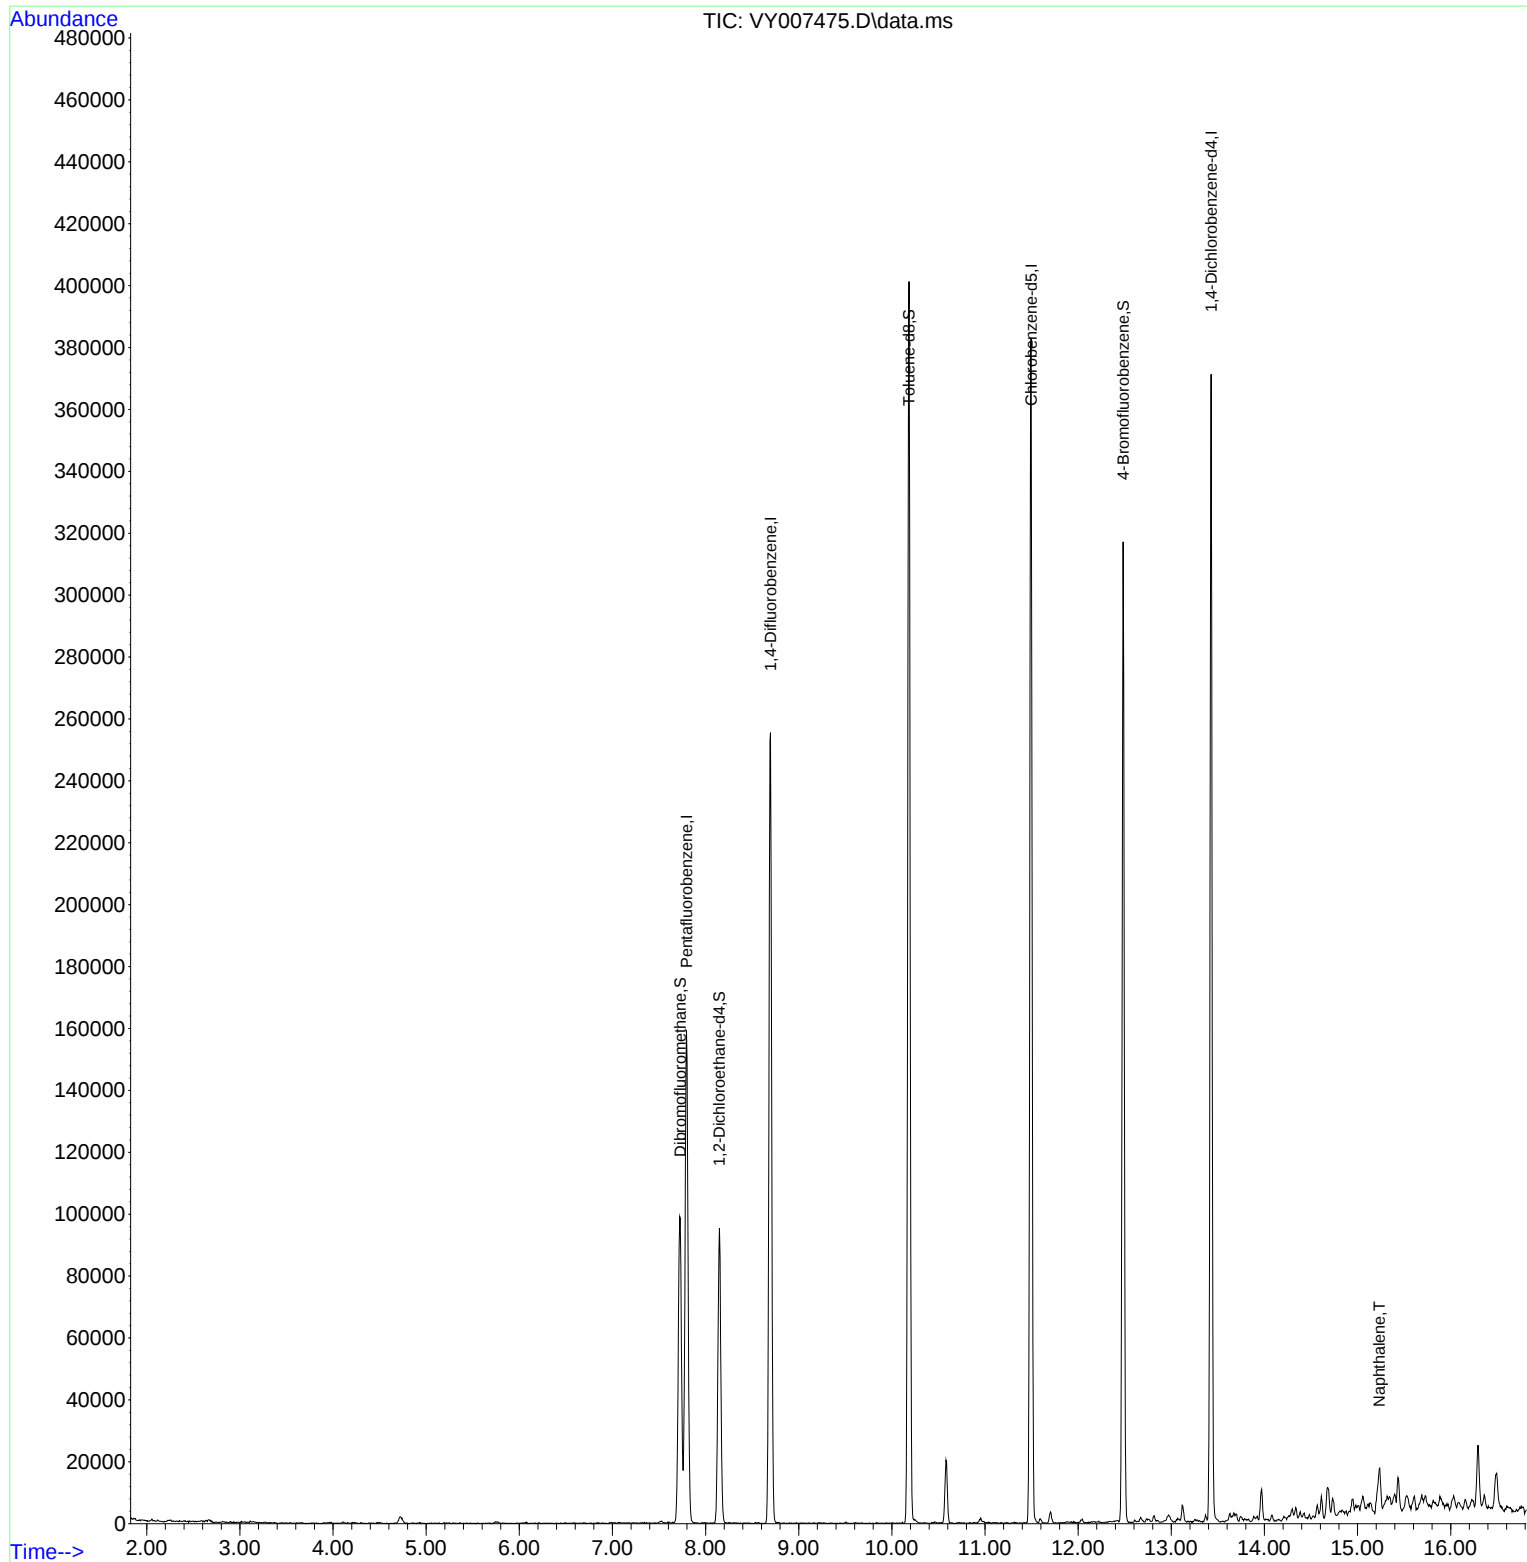


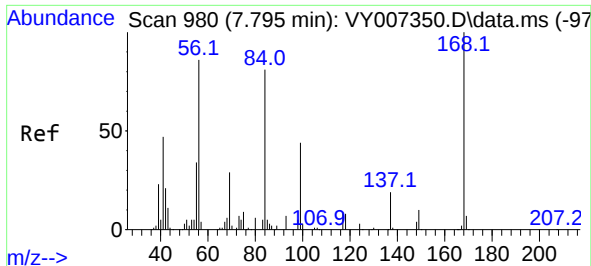

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY007475.D
Acq: 11 Feb 2022 11:24




Instrument :
MSVOA_Y
ClientSampleId :
VY0211SBL01


Tgt Ion:168 Resp: 118160
Ion Ratio Lower Upper
168 100
99 59.7 46.9 70.3

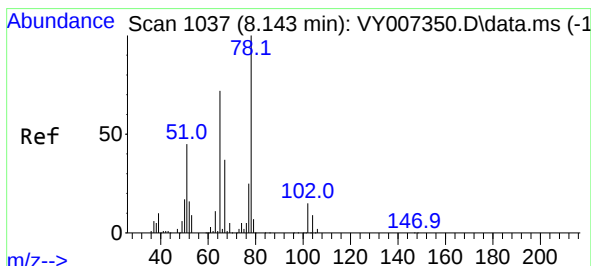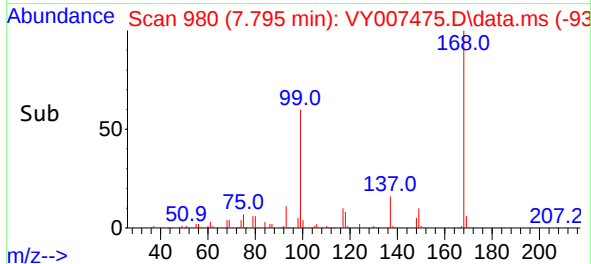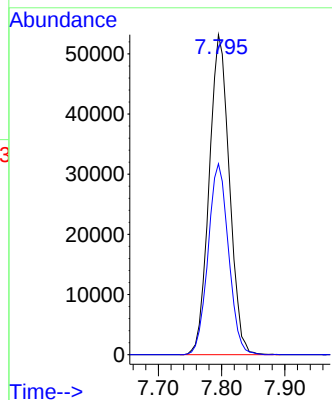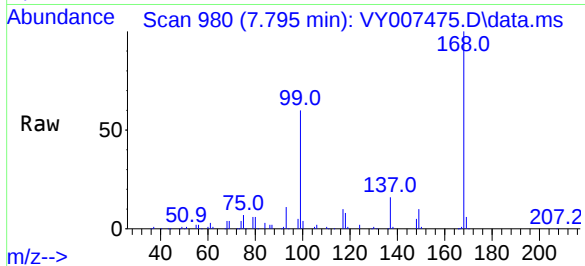

#33
1,2-Dichloroethane-d4
Concen: 54.820 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.006 min
Lab File: VY007475.D
Acq: 11 Feb 2022 11:24

Tgt Ion: 65 Resp: 74508
Ion Ratio Lower Upper
65 100
67 51.6 0.0 99.4

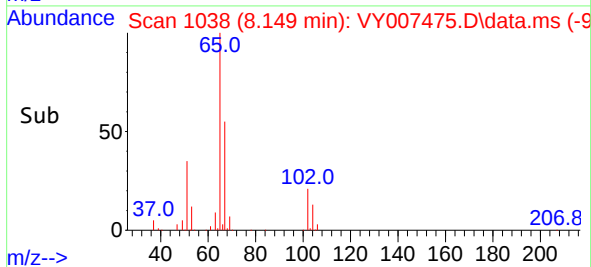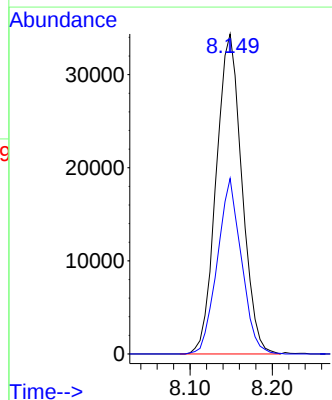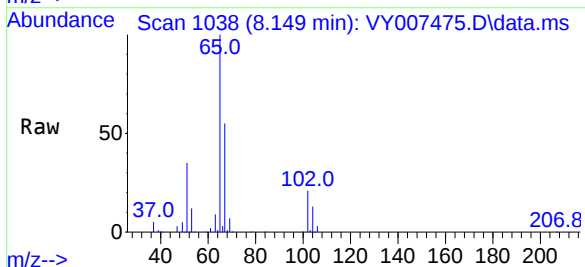

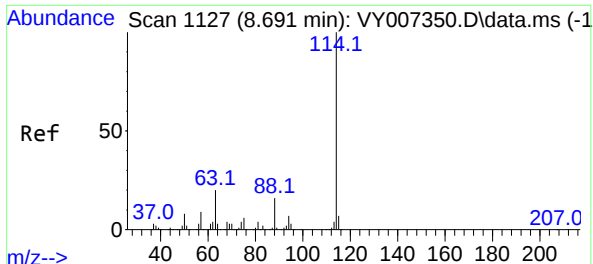

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.697 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY007475.D

Acq: 11 Feb 2022 11:24

Instrument :

MSVOA_Y

ClientSampleId :

VY0211SBL01





Tgt Ion:114 Resp: 221527

Ion Ratio Lower Upper

114 100

63 18.9 0.0 43.2

88 15.2 0.0 31.8

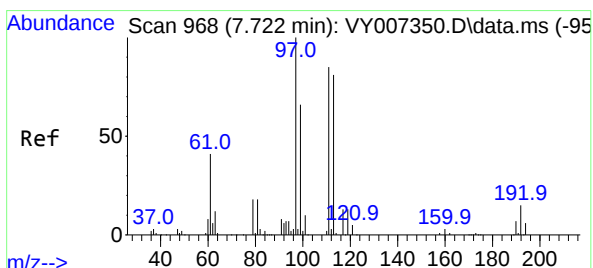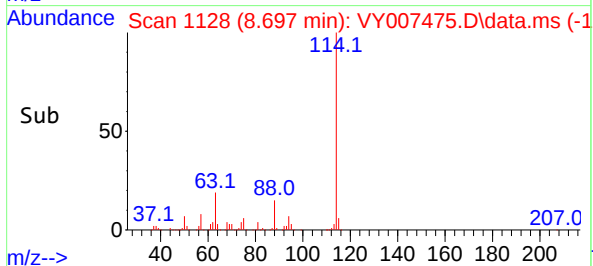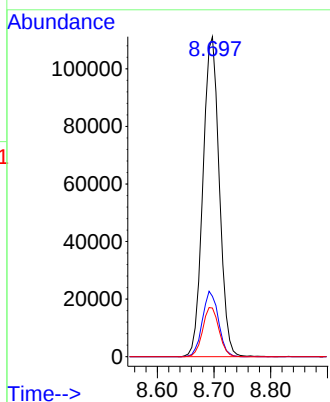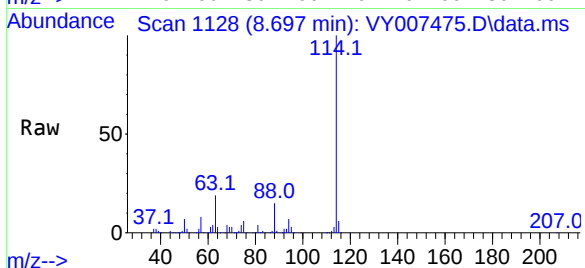

#35

Dibromofluoromethane

Concen: 50.313 ug/l

RT: 7.728 min Scan# 969

Delta R.T. 0.006 min

Lab File: VY007475.D

Acq: 11 Feb 2022 11:24




Tgt Ion:113 Resp: 71571


Ion Ratio Lower Upper

113 100

111 102.4 82.6 124.0

192 18.3 17.6 26.4


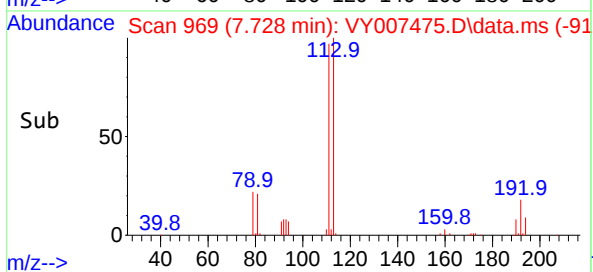
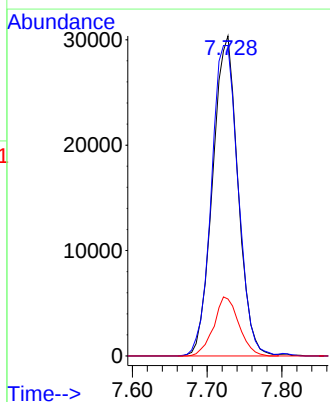
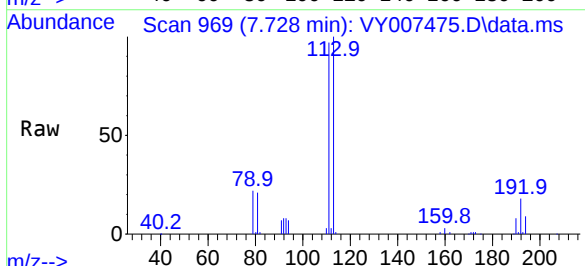


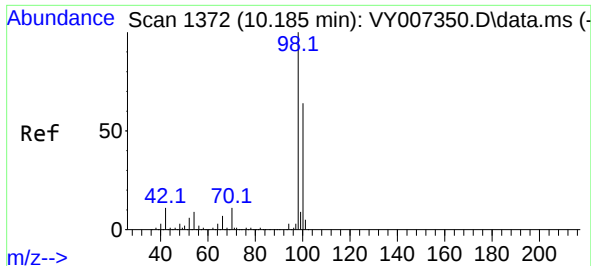

#50
Toluene-d8
Concen: 50.880 ug/l
RT: 10.185 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY007475.D
Acq: 11 Feb 2022 11:24




Instrument :
MSVOA_Y
ClientSampleId :
VY0211SBL01


Tgt Ion: 98 Resp: 267401
Ion Ratio Lower Upper
98 100
100 66.0 50.2 75.2

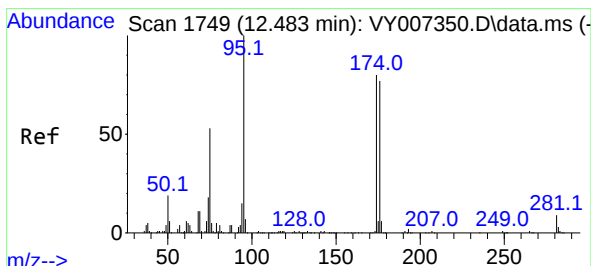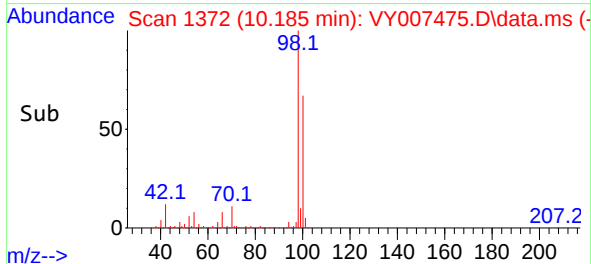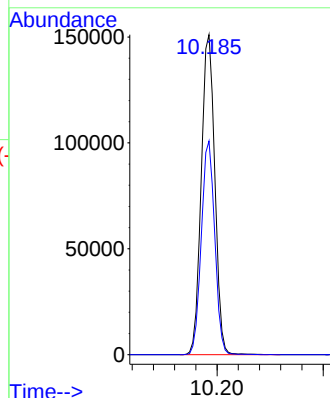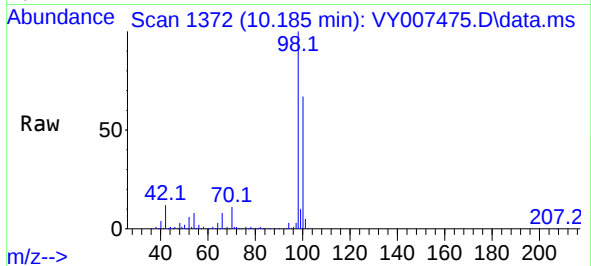

#62
4-Bromofluorobenzene
Concen: 53.617 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY007475.D
Acq: 11 Feb 2022 11:24

Tgt Ion: 95 Resp: 95774
Ion Ratio Lower Upper
95 100
174 77.7 0.0 177.0
176 75.8 0.0 175.8


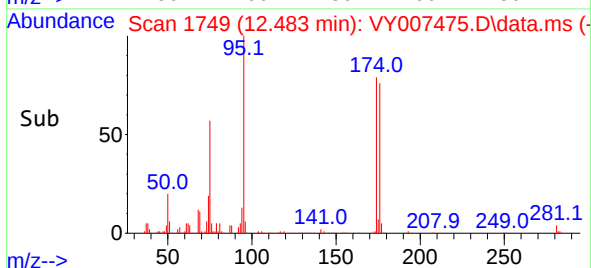
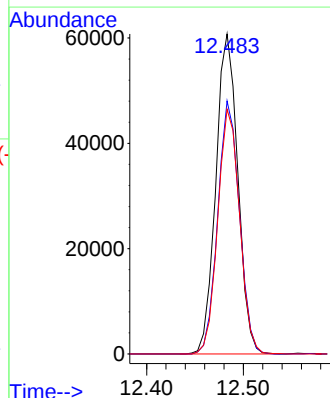
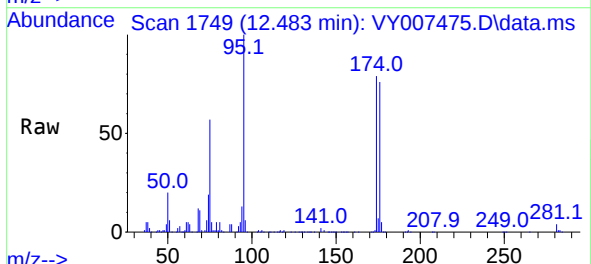


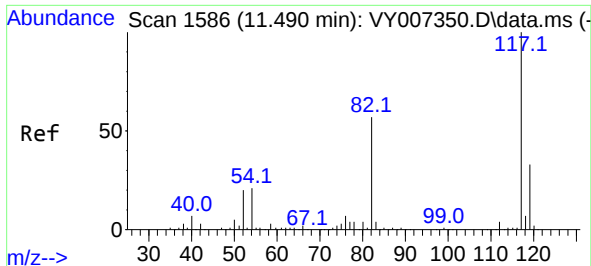

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY007475.D
Acq: 11 Feb 2022 11:24




Instrument :
MSVOA_Y
ClientSampleId :
VY0211SBL01


Tgt Ion:117 Resp: 211250
Ion Ratio Lower Upper
117 100
82 55.1 43.0 64.4
119 31.5 25.4 38.0

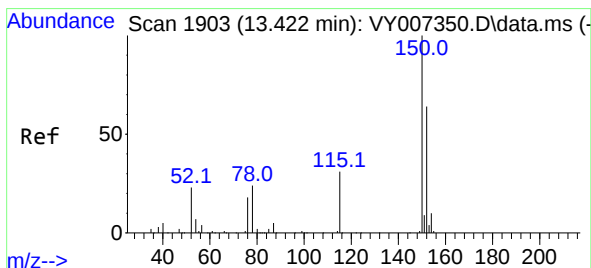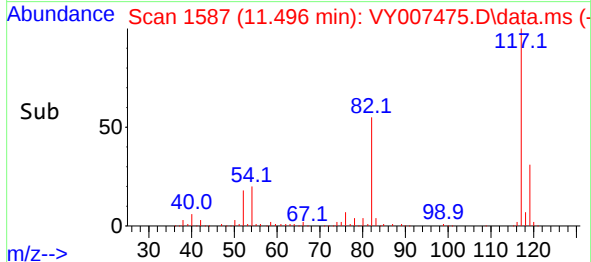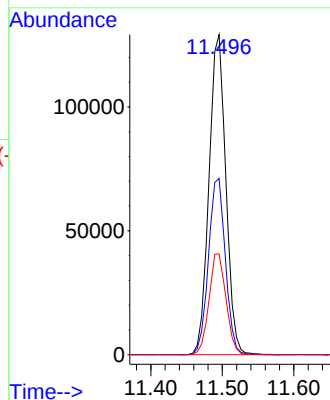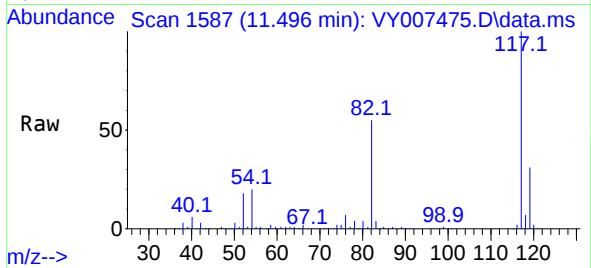

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY007475.D
Acq: 11 Feb 2022 11:24

Tgt Ion:152 Resp: 86708
Ion Ratio Lower Upper
152 100
115 63.4 28.2 84.7
150 161.0 0.0 347.6

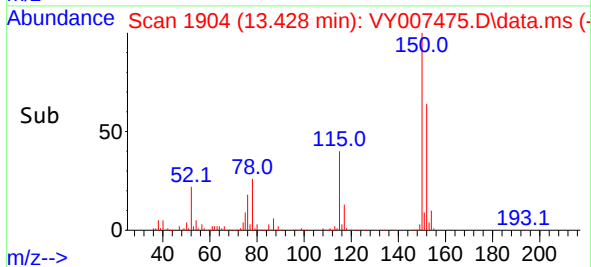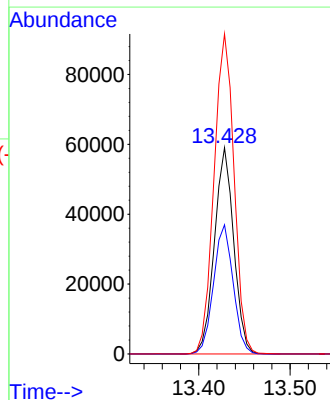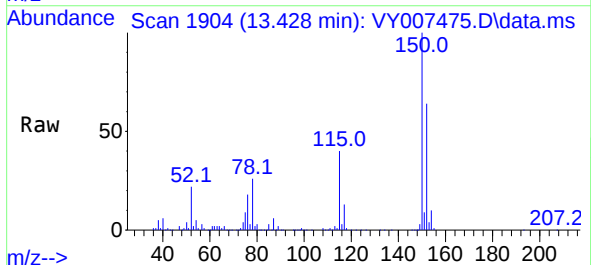

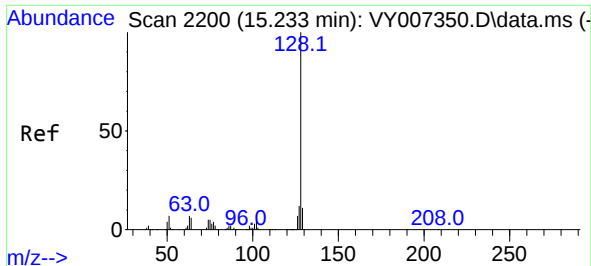

#95

Naphthalene

Concen: 2.892 ug/l

RT: 15.233 min Scan# 21

Delta R.T. -0.000 min

Lab File: VY007475.D


Acq: 11 Feb 2022 11:24

Instrument :

MSVOA_Y

ClientSampleId :

VY0211SBL01

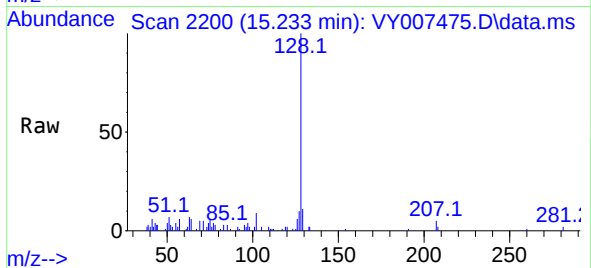

Tgt Ion:128 Resp: 10139

Ion Ratio Lower Upper

128 100

127 14.7 11.0 16.4

129 11.7 8.4 12.6

