
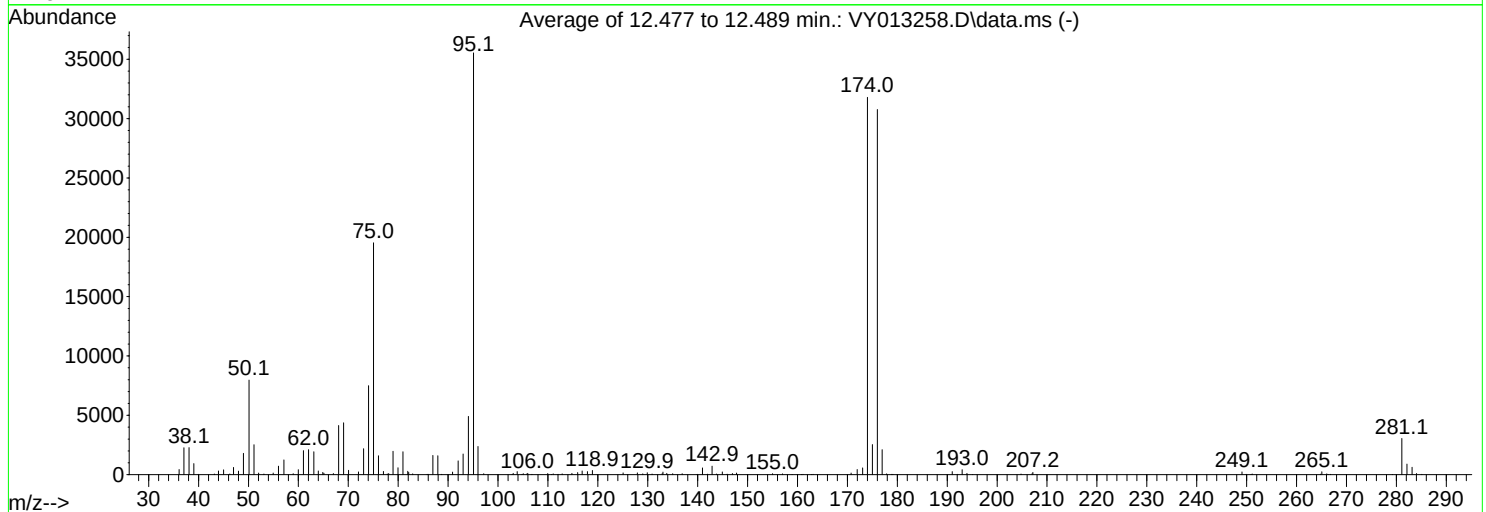


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041223\
Data File : VY013258.D
Acq On : 12 Apr 2023 09:34
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041223S.M
Title : SW846 8260
Last Update : Thu Apr 13 05:55:16 2023

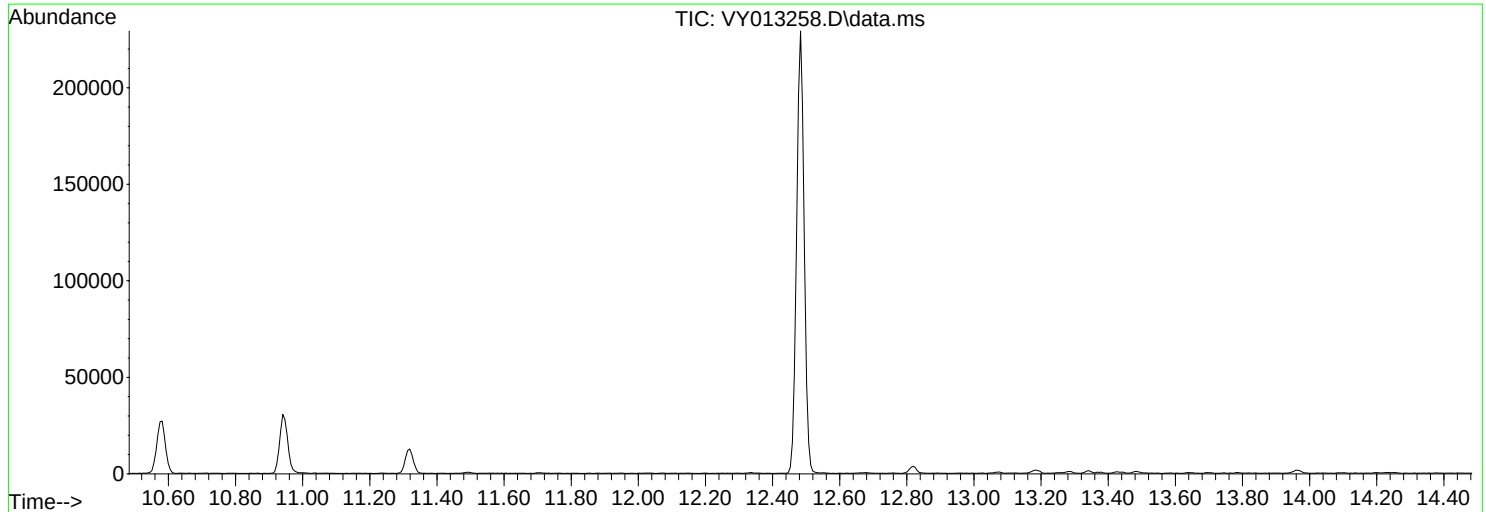

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	7970	PASS
75	95	30	60	55.0	19539	PASS
95	95	100	100	100.0	35541	PASS
96	95	5	9	6.7	2372	PASS
173	174	0.00	2	1.8	562	PASS
174	95	50	100	89.5	31797	PASS
175	174	5	9	8.0	2536	PASS
176	174	95	101	96.7	30760	PASS
177	176	5	9	6.8	2104	PASS