
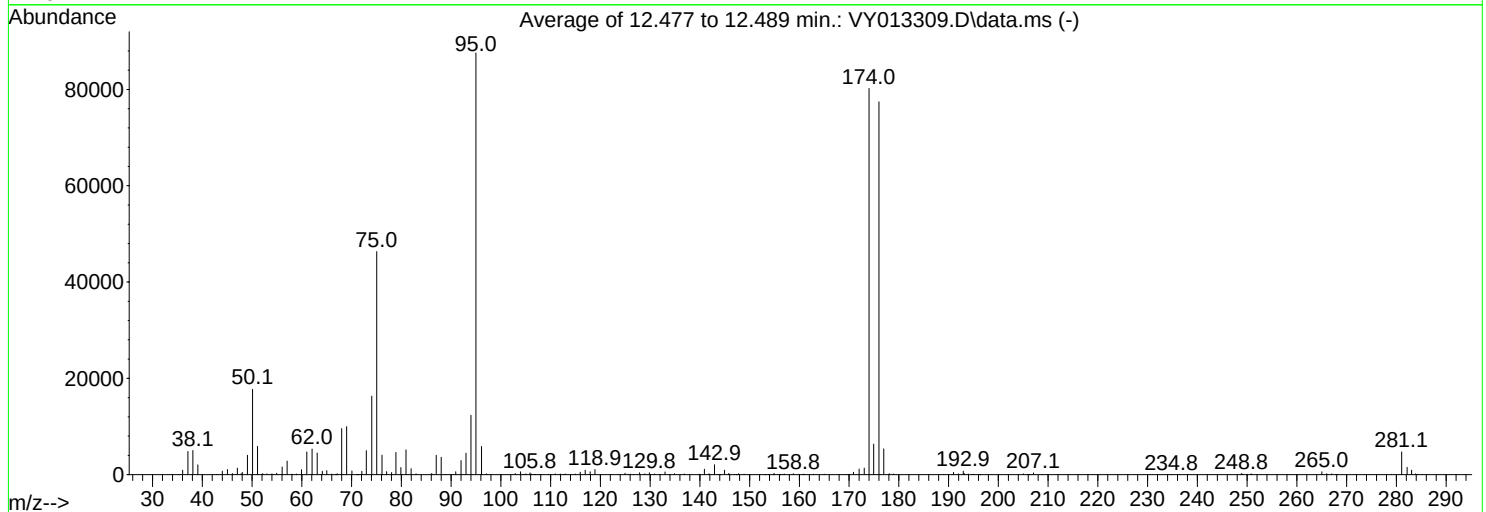


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041423\
Data File : VY013309.D
Acq On : 14 Apr 2023 09:03
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041223S.M
Title : SW846 8260
Last Update : Thu Apr 13 05:55:16 2023

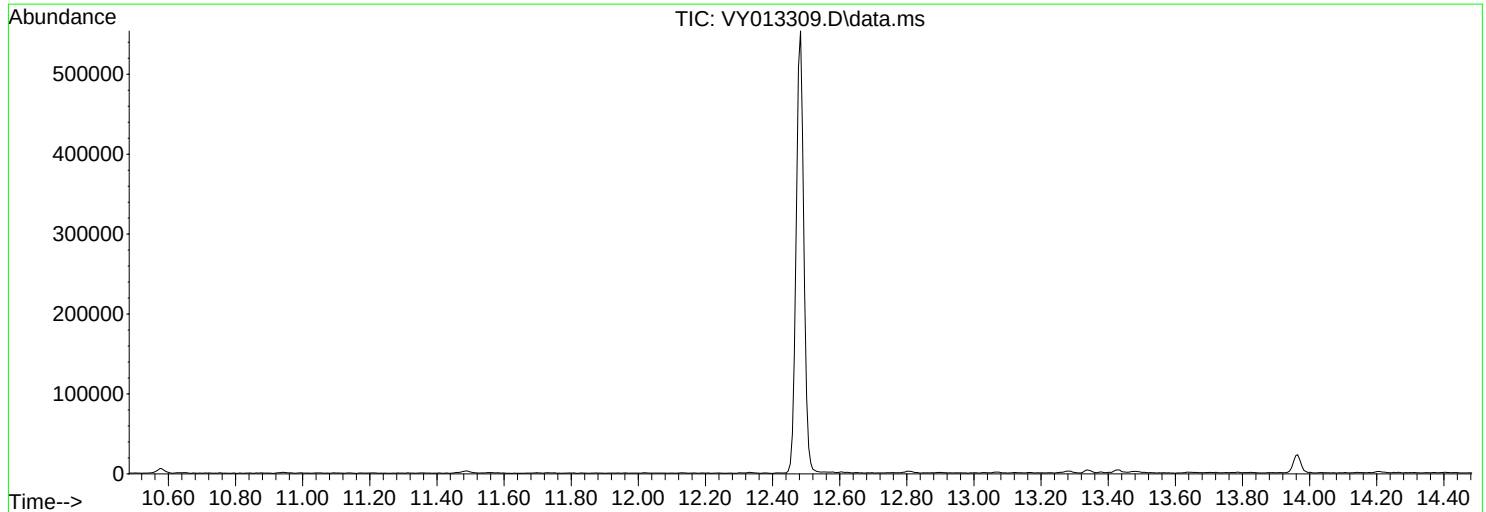

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	17727	PASS
75	95	30	60	52.9	46320	PASS
95	95	100	100	100.0	87605	PASS
96	95	5	9	6.7	5864	PASS
173	174	0.00	2	1.7	1362	PASS
174	95	50	100	91.6	80221	PASS
175	174	5	9	7.9	6360	PASS
176	174	95	101	96.5	77437	PASS
177	176	5	9	6.9	5341	PASS