
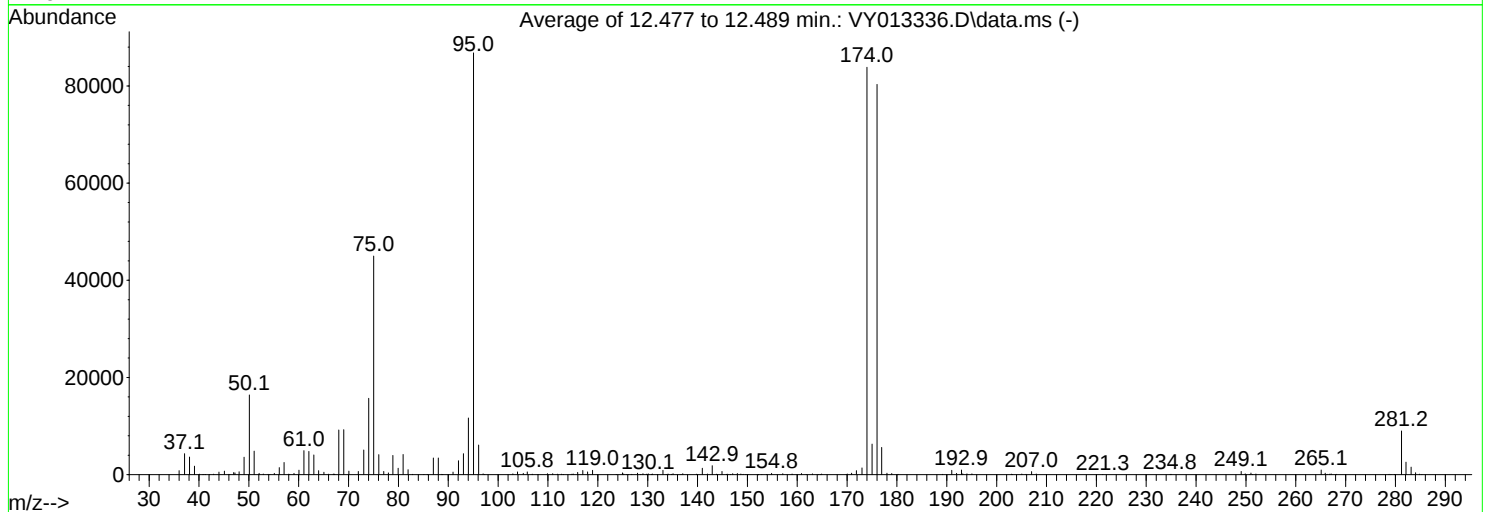


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY041923\
Data File : VY013336.D
Acq On : 19 Apr 2023 09:05
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y041223S.M
Title : SW846 8260
Last Update : Thu Apr 13 05:55:16 2023

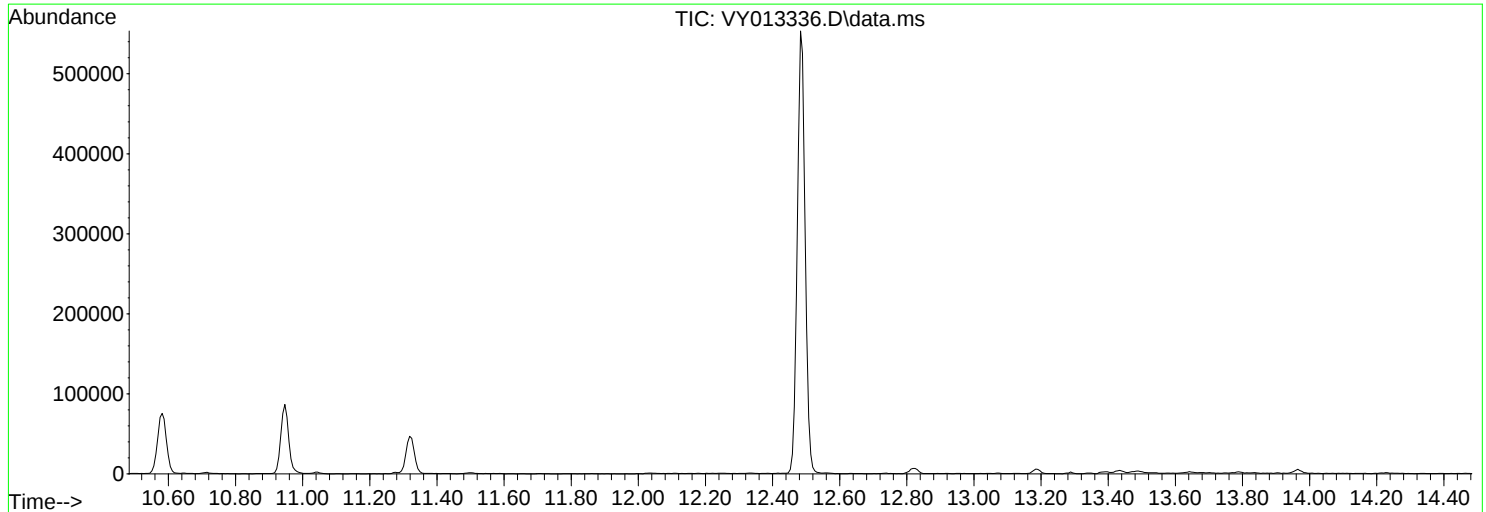

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	16418	PASS
75	95	30	60	51.8	44997	PASS
95	95	100	100	100.0	86811	PASS
96	95	5	9	7.0	6101	PASS
173	174	0.00	2	1.7	1384	PASS
174	95	50	100	96.6	83829	PASS
175	174	5	9	7.5	6282	PASS
176	174	95	101	95.8	80320	PASS
177	176	5	9	7.0	5596	PASS