
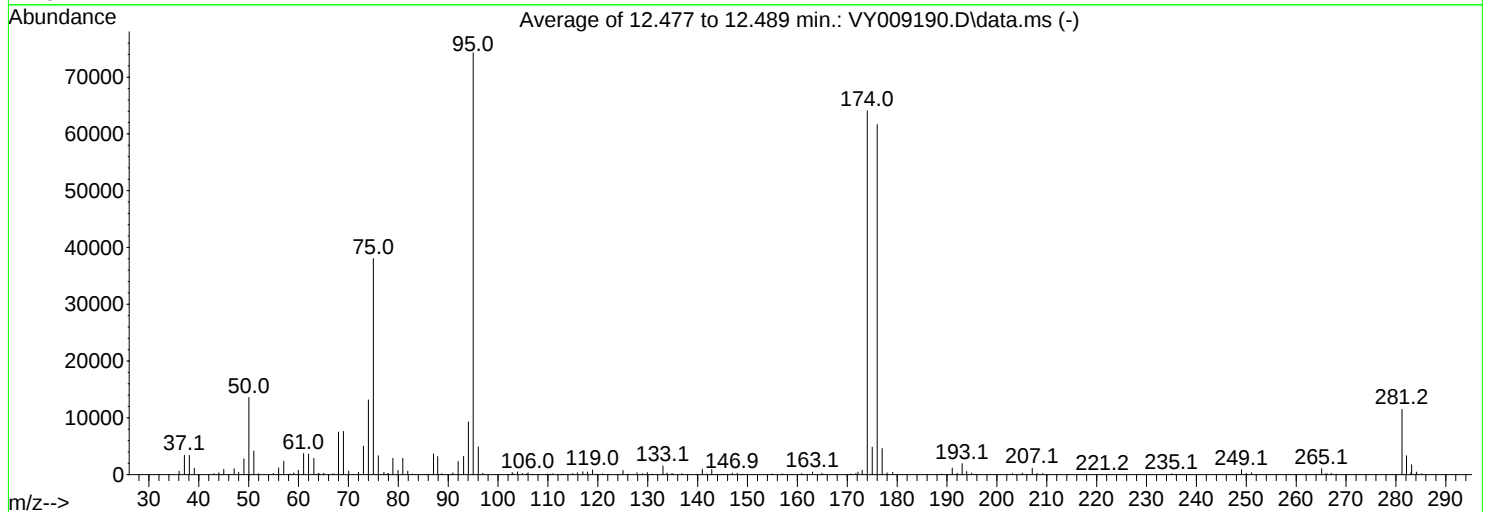


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY061622\
Data File : VY009190.D
Acq On : 16 Jun 2022 09:16
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y061522S.M
Title : SW846 8260
Last Update : Thu Jun 16 02:54:06 2022

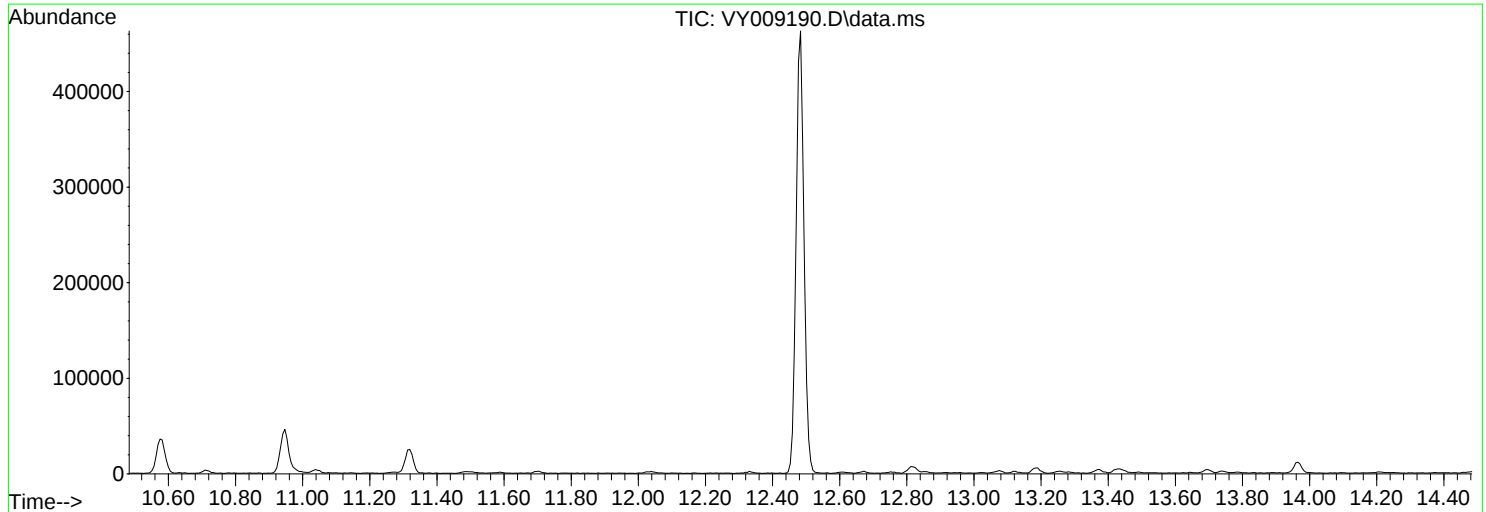

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	13568	PASS
75	95	30	60	51.2	38045	PASS
95	95	100	100	100.0	74277	PASS
96	95	5	9	6.6	4912	PASS
173	174	0.00	2	1.2	795	PASS
174	95	50	100	86.3	64080	PASS
175	174	5	9	7.6	4844	PASS
176	174	95	101	96.2	61637	PASS
177	176	5	9	7.4	4580	PASS