

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY062222\
 Data File : VY009274.D
 Acq On : 22 Jun 2022 15:11
 Operator : KP/MD
 Sample : VIBLK
 Misc : 5.00/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VIBLK


Quant Time: Jun 23 01:56:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062122S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 21 14:08:27 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	282142	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	415148	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	390832	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	199053	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	155130	50.06	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 100.12%			
35) Dibromofluoromethane	7.709	113	144674	53.81	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 107.62%			
50) Toluene-d8	10.178	98	466314	45.15	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 90.30%			
62) 4-Bromofluorobenzene	12.477	95	190018	52.36	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 104.72%			
Target Compounds						Qvalue
11) Tert butyl alcohol	4.917	59	1850	Below Cal	#	77
13) Acrolein	3.741	56	48	30.37	ug/l #	14
16) Acetone	3.942	43	2302	3.01	ug/l	96
18) Methyl Acetate	4.472	43	165	Below Cal	#	56
20) Methylene Chloride	4.710	84	16163	Below Cal	#	77
31) Cyclohexane	7.770	56	10975	2.04	ug/l #	66
36) 1,1-Dichloropropene	7.789	75	18058	4.41	ug/l #	51
38) Carbon Tetrachloride	7.783	117	24884	5.85	ug/l #	15
39) Methylcyclohexane	9.179	83	6777	1.35	ug/l	89
52) Toluene	10.239	92	16075	2.10	ug/l	99
55) 1,1,2-Trichloroethane	10.611	97	3285	1.32	ug/l #	22
59) 2-Hexanone	10.800	43	3226	2.02	ug/l #	28
67) Ethyl Benzene	11.593	91	124272	8.14	ug/l	99
68) m/p-Xylenes	11.697	106	258030	43.10	ug/l	93
69) o-Xylene	12.026	106	77543	13.62	ug/l	91
73) Isopropylbenzene	12.324	105	17758	1.14	ug/l	93
76) 1,2,3-Trichloropropane	12.733	75	3272	1.40	ug/l #	100
77) Bromobenzene	12.385	156	50595	13.34	ug/l #	1
78) n-propylbenzene	12.666	91	127342	6.77	ug/l	95
79) 2-Chlorotoluene	12.733	91	49057	4.63	ug/l #	41
80) 1,3,5-Trimethylbenzene	12.812	105	236659	18.25	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.477	75	97747	88.81	ug/l #	7
82) 4-Chlorotoluene	12.812	91	25583	2.31	ug/l #	41
83) tert-Butylbenzene	13.117	119	106186	9.39	ug/l #	70
84) 1,2,4-Trimethylbenzene	13.117	105	863977	68.01	ug/l	97
85) sec-Butylbenzene	13.117	105	863977	51.05	ug/l #	56
86) p-Isopropyltoluene	13.312	119	20896	1.49	ug/l	93
89) n-Butylbenzene	13.696	91	48375	3.69	ug/l #	73
90) Hexachloroethane	13.970	117	24400	9.14	ug/l #	6
92) 1,2-Dibromo-3-Chloropr...	14.336	75	1898	3.59	ug/l #	6
95) Naphthalene	15.232	128	439975	54.42	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 23 01:56:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y062122S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 21 14:08:27 2022
Response via : Initial Calibration







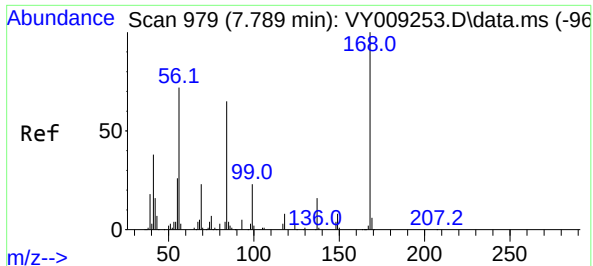

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 282142
Ion Ratio Lower Upper
168 100
99 50.8 46.9 70.3

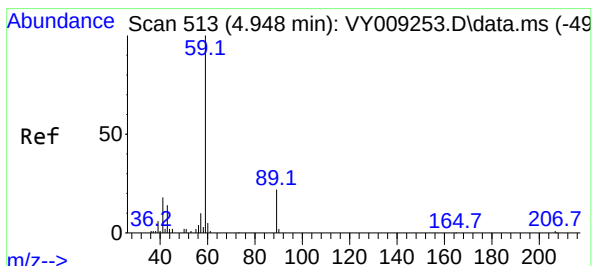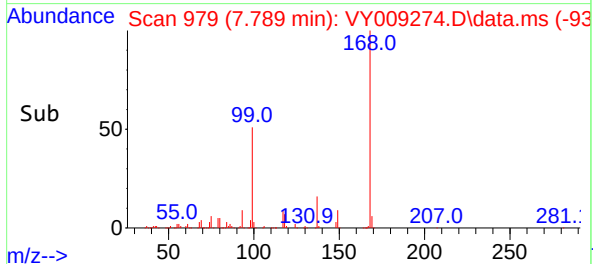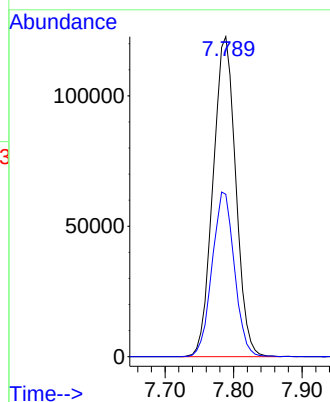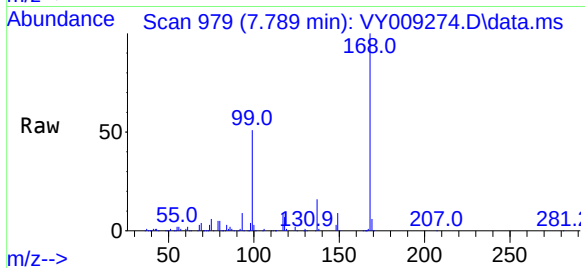

#11
Tert butyl alcohol
Concen: Below Cal
RT: 4.917 min Scan# 508
Delta R.T. -0.031 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11


Tgt Ion: 59 Resp: 1850
Ion Ratio Lower Upper
59 100
57 0.0 6.4 9.6#

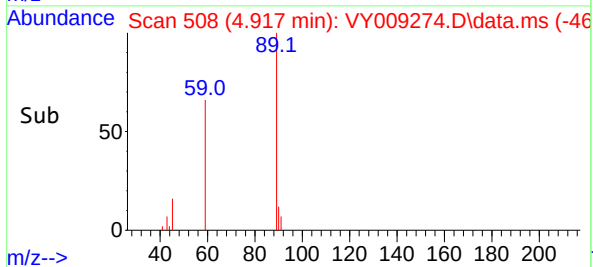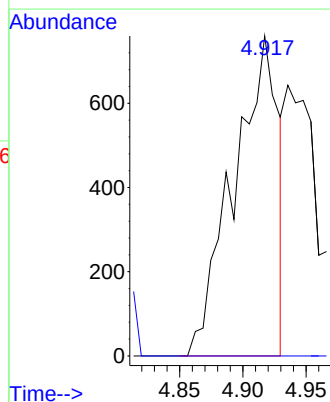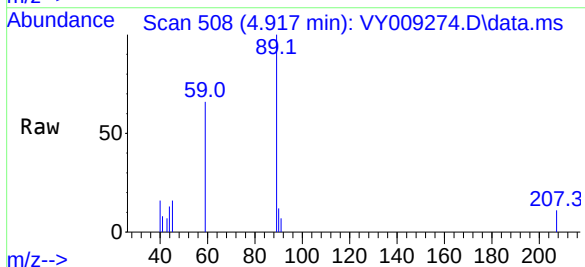






#13
Acrolein
Concen: 30.37 ug/l
RT: 3.741 min Scan# 312
Delta R.T. 0.018 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Instrument :
MSVOA_Y
ClientSampleId :
VIBLK



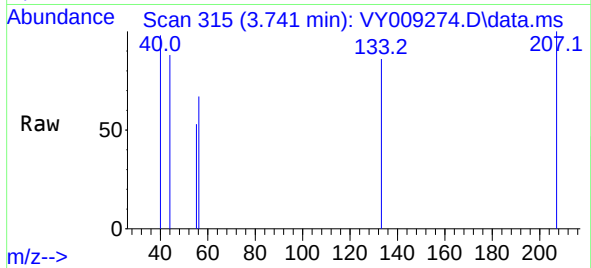



Tgt Ion: 56 Resp: 48
Ion Ratio Lower Upper
56 100
55 0.0 57.6 86.4#

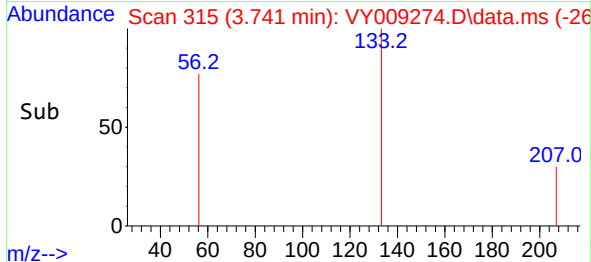

#16
Acetone
Concen: 3.01 ug/l
RT: 3.942 min Scan# 348
Delta R.T. 0.006 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion: 43 Resp: 2302
Ion Ratio Lower Upper
43 100
58 29.4 22.0 33.0







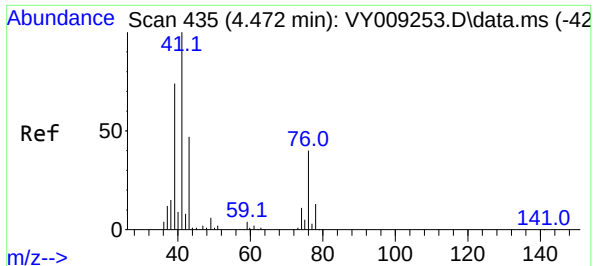

#18
Methyl Acetate
Concen: Below Cal
RT: 4.472 min Scan# 41
Delta R.T. 0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion: 43 Resp: 165
Ion Ratio Lower Upper
43 100
74 0.0 16.6 24.8#

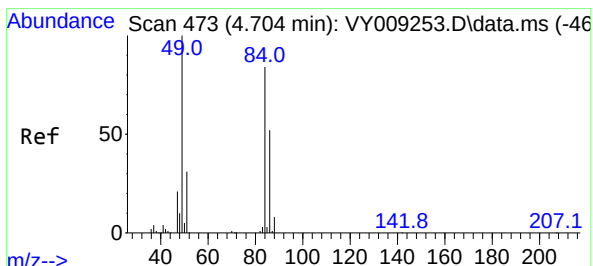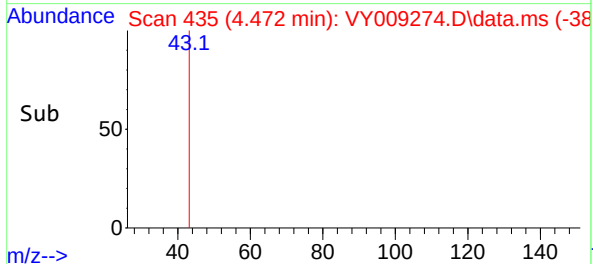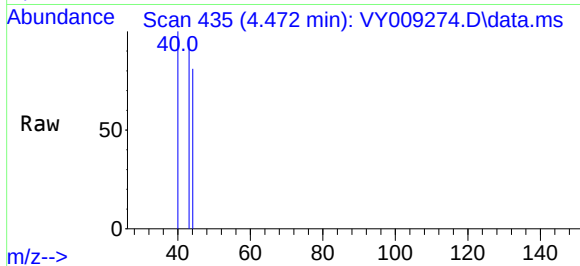

#20
Methylene Chloride
Concen: Below Cal
RT: 4.710 min Scan# 474
Delta R.T. 0.006 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion: 84 Resp: 16163
Ion Ratio Lower Upper
84 100
49 106.4 114.4 171.6#
51 33.4 35.3 52.9#
86 57.5 53.7 80.5


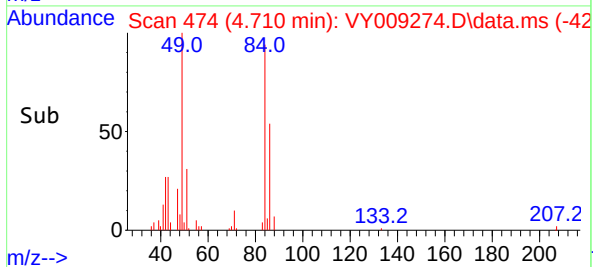

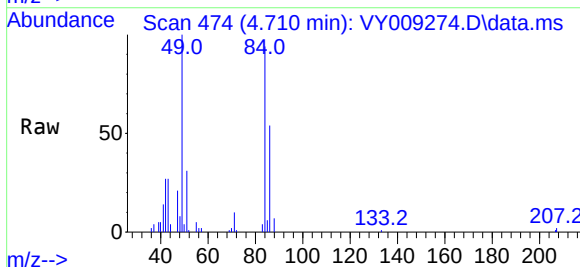




#31
Cyclohexane
Concen: 2.04 ug/l
RT: 7.770 min Scan# 91
Delta R.T. -0.007 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion: 56 Resp: 10975
Ion Ratio Lower Upper
56 100
69 84.0 26.7 40.1#
84 94.7 67.2 100.8

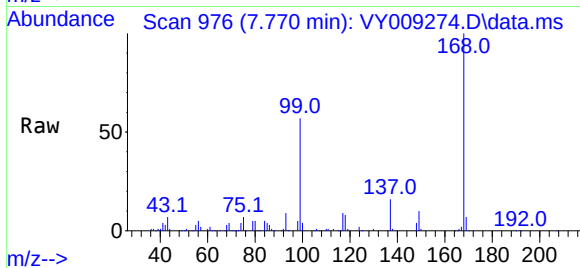

#33
1,2-Dichloroethane-d4
Concen: 50.06 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion: 65 Resp: 155130
Ion Ratio Lower Upper
65 100
67 52.5 0.0 99.4

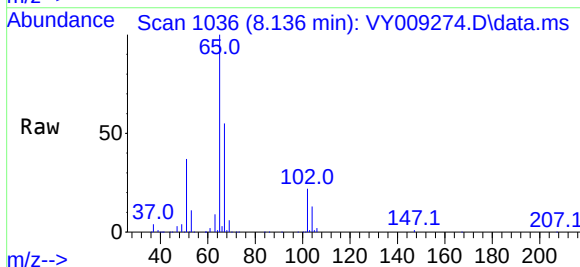



#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY009274.D

Acq: 22 Jun 2022 15:11

Instrument :

MSVOA_Y

ClientSampleId :

VIBLK





Tgt Ion:114 Resp: 415148

Ion Ratio Lower Upper

114 100

63 18.1 0.0 43.2

88 14.9 0.0 31.8

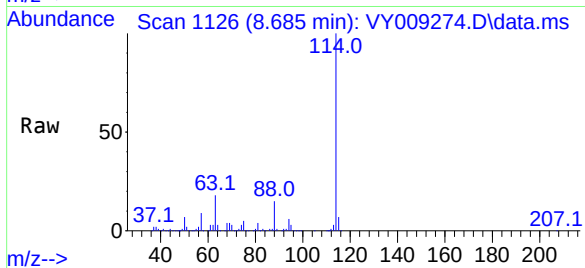

#35

Dibromofluoromethane

Concen: 53.81 ug/l

RT: 7.709 min Scan# 966

Delta R.T. -0.007 min

Lab File: VY009274.D

Acq: 22 Jun 2022 15:11




Tgt Ion:113 Resp: 144674


Ion Ratio Lower Upper

113 100

111 103.5 82.6 124.0

192 21.3 17.6 26.4




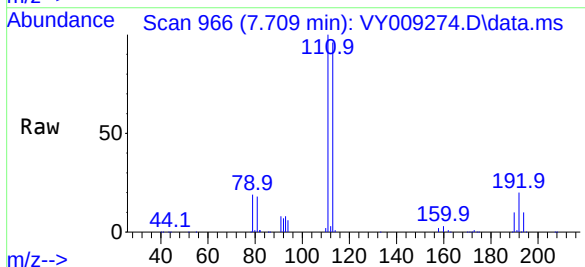


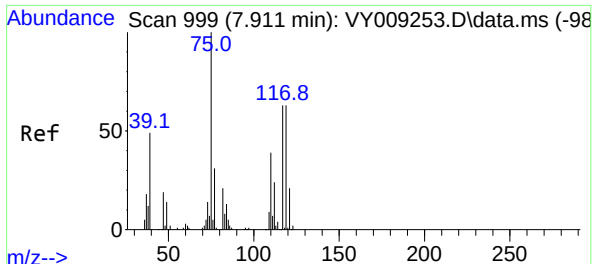

#36
1,1-Dichloropropene
Concen: 4.41 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.122 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion: 75 Resp: 18058
Ion Ratio Lower Upper
75 100
110 9.9 17.1 51.2#
77 0.0 24.4 36.6#

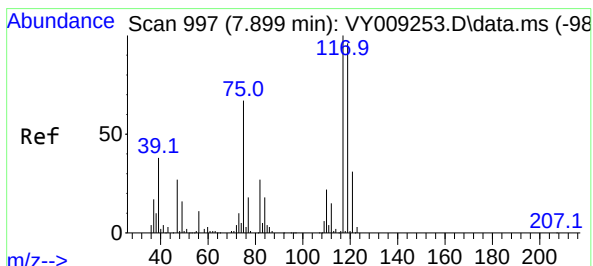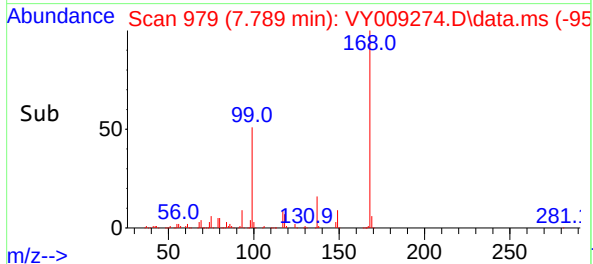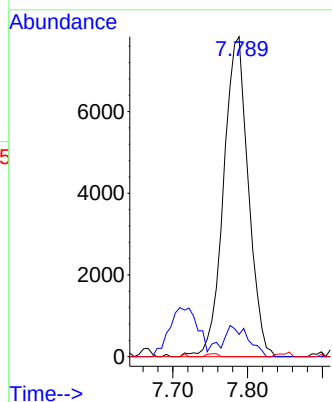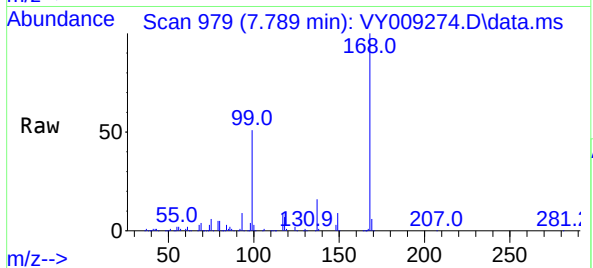

#38
Carbon Tetrachloride
Concen: 5.85 ug/l
RT: 7.783 min Scan# 978
Delta R.T. -0.116 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion: 117 Resp: 24884
Ion Ratio Lower Upper
117 100
119 5.1 77.9 116.9#
121 0.0 24.8 37.2#

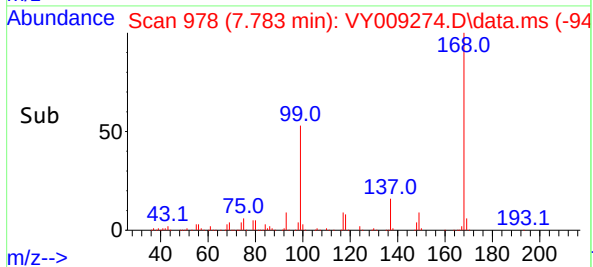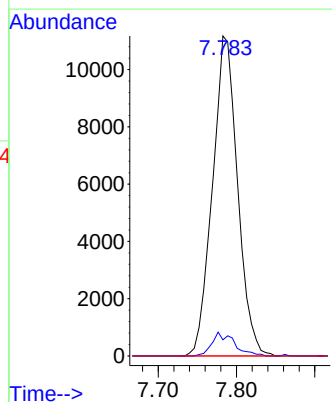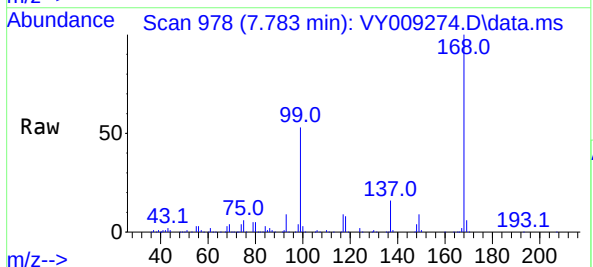



#39

Methylcyclohexane

Concen: 1.35 ug/l

RT: 9.179 min Scan# 1

Delta R.T. -0.000 min

Lab File: VY009274.D

Acq: 22 Jun 2022 15:11

Instrument :

MSVOA_Y

ClientSampleId :

VIBLK





Tgt Ion: 83 Resp: 6777

Ion Ratio Lower Upper

83 100

55 95.2 66.5 99.7

98 52.6 37.9 56.9

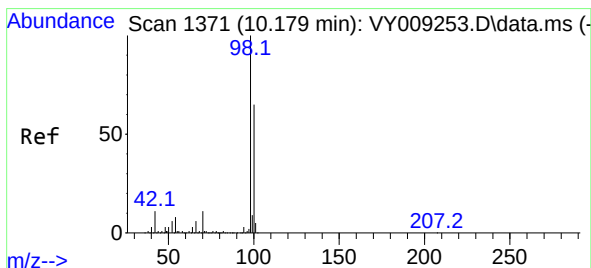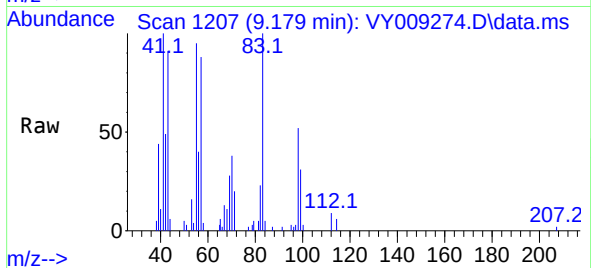

#50

Toluene-d8

Concen: 45.15 ug/l

RT: 10.178 min Scan# 1371

Delta R.T. -0.001 min

Lab File: VY009274.D




Acq: 22 Jun 2022 15:11


Tgt Ion: 98 Resp: 466314

Ion Ratio Lower Upper

98 100

100 66.1 50.2 75.2









#52
Toluene
Concen: 2.10 ug/l
RT: 10.239 min Scan# 1381
Delta R.T. -0.001 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion: 92 Resp: 16075
Ion Ratio Lower Upper
92 100
91 179.5 142.6 213.8

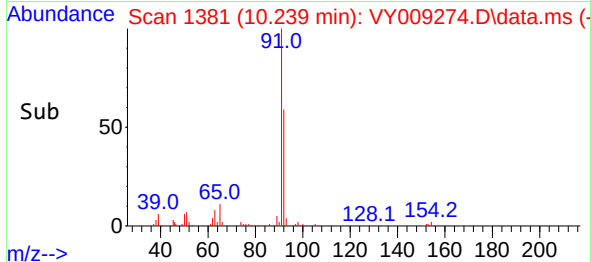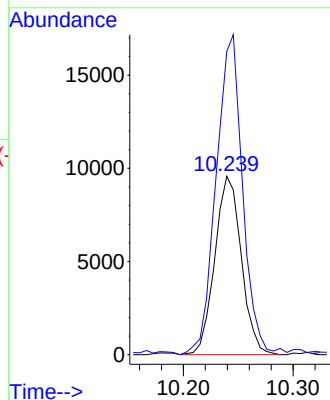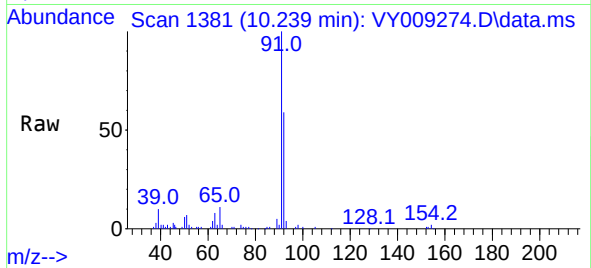

#55
1,1,2-Trichloroethane
Concen: 1.32 ug/l
RT: 10.611 min Scan# 1442
Delta R.T. -0.031 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion: 97 Resp: 3285
Ion Ratio Lower Upper
97 100
83 8.8 69.8 104.8#
85 8.9 44.3 66.5#
99 0.0 49.8 74.6#


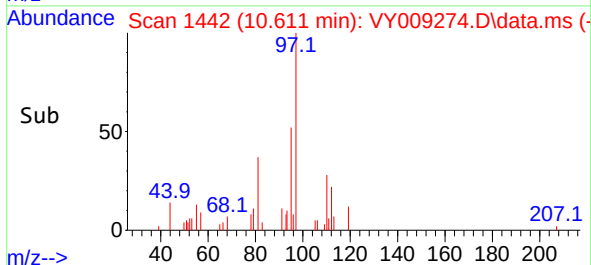
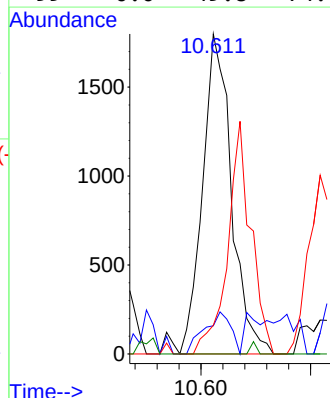





#59
2-Hexanone
Concen: 2.02 ug/l
RT: 10.800 min Scan# 1478
Delta R.T. -0.031 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion: 43 Resp: 3226
Ion Ratio Lower Upper
43 100
58 0.0 24.4 73.4#



#62
4-Bromofluorobenzene
Concen: 52.36 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion: 95 Resp: 190018
Ion Ratio Lower Upper
95 100
174 85.2 0.0 177.0
176 82.0 0.0 175.8


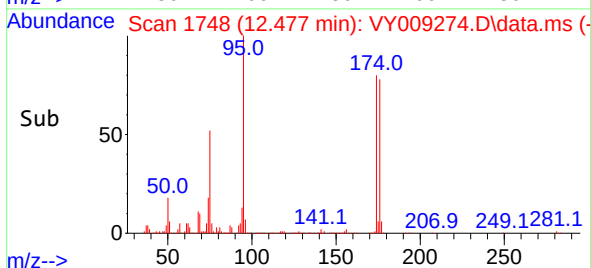
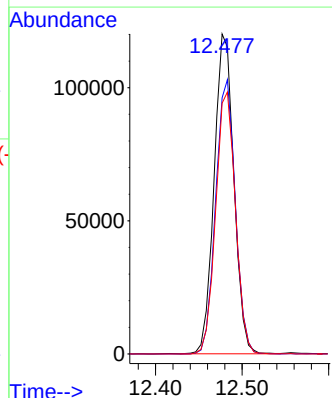





#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.489 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion:117 Resp: 390832
Ion Ratio Lower Upper
117 100
82 51.7 43.0 64.4
119 32.8 25.4 38.0



#67
Ethyl Benzene
Concen: 8.14 ug/l
RT: 11.593 min Scan# 1603
Delta R.T. -0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion: 91 Resp: 124272
Ion Ratio Lower Upper
91 100
106 31.2 24.5 36.7


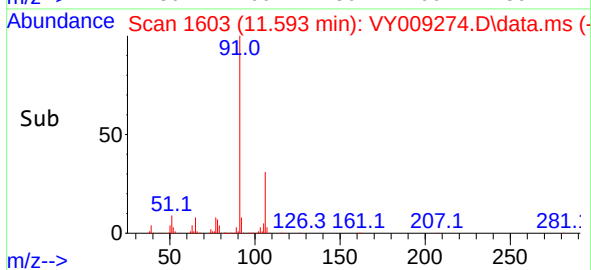






#68
m/p-Xylenes
Concen: 43.10 ug/l
RT: 11.697 min Scan# 1620
Delta R.T. -0.006 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion:106 Resp: 258030
Ion Ratio Lower Upper
106 100
91 197.6 166.6 249.8

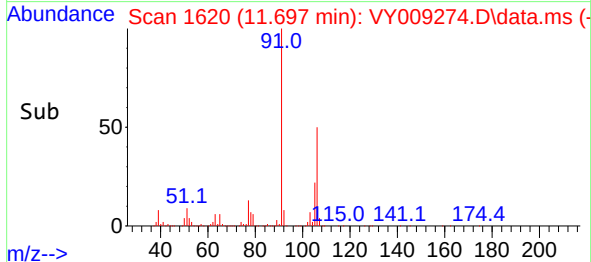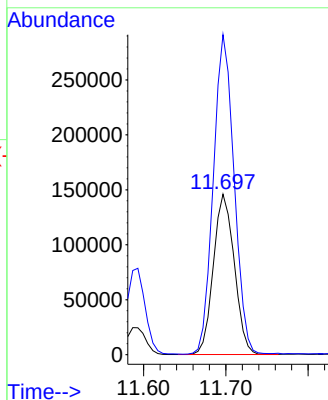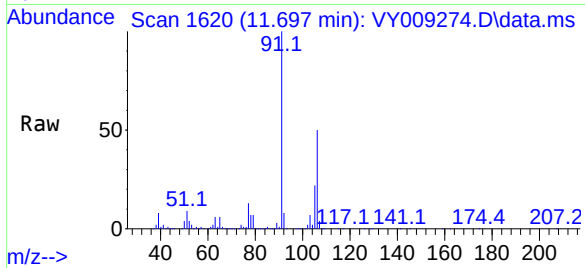

#69
o-Xylene
Concen: 13.62 ug/l
RT: 12.026 min Scan# 1674
Delta R.T. -0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion:106 Resp: 77543
Ion Ratio Lower Upper
106 100
91 206.2 110.3 331.0



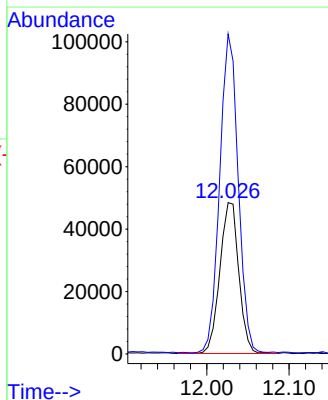
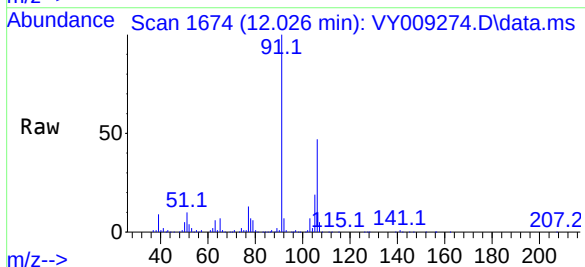




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion:152 Resp: 199053
Ion Ratio Lower Upper
152 100
115 61.2 28.2 84.7
150 157.7 0.0 347.6

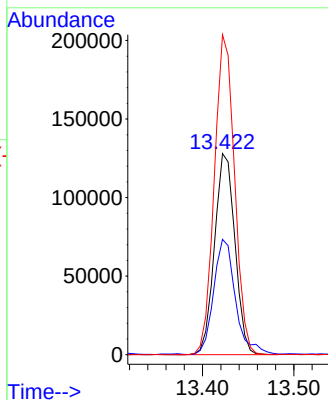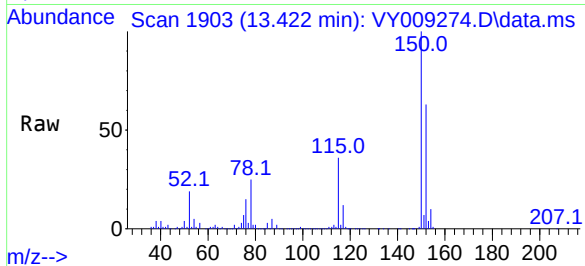

#73
Isopropylbenzene
Concen: 1.14 ug/l
RT: 12.324 min Scan# 1723
Delta R.T. -0.001 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion:105 Resp: 17758
Ion Ratio Lower Upper
105 100
120 30.6 13.4 40.2


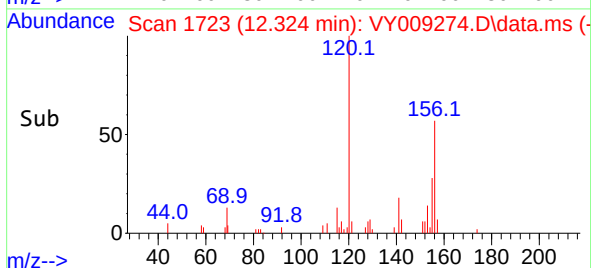
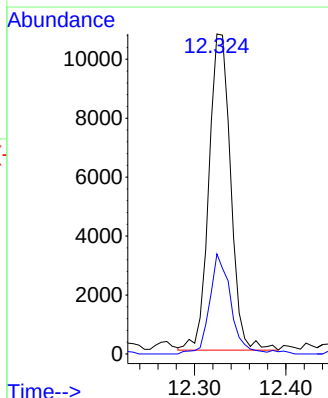
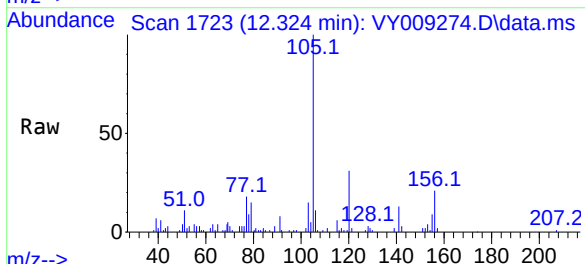




#76
1,2,3-Trichloropropane
Concen: 1.40 ug/l
RT: 12.733 min Scan# 1733
Delta R.T. 0.103 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion: 75 Resp: 3272
Ion Ratio Lower Upper
75 100
77 1431.4 0.0 0.0#

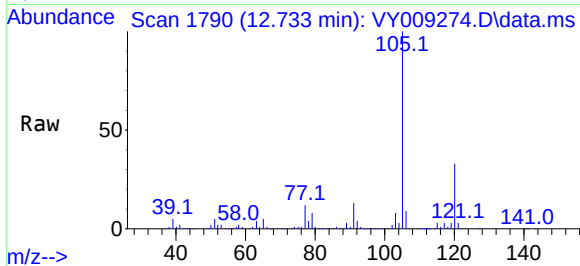

#77
Bromobenzene
Concen: 13.34 ug/l
RT: 12.385 min Scan# 1733
Delta R.T. -0.220 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion:156 Resp: 50595
Ion Ratio Lower Upper
156 100
77 0.0 95.5 286.4#
158 0.3 48.0 144.0#




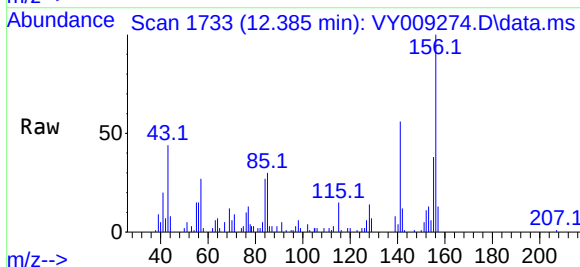




#78
n-propylbenzene
Concen: 6.77 ug/l
RT: 12.666 min Scan# 1779
Delta R.T. -0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion: 91 Resp: 127342
Ion Ratio Lower Upper
91 100
120 25.1 11.3 33.9

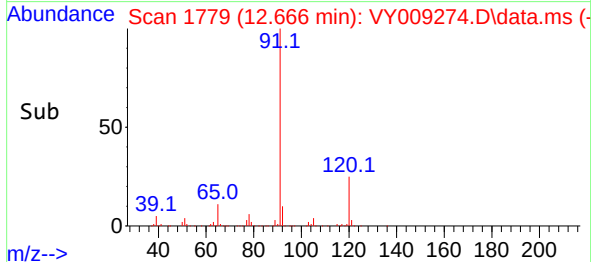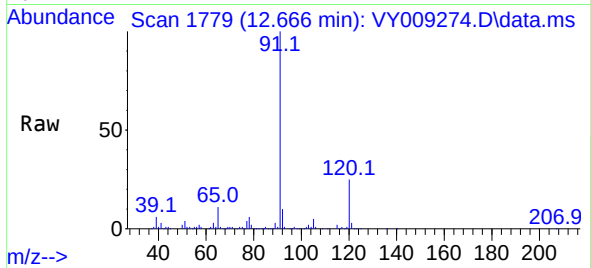

#79
2-Chlorotoluene
Concen: 4.63 ug/l
RT: 12.733 min Scan# 1790
Delta R.T. -0.025 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion: 91 Resp: 49057
Ion Ratio Lower Upper
91 100
126 0.3 16.9 50.6#


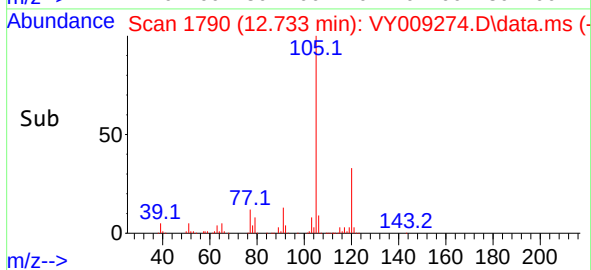






#80
1,3,5-Trimethylbenzene
Concen: 18.25 ug/l
RT: 12.812 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion:105 Resp: 236659
Ion Ratio Lower Upper
105 100
120 49.1 24.4 73.4

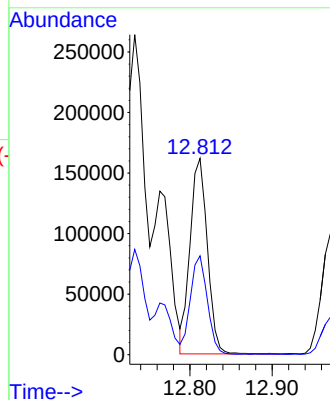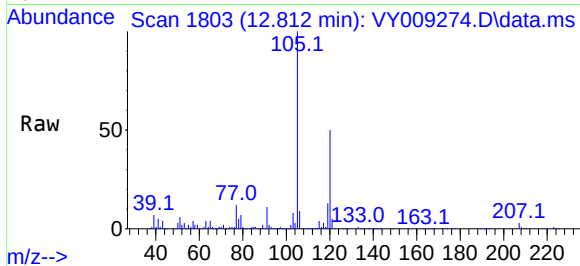

#81
trans-1,4-Dichloro-2-butene
Concen: 88.81 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.104 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion: 75 Resp: 97747
Ion Ratio Lower Upper
75 100
53 0.0 85.3 127.9#
89 0.3 37.0 55.4#


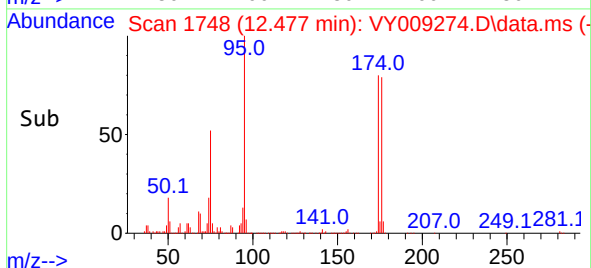
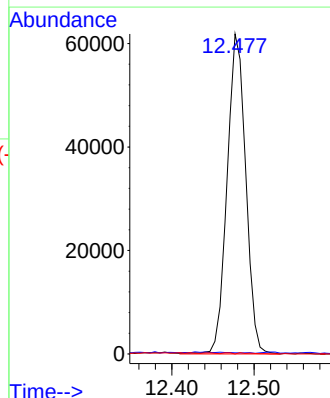





#82
4-Chlorotoluene
Concen: 2.31 ug/l
RT: 12.812 min Scan# 1810
Delta R.T. -0.043 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion: 91 Resp: 25583
Ion Ratio Lower Upper
91 100
126 0.3 17.0 51.0#

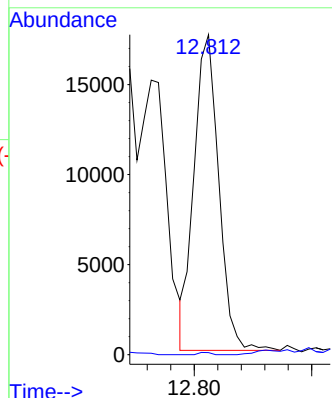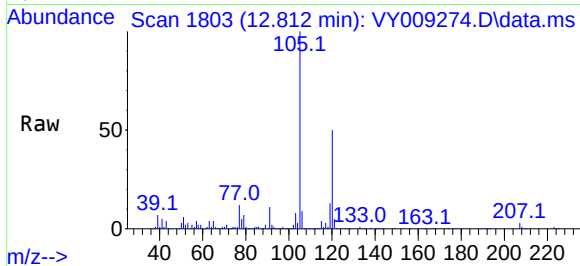

#83
tert-Butylbenzene
Concen: 9.39 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. 0.042 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion: 119 Resp: 106186
Ion Ratio Lower Upper
119 100
91 87.7 34.8 104.4
134 0.0 13.3 39.9#


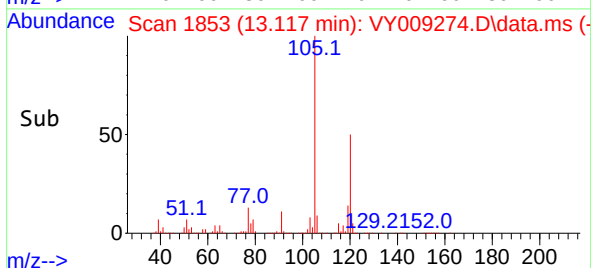
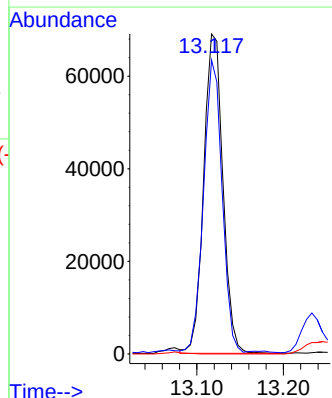
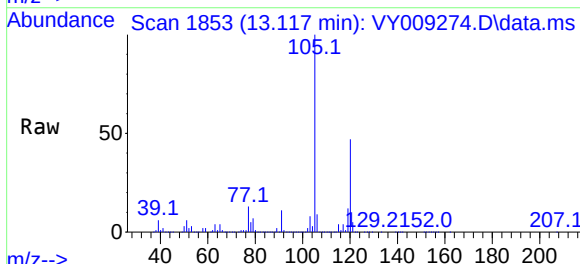




#84
1,2,4-Trimethylbenzene
Concen: 68.01 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion:105 Resp: 863977
Ion Ratio Lower Upper
105 100
120 46.7 22.3 66.9

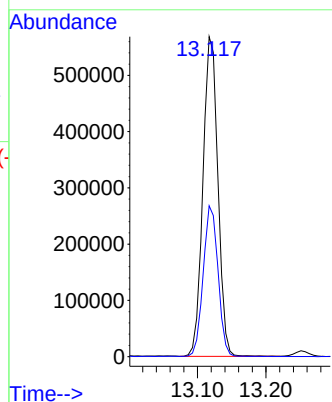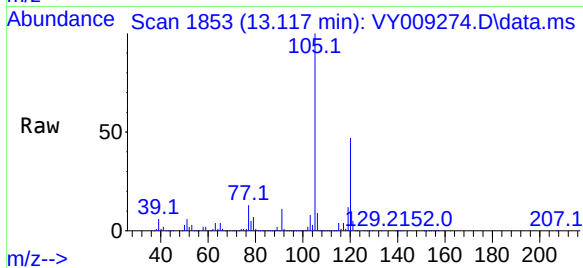

#85
sec-Butylbenzene
Concen: 51.05 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. -0.134 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion:105 Resp: 863977
Ion Ratio Lower Upper
105 100
134 0.0 10.2 30.4#



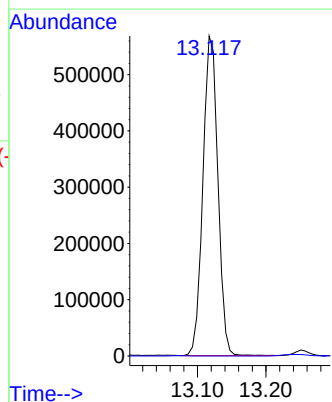
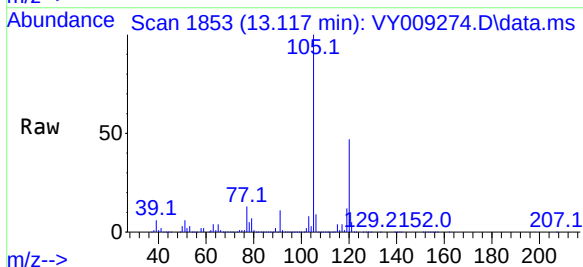




#86
p-Isopropyltoluene
Concen: 1.49 ug/l
RT: 13.312 min Scan# 119
Delta R.T. -0.055 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion:	119	Resp:	20896
Ion Ratio	Lower	Upper	
119	100		
134	30.8	13.2	39.5
91	22.3	12.4	37.2

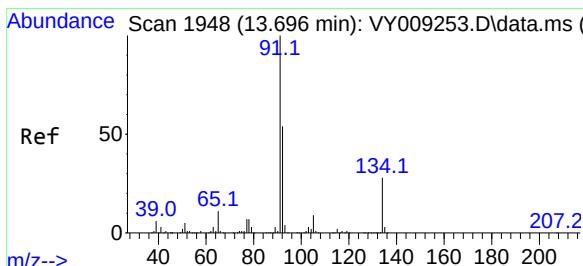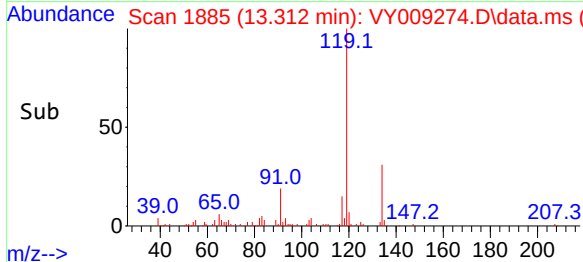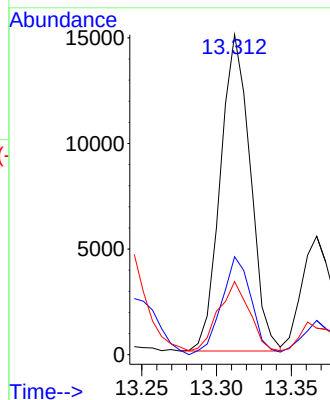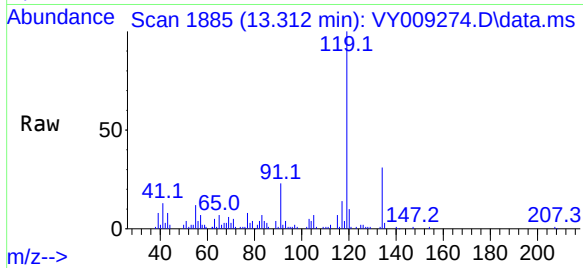

#89
n-Butylbenzene
Concen: 3.69 ug/l
RT: 13.696 min Scan# 1948
Delta R.T. 0.000 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion:	91	Resp:	48375
Ion Ratio	Lower	Upper	
91	100		
92	63.3	26.3	78.9
134	0.0	13.0	38.9


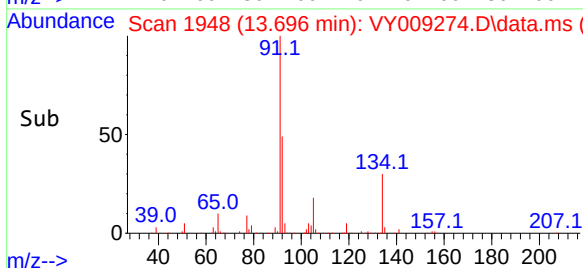
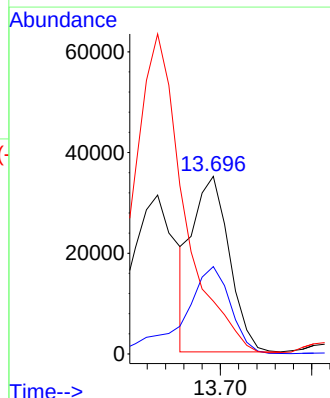
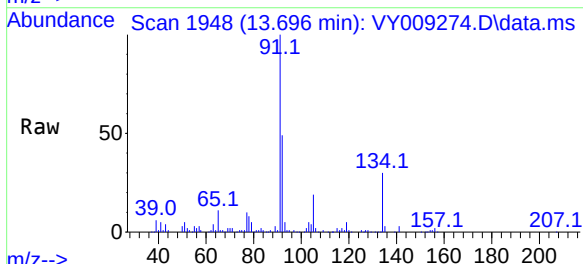




#90
Hexachloroethane
Concen: 9.14 ug/l
RT: 13.970 min Scan# 1991
Delta R.T. 0.011 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11




Instrument :
MSVOA_Y
ClientSampleId :
VIBLK


Tgt Ion:117 Resp: 24400
Ion Ratio Lower Upper
117 100
201 0.0 43.0 128.8#

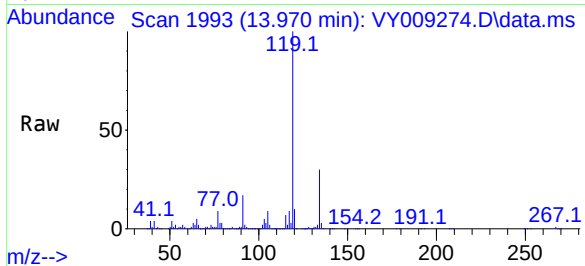

#92
1,2-Dibromo-3-Chloropropane
Concen: 3.59 ug/l
RT: 14.336 min Scan# 2053
Delta R.T. -0.019 min
Lab File: VY009274.D
Acq: 22 Jun 2022 15:11

Tgt Ion: 75 Resp: 1898
Ion Ratio Lower Upper
75 100
155 0.0 38.0 113.9#
157 0.0 47.8 143.3#

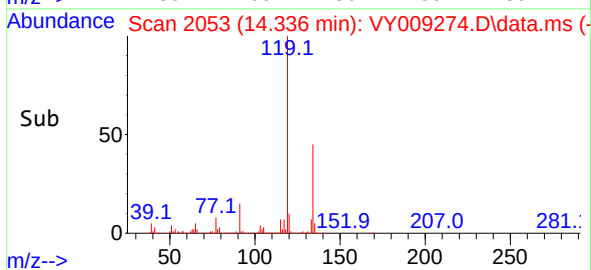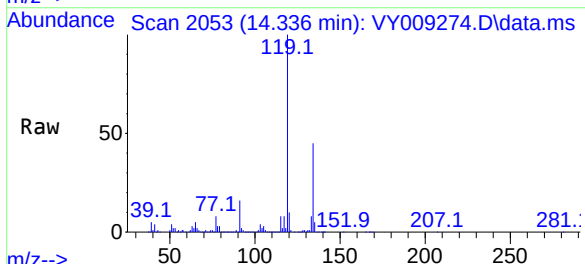



#95

Naphthalene

Concen: 54.42 ug/l

RT: 15.232 min Scan# 21

Delta R.T. -0.001 min

Lab File: VY009274.D


Acq: 22 Jun 2022 15:11

Instrument :

MSVOA_Y

ClientSampleId :

VIBLK

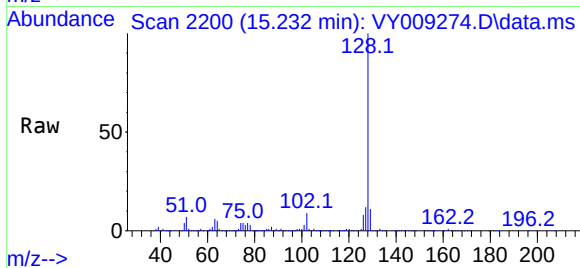

Tgt Ion:128 Resp: 439975

Ion Ratio Lower Upper

128 100

127 13.1 11.0 16.4

129 11.1 8.4 12.6

