
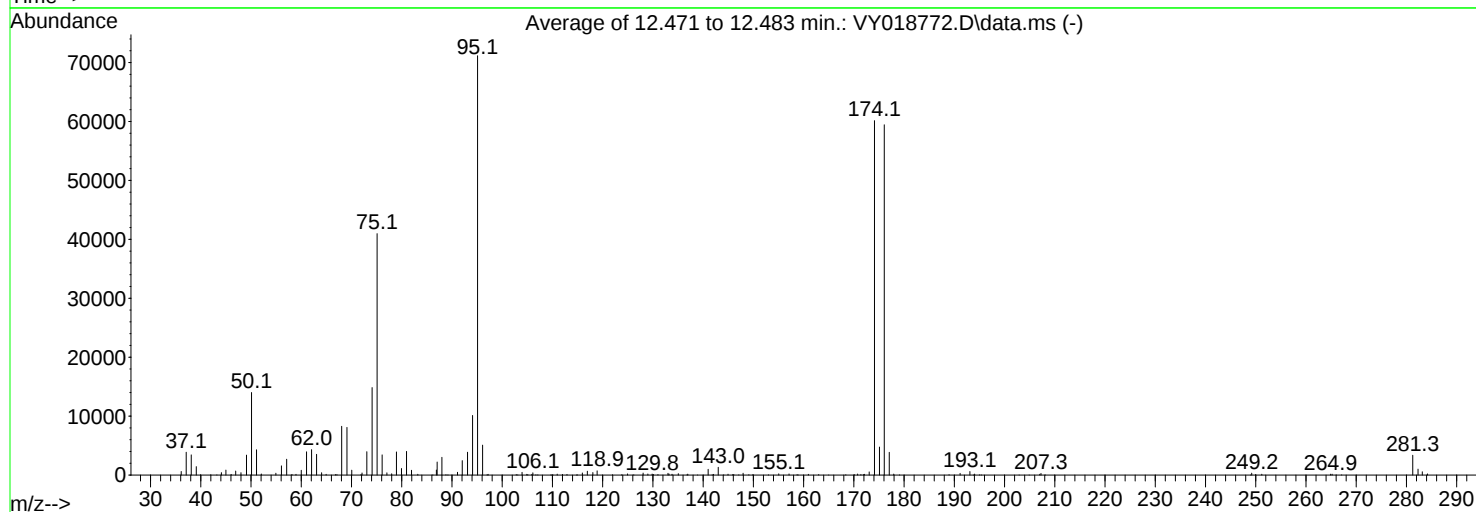


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY071124\
Data File : VY018772.D
Acq On : 11 Jul 2024 10:49
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Title : SW846 8260
Last Update : Tue Jul 09 14:28:51 2024

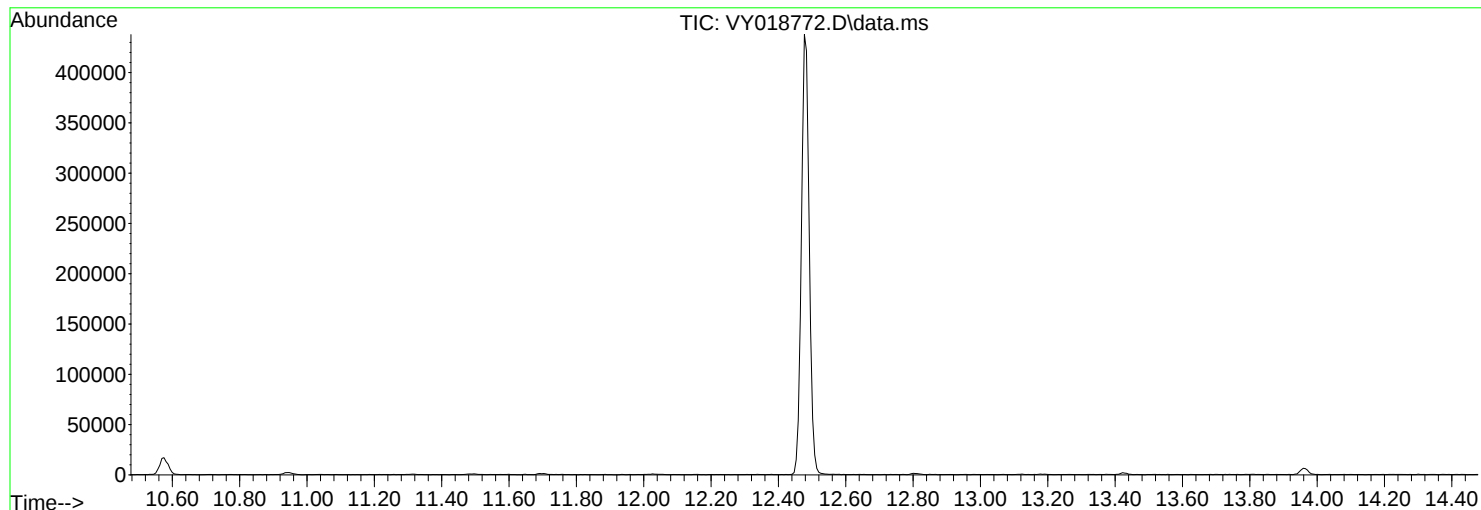

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	14011	PASS
75	95	30	60	57.6	40968	PASS
95	95	100	100	100.0	71160	PASS
96	95	5	9	7.1	5080	PASS
173	174	0.00	2	0.9	542	PASS
174	95	50	100	84.5	60149	PASS
175	174	5	9	7.9	4758	PASS
176	174	95	101	98.8	59443	PASS
177	176	5	9	6.5	3861	PASS