

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080522\
 Data File : VY009866.D
 Acq On : 05 Aug 2022 21:20
 Operator : KP/MD
 Sample : N4064-05
 Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SB-13

Quant Time: Aug 06 01:22:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080322S.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 04 02:27:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.777	168	17039	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	32143	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	33619	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	14273	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	8979	66.052	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	132.100%
35) Dibromofluoromethane	7.710	113	8426	42.994	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	85.980%
50) Toluene-d8	10.179	98	29077	50.623	ug/l	0.00
Spiked Amount	50.000	Range	78 - 125	Recovery	=	101.240%
62) 4-Bromofluorobenzene	12.477	95	7752	29.211	ug/l	0.00
Spiked Amount	50.000	Range	50 - 146	Recovery	=	58.420%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080522\
Data File : VY009866.D
Acq On : 05 Aug 2022 21:20
Operator : KP/MD
Sample : N4064-05
Misc : 5.01g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SB-13

Quant Time: Aug 06 01:22:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080322S.M
Quant Title : SW846 8260
QLast Update : Thu Aug 04 02:27:45 2022
Response via : Initial Calibration




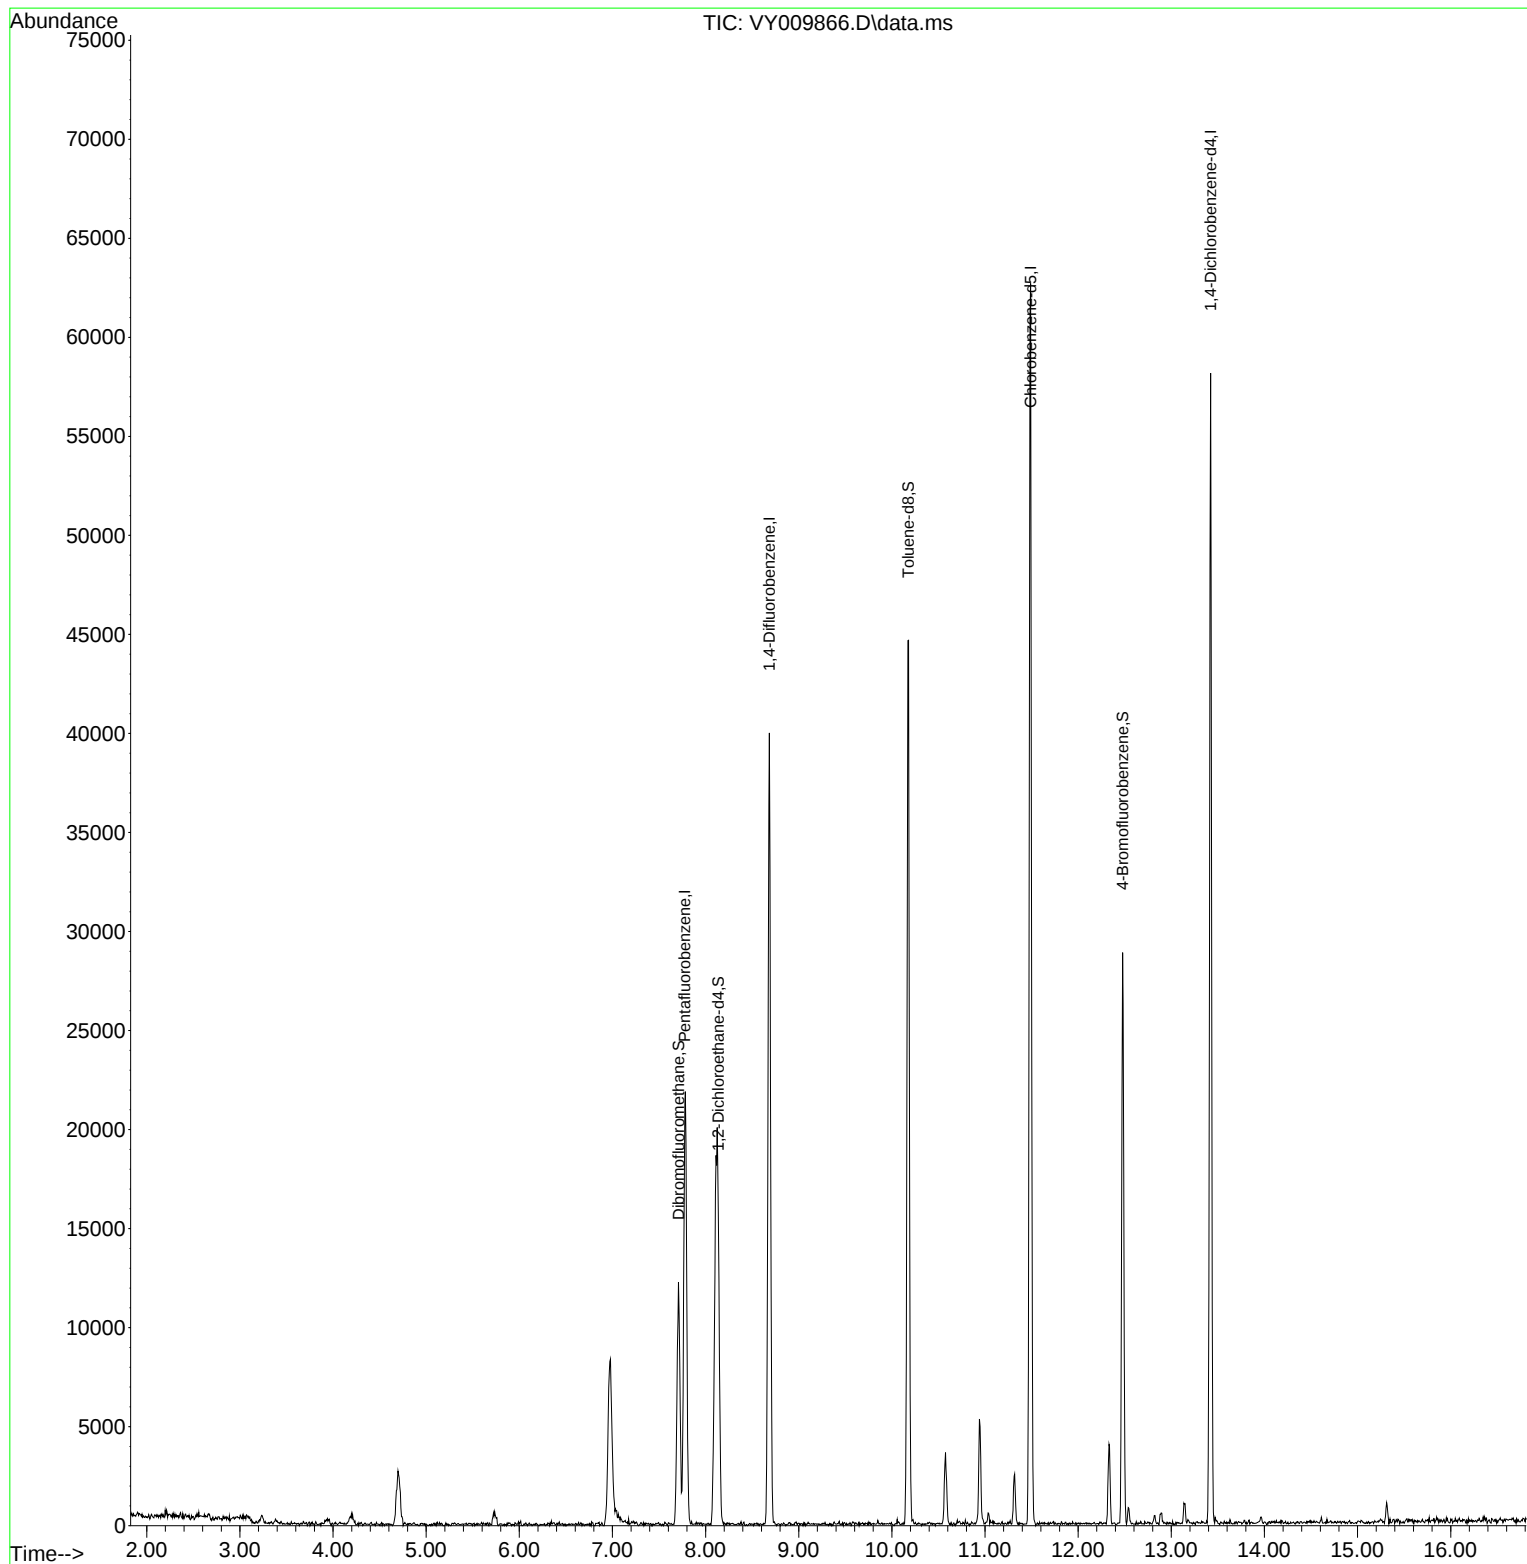




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.777 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY009866.D
Acq: 05 Aug 2022 21:20




Instrument :
MSVOA_Y
ClientSampleId :
SB-13


Tgt Ion:168 Resp: 17039
Ion Ratio Lower Upper
168 100
99 49.7 44.7 67.1

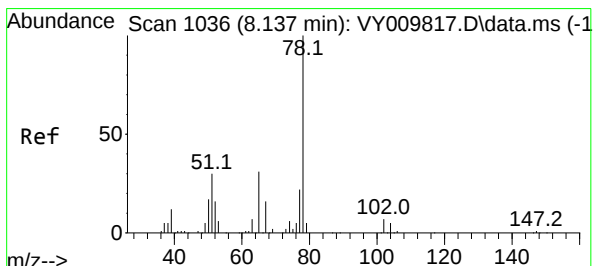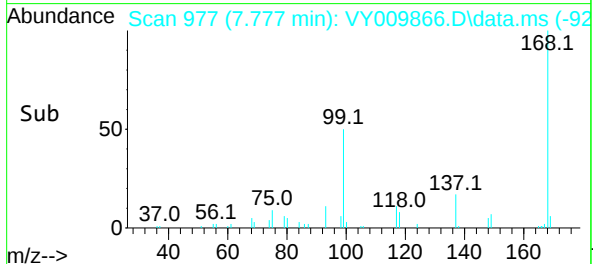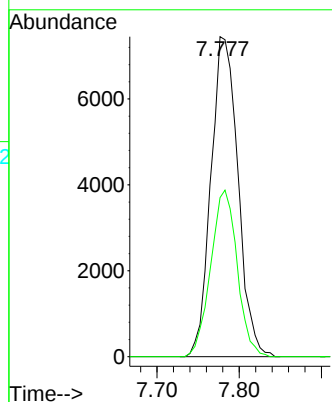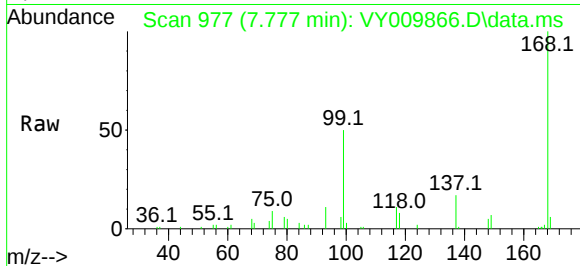

#33
1,2-Dichloroethane-d4
Concen: 66.052 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.001 min
Lab File: VY009866.D
Acq: 05 Aug 2022 21:20

Tgt Ion: 65 Resp: 8979
Ion Ratio Lower Upper
65 100
67 56.8 0.0 112.4

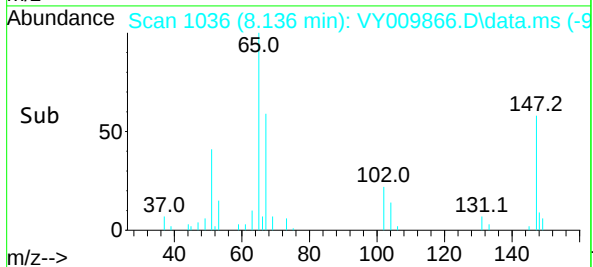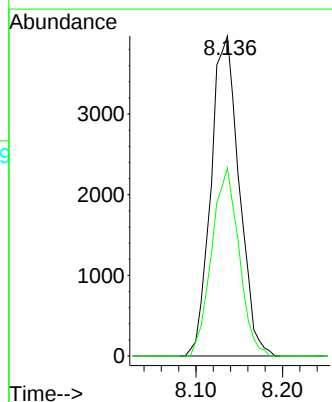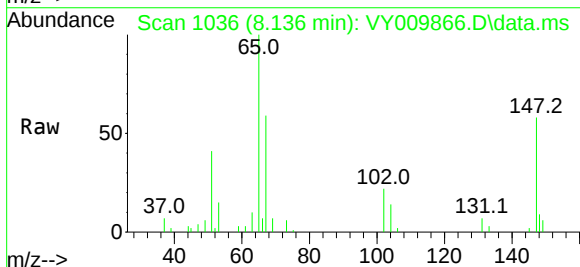

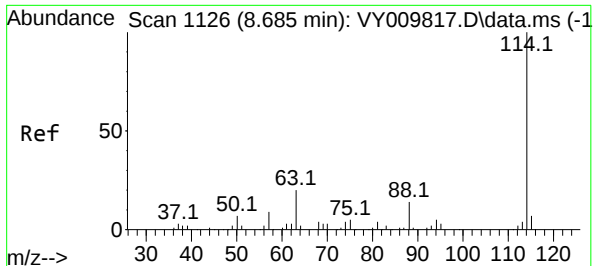

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY009866.D

Acq: 05 Aug 2022 21:20

Instrument :

MSVOA_Y

ClientSampleId :

SB-13





Tgt Ion:114 Resp: 32143

Ion Ratio Lower Upper

114 100

63 20.4 0.0 39.2

88 14.6 0.0 27.6

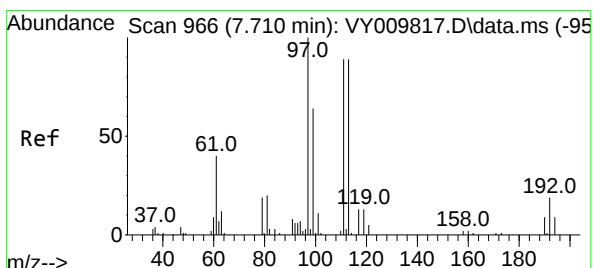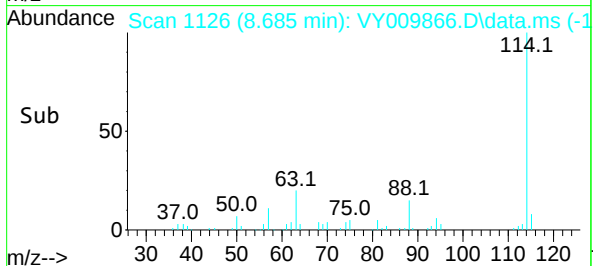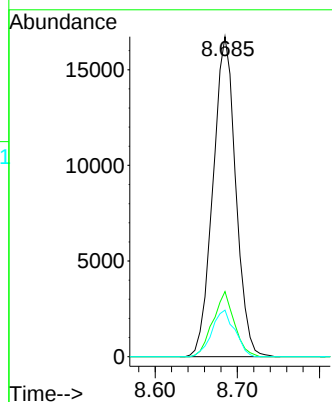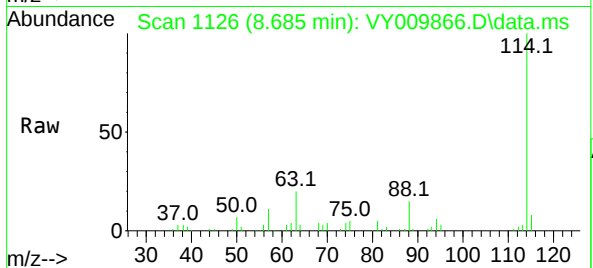

#35

Dibromofluoromethane

Concen: 42.994 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.000 min

Lab File: VY009866.D

Acq: 05 Aug 2022 21:20




Tgt Ion:113 Resp: 8426


Ion Ratio Lower Upper

113 100

111 96.4 82.4 123.6

192 20.9 16.5 24.7


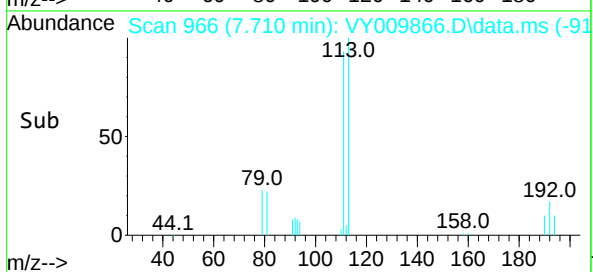
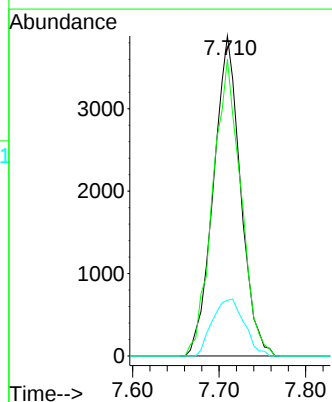
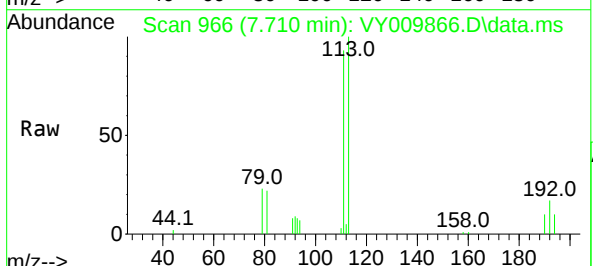


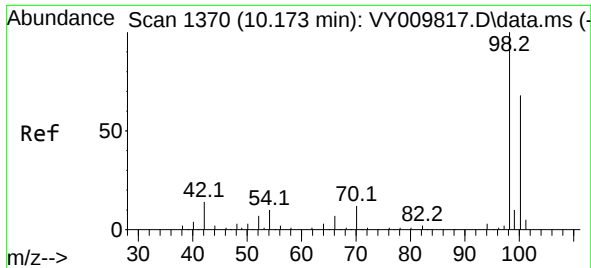

#50
Toluene-d8
Concen: 50.623 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY009866.D
Acq: 05 Aug 2022 21:20




Instrument :
MSVOA_Y
ClientSampleId :
SB-13


Tgt Ion: 98 Resp: 29077
Ion Ratio Lower Upper
98 100
100 62.7 53.4 80.2

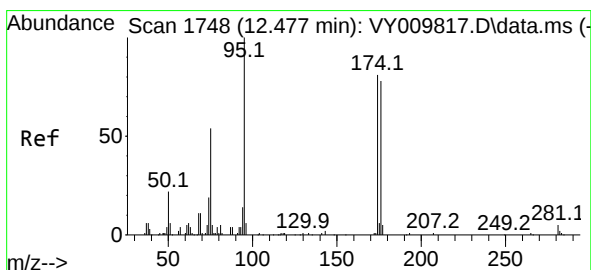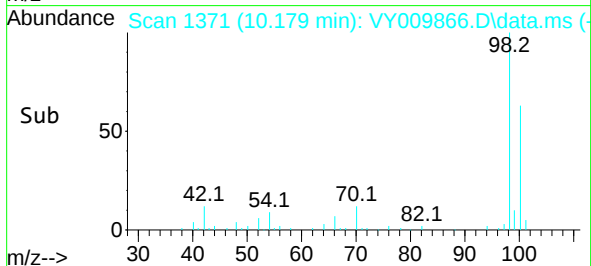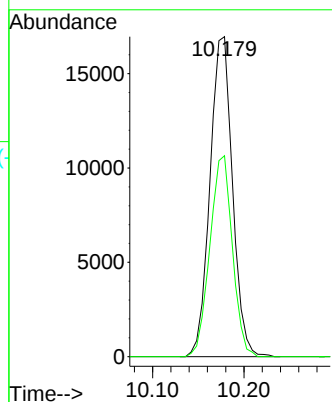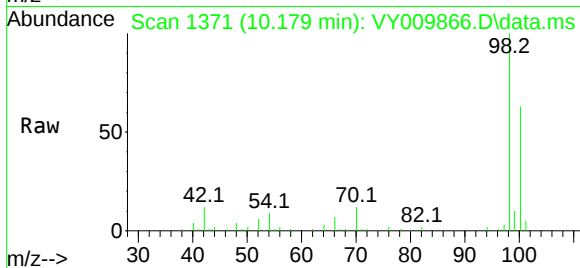

#62
4-Bromofluorobenzene
Concen: 29.211 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY009866.D
Acq: 05 Aug 2022 21:20

Tgt Ion: 95 Resp: 7752
Ion Ratio Lower Upper
95 100
174 88.3 0.0 168.6
176 85.2 0.0 163.6


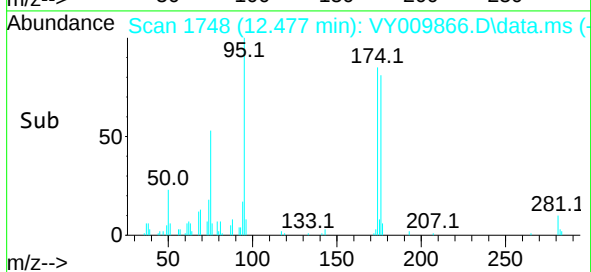
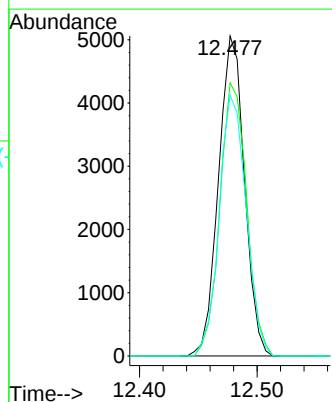
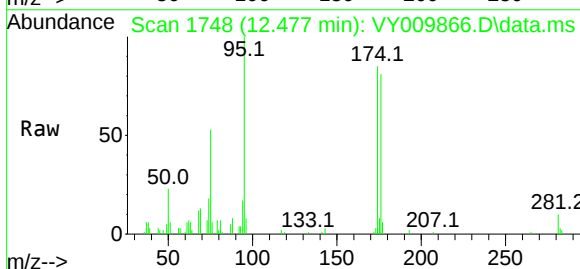


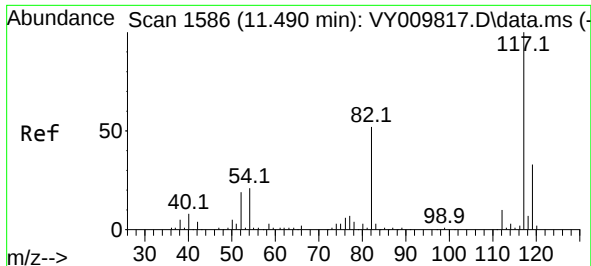

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY009866.D
Acq: 05 Aug 2022 21:20

Instrument :
MSVOA_Y
ClientSampleId :
SB-13

Tgt Ion:117 Resp: 33619
Ion Ratio Lower Upper
117 100
82 52.6 41.7 62.5
119 32.5 26.6 40.0

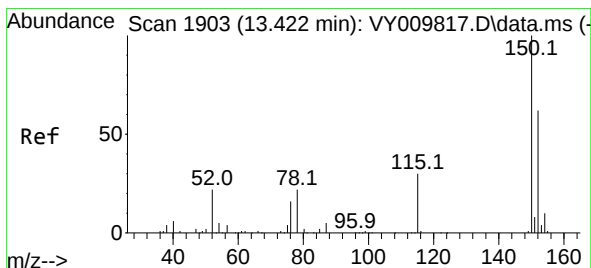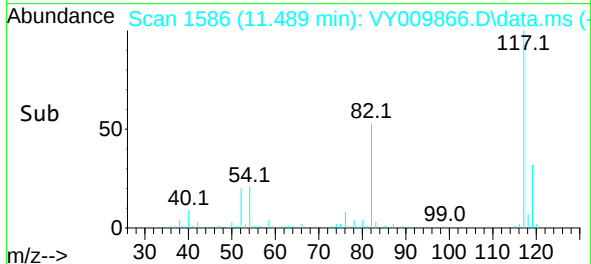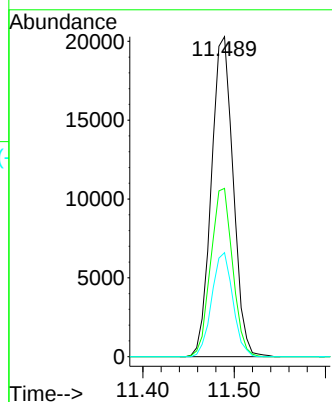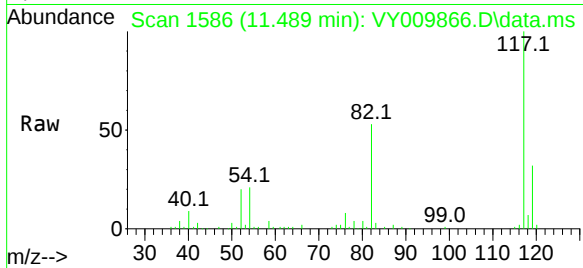

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY009866.D
Acq: 05 Aug 2022 21:20

Tgt Ion:152 Resp: 14273
Ion Ratio Lower Upper
152 100
115 58.5 28.9 86.7
150 154.3 0.0 354.2

