

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080822\
 Data File : VY009894.D
 Acq On : 09 Aug 2022 00:47
 Operator : KP/MD
 Sample : N3963-07
 Misc : 3.78g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 RVE-212

Quant Time: Aug 09 02:20:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080822S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 08 17:55:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.783	168	58153	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	115742	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	112590	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	50553	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	27983	62.957	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	125.920%
35) Dibromofluoromethane	7.710	113	25521	40.619	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	81.240%
50) Toluene-d8	10.173	98	92895	48.624	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	97.240%
62) 4-Bromofluorobenzene	12.477	95	30287	34.524	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	69.040%
Target Compounds						
					Qvalue	
18) Methyl Acetate	4.466	43	264	Below Cal	#	52
20) Methylene Chloride	4.698	84	6161	Below Cal		84
25) 2-Butanone	6.972	43	544	2.014	ug/l #	48
31) Cyclohexane	7.771	56	1216	1.077	ug/l #	1
36) 1,1-Dichloropropene	7.777	75	5075	4.787	ug/l #	48
38) Carbon Tetrachloride	7.783	117	5724	5.440	ug/l #	16
76) 1,2,3-Trichloropropane	12.477	75	15823	28.608	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.477	75	15823	57.839	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080822\
Data File : VY009894.D
Acq On : 09 Aug 2022 00:47
Operator : KP/MD
Sample : N3963-07
Misc : 3.78g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
RVE-212


Quant Time: Aug 09 02:20:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080822S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 08 17:55:50 2022
Response via : Initial Calibration

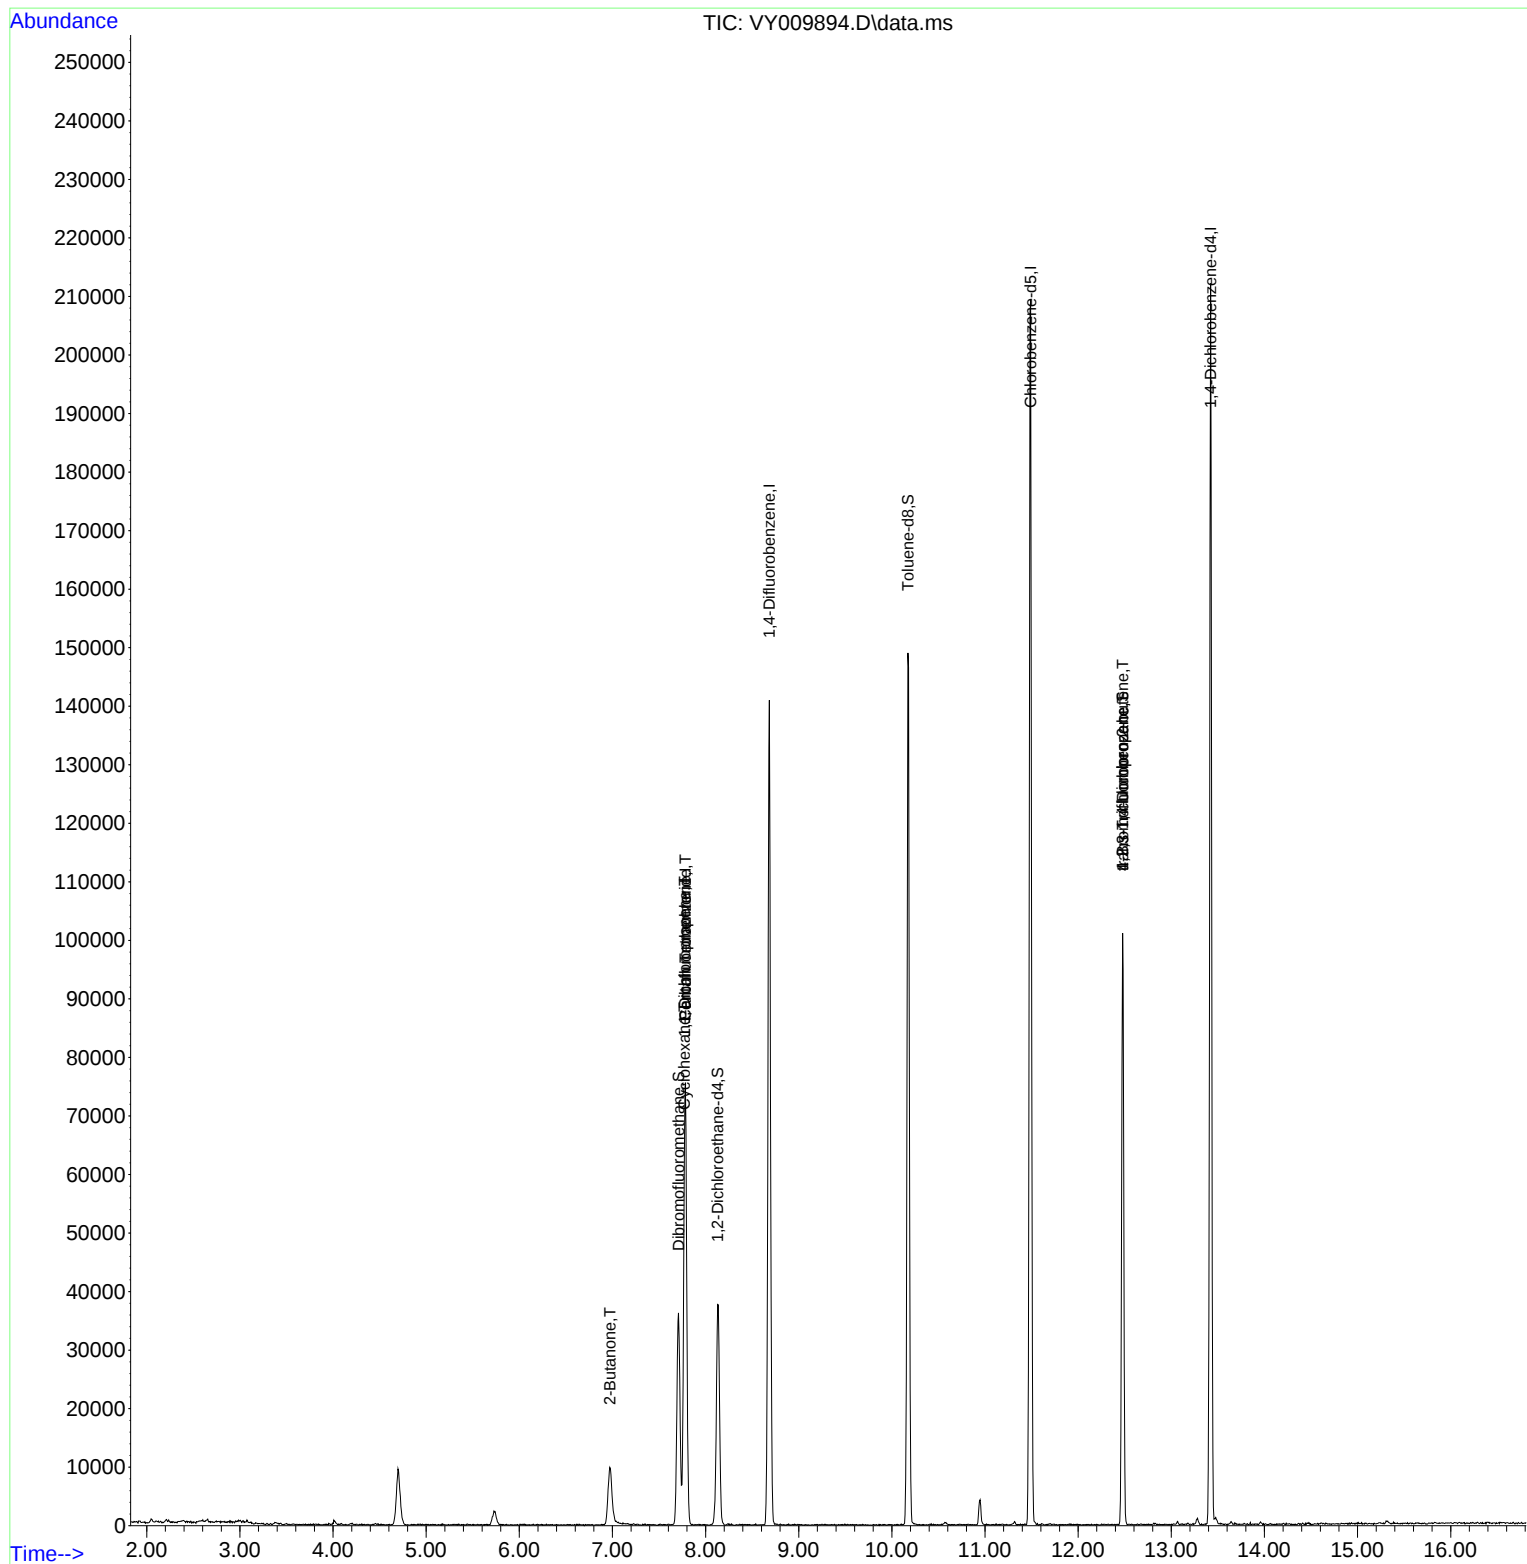



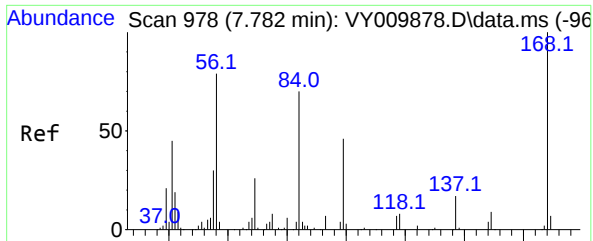


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. 0.001 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47

Instrument :
MSVOA_Y
ClientSampleId :
RVE-212



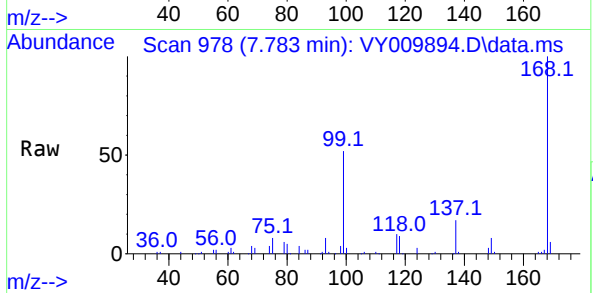



Tgt Ion:168 Resp: 58153
Ion Ratio Lower Upper
168 100
99 52.2 42.1 63.1

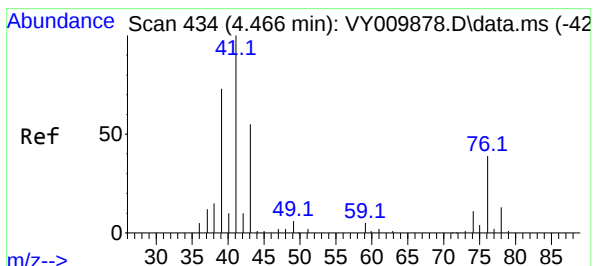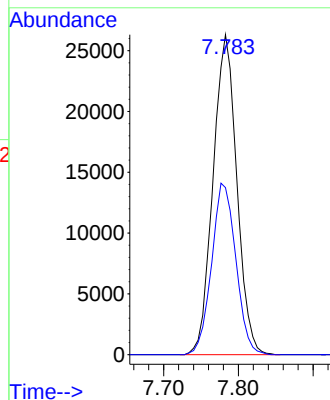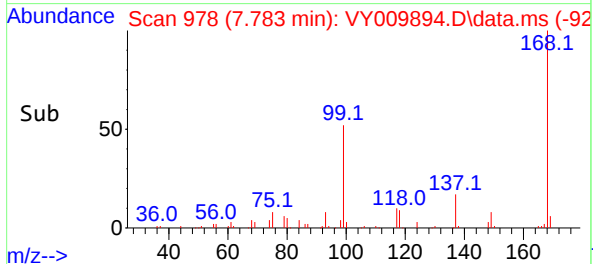

#18
Methyl Acetate
Concen: Below Cal
RT: 4.466 min Scan# 434
Delta R.T. 0.000 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47


Tgt Ion: 43 Resp: 264
Ion Ratio Lower Upper
43 100
74 0.0 18.8 28.2#

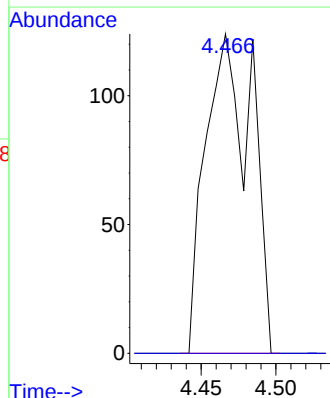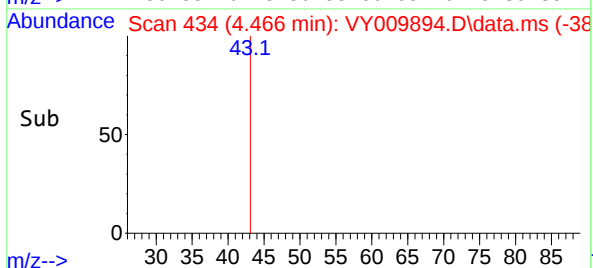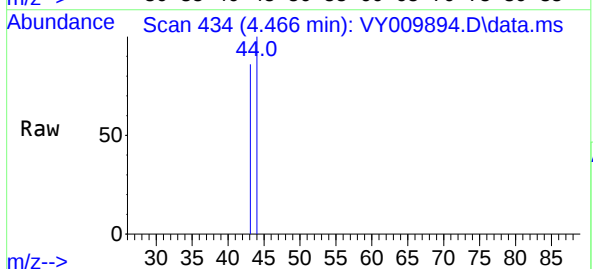

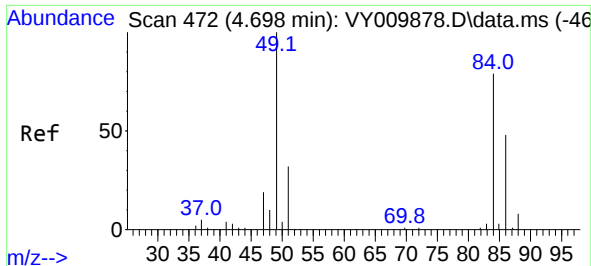




#20
Methylene Chloride
Concen: Below Cal
RT: 4.698 min Scan# 41
Delta R.T. -0.000 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47

Instrument :
MSVOA_Y
ClientSampleId :
RVE-212



Tgt Ion: 84 Resp: 6161




Ion	Ratio	Lower	Upper
84	100		
49	143.4	98.2	147.4
51	48.4	33.4	50.0
86	77.6	52.3	78.5

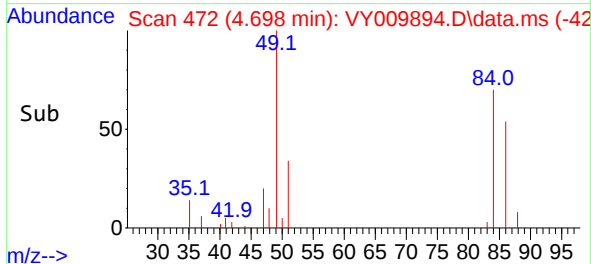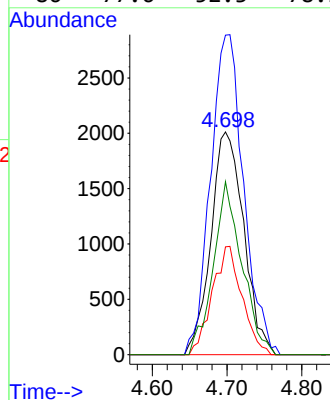


#25
2-Butanone
Concen: 2.014 ug/l
RT: 6.972 min Scan# 845
Delta R.T. -0.006 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47

Tgt Ion: 43 Resp: 544


Ion	Ratio	Lower	Upper
43	100		
72	0.0	21.5	32.3#

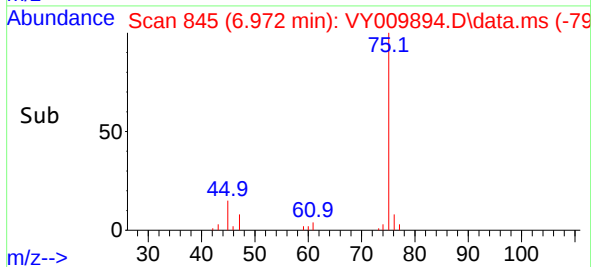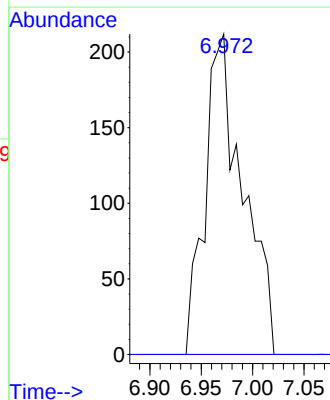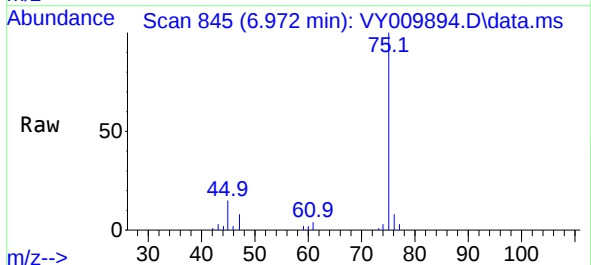



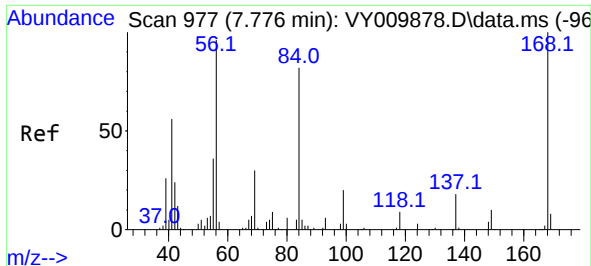


#31
Cyclohexane
Concen: 1.077 ug/l
RT: 7.771 min Scan# 91
Delta R.T. -0.005 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47


Instrument :
MSVOA_Y
ClientSampleId :
RVE-212





Tgt Ion: 56 Resp: 1216
Ion Ratio Lower Upper
56 100
69 153.9 26.0 39.0#
84 193.4 69.5 104.3#

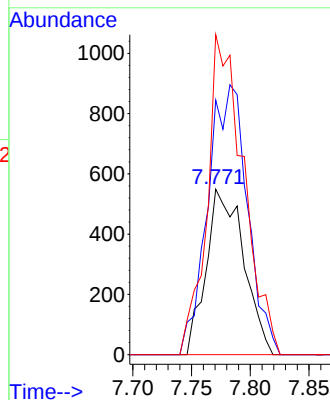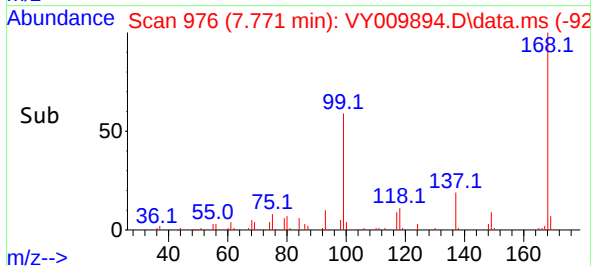


#33
1,2-Dichloroethane-d4
Concen: 62.957 ug/l
RT: 8.130 min Scan# 1035
Delta R.T. 0.000 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47

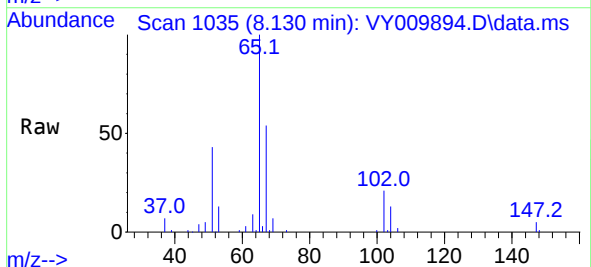

Tgt Ion: 65 Resp: 27983
Ion Ratio Lower Upper
65 100
67 55.2 0.0 108.4

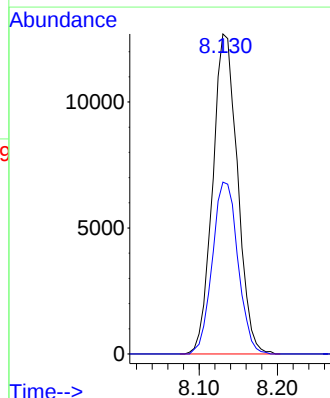

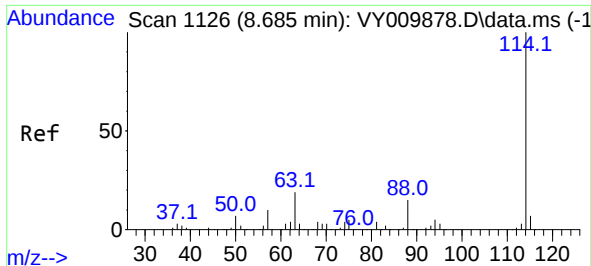

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY009894.D

Acq: 09 Aug 2022 00:47

Instrument :

MSVOA_Y

ClientSampleId :

RVE-212





Tgt Ion:114 Resp: 115742

Ion Ratio Lower Upper

114 100

63 19.3 0.0 38.0

88 14.6 0.0 30.0

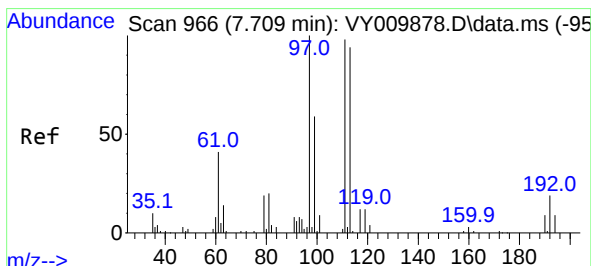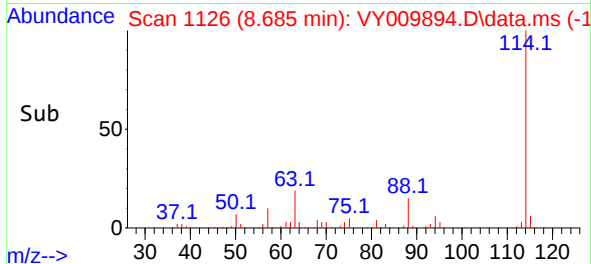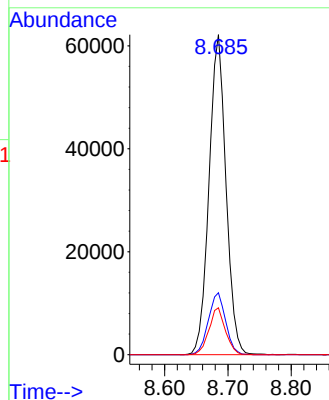

#35

Dibromofluoromethane

Concen: 40.619 ug/l

RT: 7.710 min Scan# 966

Delta R.T. 0.001 min

Lab File: VY009894.D

Acq: 09 Aug 2022 00:47




Tgt Ion:113 Resp: 25521


Ion Ratio Lower Upper

113 100

111 103.1 80.6 120.8

192 19.4 16.2 24.4



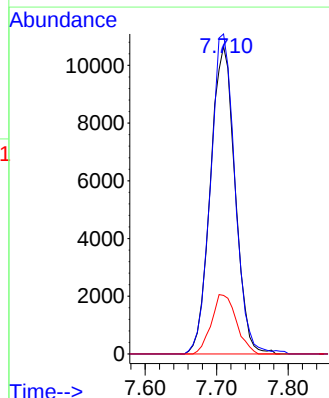
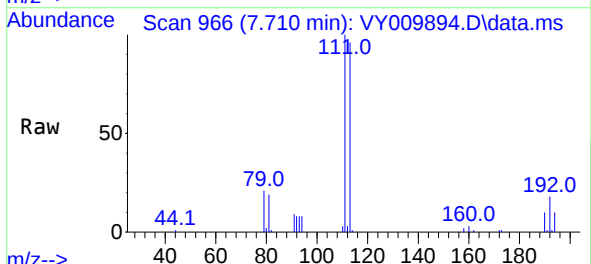


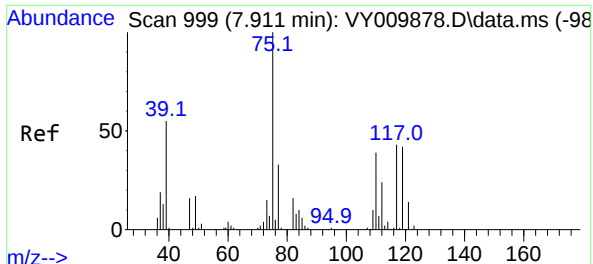

#36
1,1-Dichloropropene
Concen: 4.787 ug/l
RT: 7.777 min Scan# 91
Delta R.T. -0.134 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47




Instrument :
MSVOA_Y
ClientSampleId :
RVE-212


Tgt Ion: 75 Resp: 5075
Ion Ratio Lower Upper
75 100
110 8.0 18.6 56.0#
77 0.0 25.0 37.4#

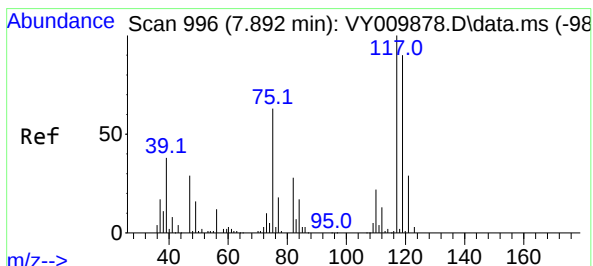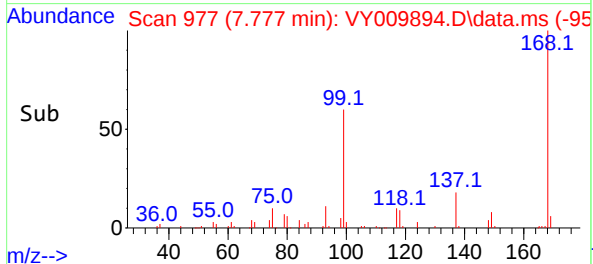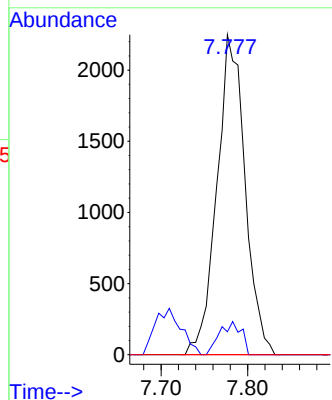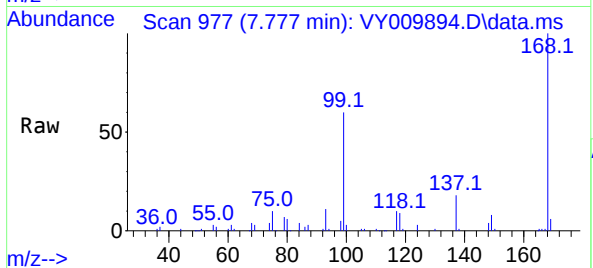

#38
Carbon Tetrachloride
Concen: 5.440 ug/l
RT: 7.783 min Scan# 978
Delta R.T. -0.109 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47

Tgt Ion: 117 Resp: 5724
Ion Ratio Lower Upper
117 100
119 5.1 75.9 113.9#
121 0.0 24.9 37.3#


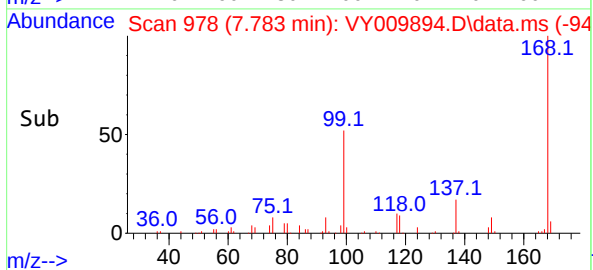
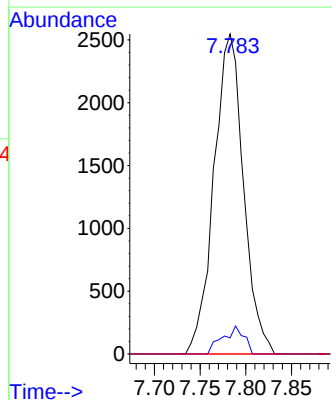
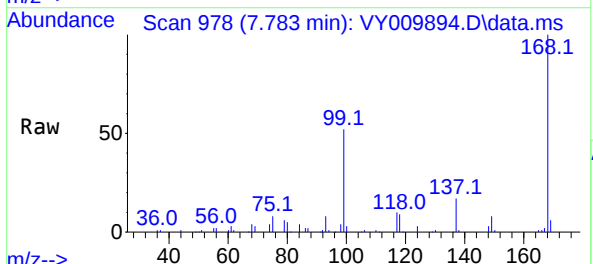


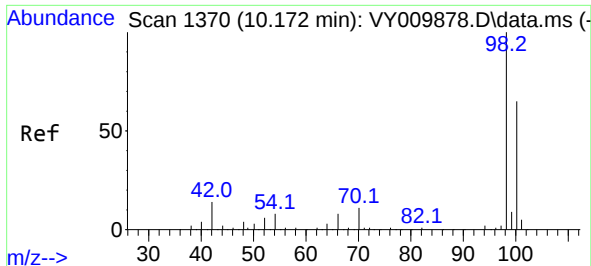

#50
Toluene-d8
Concen: 48.624 ug/l
RT: 10.173 min Scan# 11
Delta R.T. 0.001 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47




Instrument :
MSVOA_Y
ClientSampleId :
RVE-212


Tgt Ion: 98 Resp: 92895
Ion Ratio Lower Upper
98 100
100 66.3 52.9 79.3

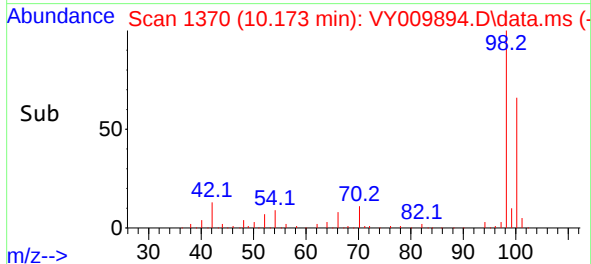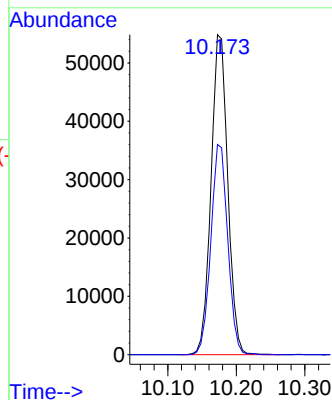

#62
4-Bromofluorobenzene
Concen: 34.524 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47

Tgt Ion: 95 Resp: 30287
Ion Ratio Lower Upper
95 100
174 83.4 0.0 173.8
176 80.0 0.0 167.0


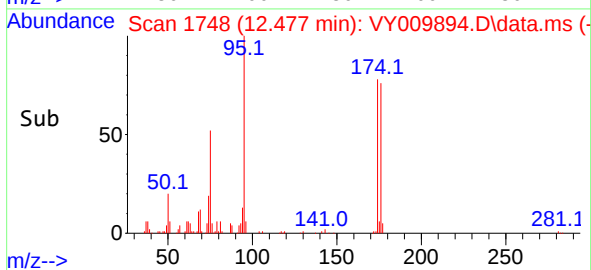
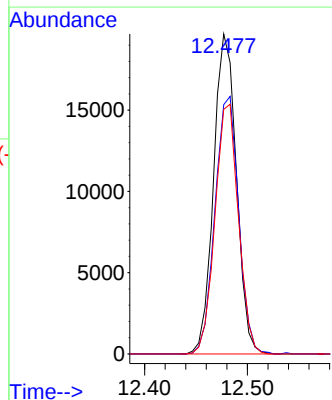
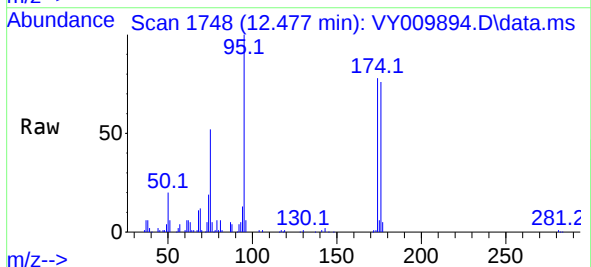


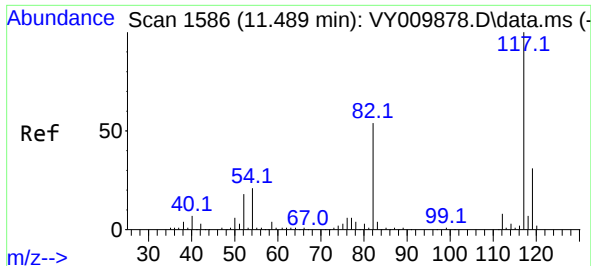

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47




Instrument :
MSVOA_Y
ClientSampleId :
RVE-212


Tgt Ion:117 Resp: 112590
Ion Ratio Lower Upper
117 100
82 52.4 41.8 62.6
119 33.0 25.6 38.4

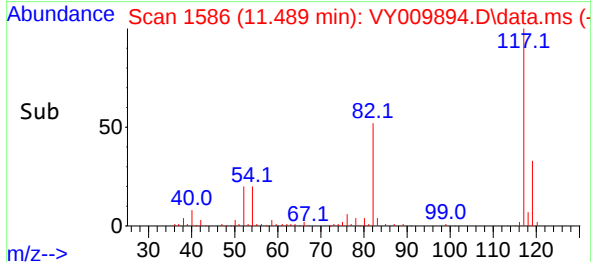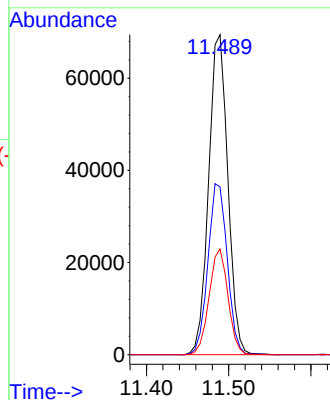

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47

Tgt Ion:152 Resp: 50553
Ion Ratio Lower Upper
152 100
115 57.9 28.6 85.9
150 157.6 0.0 349.8


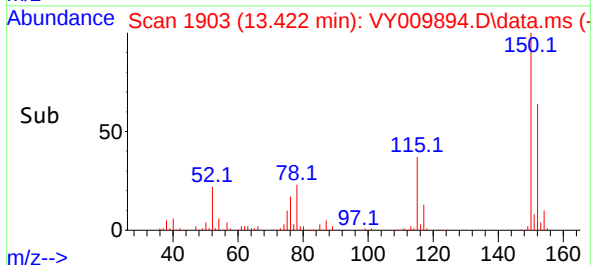
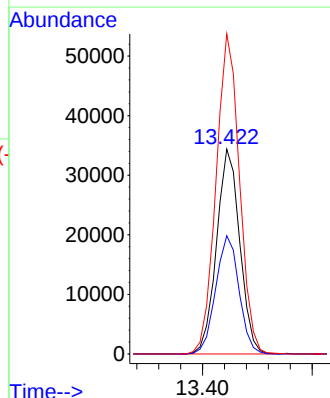
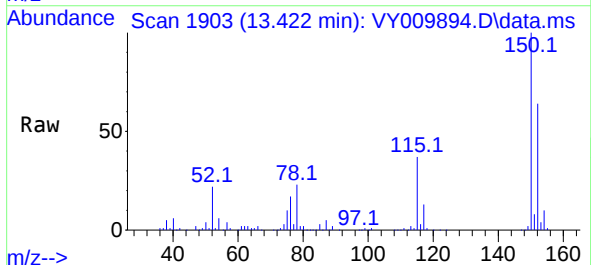


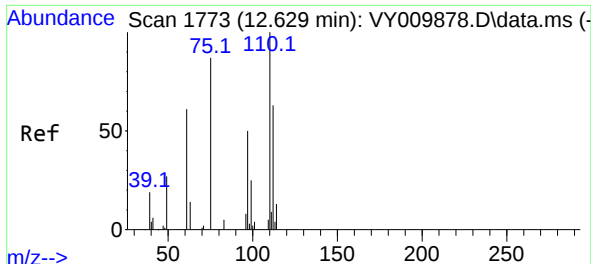

#76
1,2,3-Trichloropropane
Concen: 28.608 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.152 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47

Instrument :
MSVOA_Y
ClientSampleId :
RVE-212

Tgt Ion: 75 Resp: 15823
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#

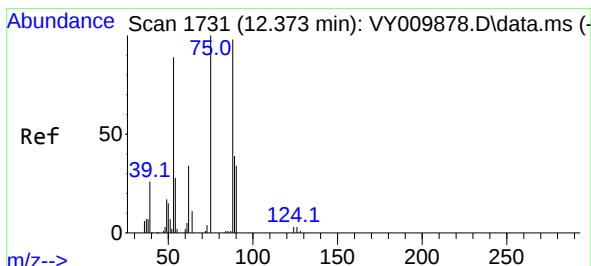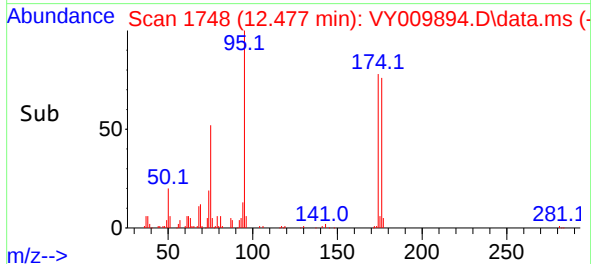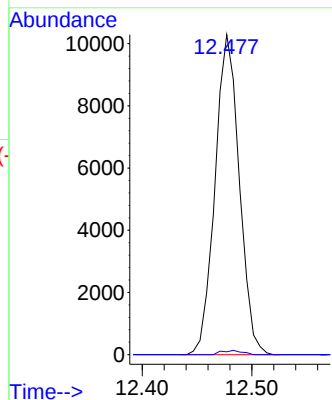

#81
trans-1,4-Dichloro-2-butene
Concen: 57.839 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.104 min
Lab File: VY009894.D
Acq: 09 Aug 2022 00:47

Tgt Ion: 75 Resp: 15823
Ion Ratio Lower Upper
75 100
53 0.0 71.4 107.2#
89 0.0 38.1 57.1#

