

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080822\
 Data File : VY009895.D
 Acq On : 09 Aug 2022 01:10
 Operator : KP/MD
 Sample : N3963-11
 Misc : 3.89g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 RVE-216

Quant Time: Aug 09 02:20:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080822S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 08 17:55:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.782	168	56056	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	113450	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	112302	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	52546	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	27528	64.383	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	128.760%
35) Dibromofluoromethane	7.709	113	25332	41.133	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	82.260%
50) Toluene-d8	10.178	98	92622	49.595	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	99.180%
62) 4-Bromofluorobenzene	12.477	95	30008	34.897	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	69.800%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080822\
Data File : VY009895.D
Acq On : 09 Aug 2022 01:10
Operator : KP/MD
Sample : N3963-11
Misc : 3.89g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
RVE-216

Quant Time: Aug 09 02:20:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080822S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 08 17:55:50 2022
Response via : Initial Calibration




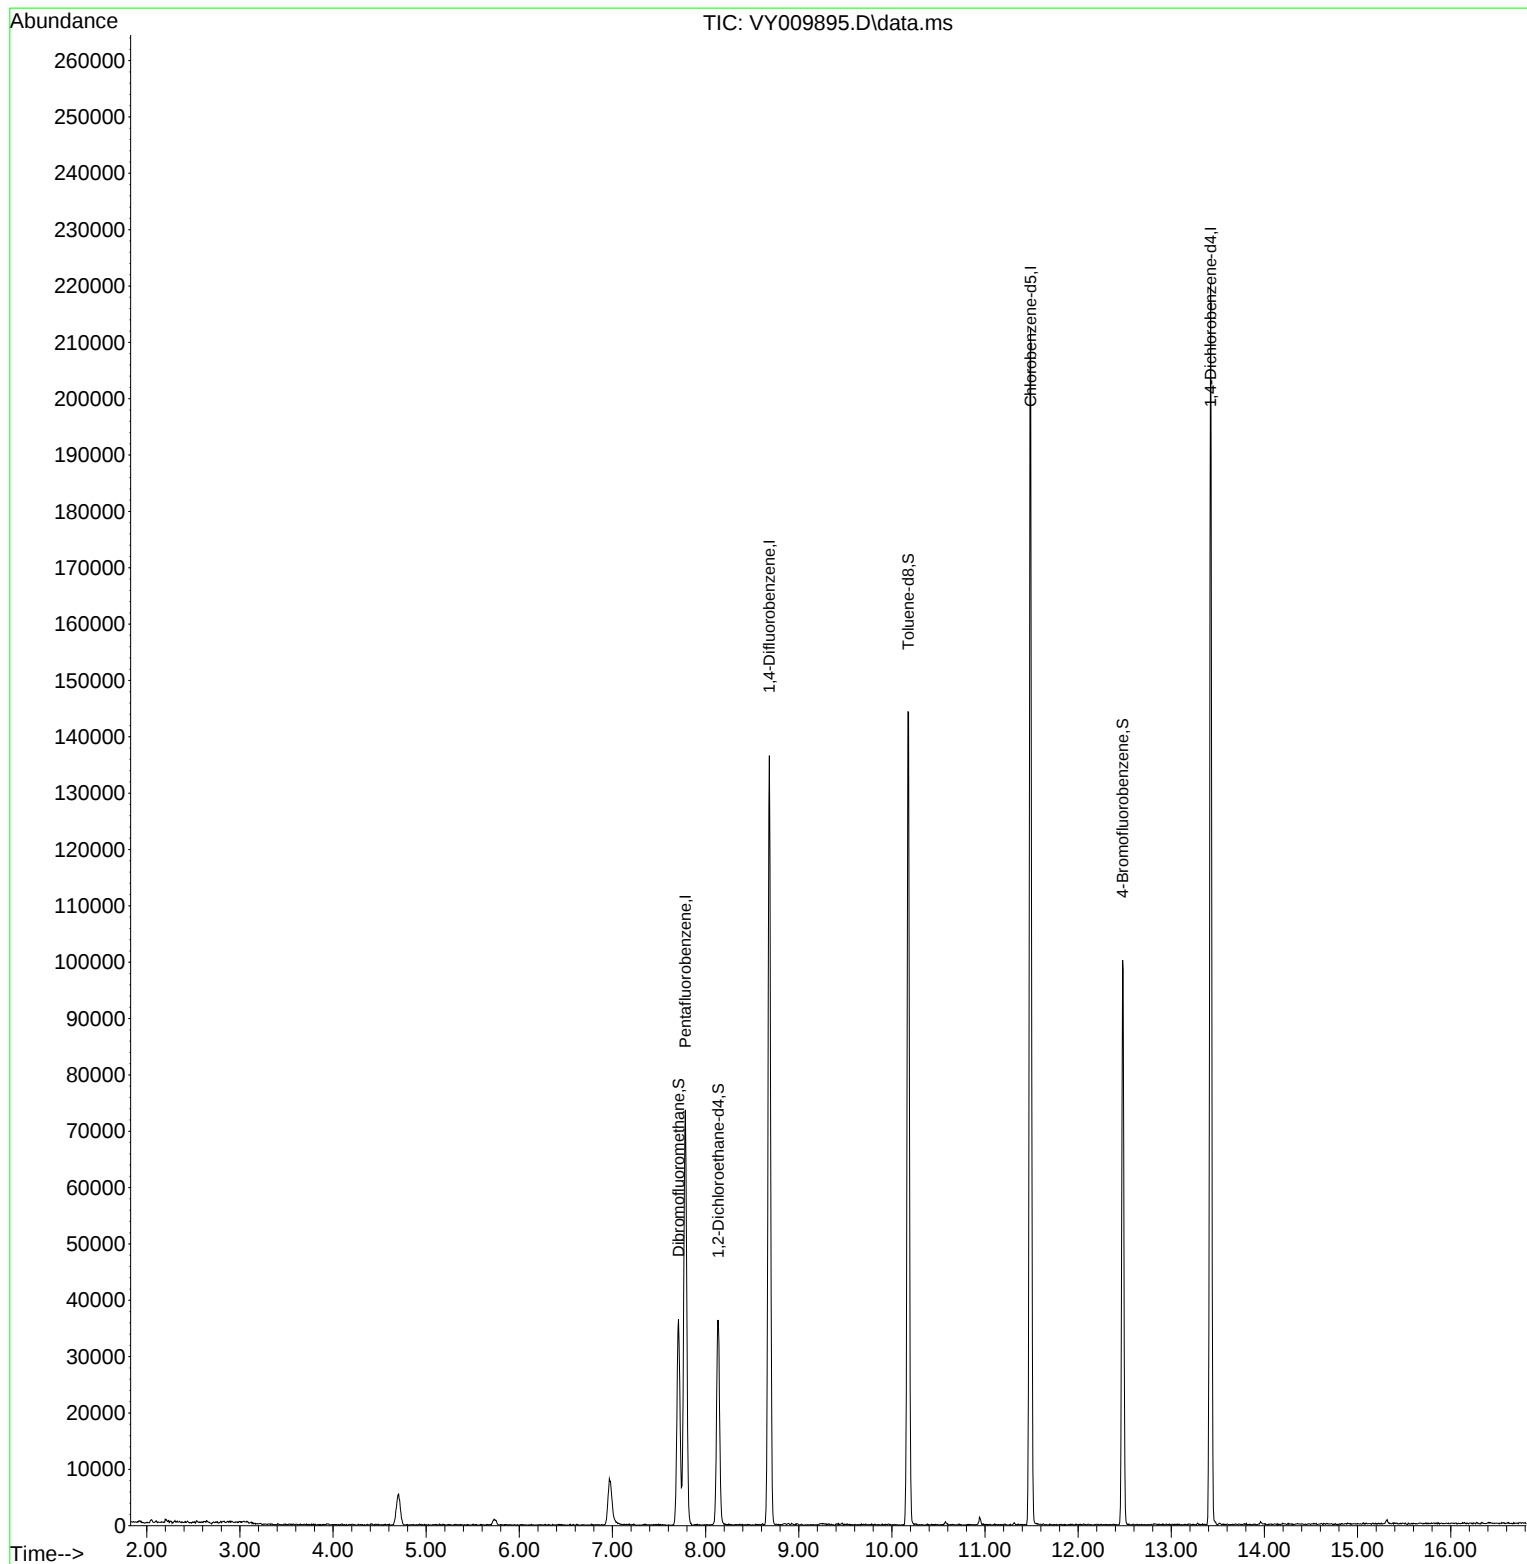


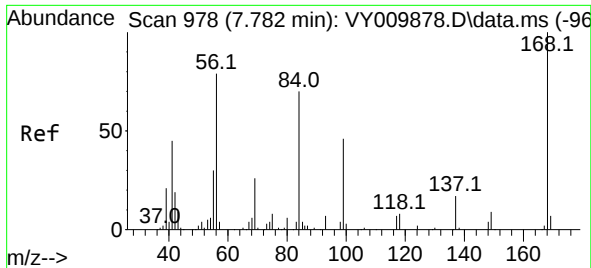

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.782 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY009895.D
Acq: 09 Aug 2022 01:10




Instrument :
MSVOA_Y
ClientSampleId :
RVE-216


Tgt Ion:168 Resp: 56056
Ion Ratio Lower Upper
168 100
99 53.8 42.1 63.1

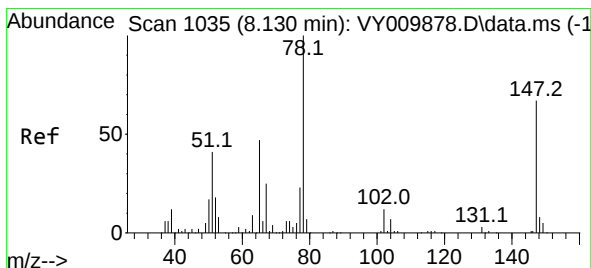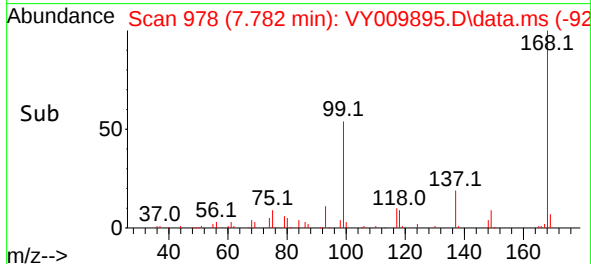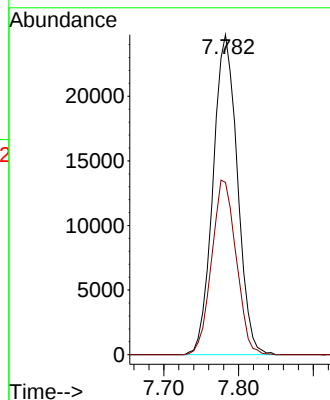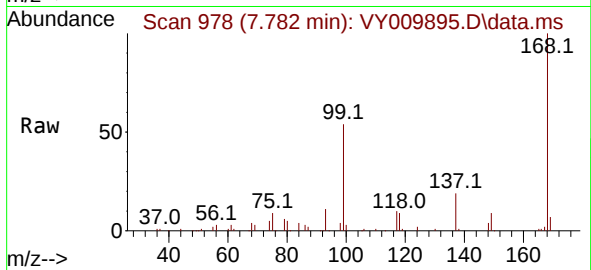

#33
1,2-Dichloroethane-d4
Concen: 64.383 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.006 min
Lab File: VY009895.D
Acq: 09 Aug 2022 01:10

Tgt Ion: 65 Resp: 27528
Ion Ratio Lower Upper
65 100
67 54.1 0.0 108.4

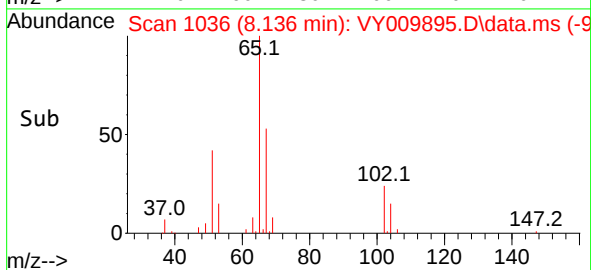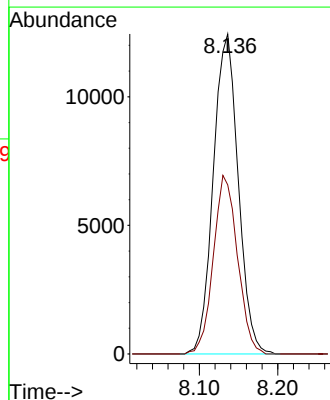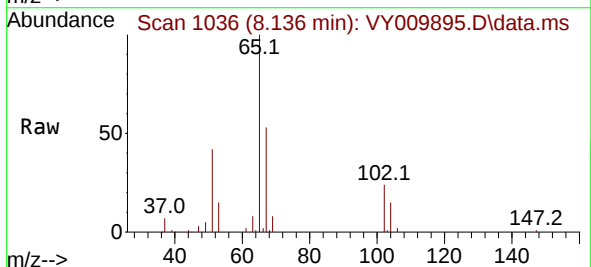

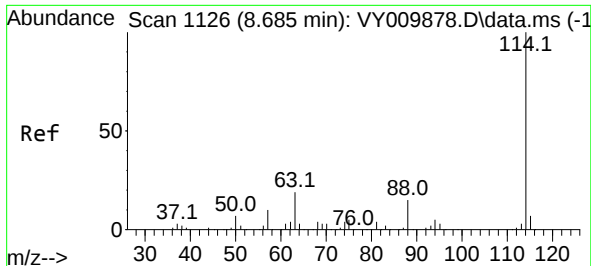

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY009895.D

Acq: 09 Aug 2022 01:10

Instrument :

MSVOA_Y

ClientSampleId :

RVE-216





Tgt Ion:114 Resp: 113450

Ion Ratio Lower Upper

114 100

63 18.8 0.0 38.0

88 14.6 0.0 30.0

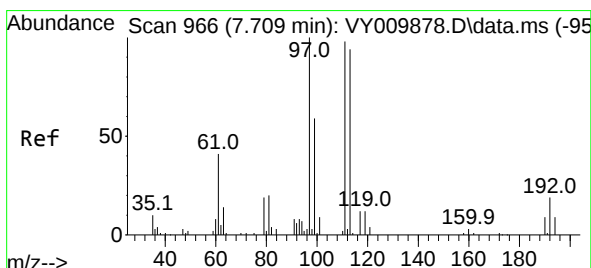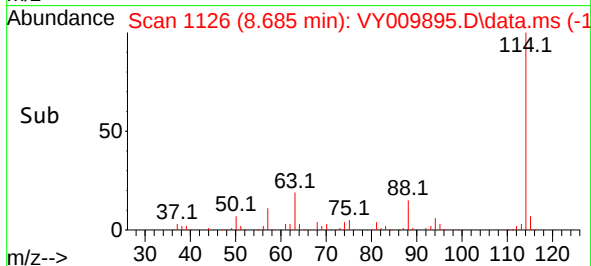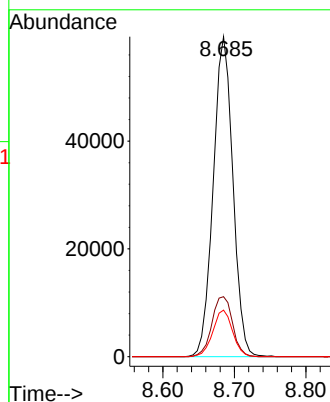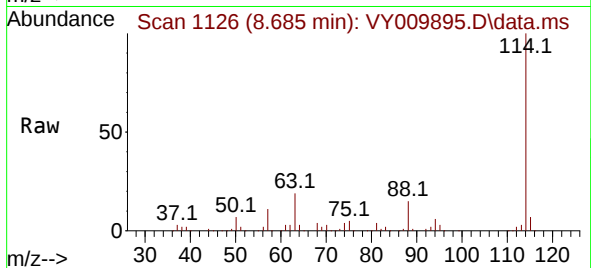

#35

Dibromofluoromethane

Concen: 41.133 ug/l

RT: 7.709 min Scan# 966

Delta R.T. 0.000 min

Lab File: VY009895.D

Acq: 09 Aug 2022 01:10




Tgt Ion:113 Resp: 25332


Ion Ratio Lower Upper

113 100

111 102.8 80.6 120.8

192 19.8 16.2 24.4


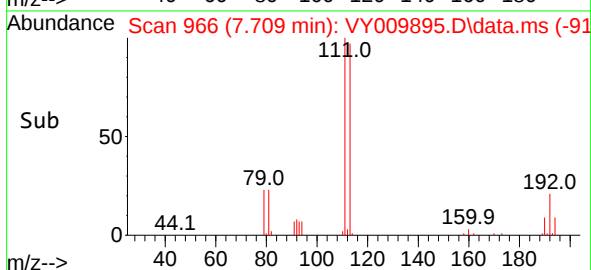
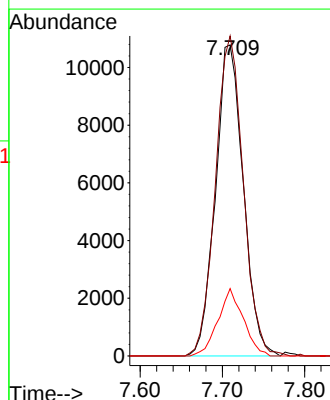
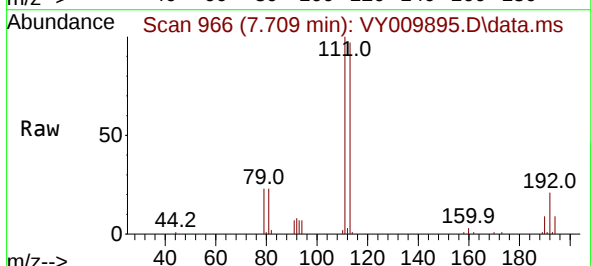


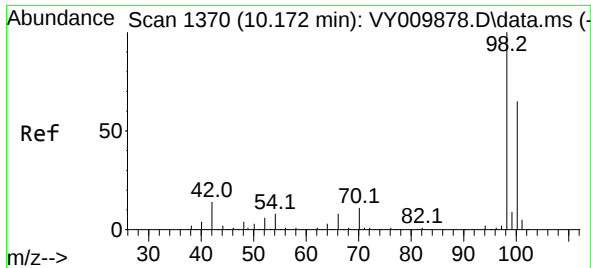

#50
Toluene-d8
Concen: 49.595 ug/l
RT: 10.178 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY009895.D
Acq: 09 Aug 2022 01:10




Instrument :
MSVOA_Y
ClientSampleId :
RVE-216


Tgt Ion: 98 Resp: 92622
Ion Ratio Lower Upper
98 100
100 67.0 52.9 79.3

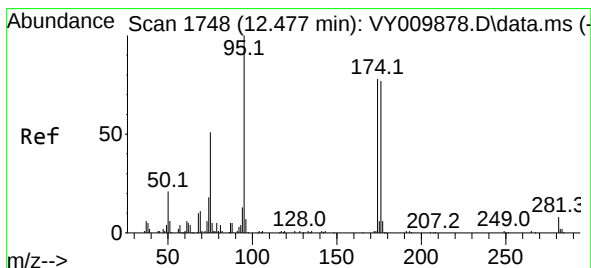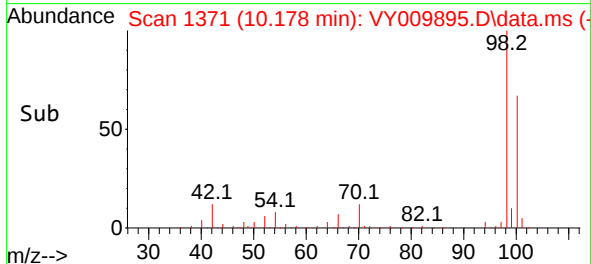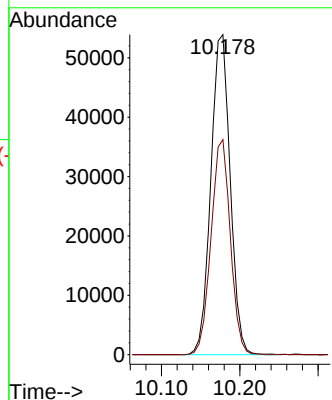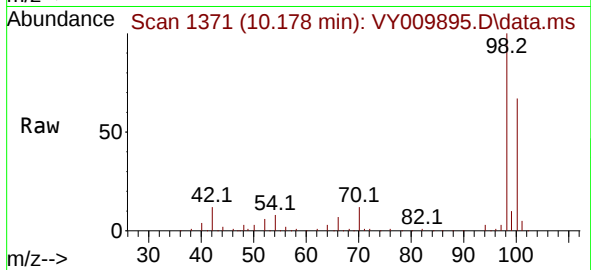

#62
4-Bromofluorobenzene
Concen: 34.897 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY009895.D
Acq: 09 Aug 2022 01:10

Tgt Ion: 95 Resp: 30008
Ion Ratio Lower Upper
95 100
174 85.1 0.0 173.8
176 81.7 0.0 167.0


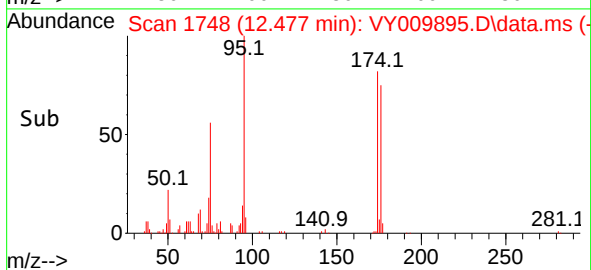
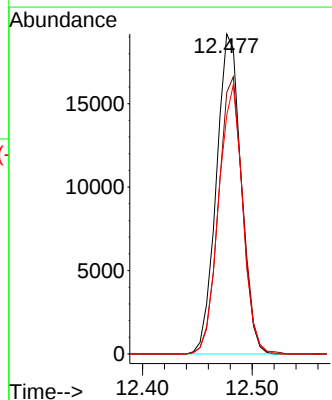
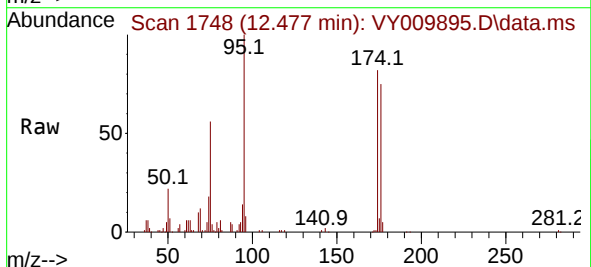


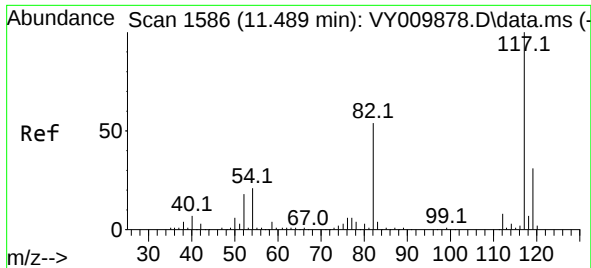

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY009895.D
Acq: 09 Aug 2022 01:10

Instrument :
MSVOA_Y
ClientSampleId :
RVE-216

Tgt Ion:117 Resp: 112302
Ion Ratio Lower Upper
117 100
82 53.8 41.8 62.6
119 31.4 25.6 38.4

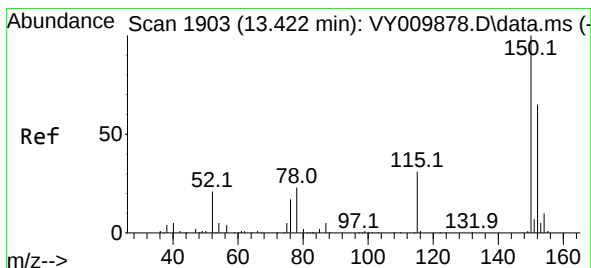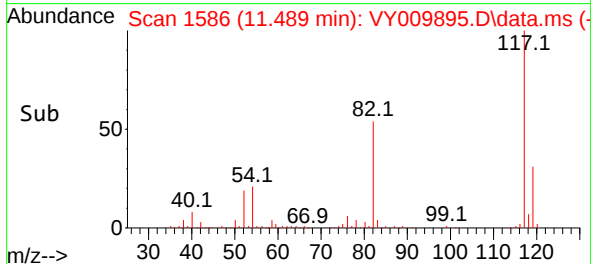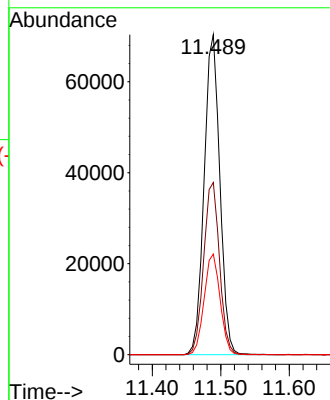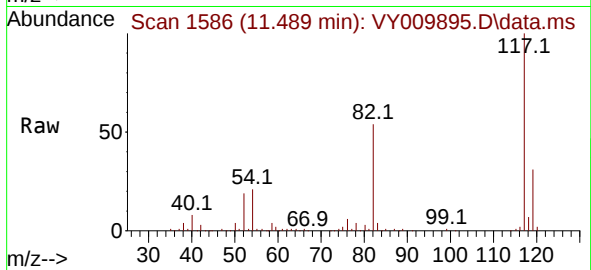

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY009895.D
Acq: 09 Aug 2022 01:10

Tgt Ion:152 Resp: 52546
Ion Ratio Lower Upper
152 100
115 57.5 28.6 85.9
150 157.2 0.0 349.8

